

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060622\
 Data File : PD070125.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Jun 2022 15:09
 Operator : AR\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 07 05:43:57 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060622.M
 Quant Title : GC Extractables
 QLast Update : Tue Jun 07 05:42:55 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.440	4.167	63415161	482.8E6	50.000	50.000
28)	SA Decachlor...	8.190	9.360	55033046	280.7E6	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.308	5.189	19922688	202.1E6	500.000	500.000
24)	Chlordane-2	4.808	5.662	23249515	227.3E6	500.000	500.000
25)	Chlordane-3	5.375	6.318	63711880	732.7E6	500.000	500.000
26)	Chlordane-4	5.433	6.395	54107347	851.9E6	500.000	500.000
27)	Chlordane-5	6.270	7.206	22478199	154.1E6	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060622\
Data File : PD070125.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Jun 2022 15:09
Operator : AR\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 07 05:43:57 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060622.M
Quant Title : GC Extractables
QLast Update : Tue Jun 07 05:42:55 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

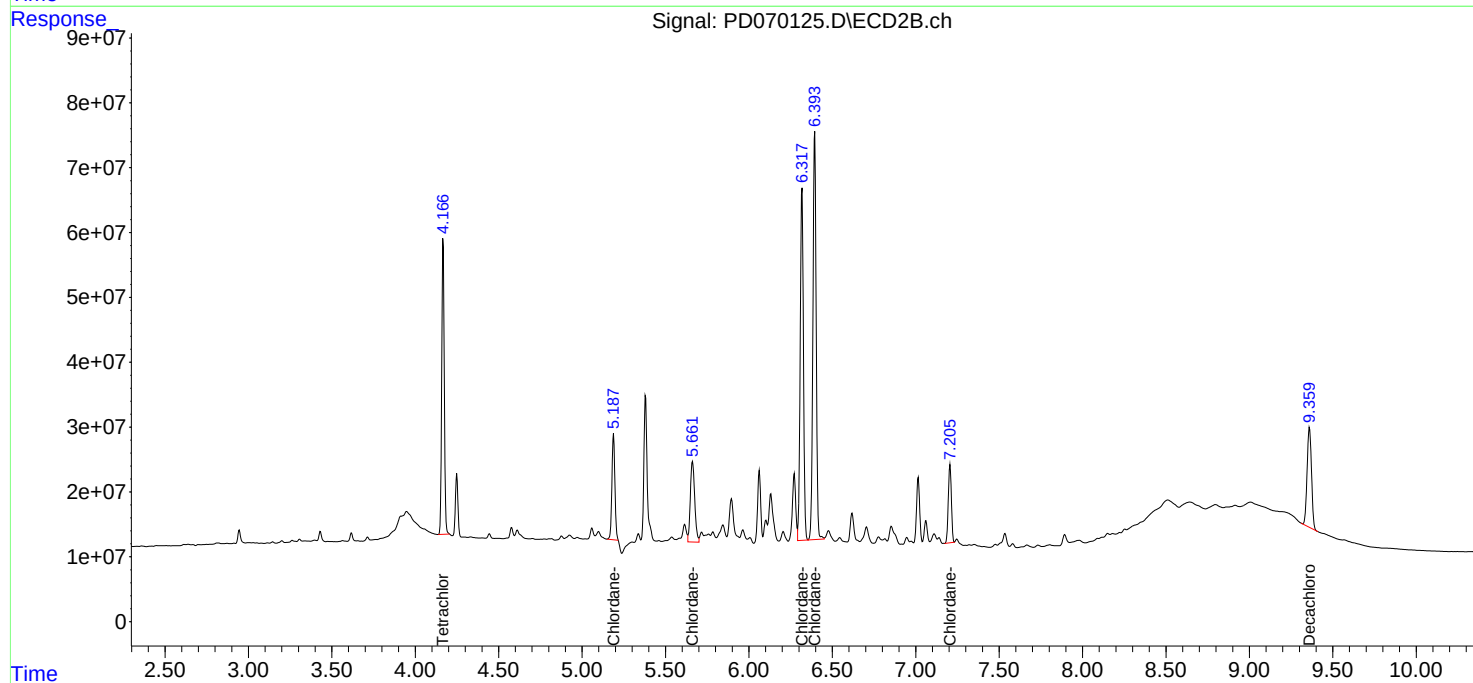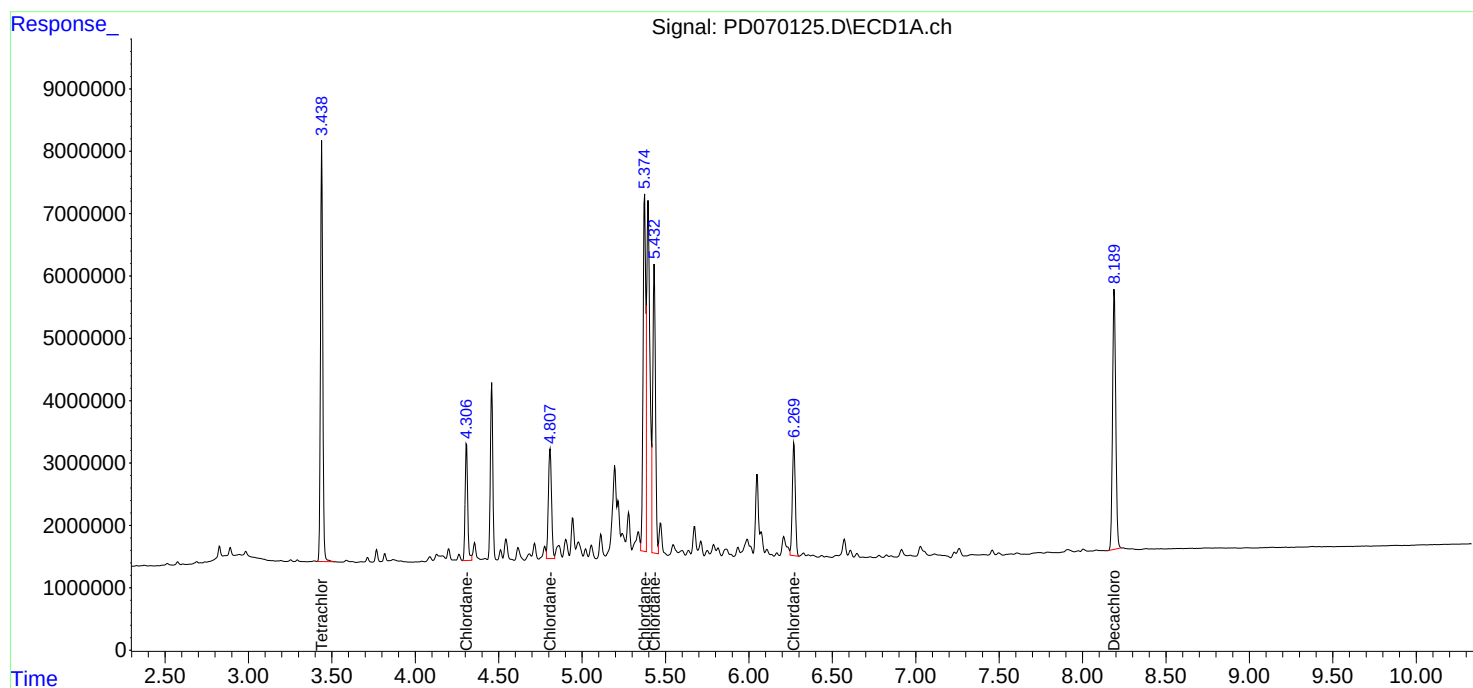


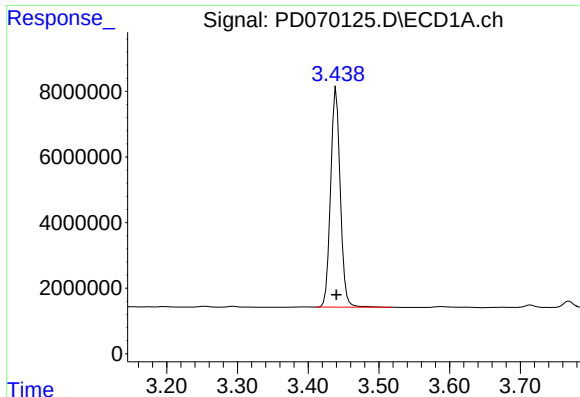

#1 Tetrachloro-m-xylene


R.T.: 3.440 min
Delta R.T.: 0.000 min
Response: 63415161
Conc: 50.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

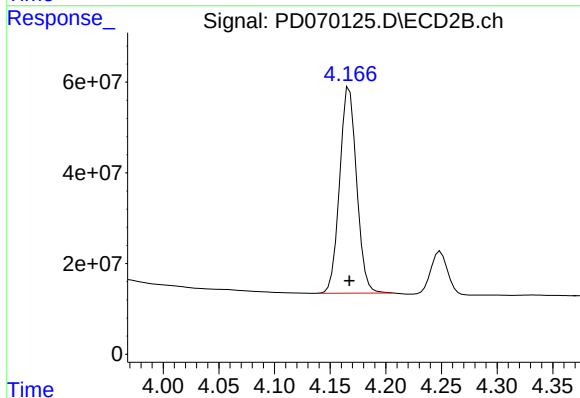


#1 Tetrachloro-m-xylene

R.T.: 4.167 min
Delta R.T.: 0.000 min
Response: 482836640
Conc: 50.00 ng/ml

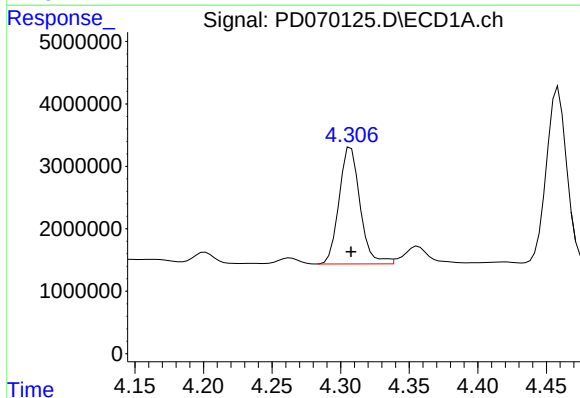


#23 Chlordane-1

R.T.: 4.308 min
Delta R.T.: 0.000 min
Response: 19922688
Conc: 500.00 ng/ml

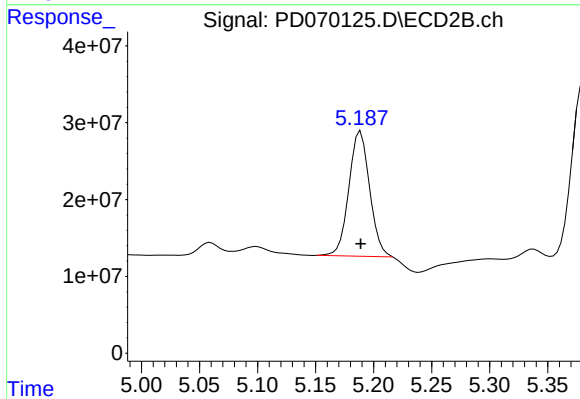

#23 Chlordane-1


R.T.: 5.189 min
Delta R.T.: 0.000 min
Response: 202058974
Conc: 500.00 ng/ml

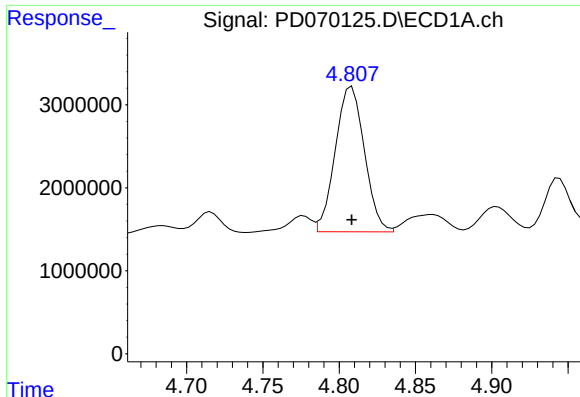

#24 Chlordane-2


R.T.: 4.808 min
Delta R.T.: 0.000 min
Response: 23249515
Conc: 500.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

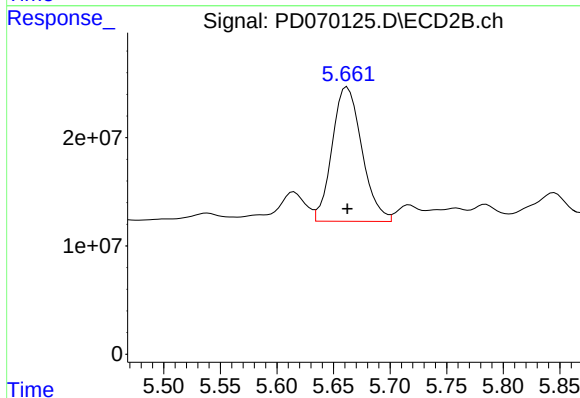


#24 Chlordane-2

R.T.: 5.662 min
Delta R.T.: 0.000 min
Response: 227305227
Conc: 500.00 ng/ml

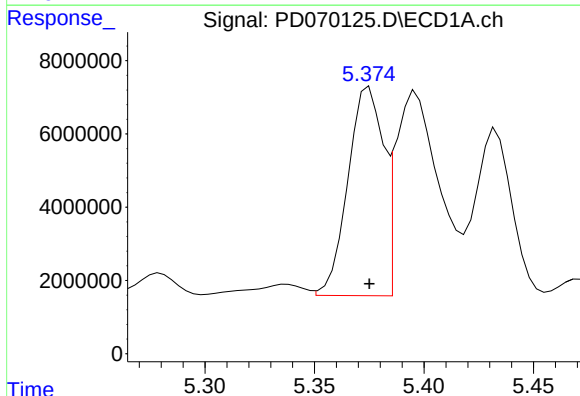


#25 Chlordane-3

R.T.: 5.375 min
Delta R.T.: 0.000 min
Response: 63711880
Conc: 500.00 ng/ml

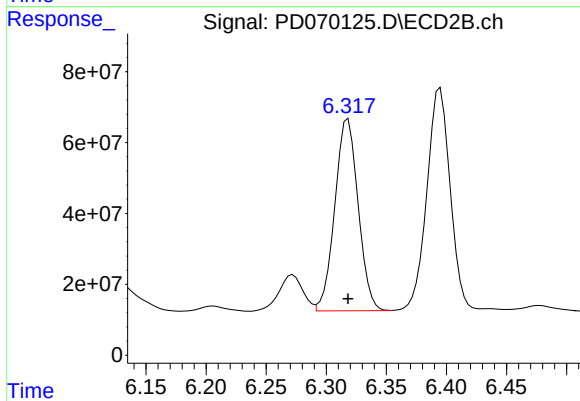

#25 Chlordane-3


R.T.: 6.318 min
Delta R.T.: 0.000 min
Response: 732722564
Conc: 500.00 ng/ml

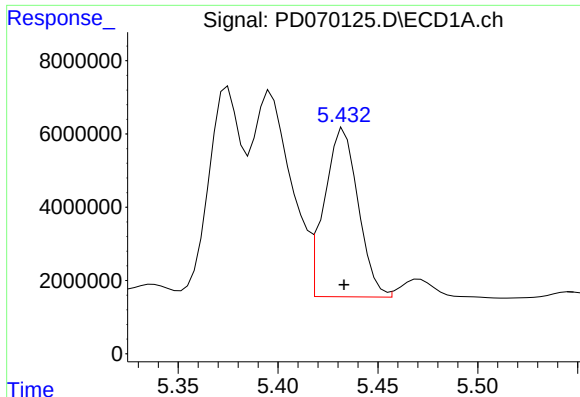

#26 Chlordane-4


R.T.: 5.433 min
Delta R.T.: 0.000 min
Response: 54107347
Conc: 500.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

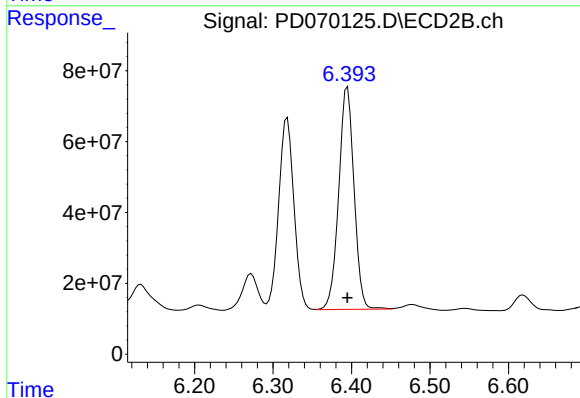


#26 Chlordane-4

R.T.: 6.395 min
Delta R.T.: 0.000 min
Response: 851866069
Conc: 500.00 ng/ml

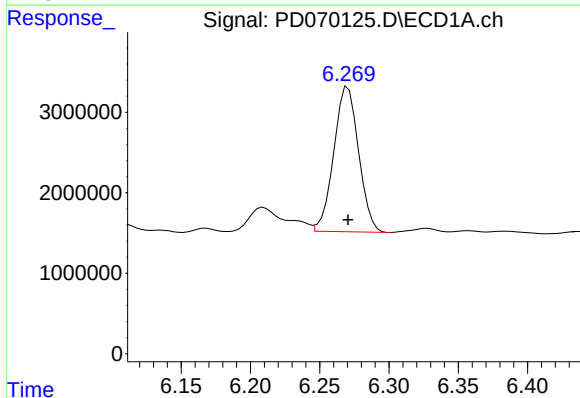


#27 Chlordane-5

R.T.: 6.270 min
Delta R.T.: 0.000 min
Response: 22478199
Conc: 500.00 ng/ml

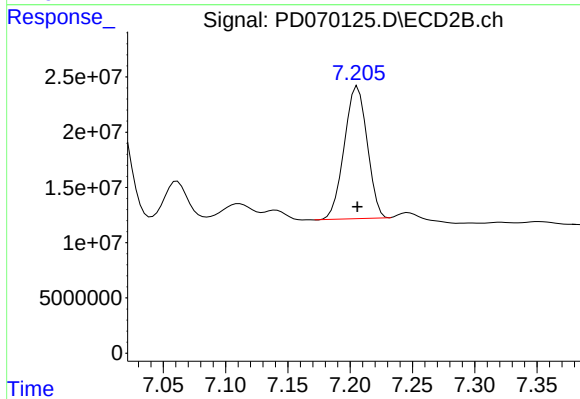

#27 Chlordane-5


R.T.: 7.206 min
Delta R.T.: 0.000 min
Response: 154127614
Conc: 500.00 ng/ml

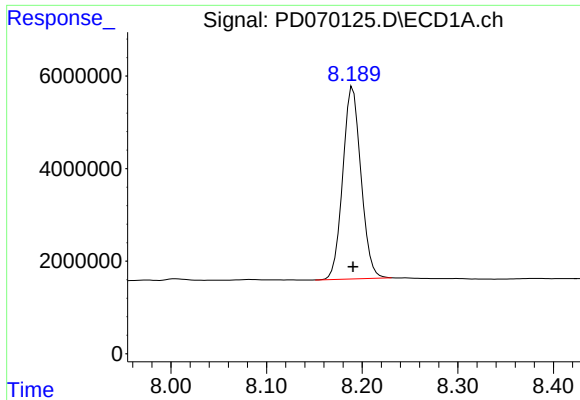

#28 Decachlorobiphenyl

R.T.: 8.190 min
Delta R.T.: 0.000 min
Response: 55033046
Conc: 50.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

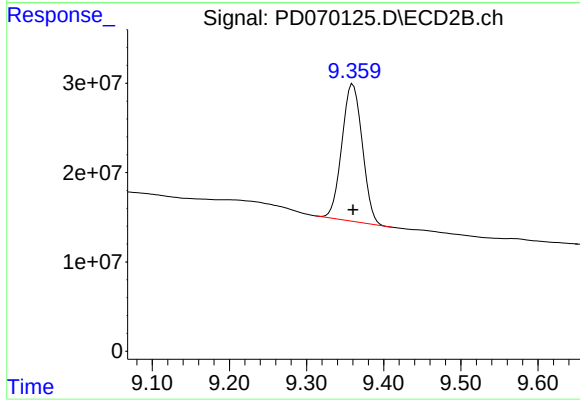

#28 Decachlorobiphenyl

R.T.: 9.360 min
Delta R.T.: 0.000 min
Response: 280736537
Conc: 50.00 ng/ml