

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060622\
 Data File : PD070134.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Jun 2022 19:09
 Operator : AR\AJ
 Sample : PCHLORICV500
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 ICVPD060622CHLOR

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 07 05:56:40 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060622.M
 Quant Title : GC Extractables
 QLast Update : Tue Jun 07 05:56:19 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.448	4.168	62941575	472.1E6	47.424	45.549
28)	SA Decachlor...	8.203	9.365	54198465	312.3E6	45.566	48.307
Target Compounds							
23)	Chlordane-1	4.317	5.190	19459533	167.3E6	454.584	392.149
24)	Chlordane-2	4.819	5.664	22957519	229.5E6	462.563	475.488
25)	Chlordane-3	5.386	6.320	63810992	737.3E6	475.460	465.367
26)	Chlordane-4	5.444	6.397	53608705	850.6E6	468.535	459.223
27)	Chlordane-5	6.282	7.209	21841967	152.0E6	464.366	462.277



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060622\
Data File : PD070134.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Jun 2022 19:09
Operator : AR\AJ
Sample : PCHLORICV500
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
ICVPD060622CHLOR

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 07 05:56:40 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060622.M
Quant Title : GC Extractables
QLast Update : Tue Jun 07 05:56:19 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

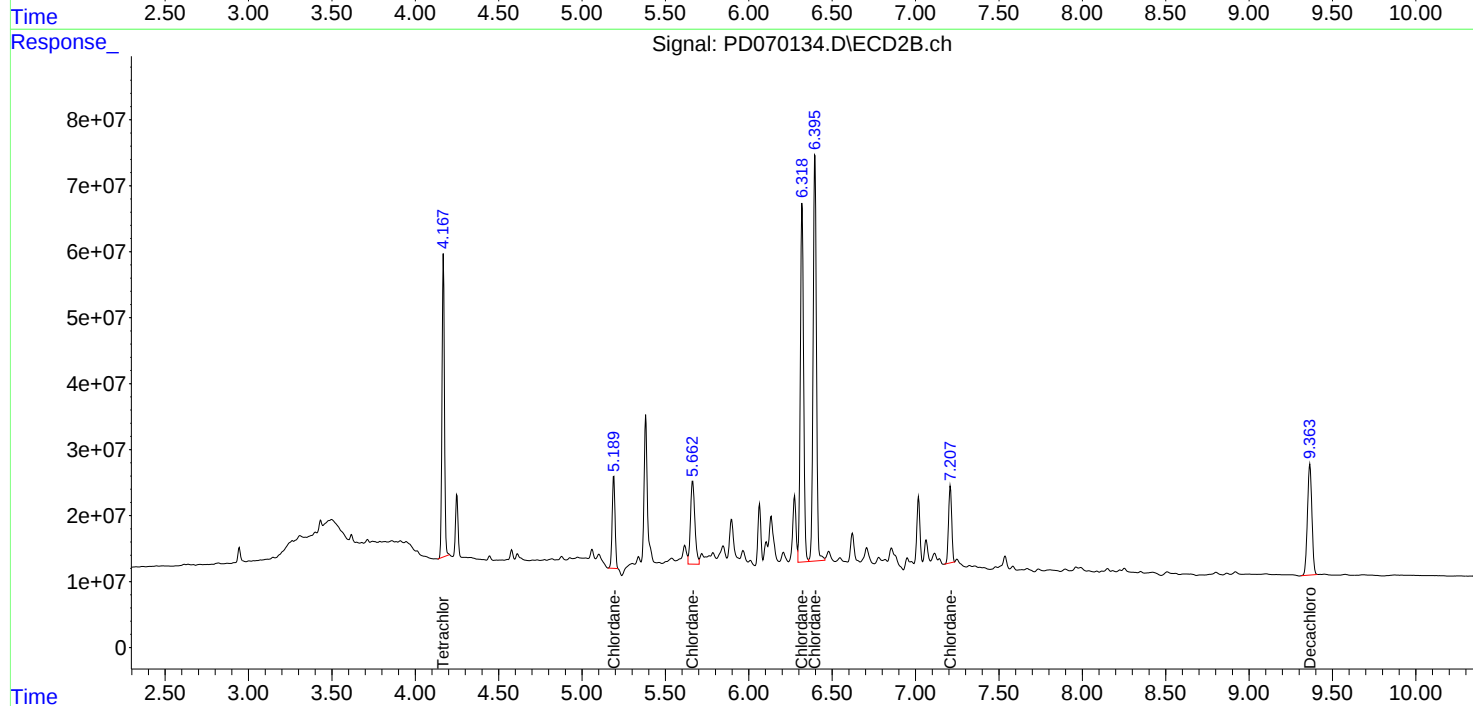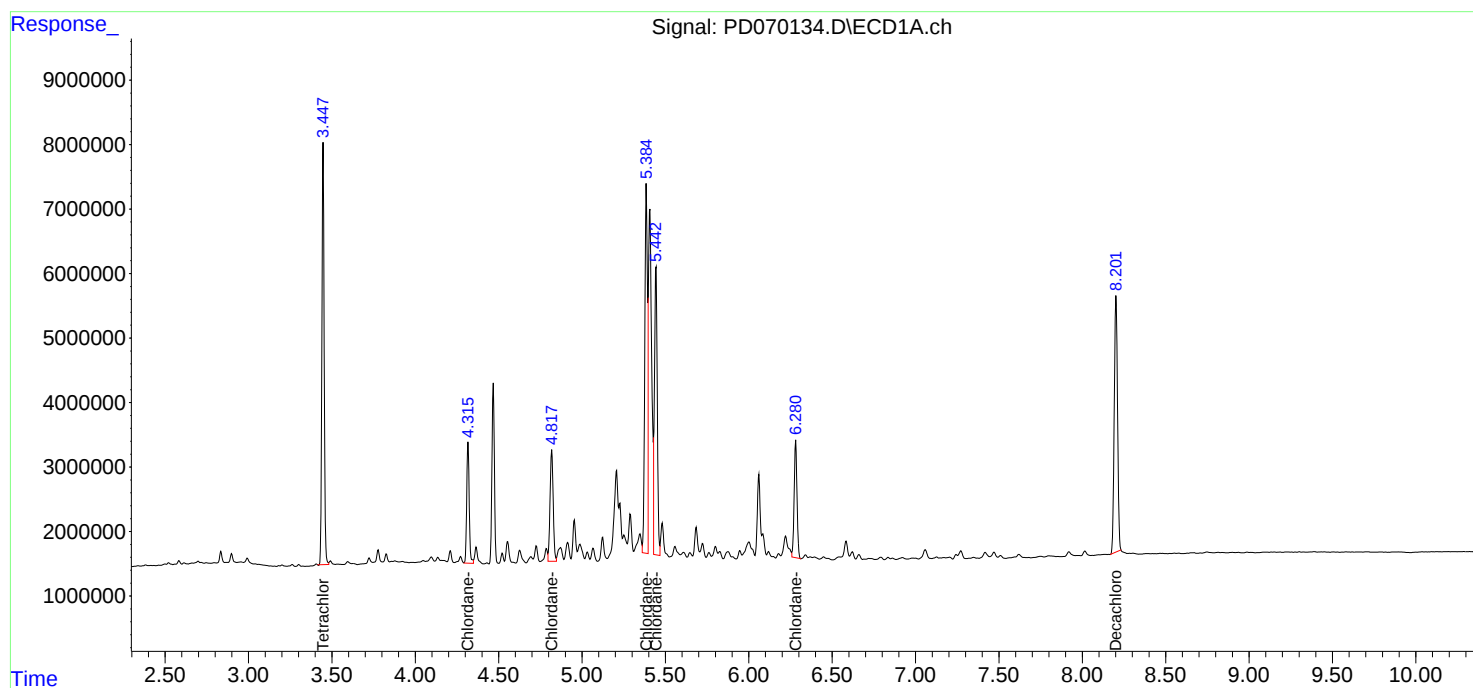


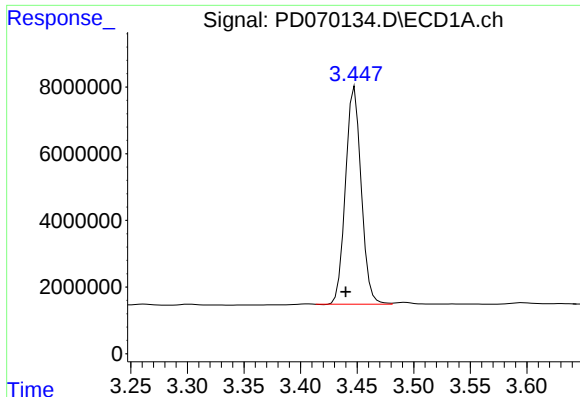

#1 Tetrachloro-m-xylene


R.T.: 3.448 min
Delta R.T.: 0.008 min
Response: 62941575
Conc: 47.42 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD060622CHLOR

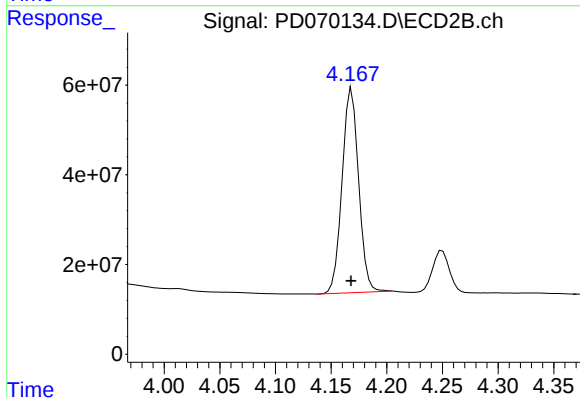


#1 Tetrachloro-m-xylene

R.T.: 4.168 min
Delta R.T.: 0.000 min
Response: 472082885
Conc: 45.55 ng/ml

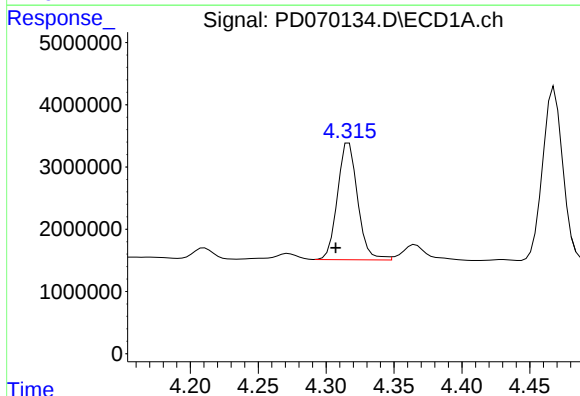


#23 Chlordane-1

R.T.: 4.317 min
Delta R.T.: 0.010 min
Response: 19459533
Conc: 454.58 ng/ml

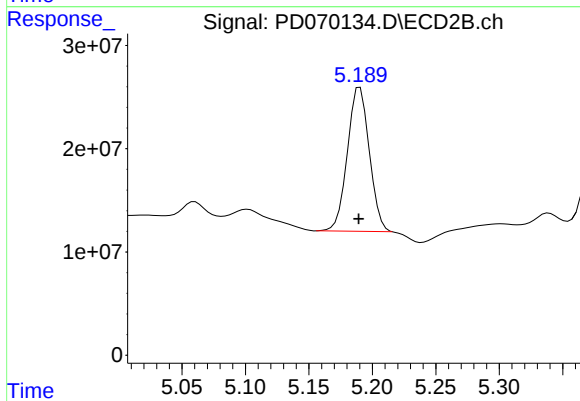

#23 Chlordane-1


R.T.: 5.190 min
Delta R.T.: 0.001 min
Response: 167258465
Conc: 392.15 ng/ml

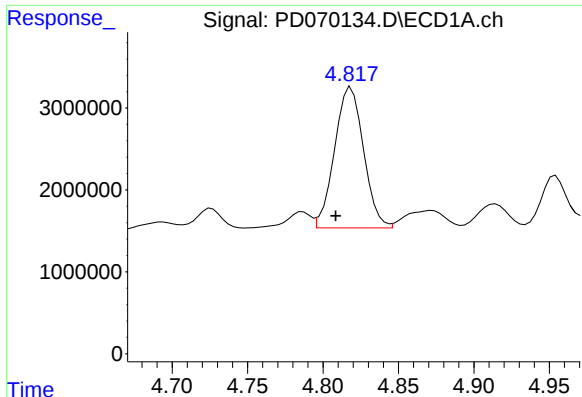

#24 Chlordane-2


R.T.: 4.819 min
Delta R.T.: 0.010 min
Response: 22957519
Conc: 462.56 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD060622CHLOR

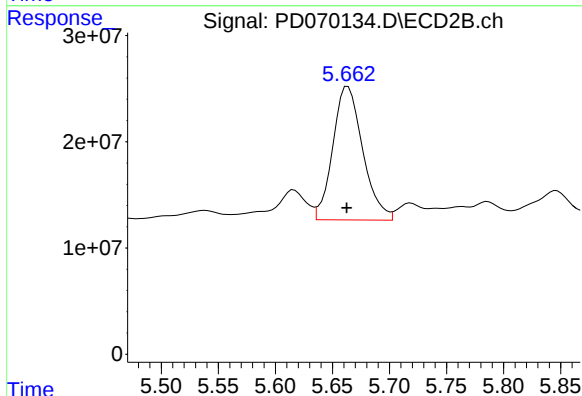


#24 Chlordane-2

R.T.: 5.664 min
Delta R.T.: 0.000 min
Response: 229530098
Conc: 475.49 ng/ml

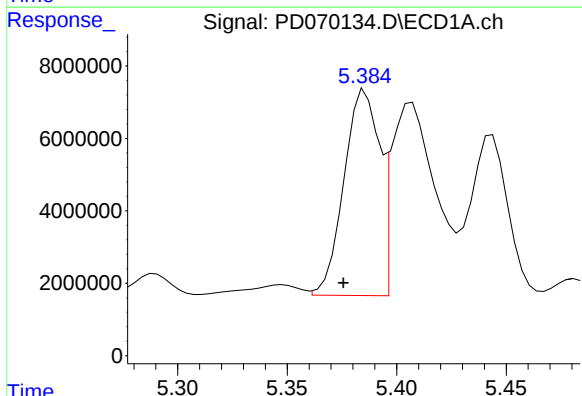


#25 Chlordane-3

R.T.: 5.386 min
Delta R.T.: 0.010 min
Response: 63810992
Conc: 475.46 ng/ml

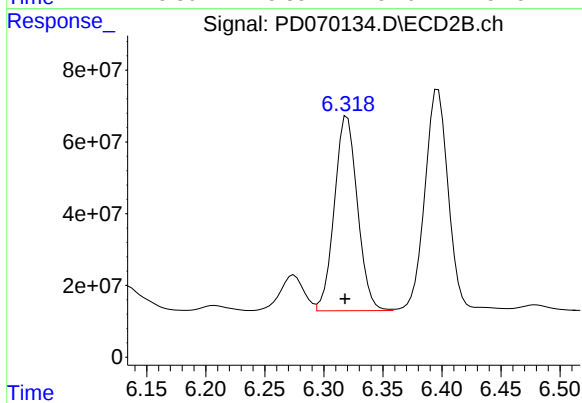

#25 Chlordane-3


R.T.: 6.320 min
Delta R.T.: 0.002 min
Response: 737267632
Conc: 465.37 ng/ml

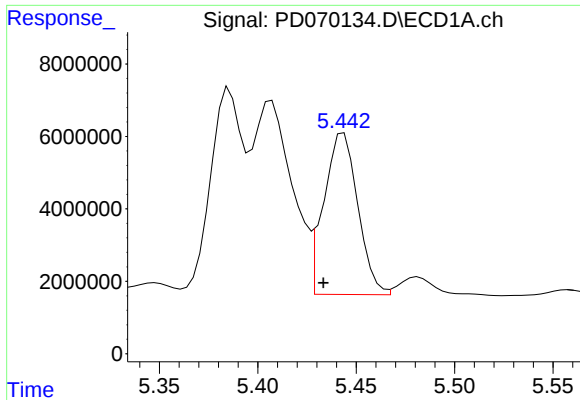

#26 Chlordane-4


R.T.: 5.444 min
Delta R.T.: 0.010 min
Response: 53608705
Conc: 468.53 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD060622CHLOR

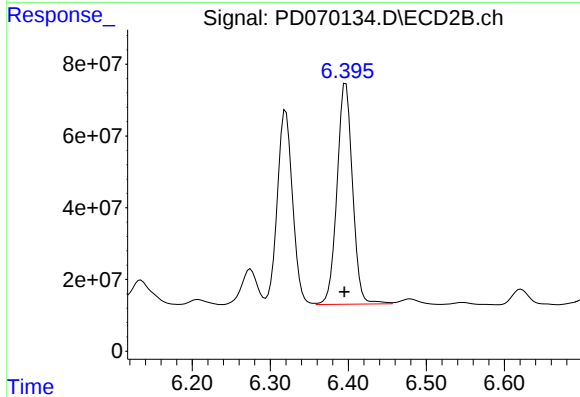


#26 Chlordane-4

R.T.: 6.397 min
Delta R.T.: 0.002 min
Response: 850582260
Conc: 459.22 ng/ml

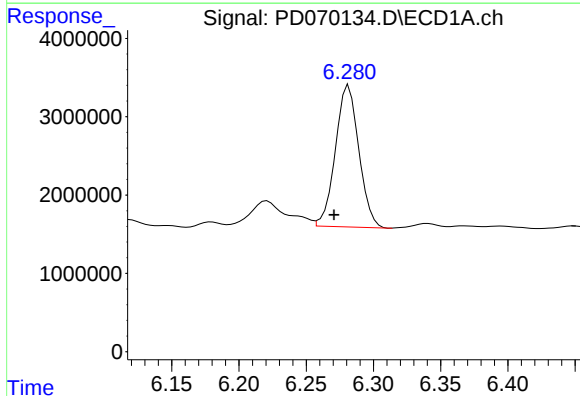


#27 Chlordane-5

R.T.: 6.282 min
Delta R.T.: 0.011 min
Response: 21841967
Conc: 464.37 ng/ml

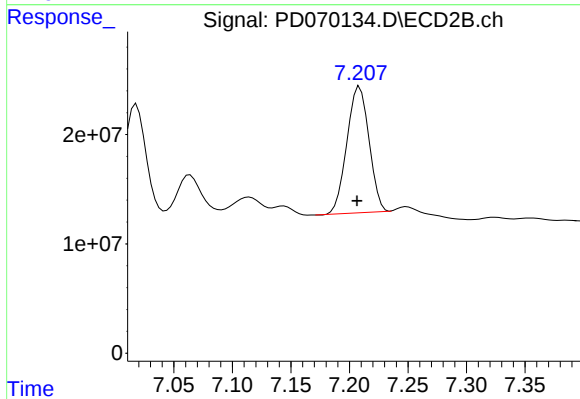

#27 Chlordane-5


R.T.: 7.209 min
Delta R.T.: 0.002 min
Response: 152043033
Conc: 462.28 ng/ml

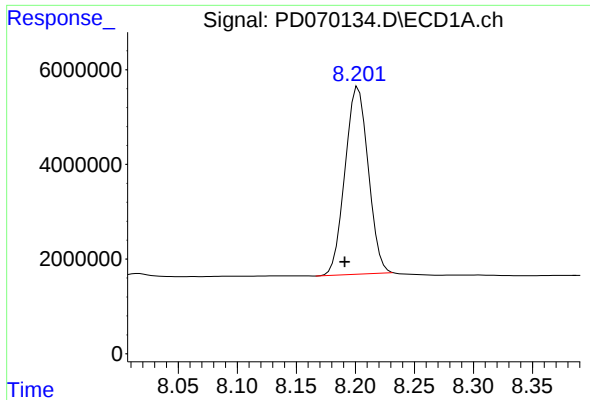

#28 Decachlorobiphenyl

R.T.: 8.203 min
Delta R.T.: 0.011 min
Response: 54198465
Conc: 45.57 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD060622CHLOR

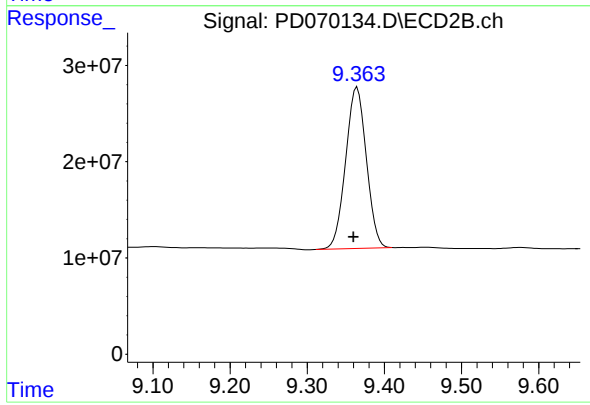

#28 Decachlorobiphenyl

R.T.: 9.365 min
Delta R.T.: 0.005 min
Response: 312269556
Conc: 48.31 ng/ml