

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060622\
 Data File : PD070139.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Jun 2022 21:16
 Operator : AR\AJ
 Sample : N2936-01RE
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 SEMI-ANNUAL-CONDENSATERE

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 06/07/2022
 Supervised By :Ankita Jodhani 06/07/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 07 06:29:38 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060622.M
 Quant Title : GC Extractables
 QLast Update : Tue Jun 07 06:00:04 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.427	4.163	37206554	31757836	34.271	3.253m#
28) SA Decachlor...	8.186	9.364	6056037	93296756	5.446m	15.169 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060622\
Data File : PD070139.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Jun 2022 21:16
Operator : AR\AJ
Sample : N2936-01RE
Misc :
ALS Vial : 23 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
SEMI-ANNUAL-CONDENSATERE


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 06/07/2022
Supervised By : Ankita Jodhani 06/07/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 07 06:29:38 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060622.M
Quant Title : GC Extractables
QLast Update : Tue Jun 07 06:00:04 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

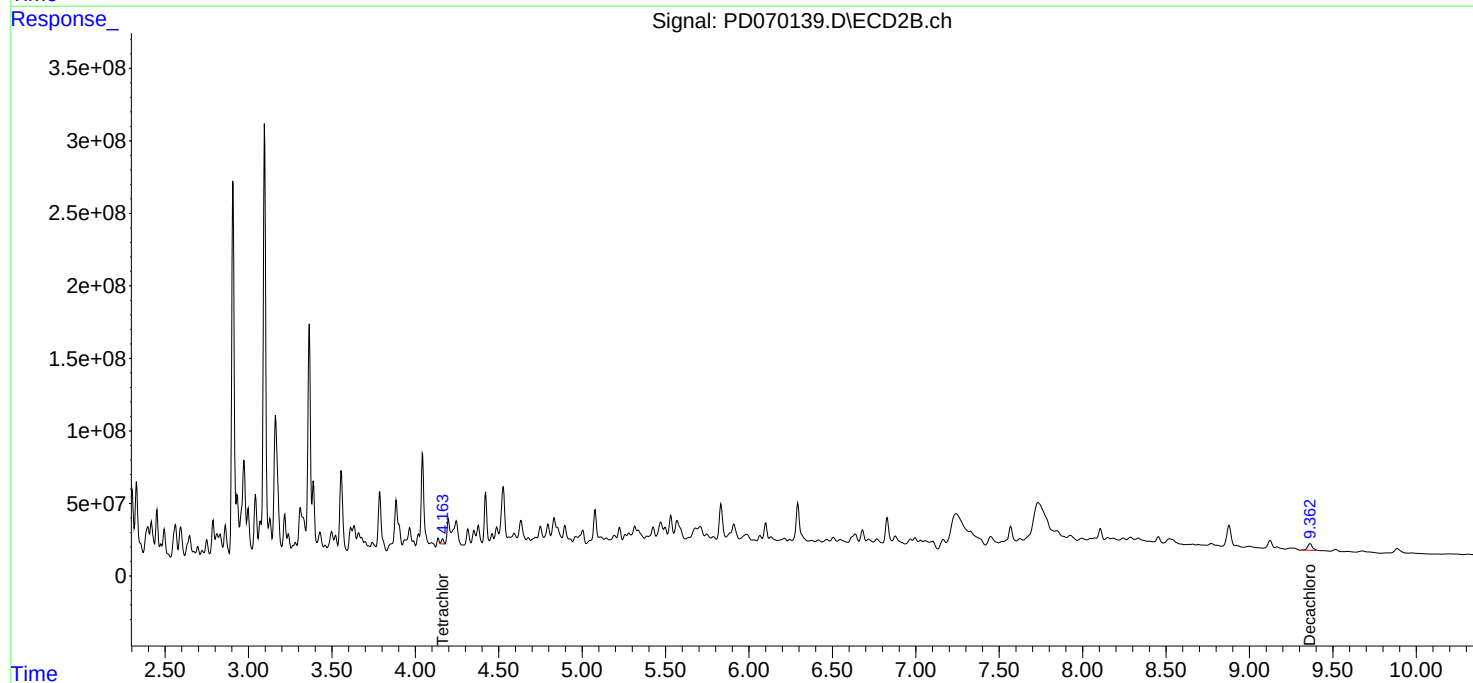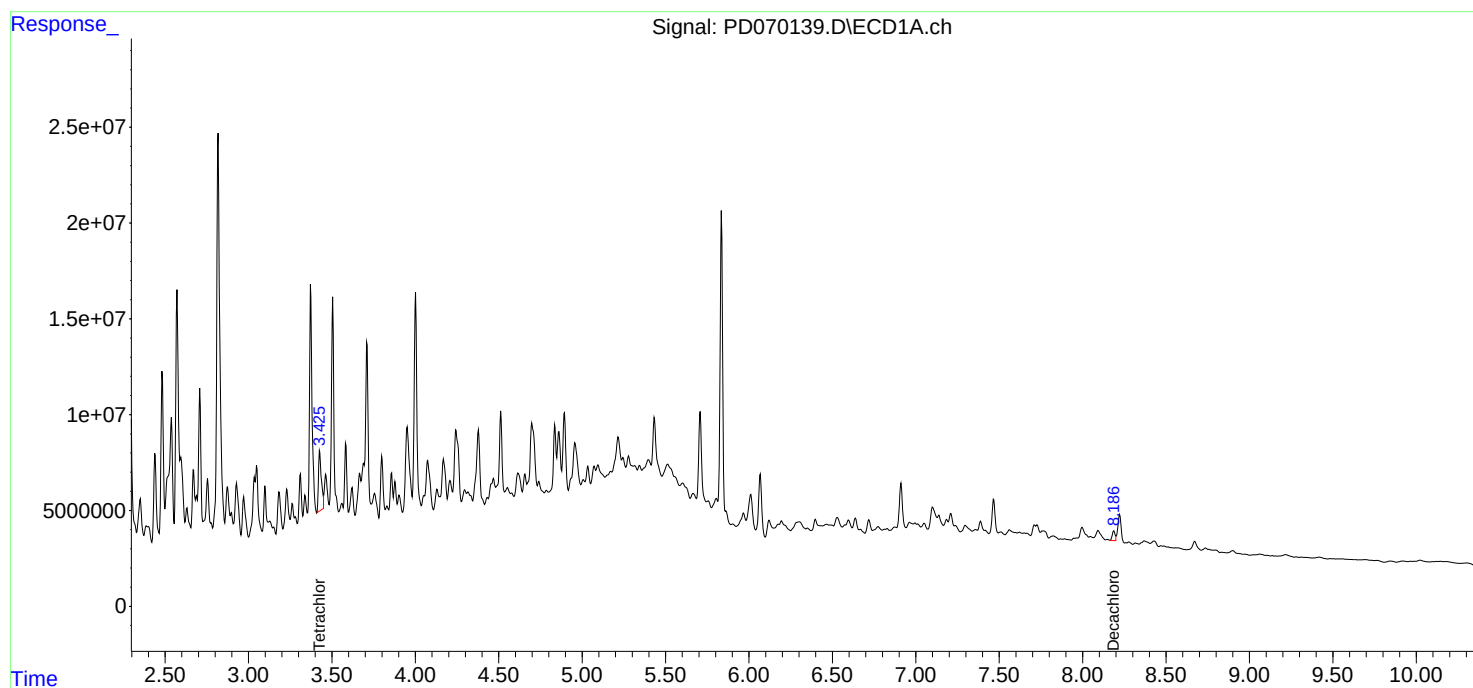

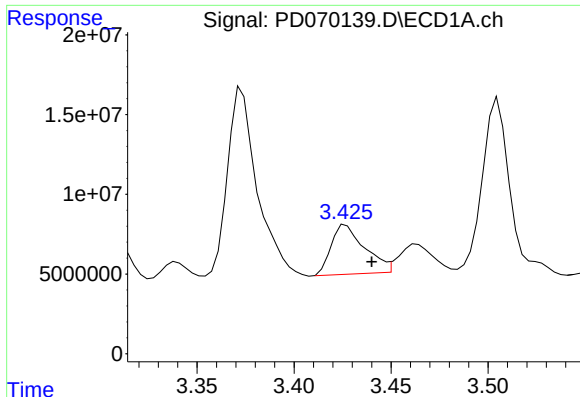


#1 Tetrachloro-m-xylene

R.T.: 3.427 min
Delta R.T.: -0.013 min
Response: 37206554
Conc: 34.27 ng/ml

Instrument :
ECD_D
ClientSampleId :
SEMI-ANNUAL-CONDENSATERE


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 06/07/2022
Supervised By :Ankita Jodhani 06/07/2022

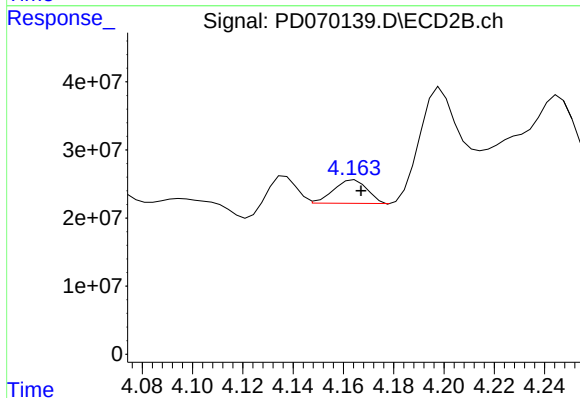


#1 Tetrachloro-m-xylene

R.T.: 4.163 min
Delta R.T.: -0.004 min
Response: 31757836
Conc: 3.25 ng/ml m

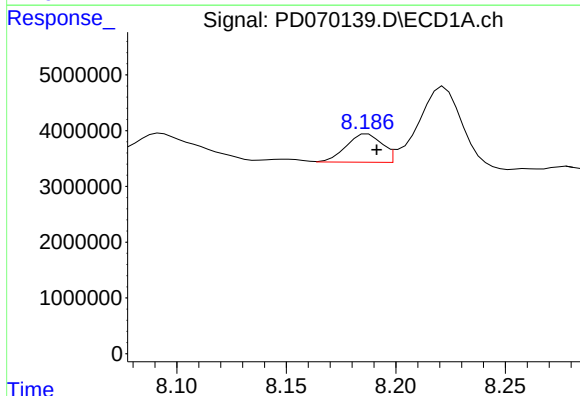

#28 Decachlorobiphenyl

R.T.: 8.186 min
Delta R.T.: -0.005 min
Response: 6056037
Conc: 5.45 ng/ml m

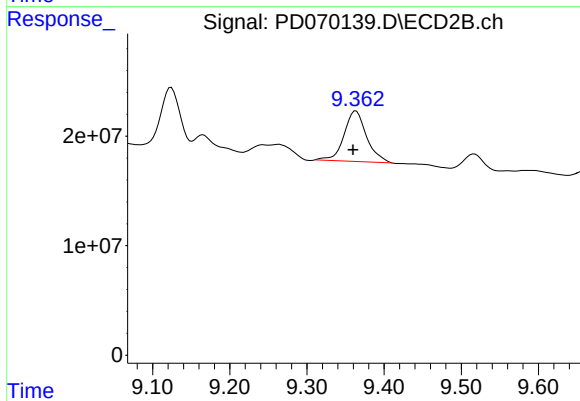

#28 Decachlorobiphenyl

R.T.: 9.364 min
Delta R.T.: 0.004 min
Response: 93296756
Conc: 15.17 ng/ml