

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060622\
 Data File : PD070143.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Jun 2022 22:12
 Operator : AR\AJ
 Sample : N3155-01
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 MONTHLY-OUTFALL-002

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 06/08/2022
 Supervised By : Ankita Jodhani 06/08/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 07 06:31:06 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060622.M
 Quant Title : GC Extractables
 QLast Update : Tue Jun 07 06:00:04 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.441	4.168	16592635	128.0E6	15.284	13.114m
28) SA Decachlor...	8.189	9.361	13253558	70050578	11.917	11.389

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060622\
Data File : PD070143.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Jun 2022 22:12
Operator : AR\AJ
Sample : N3155-01
Misc :
ALS Vial : 27 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
MONTHLY-OUTFALL-002


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 06/08/2022
Supervised By : Ankita Jodhani 06/08/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 07 06:31:06 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060622.M
Quant Title : GC Extractables
QLast Update : Tue Jun 07 06:00:04 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

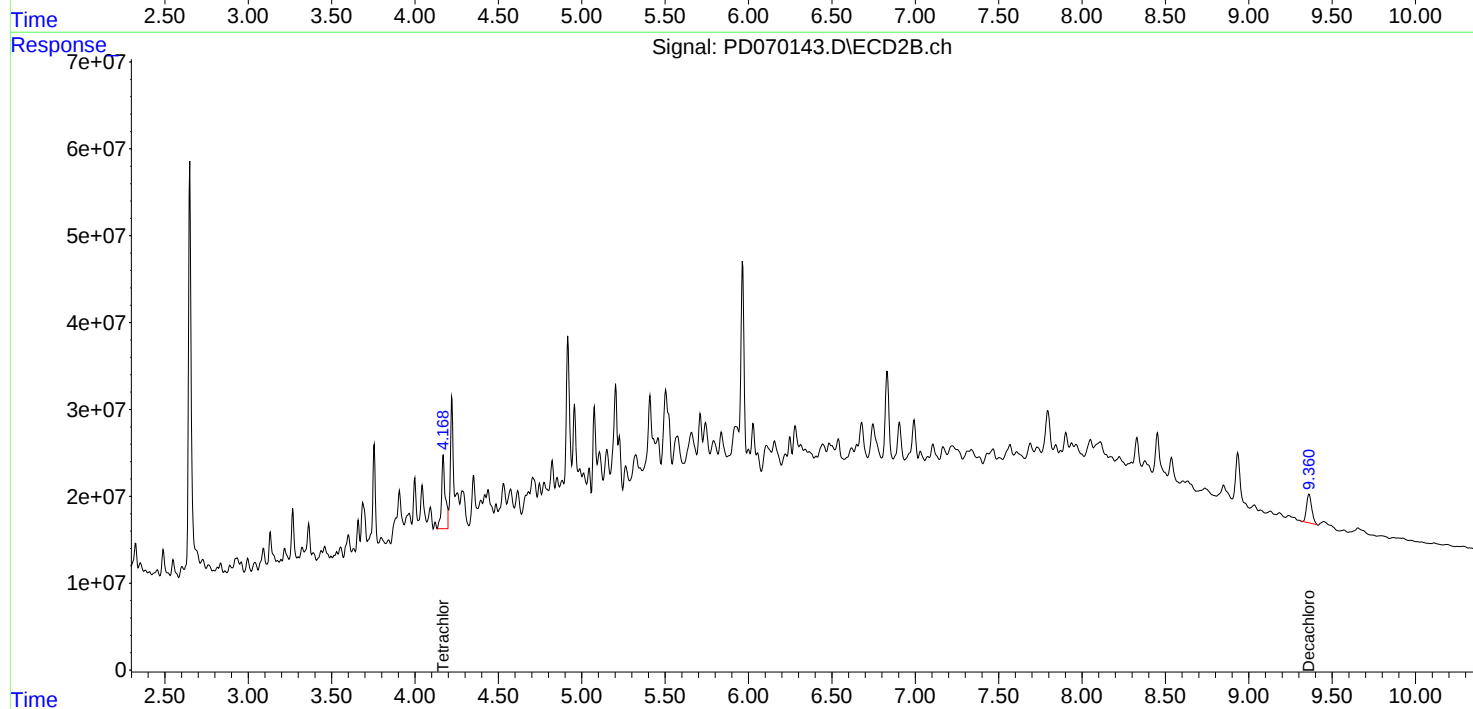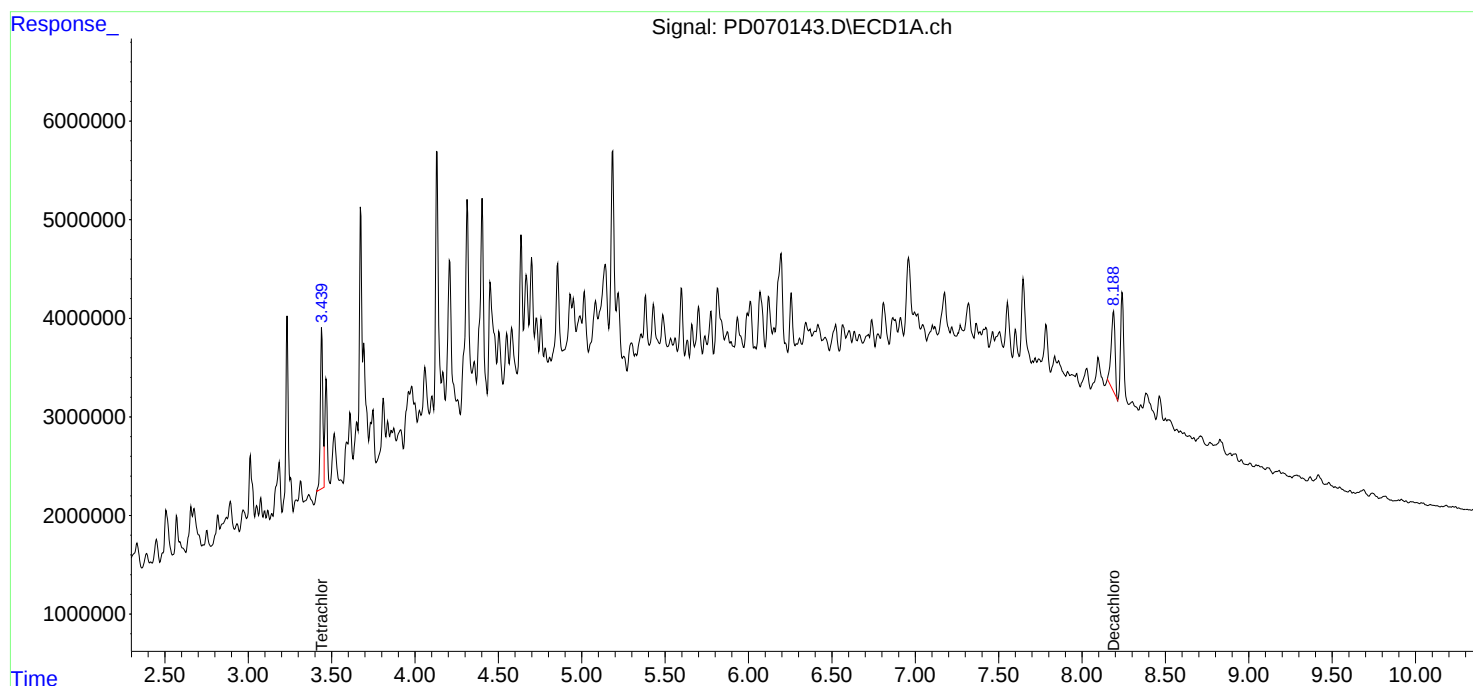

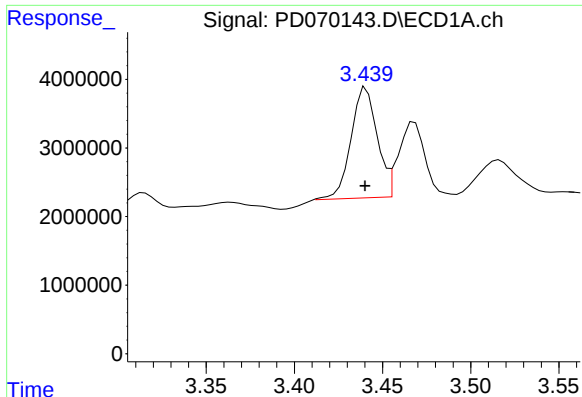


#1 Tetrachloro-m-xylene

R.T.: 3.441 min
Delta R.T.: 0.000 min
Response: 16592635
Conc: 15.28 ng/ml

Instrument :
ECD_D
ClientSampleId :
MONTHLY-OUTFALL-002


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 06/08/2022
Supervised By :Ankita Jodhani 06/08/2022

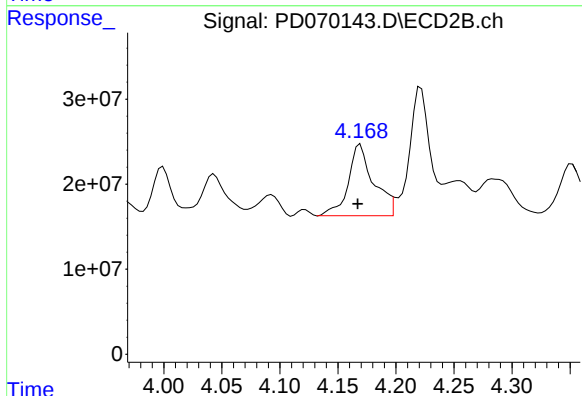


#1 Tetrachloro-m-xylene

R.T.: 4.168 min
Delta R.T.: 0.000 min
Response: 128008207
Conc: 13.11 ng/ml m

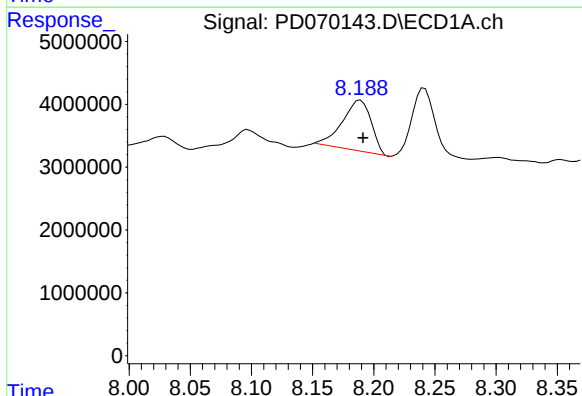

#28 Decachlorobiphenyl

R.T.: 8.189 min
Delta R.T.: -0.002 min
Response: 13253558
Conc: 11.92 ng/ml

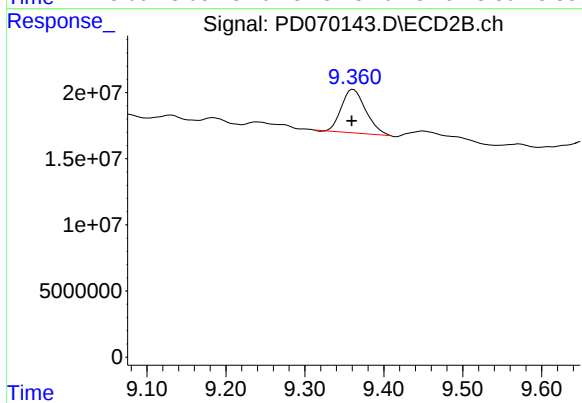

#28 Decachlorobiphenyl

R.T.: 9.361 min
Delta R.T.: 0.002 min
Response: 70050578
Conc: 11.39 ng/ml