

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060624\
 Data File : PD083444.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Jun 2024 06:29
 Operator : AR\AJ
 Sample : P2634-21
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BHB5

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 06/06/2024
 Supervised By : Ankita Jodhani 06/06/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 06 11:34:08 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060424CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Jun 04 07:04:40 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.561	2.771	15484241	64800606	10.793m	13.681m#
2) SA Decachlor...	9.115	7.900	20781012	70129987	10.169m	14.061 #
Target Compounds						
9) A Endosulfan I	6.138	5.116	11479230	46239437	5.404m	8.482m#
13) MA Dieldrin	6.402	5.360	6084747	24799916	2.691m	4.089m#
16) A 4,4'-DDD	6.731	5.776	6971988	15966053	4.340m	3.446m
17) MA 4,4'-DDT	7.066	6.021	1164489	7414058	0.713	1.588m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060624\
Data File : PD083444.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Jun 2024 06:29
Operator : AR\AJ
Sample : P2634-21
Misc :
ALS Vial : 44 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 06 11:34:08 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060424CLP.M
Quant Title : GC Extractables
QLast Update : Tue Jun 04 07:04:40 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

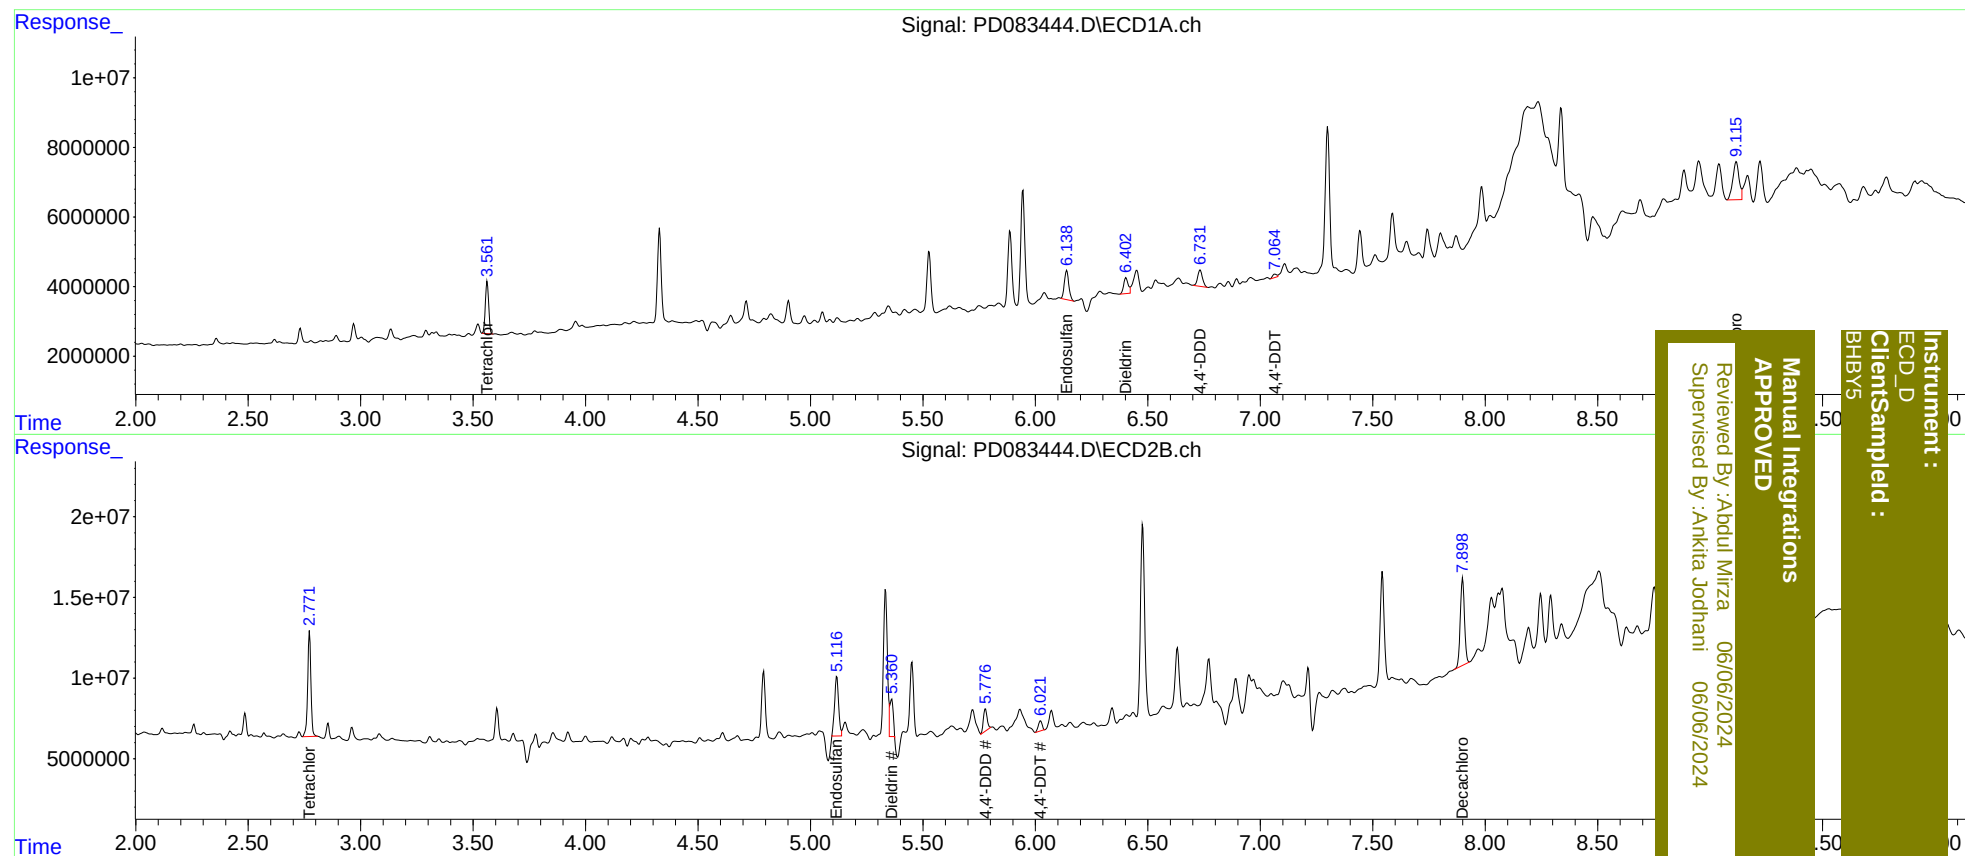

Instrument :
ECD_D
ClientSampled :
BHBYS

Manual Integrations
APPROVED

Reviewed By: Abdul Mirza 06/06/2024
Supervised By: Ankita Jodhani 06/06/2024