

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060721\
 Data File : PD063533.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Jun 2021 12:03
 Operator : AR\AJ
 Sample : M2613-06
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 18-B12(106-110)

Manual Integrations
 APPROVED

Ankita
 6/8/2021 11:52:41 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 08 04:12:31 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060221.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 03 01:33:41 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.439	3.970	26921375	284.6E6	19.455	21.241
28)	SA Decachlor...	8.194	9.023	23452599	214.1E6	14.912	15.494
Target Compounds							
17)	MA 4,4'-DDT	6.354	7.092	790921	10314923	0.547m	0.685 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060721\
Data File : PD063533.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Jun 2021 12:03
Operator : AR\AJ
Sample : M2613-06
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampled :
18-B12(106-110)


Manual Integrations
APPROVED

Ankita
6/8/2021 11:52:41 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 08 04:12:31 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060221.M
Quant Title : GC Extractables
QLast Update : Thu Jun 03 01:33:41 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

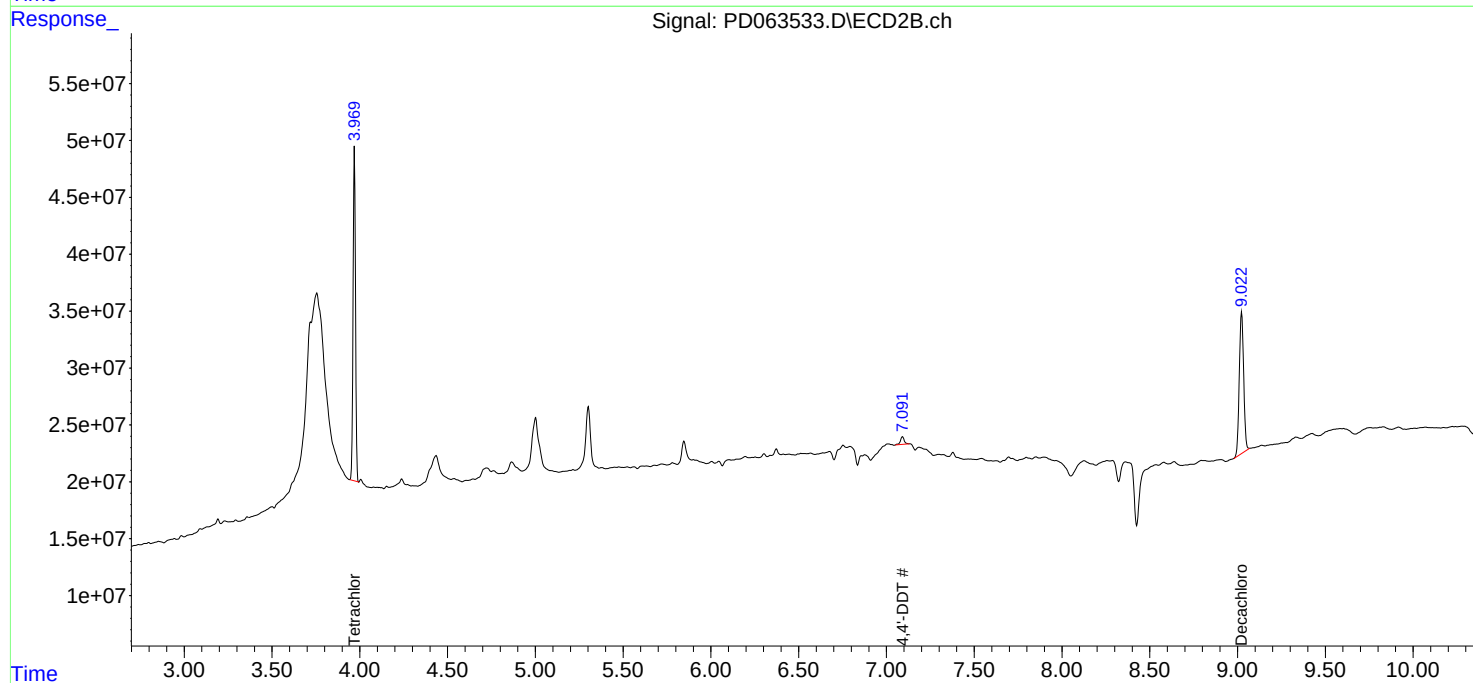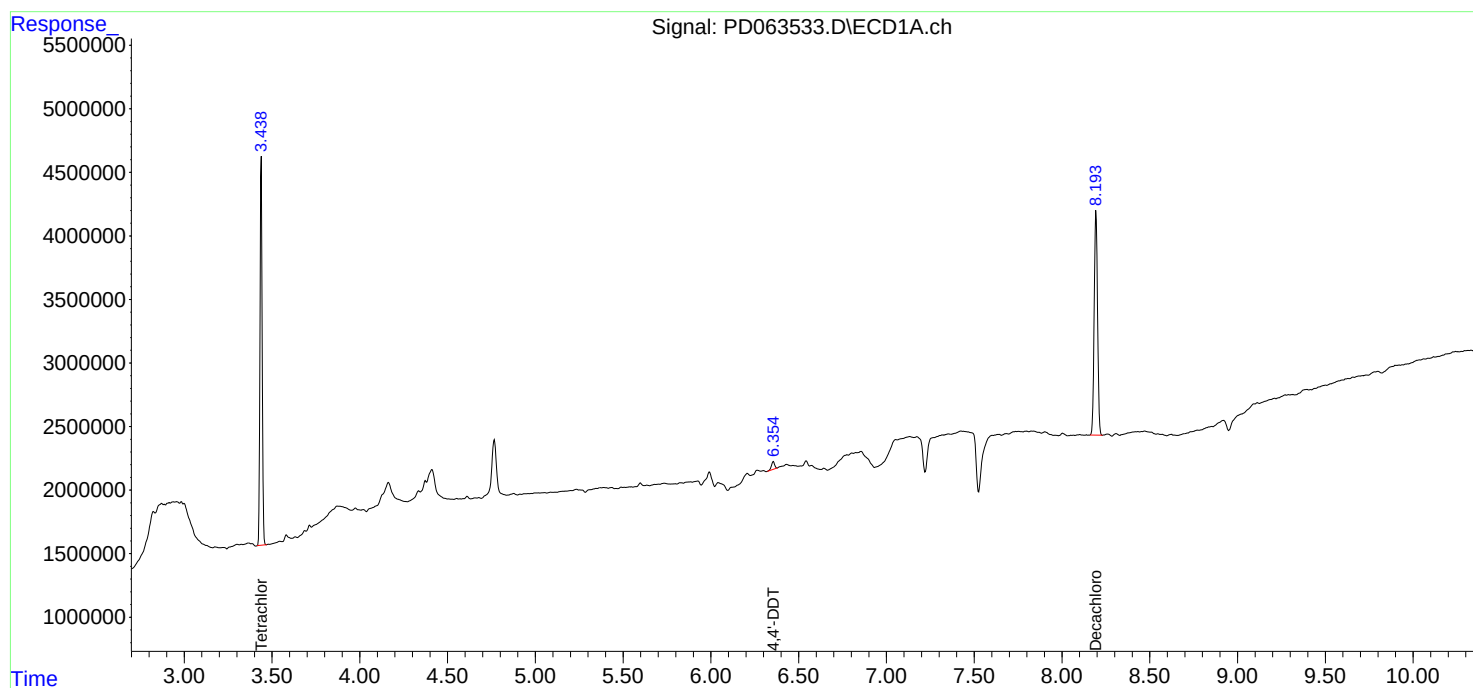

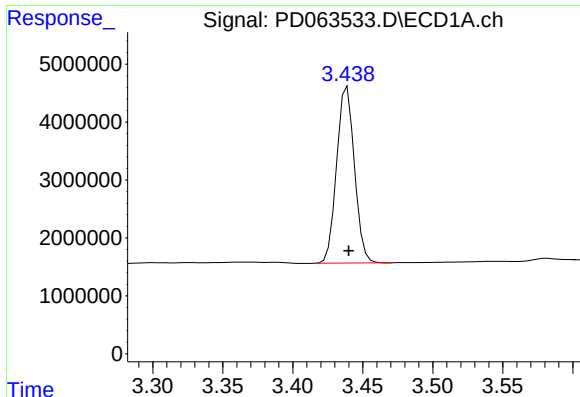


#1 Tetrachloro-m-xylene

R.T.: 3.439 min
Delta R.T.: -0.001 min
Response: 26921375
Conc: 19.46 ng/ml

Instrument :
ECD_D
ClientSampleId :
18-B12(106-110)


Manual Integrations
APPROVED

Ankita
6/8/2021 11:52:41 AM

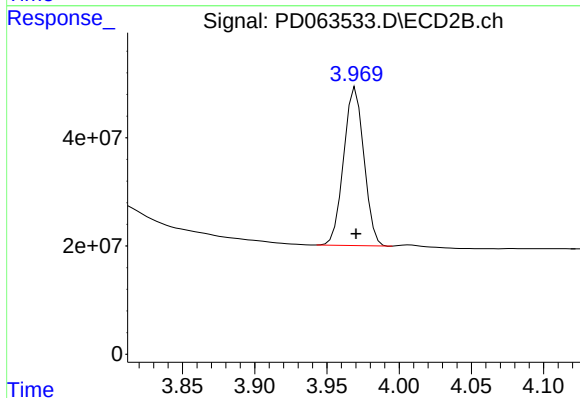


#1 Tetrachloro-m-xylene

R.T.: 3.970 min
Delta R.T.: 0.000 min
Response: 284605868
Conc: 21.24 ng/ml

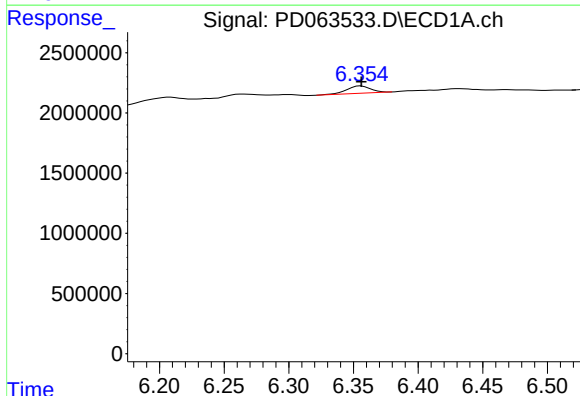


#17 4,4'-DDT

R.T.: 6.354 min
Delta R.T.: -0.002 min
Response: 790921
Conc: 0.55 ng/ml m

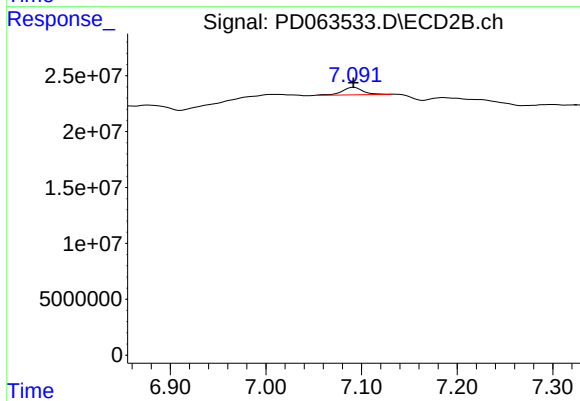

#17 4,4'-DDT

R.T.: 7.092 min
Delta R.T.: 0.000 min
Response: 10314923
Conc: 0.69 ng/ml

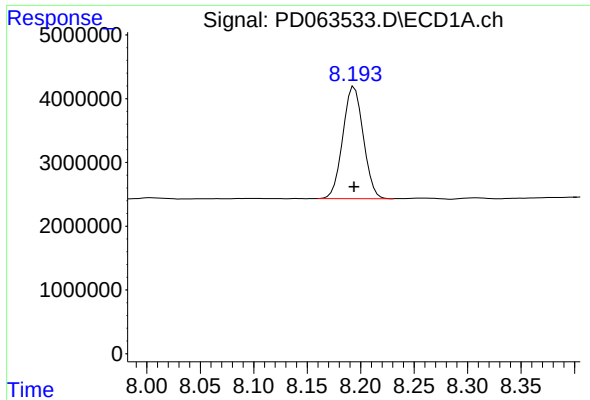


#28 Decachlorobiphenyl

R.T.: 8.194 min
Delta R.T.: 0.000 min
Response: 23452599
Conc: 14.91 ng/ml

Instrument :
ECD_D
ClientSampleId :
18-B12(106-110)

Manual Integrations
APPROVED

Ankita
6/8/2021 11:52:41 AM

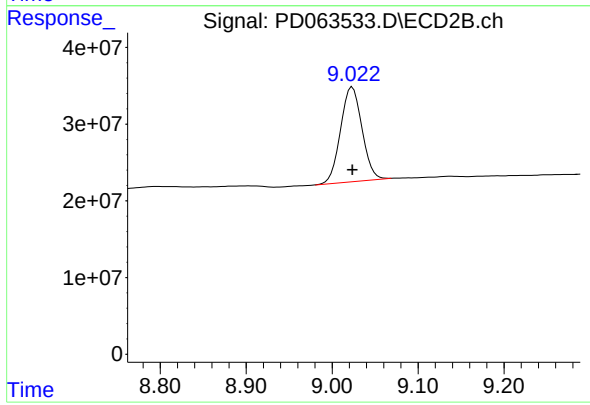

#28 Decachlorobiphenyl

R.T.: 9.023 min
Delta R.T.: 0.000 min
Response: 214099562
Conc: 15.49 ng/ml