

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060721\
 Data File : PD063544.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Jun 2021 14:37
 Operator : AR\AJ
 Sample : M2624-01
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 G-1

Manual Integrations
 APPROVED

Ankita
 6/8/2021 11:53:05 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 08 04:15:18 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060221.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 03 01:33:41 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.439	3.970	11083988	124.1E6	8.010	9.265
28) SA Decachlor...	8.194	9.024	11997110	109.5E6	7.628	7.925
Target Compounds						
5) MB Aldrin	4.707	5.454	52011285	590.8E6	27.521	30.384
11) B alpha-Chl...	5.433	6.148	883114	25736139	0.499m	1.448 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060721\
Data File : PD063544.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Jun 2021 14:37
Operator : AR\AJ
Sample : M2624-01
Misc :
ALS Vial : 24 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
G-1


Manual Integrations
APPROVED

Ankita
6/8/2021 11:53:05 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 08 04:15:18 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060221.M
Quant Title : GC Extractables
QLast Update : Thu Jun 03 01:33:41 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

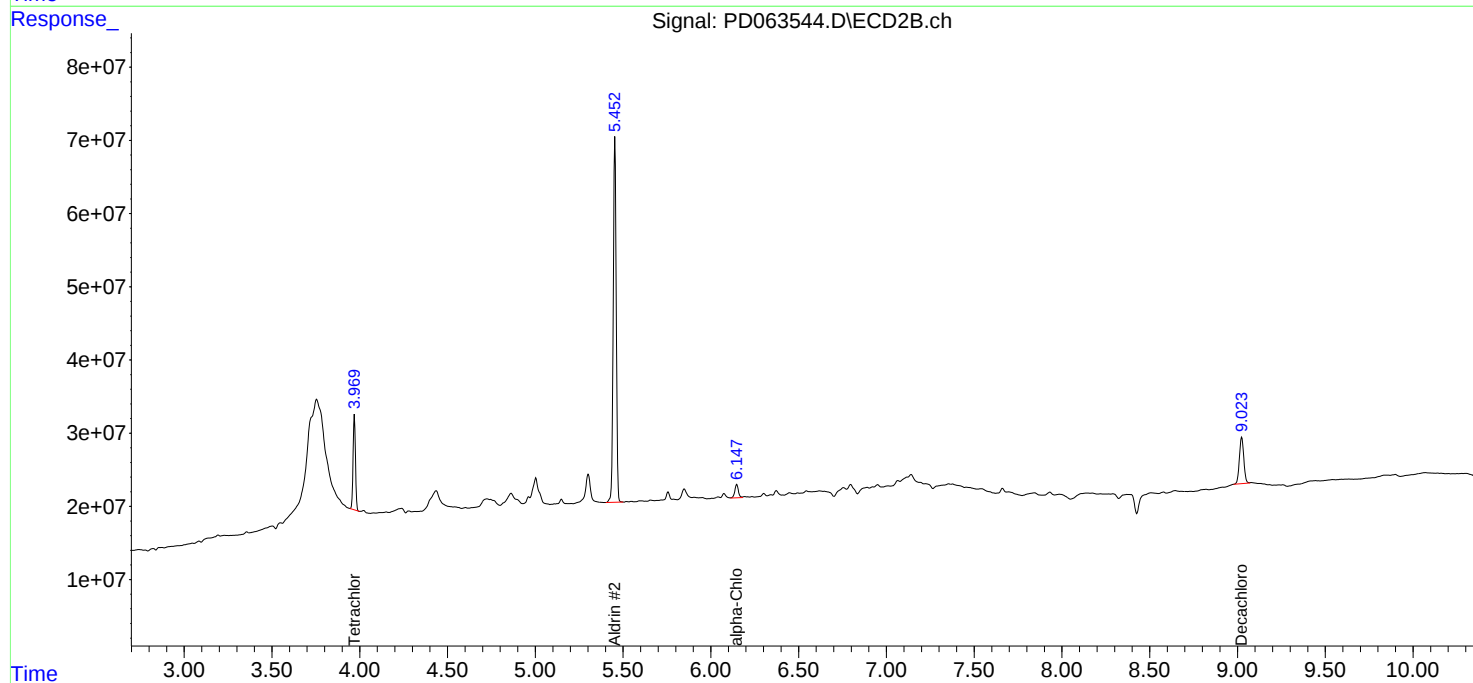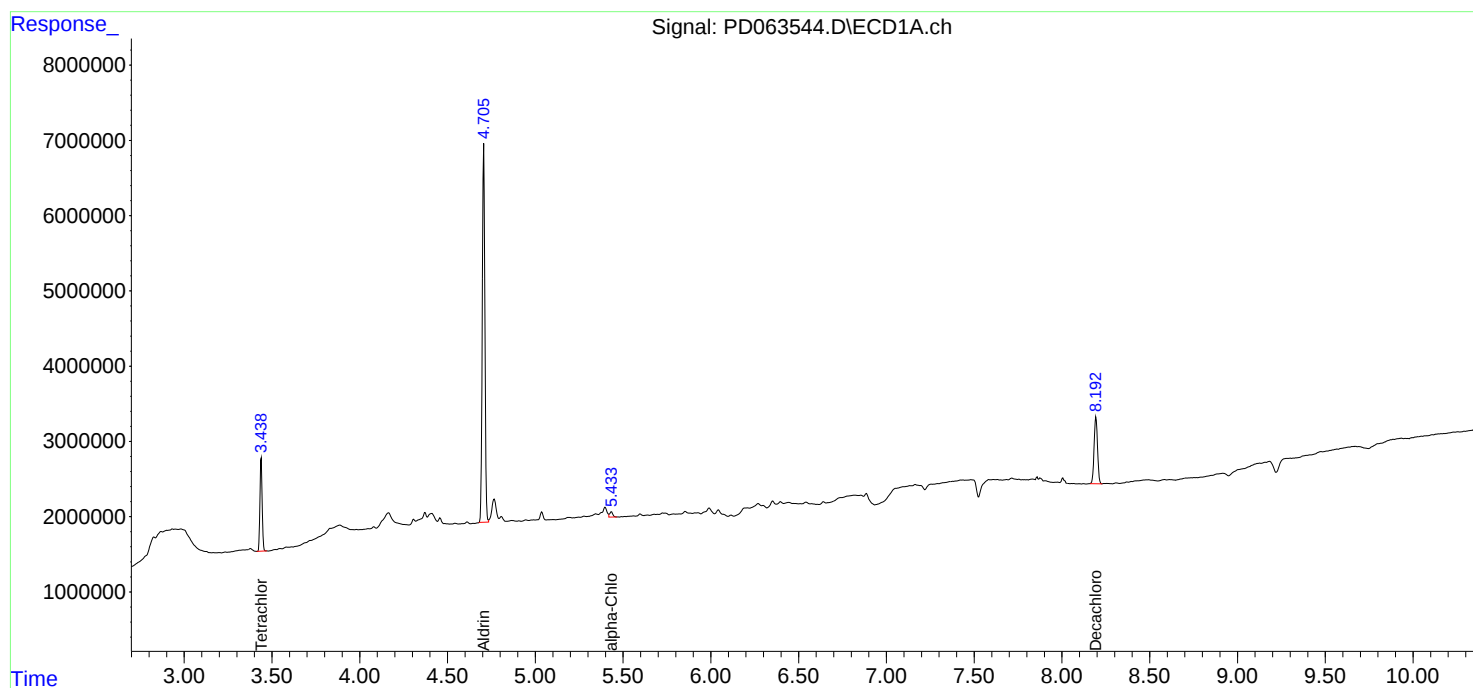

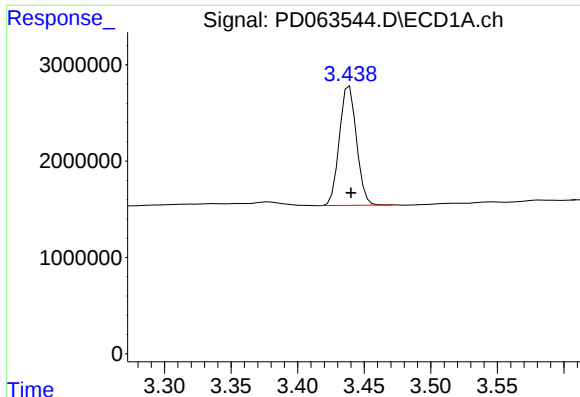


#1 Tetrachloro-m-xylene

R.T.: 3.439 min
Delta R.T.: -0.001 min
Response: 11083988
Conc: 8.01 ng/ml

Instrument :
ECD_D
ClientSampleId :
G-1


Manual Integrations
APPROVED

Ankita
6/8/2021 11:53:05 AM

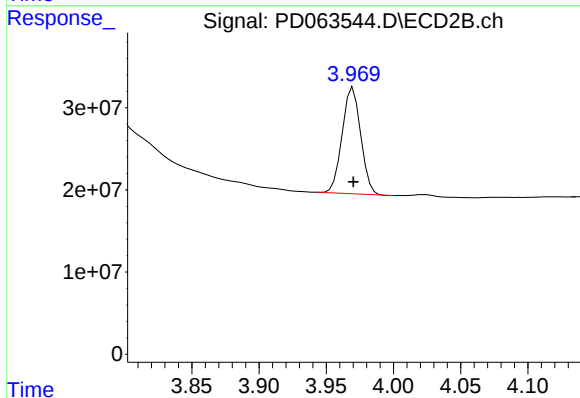


#1 Tetrachloro-m-xylene

R.T.: 3.970 min
Delta R.T.: 0.000 min
Response: 124135778
Conc: 9.26 ng/ml

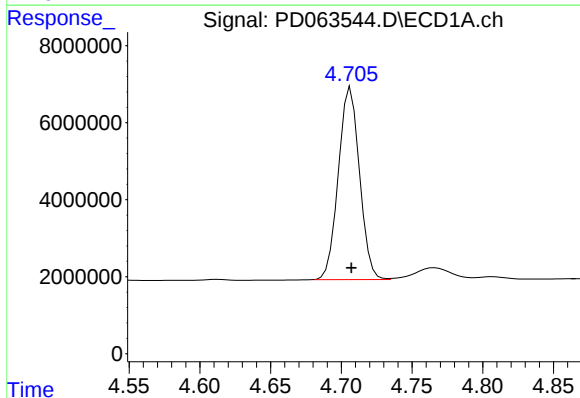


#5 Aldrin

R.T.: 4.707 min
Delta R.T.: 0.000 min
Response: 52011285
Conc: 27.52 ng/ml

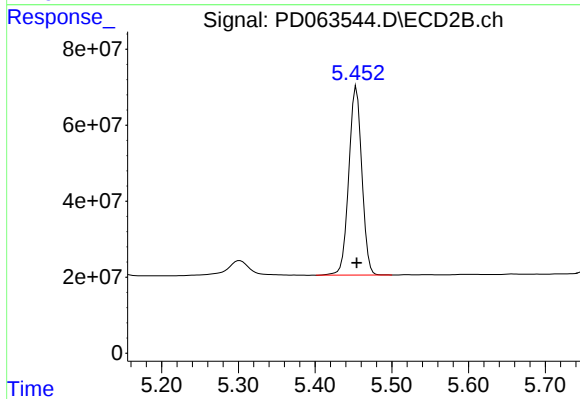

#5 Aldrin

R.T.: 5.454 min
Delta R.T.: 0.000 min
Response: 590782773
Conc: 30.38 ng/ml

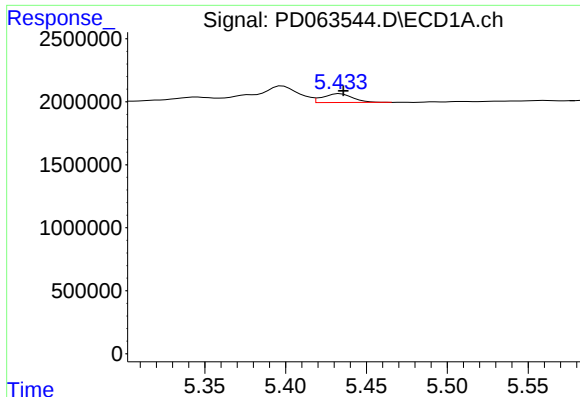


#11 alpha-Chlordane

R.T.: 5.433 min
Delta R.T.: -0.003 min
Response: 883114
Conc: 0.50 ng/ml m

Instrument :
ECD_D
ClientSampleId :
G-1


Manual Integrations
APPROVED

Ankita
6/8/2021 11:53:05 AM

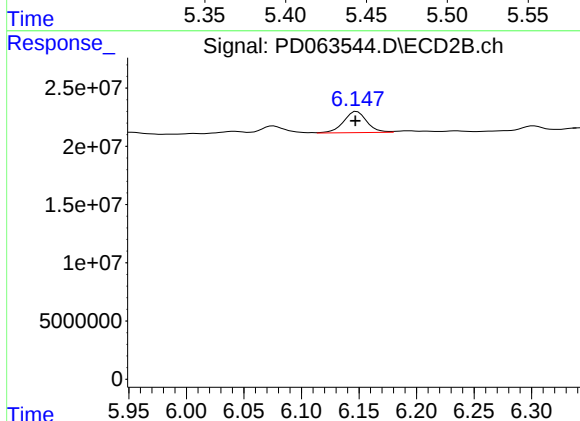


#11 alpha-Chlordane

R.T.: 6.148 min
Delta R.T.: 0.001 min
Response: 25736139
Conc: 1.45 ng/ml

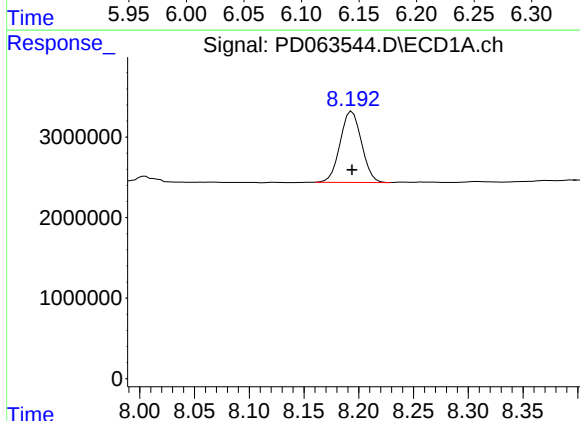

#28 Decachlorobiphenyl

R.T.: 8.194 min
Delta R.T.: 0.000 min
Response: 11997110
Conc: 7.63 ng/ml

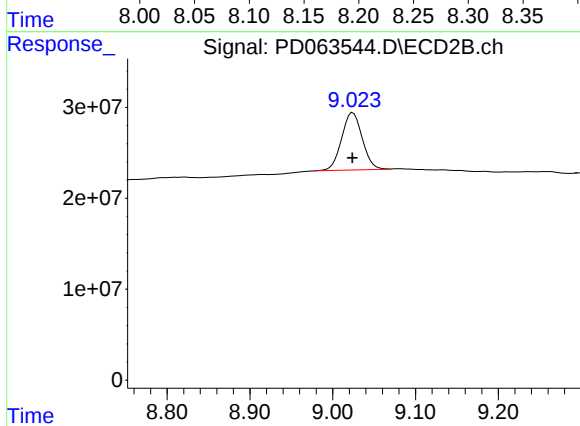

#28 Decachlorobiphenyl

R.T.: 9.024 min
Delta R.T.: 0.000 min
Response: 109506500
Conc: 7.92 ng/ml