

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD060721\  
 Data File : PD063558.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 07 Jun 2021 18:08  
 Operator : AR\AJ  
 Sample : M2603-26  
 Misc :  
 ALS Vial : 36 Sample Multiplier: 1

Instrument :  
 ECD\_D  
 ClientSampleId :  
 FAM4-WC7

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Jun 08 04:18:46 2021  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD060221.M  
 Quant Title : GC Extractables  
 QLast Update : Thu Jun 03 01:33:41 2021  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2 µl  
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1  
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

|                             | Compound        | RT#1  | RT#2  | Resp#1   | Resp#2  | ng/ml  | ng/ml  |
|-----------------------------|-----------------|-------|-------|----------|---------|--------|--------|
| -----                       |                 |       |       |          |         |        |        |
| System Monitoring Compounds |                 |       |       |          |         |        |        |
| 1)                          | SA Tetrachlo... | 3.439 | 3.970 | 31895739 | 332.0E6 | 23.050 | 24.782 |
| 28)                         | SA Decachlor... | 8.195 | 9.025 | 35939265 | 313.0E6 | 22.852 | 22.647 |

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD060721\  
Data File : PD063558.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 07 Jun 2021 18:08  
Operator : AR\AJ  
Sample : M2603-26  
Misc :  
ALS Vial : 36 Sample Multiplier: 1

Instrument :  
ECD\_D  
ClientSampleId :  
FAM4-WC7

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Jun 08 04:18:46 2021  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD060221.M  
Quant Title : GC Extractables  
QLast Update : Thu Jun 03 01:33:41 2021  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 2 µl  
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1  
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

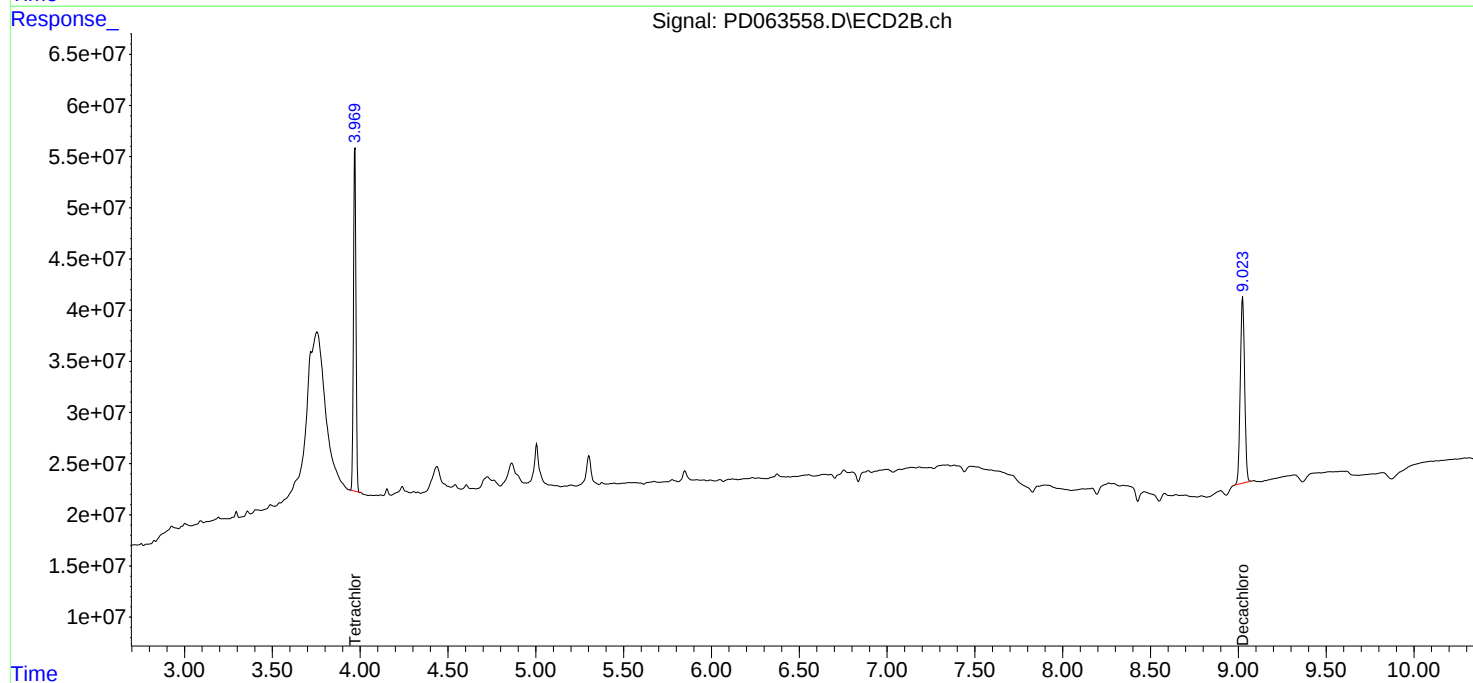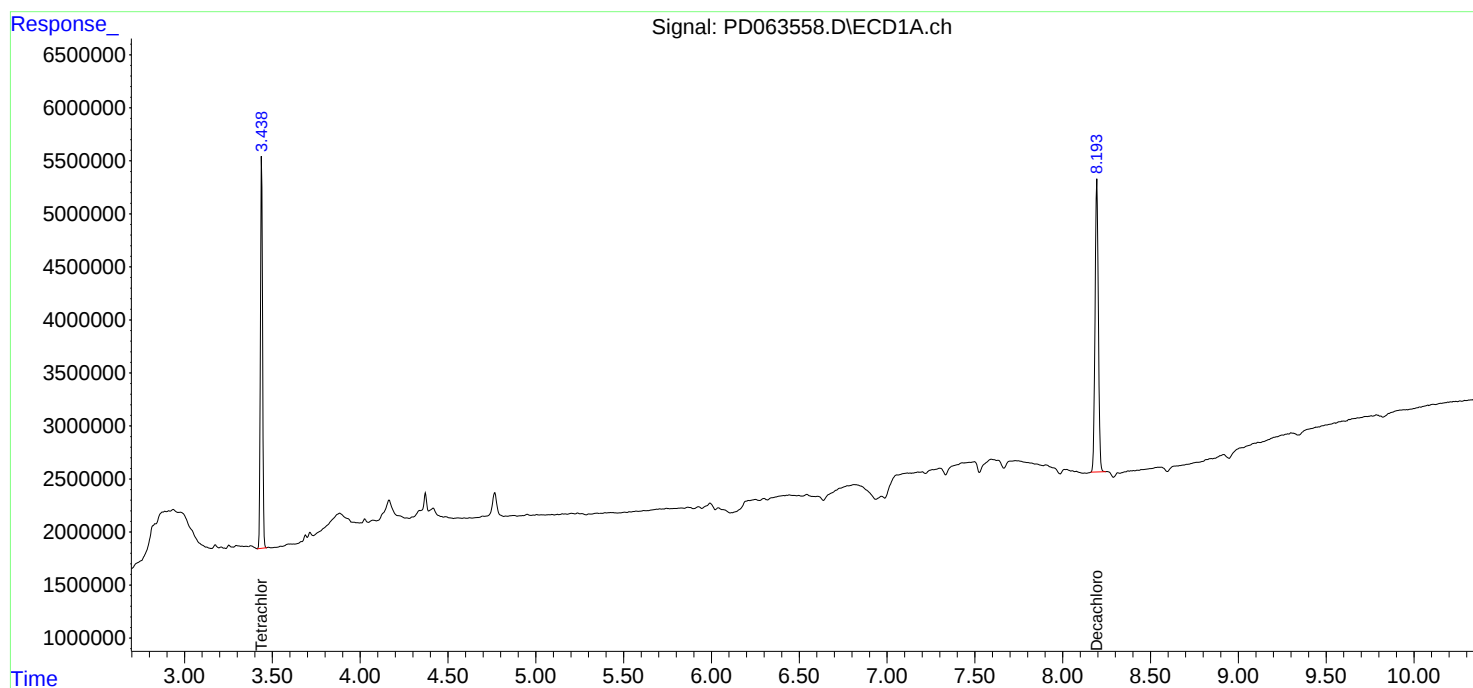


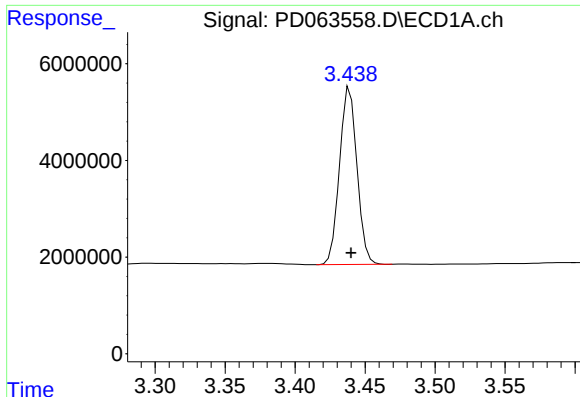

#1 Tetrachloro-m-xylene


R.T.: 3.439 min  
Delta R.T.: 0.000 min  
Response: 31895739  
Conc: 23.05 ng/ml

Instrument :  
ECD\_D  
ClientSampleId :  
FAM4-WC7

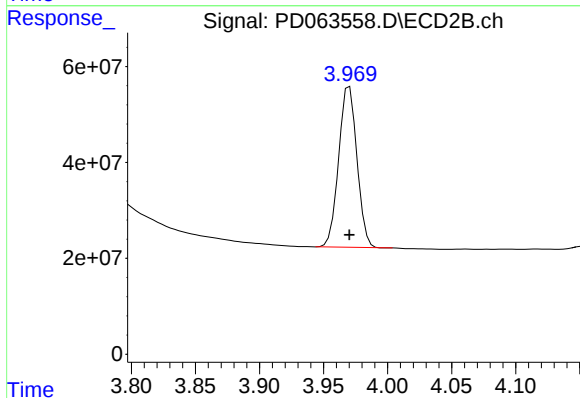


#1 Tetrachloro-m-xylene

R.T.: 3.970 min  
Delta R.T.: 0.000 min  
Response: 332046265  
Conc: 24.78 ng/ml

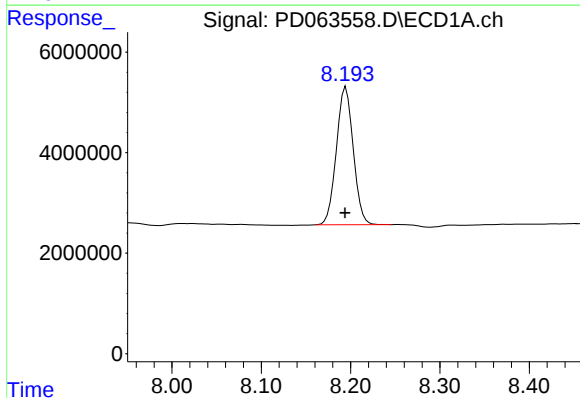

#28 Decachlorobiphenyl

R.T.: 8.195 min  
Delta R.T.: 0.001 min  
Response: 35939265  
Conc: 22.85 ng/ml

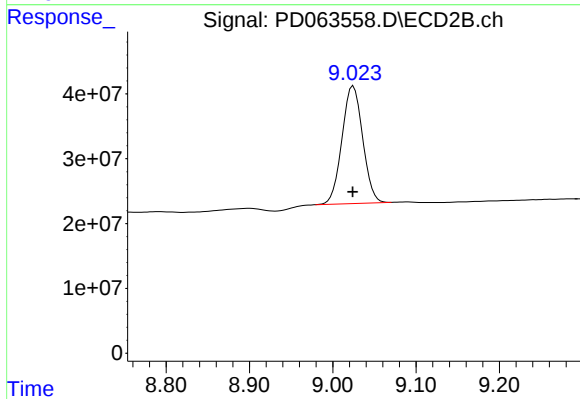

#28 Decachlorobiphenyl

R.T.: 9.025 min  
Delta R.T.: 0.001 min  
Response: 312950010  
Conc: 22.65 ng/ml