

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060721\
 Data File : PD063565.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Jun 2021 20:01
 Operator : AR\AJ
 Sample : M2612-02
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 18-B12(10-14)

Manual Integrations
 APPROVED

Ankita
 6/8/2021 11:53:12 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 08 04:20:32 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060221.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 03 01:33:41 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.439	3.970	15516648	158.9E6	11.214	11.861
28)	SA Decachlor...	8.195	9.024	16731147	154.3E6	10.638	11.164
Target Compounds							
12)	B 4,4'-DDE	5.597	6.299	2617882	25880212	1.506m	1.424m
14)	MA Endrin	5.986	6.664	877712	9562299	0.552m	0.622

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060721\
Data File : PD063565.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Jun 2021 20:01
Operator : AR\AJ
Sample : M2612-02
Misc :
ALS Vial : 40 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampled :
18-B12(10-14)


Manual Integrations
APPROVED

Ankita
6/8/2021 11:53:12 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 08 04:20:32 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060221.M
Quant Title : GC Extractables
QLast Update : Thu Jun 03 01:33:41 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

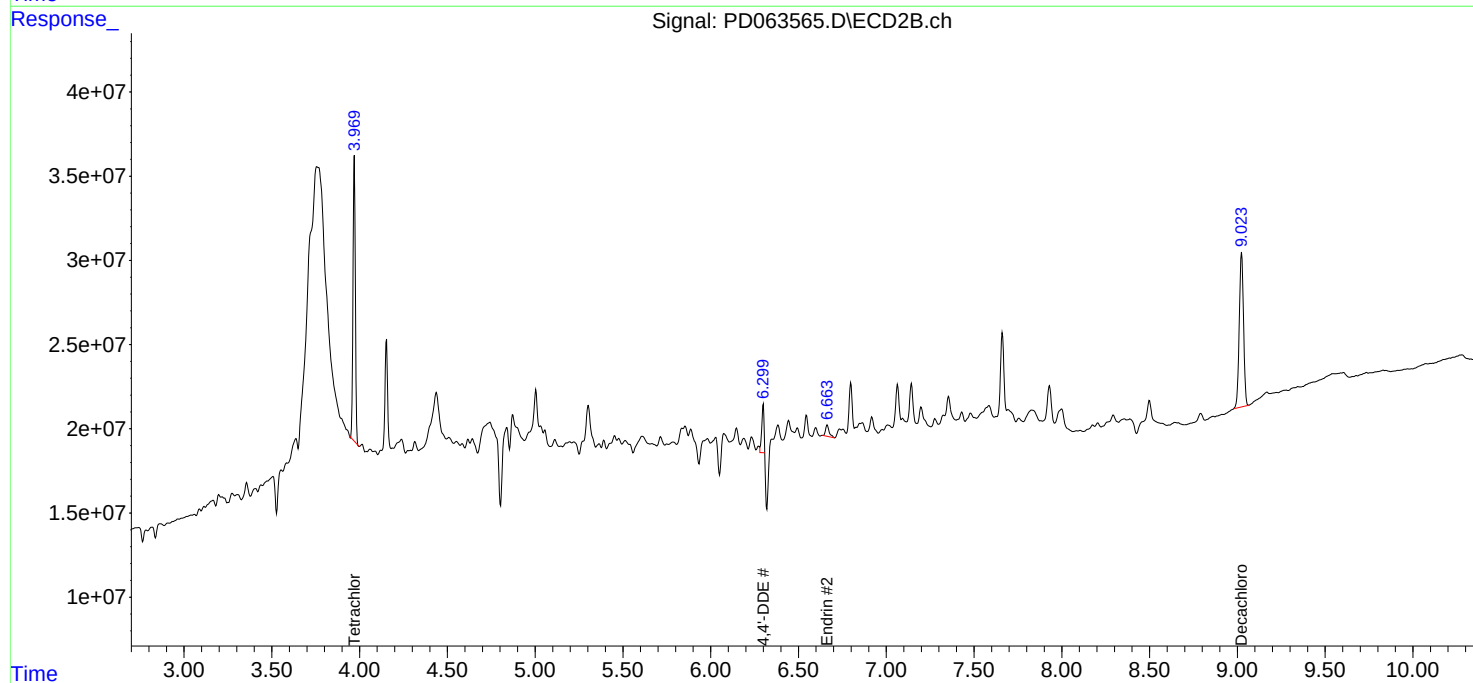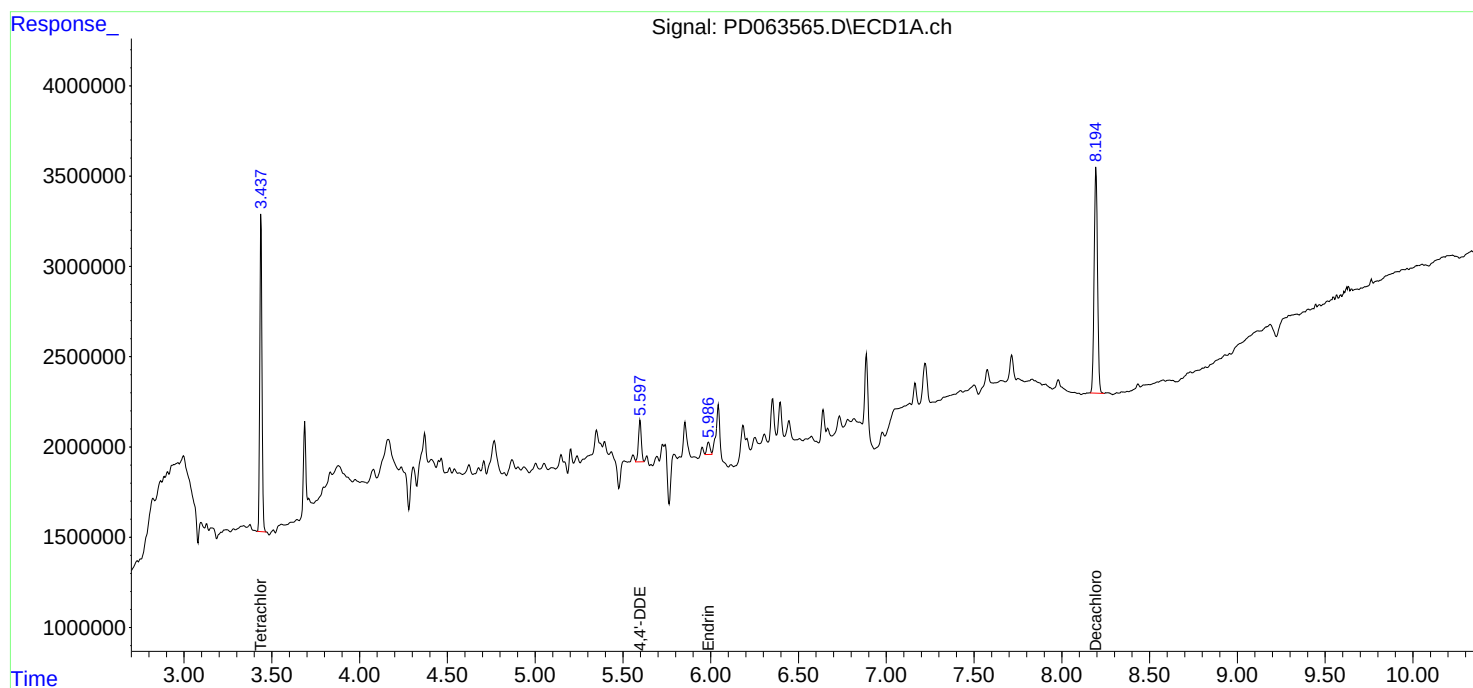

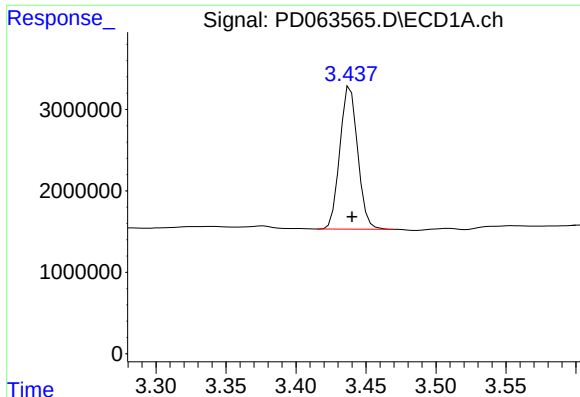


#1 Tetrachloro-m-xylene

R.T.: 3.439 min
Delta R.T.: -0.001 min
Response: 15516648
Conc: 11.21 ng/ml

Instrument :
ECD_D
ClientSampleId :
18-B12(10-14)


Manual Integrations
APPROVED

Ankita
6/8/2021 11:53:12 AM

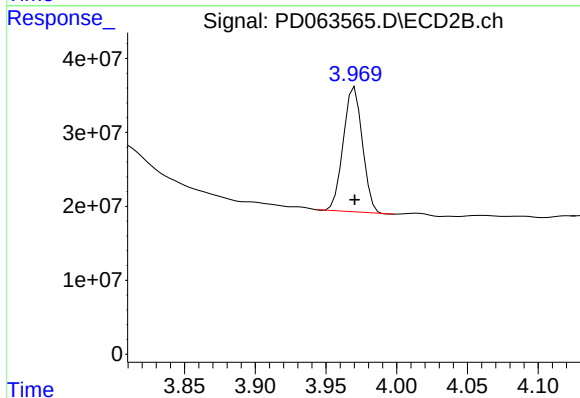


#1 Tetrachloro-m-xylene

R.T.: 3.970 min
Delta R.T.: 0.000 min
Response: 158925896
Conc: 11.86 ng/ml

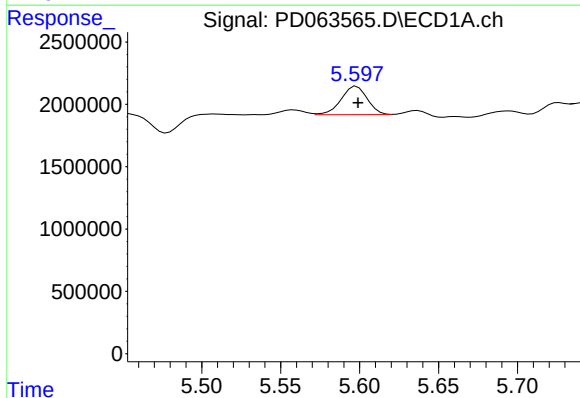


#12 4,4'-DDE

R.T.: 5.597 min
Delta R.T.: -0.002 min
Response: 2617882
Conc: 1.51 ng/ml m

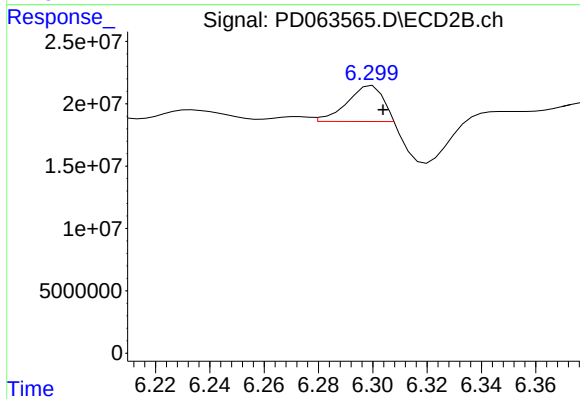

#12 4,4'-DDE

R.T.: 6.299 min
Delta R.T.: -0.005 min
Response: 25880212
Conc: 1.42 ng/ml m

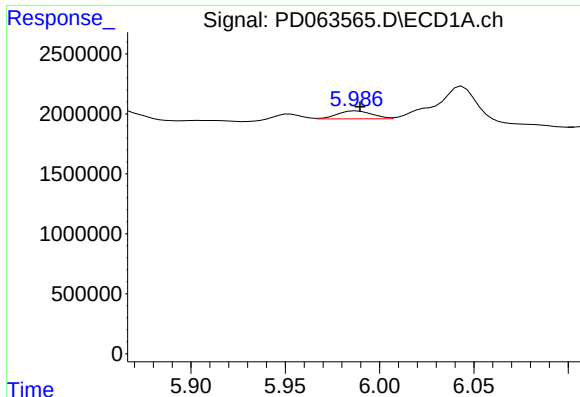


#14 Endrin

R.T.: 5.986 min
Delta R.T.: -0.003 min
Response: 877712
Conc: 0.55 ng/ml m

Instrument :
ECD_D
ClientSampleId :
18-B12(10-14)


Manual Integrations
APPROVED

Ankita
6/8/2021 11:53:12 AM

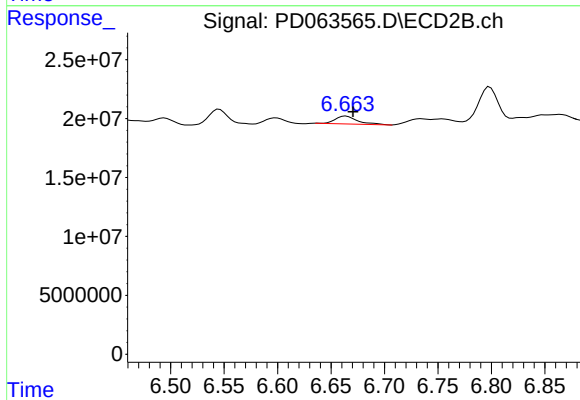


#14 Endrin

R.T.: 6.664 min
Delta R.T.: -0.007 min
Response: 9562299
Conc: 0.62 ng/ml

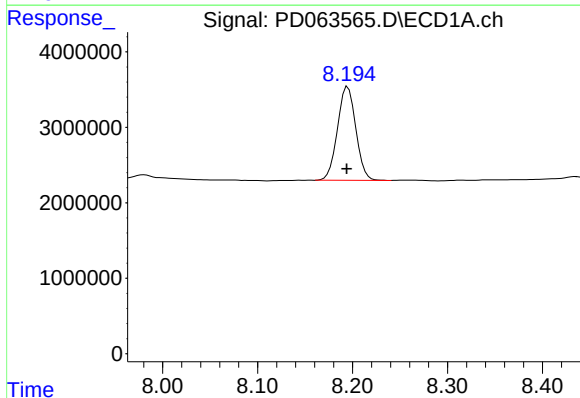

#28 Decachlorobiphenyl

R.T.: 8.195 min
Delta R.T.: 0.001 min
Response: 16731147
Conc: 10.64 ng/ml

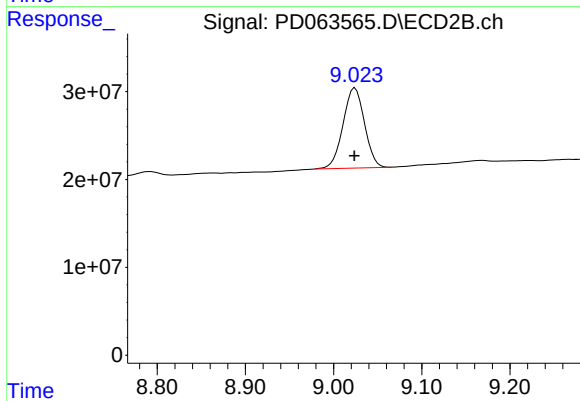

#28 Decachlorobiphenyl

R.T.: 9.024 min
Delta R.T.: 0.000 min
Response: 154271780
Conc: 11.16 ng/ml