

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060722\
 Data File : PD070174.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Jun 2022 20:05
 Operator : AR\AJ
 Sample : N3189-01
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 08 01:18:18 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060622.M
 Quant Title : GC Extractables
 QLast Update : Tue Jun 07 06:00:04 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.440	4.168	18997148	176.1E6	17.498	18.038
2)	SA Decachlor...	8.192	9.360	12792733	73843924	11.503	12.006
Target Compounds							
10)	B gamma-Chl...	0.000	6.317	0	9280361	N.D.	0.807 #
25)	Chlordane-3	0.000	6.317	0	9280361	N.D.	5.858 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060722\
Data File : PD070174.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Jun 2022 20:05
Operator : AR\AJ
Sample : N3189-01
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 08 01:18:18 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060622.M
Quant Title : GC Extractables
QLast Update : Tue Jun 07 06:00:04 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

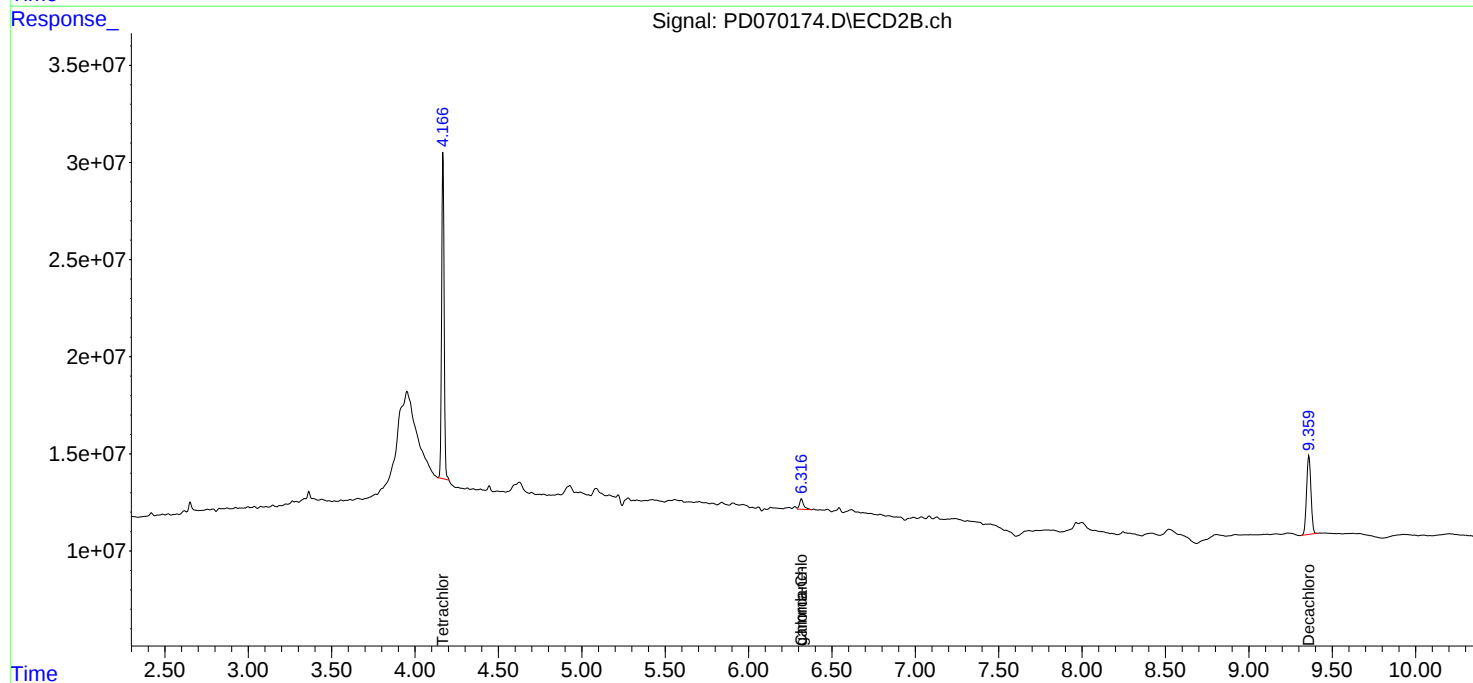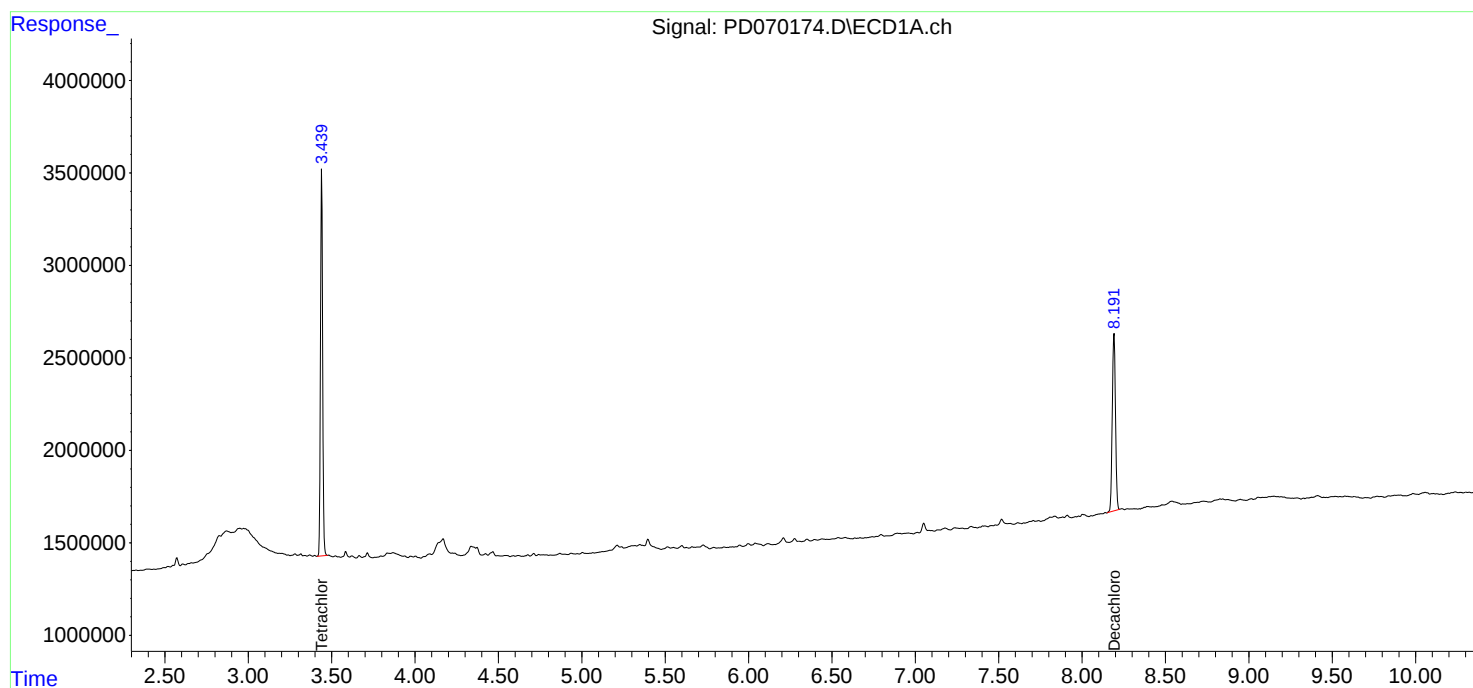


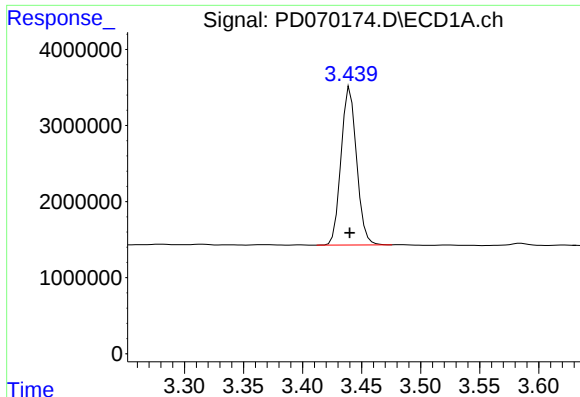

#1 Tetrachloro-m-xylene


R.T.: 3.440 min
Delta R.T.: 0.000 min
Response: 18997148
Conc: 17.50 ng/ml

Instrument :
ECD_D
ClientSampleId :

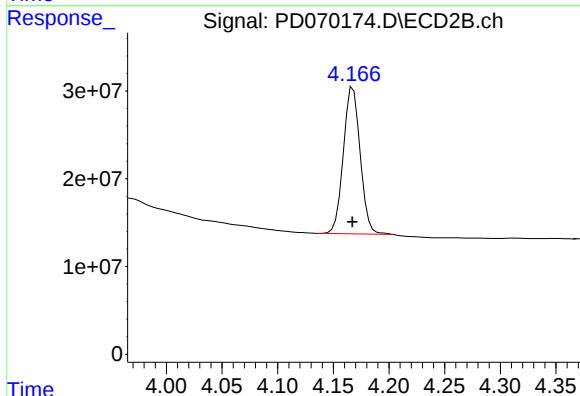


#1 Tetrachloro-m-xylene

R.T.: 4.168 min
Delta R.T.: 0.000 min
Response: 176079186
Conc: 18.04 ng/ml

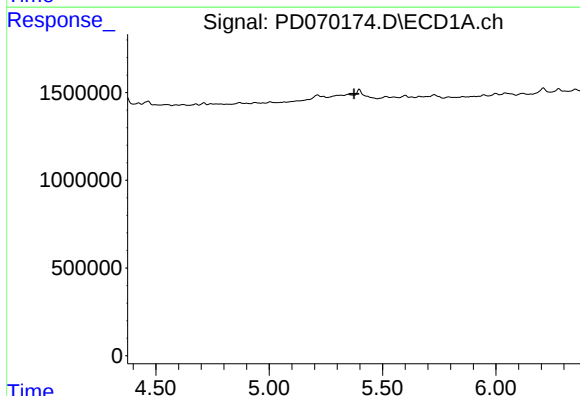


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.375 min
Response: 0
Conc: N.D.

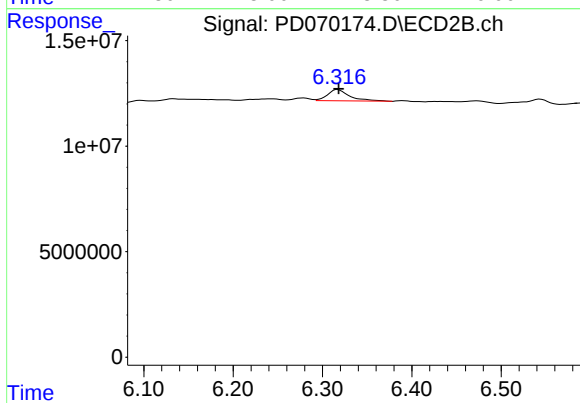

#10 gamma-Chlordane


R.T.: 6.317 min
Delta R.T.: 0.000 min
Response: 9280361
Conc: 0.81 ng/ml

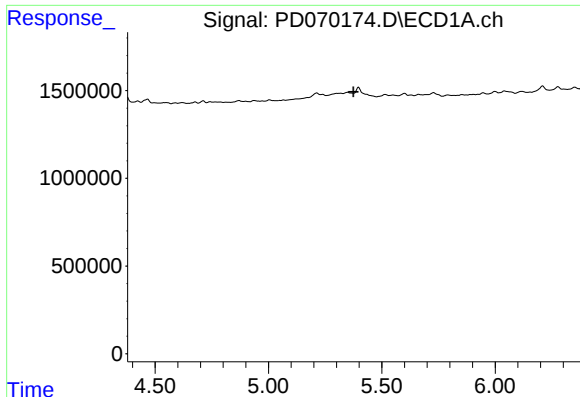

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.376 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

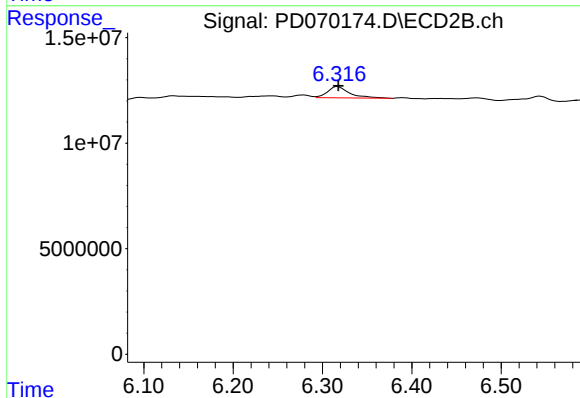


#25 Chlordane-3

R.T.: 6.317 min
Delta R.T.: 0.000 min
Response: 9280361
Conc: 5.86 ng/ml

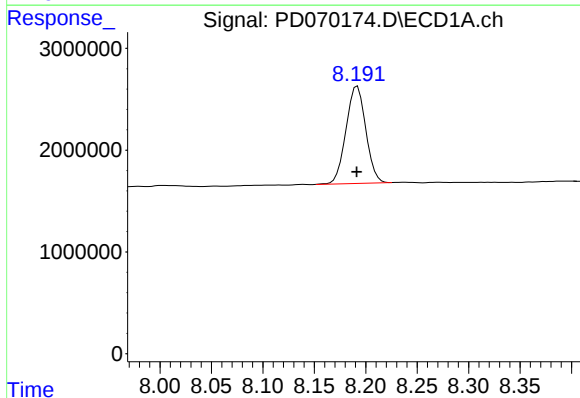

#28 Decachlorobiphenyl

R.T.: 8.192 min
Delta R.T.: 0.000 min
Response: 12792733
Conc: 11.50 ng/ml

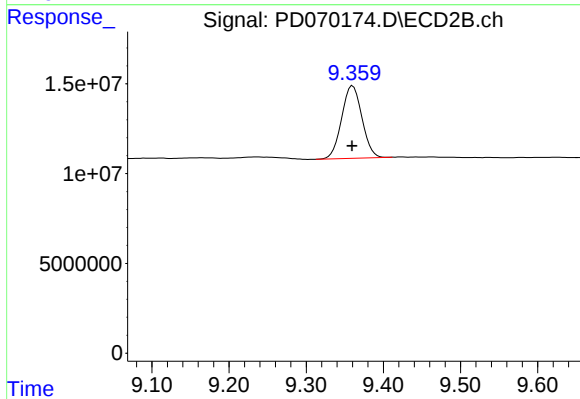

#28 Decachlorobiphenyl

R.T.: 9.360 min
Delta R.T.: 0.000 min
Response: 73843924
Conc: 12.01 ng/ml