

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060722\
 Data File : PD070167.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Jun 2022 15:54
 Operator : AR\AJ
 Sample : N2985-19DL 5X
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 P021-SS007-0006-01DL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 08 05:41:56 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060622.M
 Quant Title : GC Extractables
 QLast Update : Wed Jun 08 02:48:31 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.441	4.167	4428103	45647913	4.079	4.676
28) SA Decachlor...	8.193	9.361	4307194	24169470	3.873	3.930
Target Compounds						
12) B 4,4'-DDE	5.600	6.543	1655618	18378141	1.324	1.753 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060722\
Data File : PD070167.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Jun 2022 15:54
Operator : AR\AJ
Sample : N2985-19DL 5X
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
P021-SS007-0006-01DL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 08 05:41:56 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060622.M
Quant Title : GC Extractables
QLast Update : Wed Jun 08 02:48:31 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

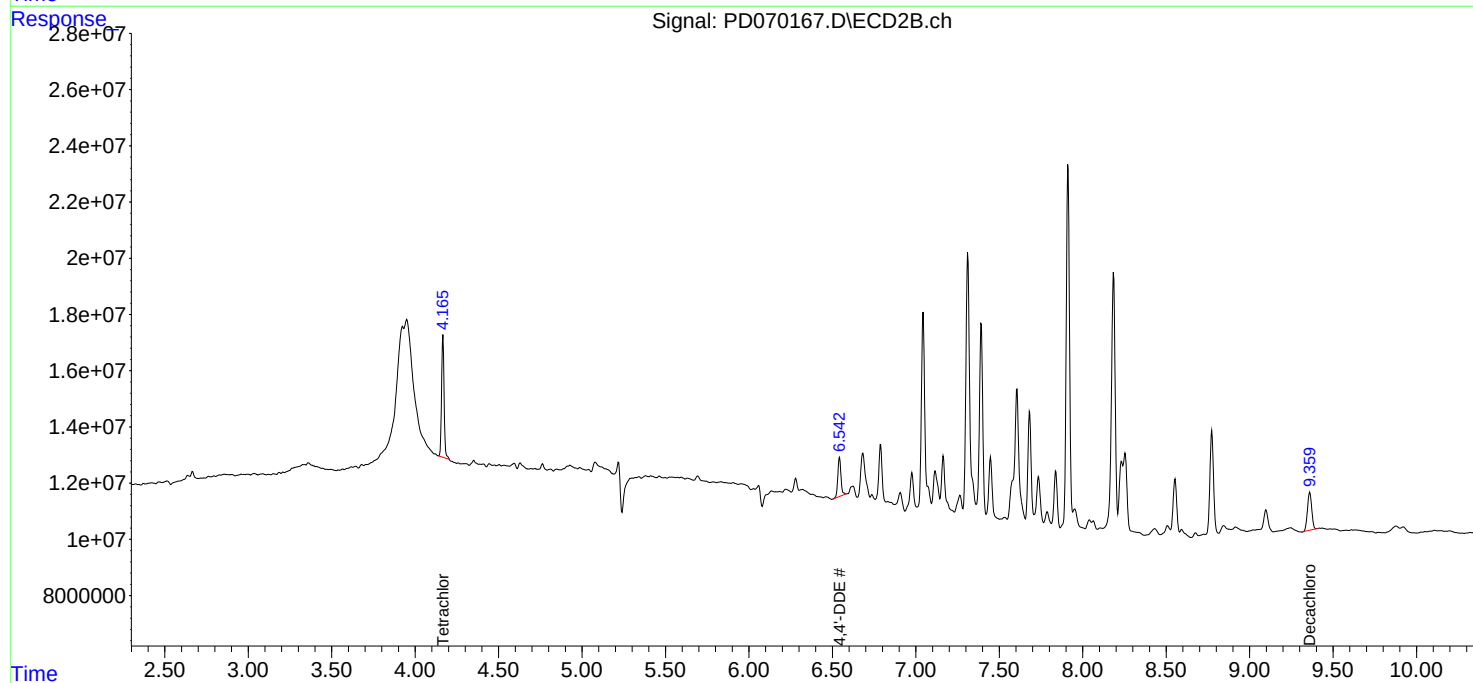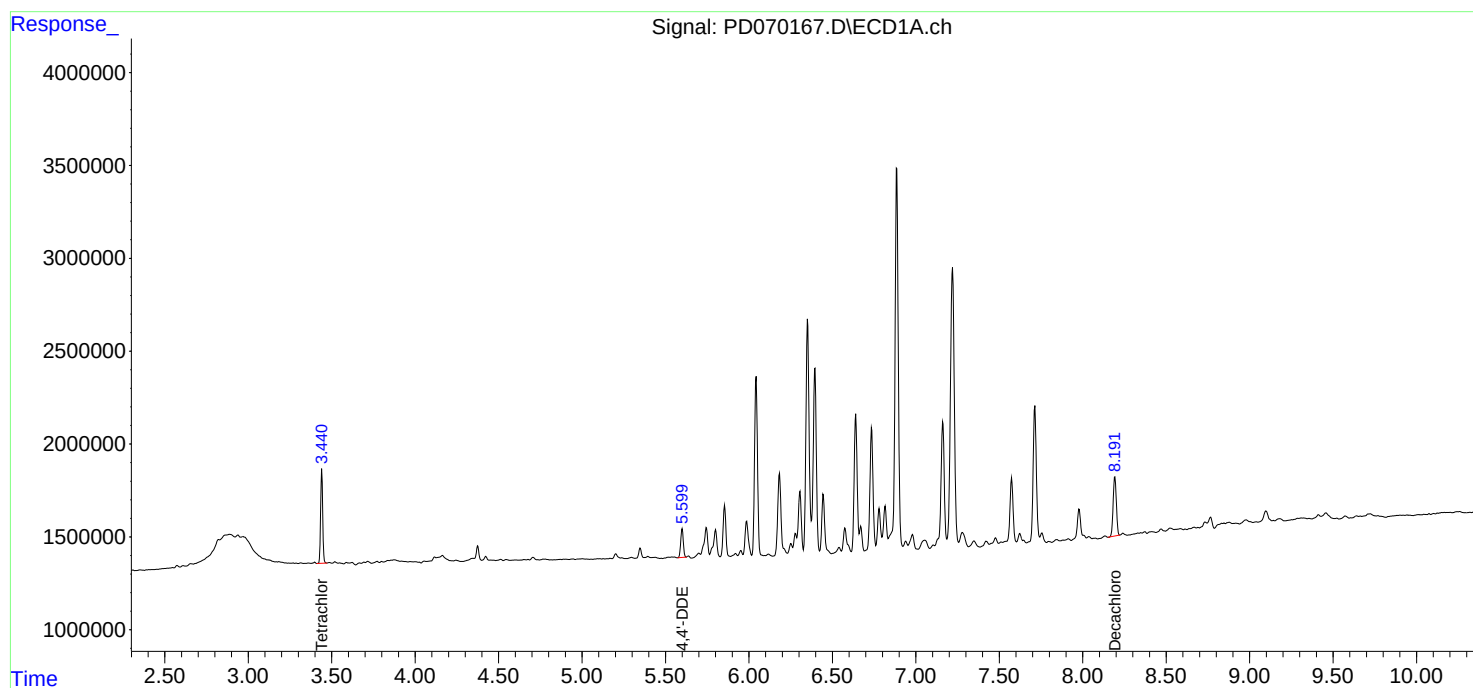


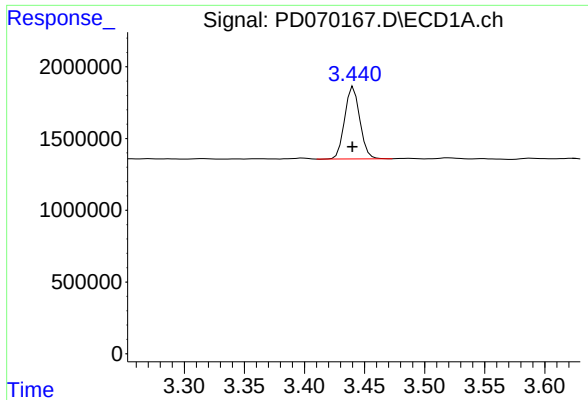

#1 Tetrachloro-m-xylene


R.T.: 3.441 min
Delta R.T.: 0.000 min
Response: 4428103
Conc: 4.08 ng/ml

Instrument :
ECD_D
ClientSampleId :
P021-SS007-0006-01DL

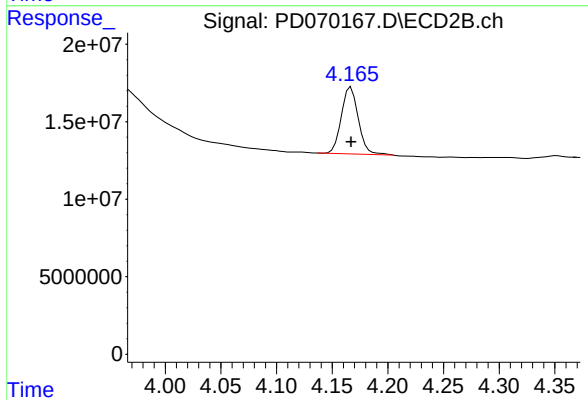


#1 Tetrachloro-m-xylene

R.T.: 4.167 min
Delta R.T.: 0.000 min
Response: 45647913
Conc: 4.68 ng/ml

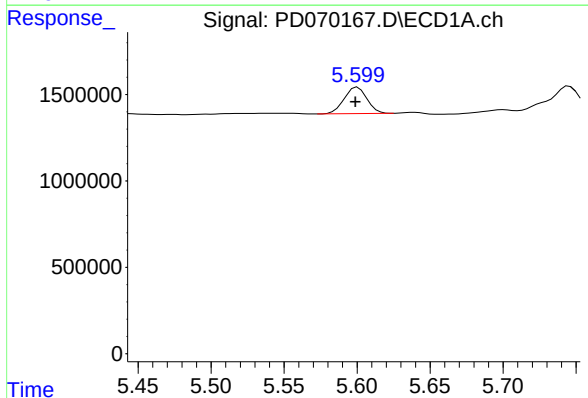


#12 4,4'-DDE

R.T.: 5.600 min
Delta R.T.: 0.002 min
Response: 1655618
Conc: 1.32 ng/ml

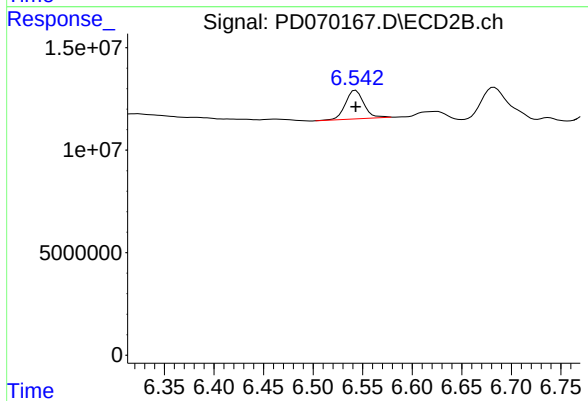

#12 4,4'-DDE


R.T.: 6.543 min
Delta R.T.: 0.000 min
Response: 18378141
Conc: 1.75 ng/ml

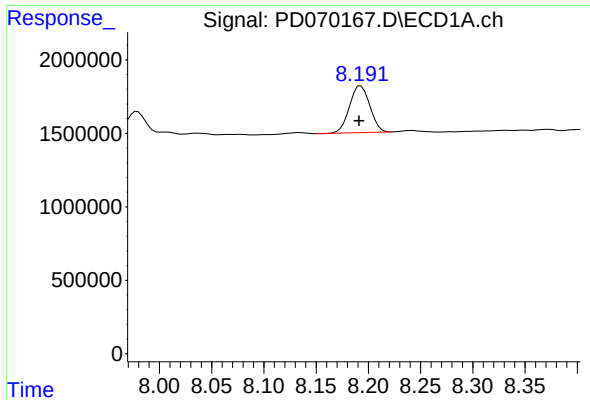

#28 Decachlorobiphenyl

R.T.: 8.193 min
Delta R.T.: 0.002 min
Response: 4307194
Conc: 3.87 ng/ml

Instrument :
ECD_D
ClientSampleId :
P021-SS007-0006-01DL

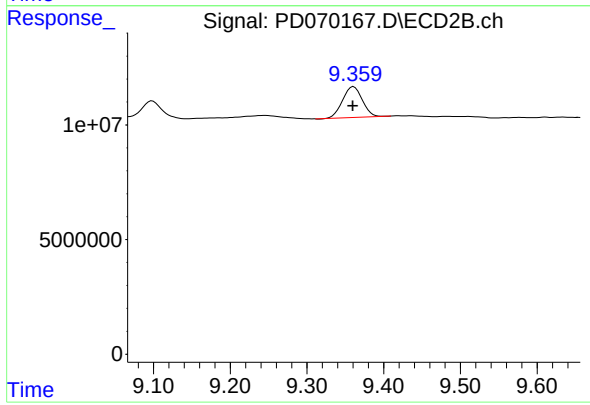

#28 Decachlorobiphenyl

R.T.: 9.361 min
Delta R.T.: 0.001 min
Response: 24169470
Conc: 3.93 ng/ml