

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060724\
 Data File : PD083457.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Jun 2024 17:10
 Operator : AR\AJ
 Sample : INDA101
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 07 03:45:13 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060724CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 07 03:41:46 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.563	2.773	6467329	28020724	4.952	5.132
27)	SA Decachlor...	9.122	7.902	20226129	63870002	10.445	10.554
Target Compounds							
2)	A alpha-BHC	4.020	3.273	10154726	41267618	4.696	4.820
3)	MA gamma-BHC...	4.354	3.601	10018954	38123821	4.683	4.870
4)	MA Heptachlor	4.946	3.940	11579725	38780463	4.827	4.929
9)	A Endosulfan I	6.106	5.089	9469988	33314931	4.868	5.006
13)	MA Dieldrin	6.381	5.353	19589857	72131815	9.595	9.789
14)	MA Endrin	6.612	5.629	16008427	64649762	9.525	9.900
16)	A 4,4'-DDD	6.745	5.775	13748681	54959069	9.502	9.660
17)	MA 4,4'-DDT	7.061	6.026	13783912	51924082	9.198	9.042
20)	A Methoxychlor	7.538	6.601	43991784	158.1E6	50.828	53.263


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060724\
Data File : PD083457.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Jun 2024 17:10
Operator : AR\AJ
Sample : INDA101
Misc :
ALS Vial : 9 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 07 03:45:13 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060724CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jun 07 03:41:46 2024
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

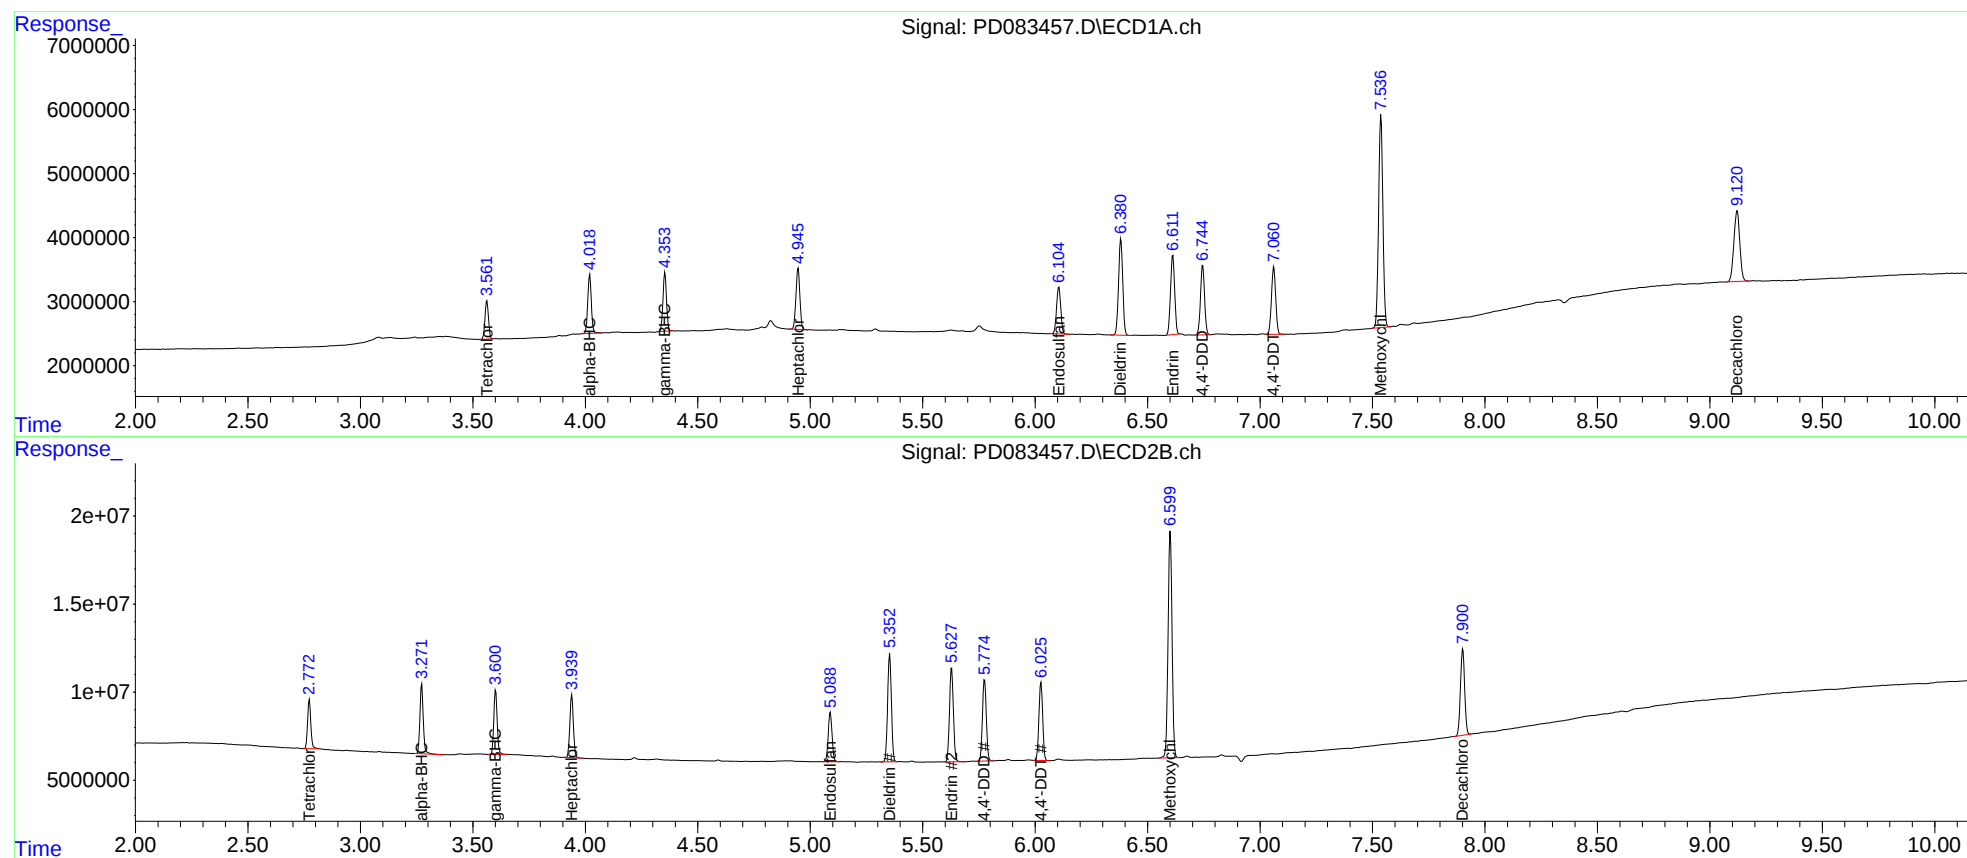

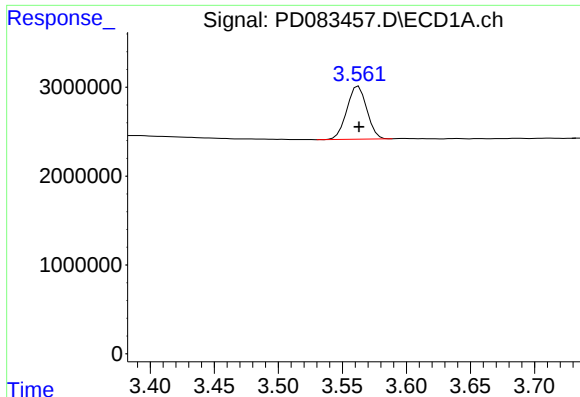


#1 Tetrachloro-m-xylene

R.T.: 3.563 min
Delta R.T.: 0.000 min
Response: 6467329
Conc: 4.95 ng/ml

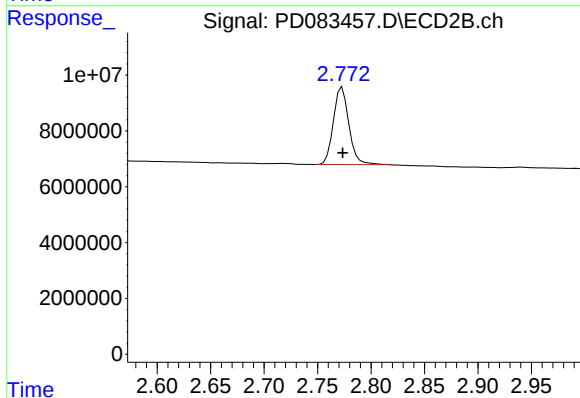


#1 Tetrachloro-m-xylene

R.T.: 2.773 min
Delta R.T.: 0.000 min
Response: 28020724
Conc: 5.13 ng/ml

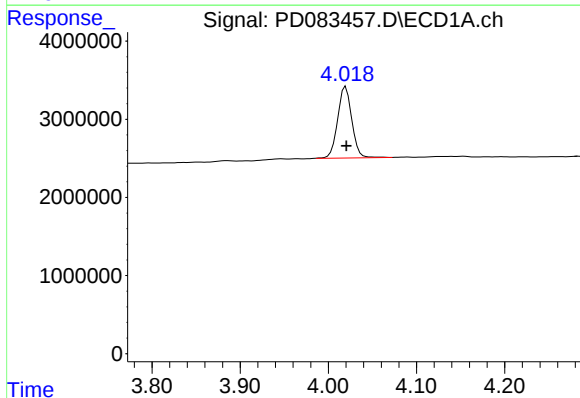


#2 alpha-BHC

R.T.: 4.020 min
Delta R.T.: 0.000 min
Response: 10154726
Conc: 4.70 ng/ml

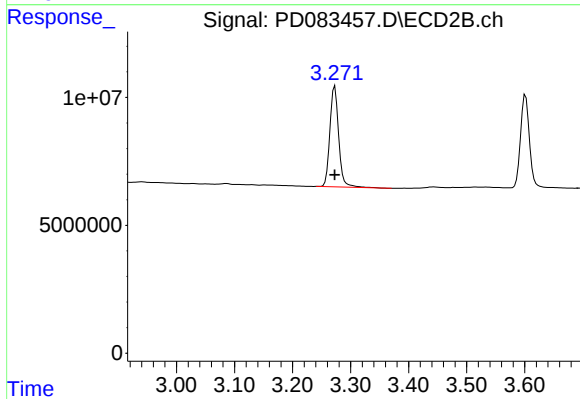


#2 alpha-BHC

R.T.: 3.273 min
Delta R.T.: 0.000 min
Response: 41267618
Conc: 4.82 ng/ml

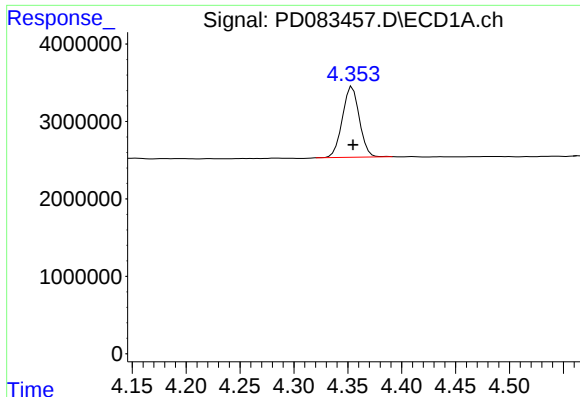


#3 gamma-BHC (Lindane)

R.T.: 4.354 min
Delta R.T.: 0.000 min
Response: 10018954
Conc: 4.68 ng/ml

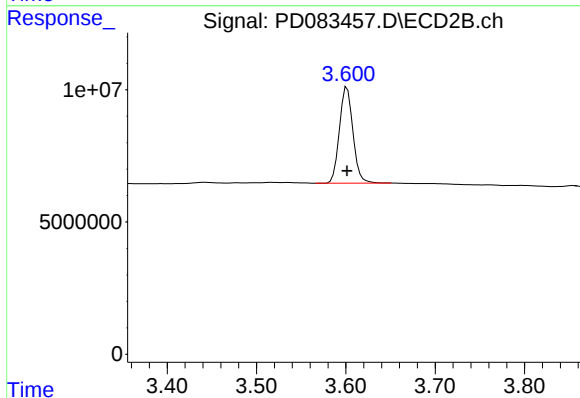


#3 gamma-BHC (Lindane)

R.T.: 3.601 min
Delta R.T.: 0.000 min
Response: 38123821
Conc: 4.87 ng/ml

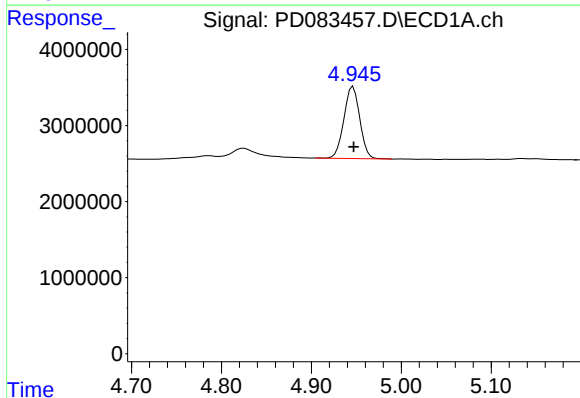


#4 Heptachlor

R.T.: 4.946 min
Delta R.T.: 0.000 min
Response: 11579725
Conc: 4.83 ng/ml

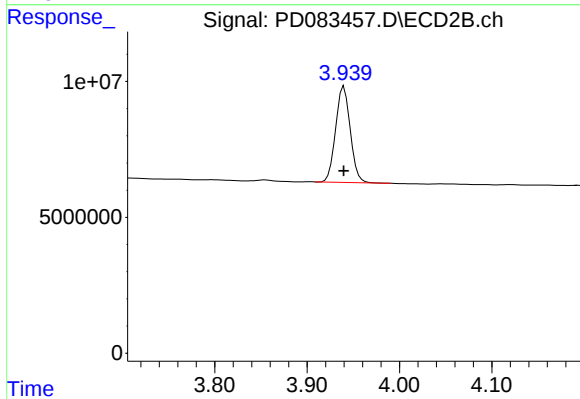


#4 Heptachlor

R.T.: 3.940 min
Delta R.T.: 0.000 min
Response: 38780463
Conc: 4.93 ng/ml

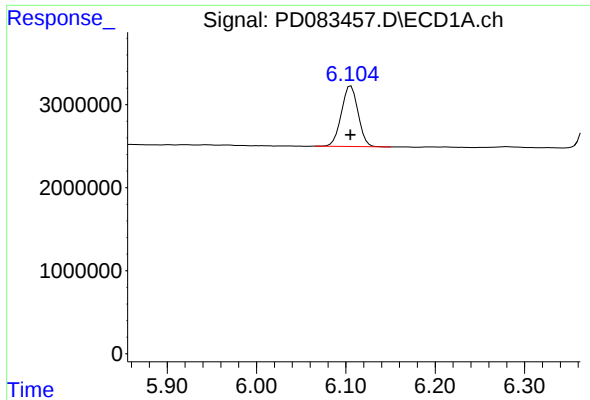


#9 Endosulfan I

R.T.: 6.106 min
Delta R.T.: 0.000 min
Response: 9469988
Conc: 4.87 ng/ml

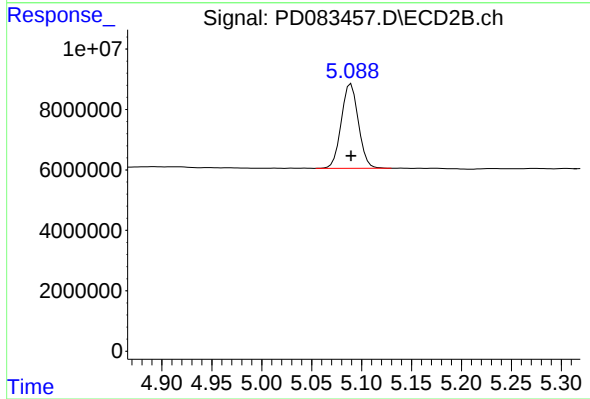


#9 Endosulfan I

R.T.: 5.089 min
Delta R.T.: 0.000 min
Response: 33314931
Conc: 5.01 ng/ml

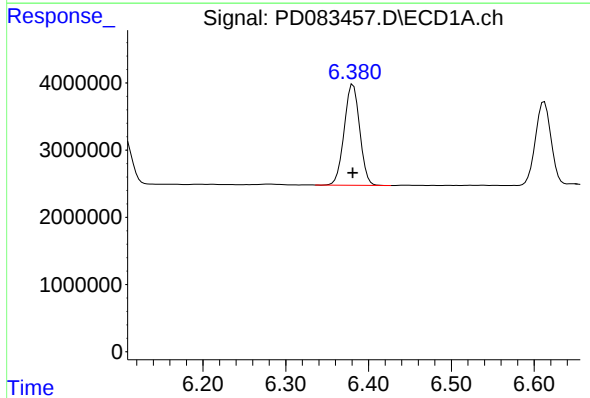


#13 Dieldrin

R.T.: 6.381 min
Delta R.T.: 0.000 min
Response: 19589857
Conc: 9.59 ng/ml

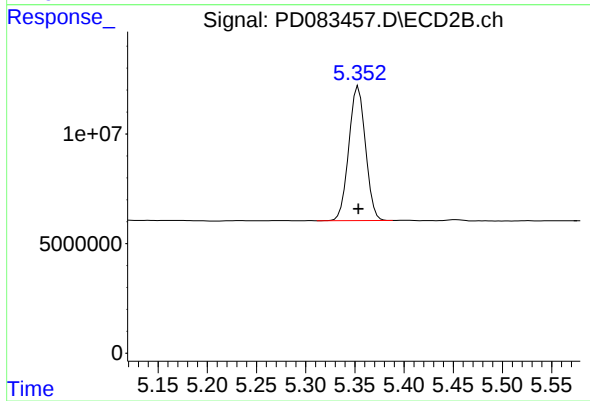


#13 Dieldrin

R.T.: 5.353 min
Delta R.T.: 0.000 min
Response: 72131815
Conc: 9.79 ng/ml

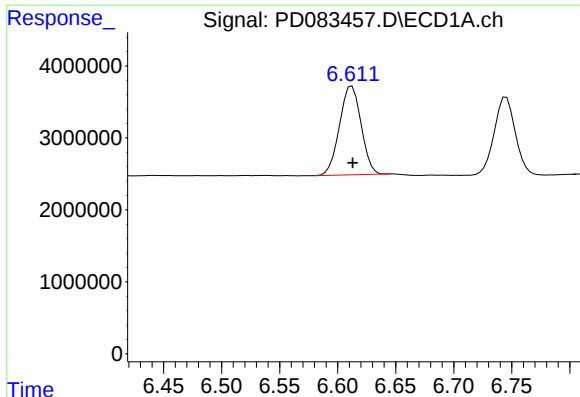


#14 Endrin

R.T.: 6.612 min
Delta R.T.: 0.000 min
Response: 16008427
Conc: 9.52 ng/ml

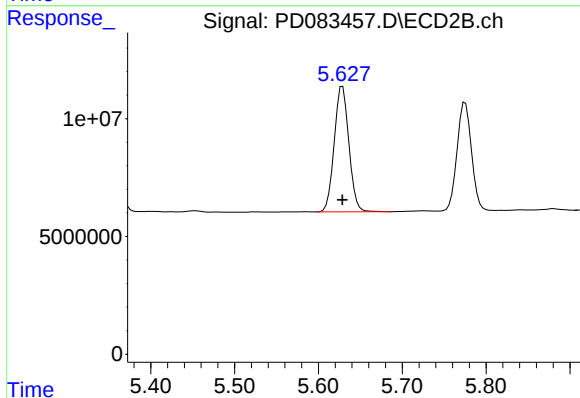


#14 Endrin

R.T.: 5.629 min
Delta R.T.: 0.000 min
Response: 64649762
Conc: 9.90 ng/ml

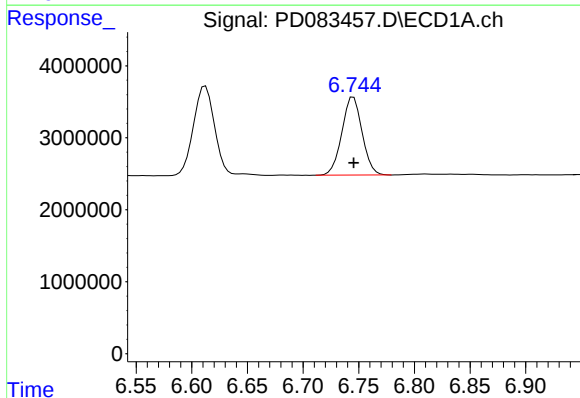


#16 4,4'-DDD

R.T.: 6.745 min
Delta R.T.: 0.000 min
Response: 13748681
Conc: 9.50 ng/ml

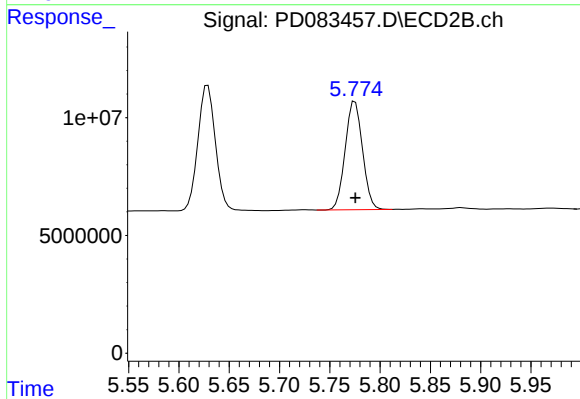


#16 4,4'-DDD

R.T.: 5.775 min
Delta R.T.: 0.000 min
Response: 54959069
Conc: 9.66 ng/ml

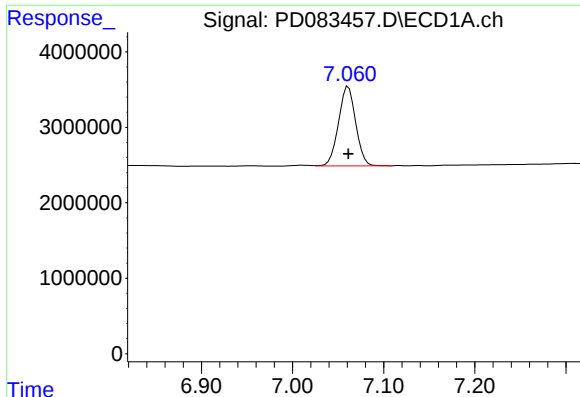


#17 4,4'-DDT

R.T.: 7.061 min
Delta R.T.: 0.000 min
Response: 13783912
Conc: 9.20 ng/ml

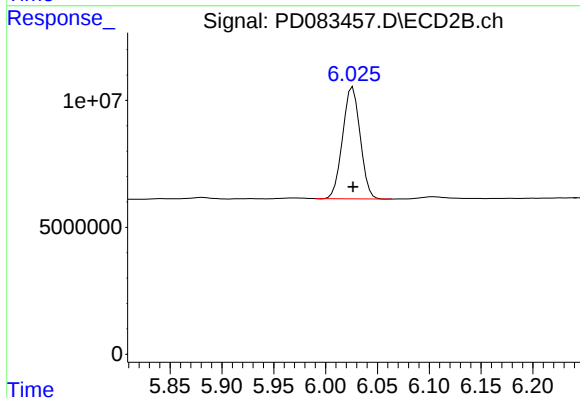


#17 4,4'-DDT

R.T.: 6.026 min
Delta R.T.: 0.000 min
Response: 51924082
Conc: 9.04 ng/ml

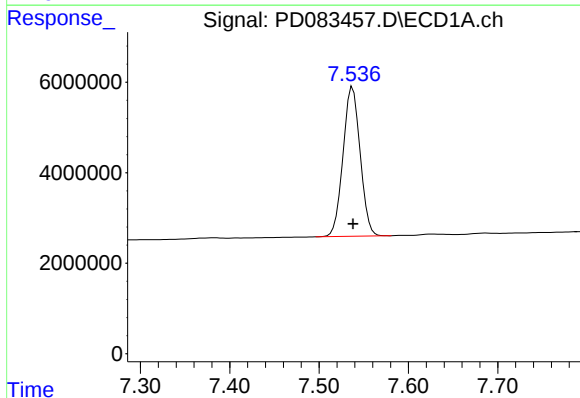


#20 Methoxychlor

R.T.: 7.538 min
Delta R.T.: 0.000 min
Response: 43991784
Conc: 50.83 ng/ml

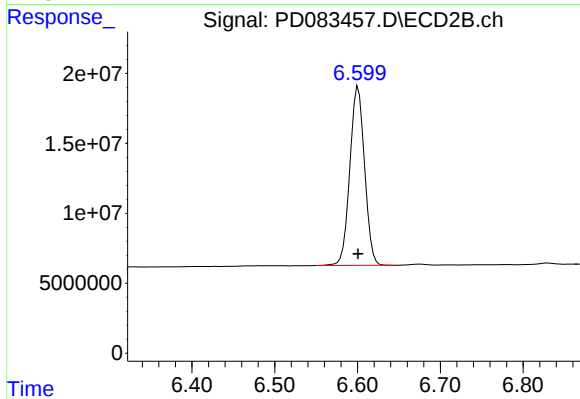


#20 Methoxychlor

R.T.: 6.601 min
Delta R.T.: 0.000 min
Response: 158093919
Conc: 53.26 ng/ml

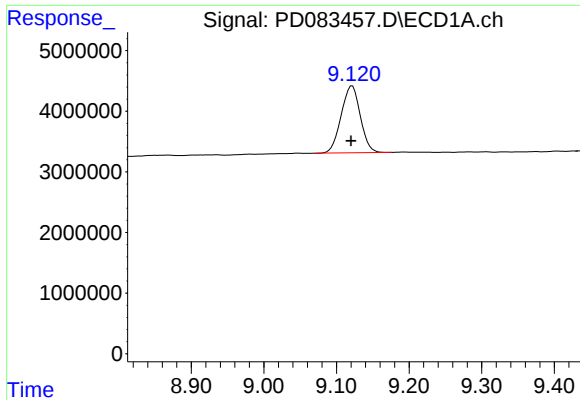

#27 Decachlorobiphenyl

R.T.: 9.122 min
Delta R.T.: 0.002 min
Response: 20226129
Conc: 10.44 ng/ml

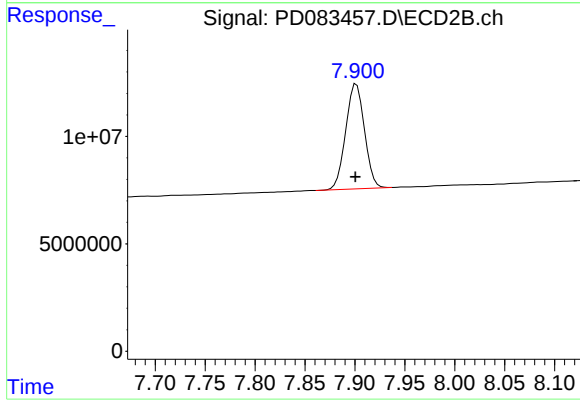

#27 Decachlorobiphenyl

R.T.: 7.902 min
Delta R.T.: 0.001 min
Response: 63870002
Conc: 10.55 ng/ml