

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060724\
 Data File : PD083459.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Jun 2024 17:36
 Operator : AR\AJ
 Sample : INDA201
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 07 03:45:42 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060724CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 07 03:41:46 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.563	2.773	13080342	55477639	10.016	10.160
27)	SA Decachlor...	9.119	7.901	39601613	125.3E6	20.451	20.712
Target Compounds							
2)	A alpha-BHC	4.020	3.273	20739675	83646820	9.590	9.770
3)	MA gamma-BHC...	4.354	3.601	20688082	77325065	9.671	9.878
4)	MA Heptachlor	4.947	3.939	23449027	78246665	9.775	9.946
9)	A Endosulfan I	6.106	5.089	19446919	66990524	9.997	10.066
13)	MA Dieldrin	6.382	5.353	39876137	146.4E6	19.531	19.874
14)	MA Endrin	6.613	5.629	32711279	130.9E6	19.462	20.038
16)	A 4,4'-DDD	6.745	5.775	28061549	112.9E6	19.395	19.849
17)	MA 4,4'-DDT	7.061	6.026	28677716	110.8E6	19.137	19.289
20)	A Methoxychlor	7.538	6.601	86875768	311.4E6	100.375	104.901


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060724\
Data File : PD083459.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Jun 2024 17:36
Operator : AR\AJ
Sample : INDA201
Misc :
ALS Vial : 11 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 07 03:45:42 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060724CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jun 07 03:41:46 2024
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

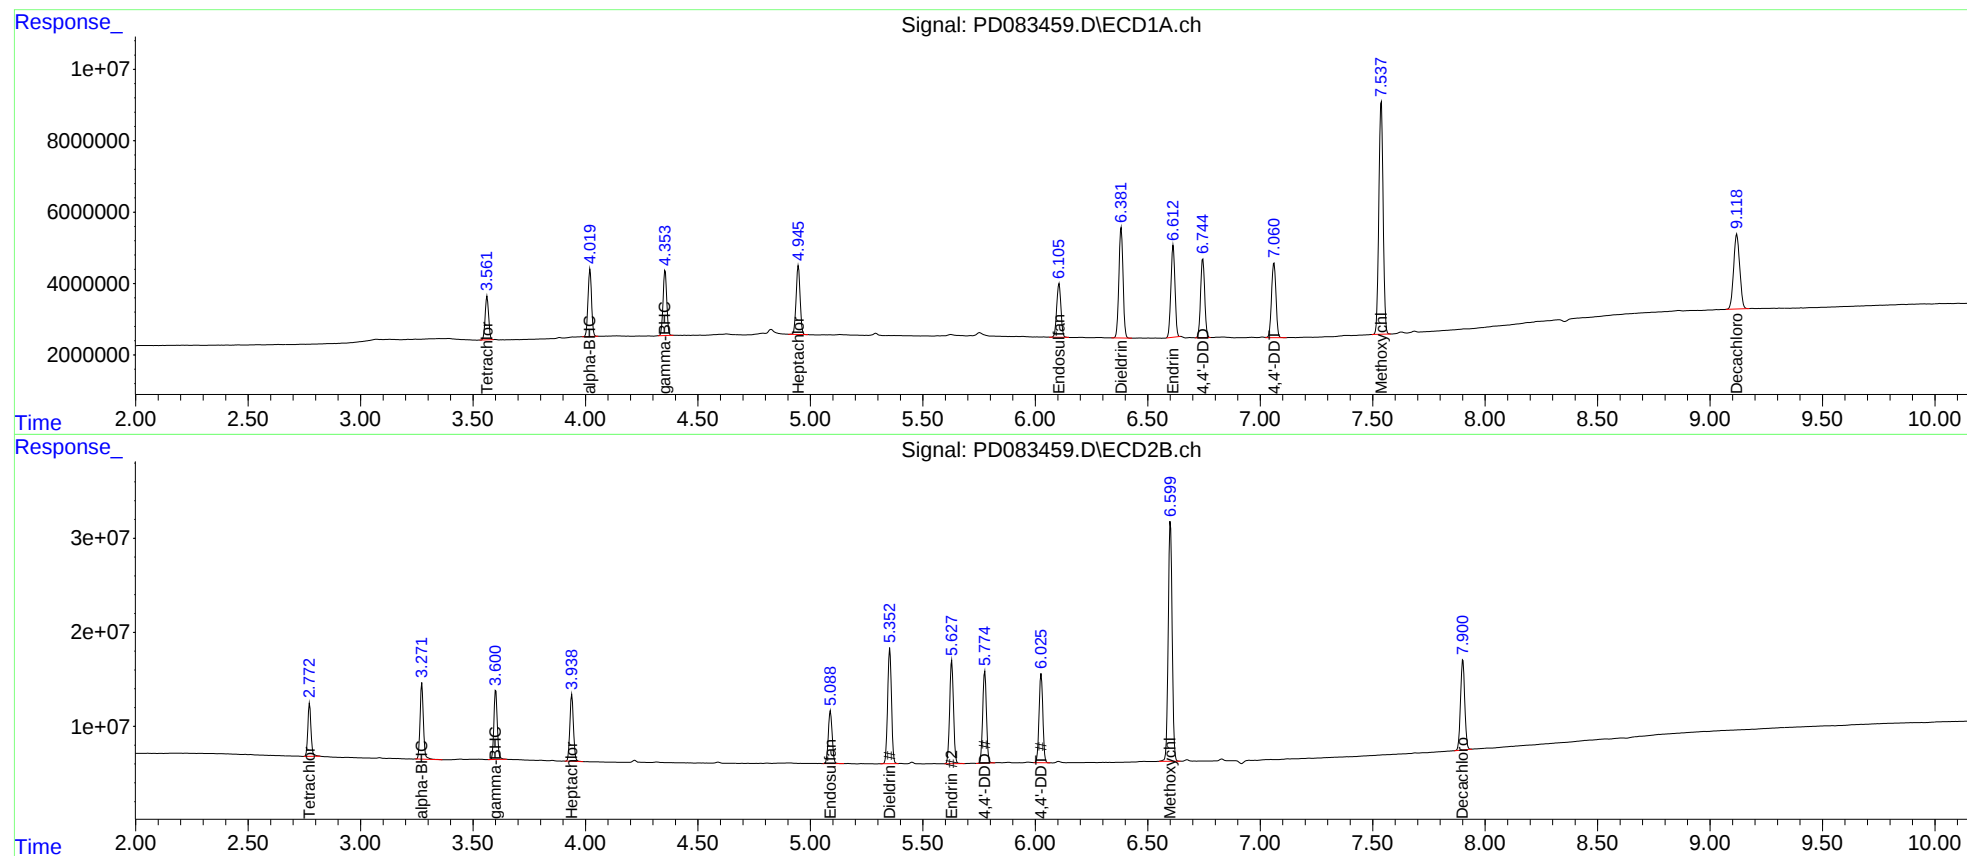

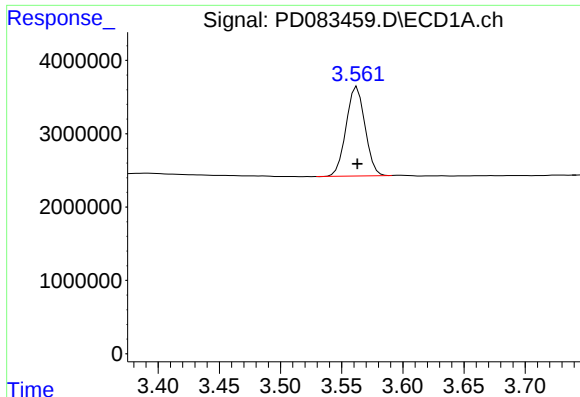


#1 Tetrachloro-m-xylene

R.T.: 3.563 min
Delta R.T.: 0.000 min
Response: 13080342
Conc: 10.02 ng/ml

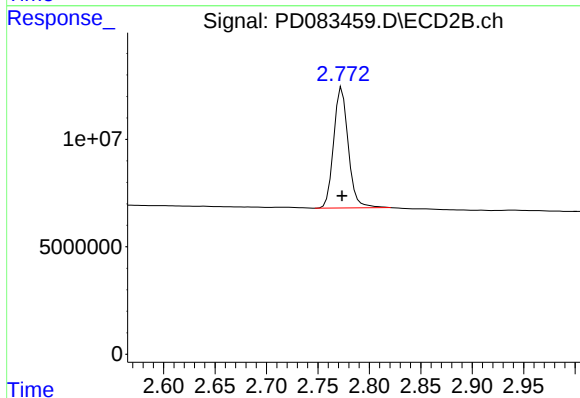


#1 Tetrachloro-m-xylene

R.T.: 2.773 min
Delta R.T.: 0.000 min
Response: 55477639
Conc: 10.16 ng/ml

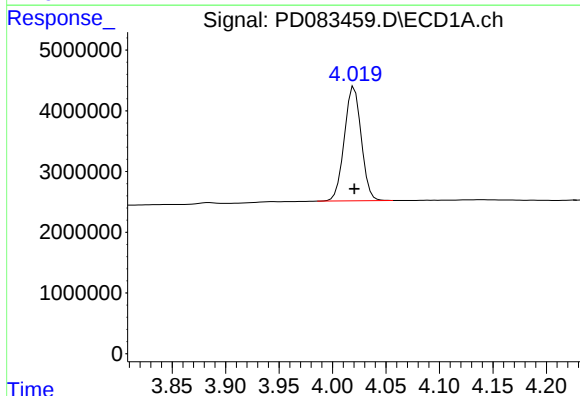


#2 alpha-BHC

R.T.: 4.020 min
Delta R.T.: 0.000 min
Response: 20739675
Conc: 9.59 ng/ml

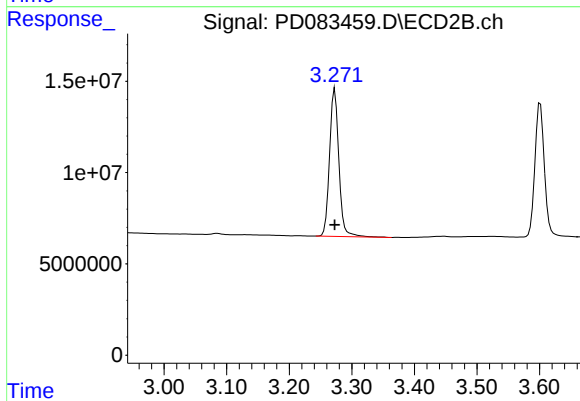


#2 alpha-BHC

R.T.: 3.273 min
Delta R.T.: 0.000 min
Response: 83646820
Conc: 9.77 ng/ml

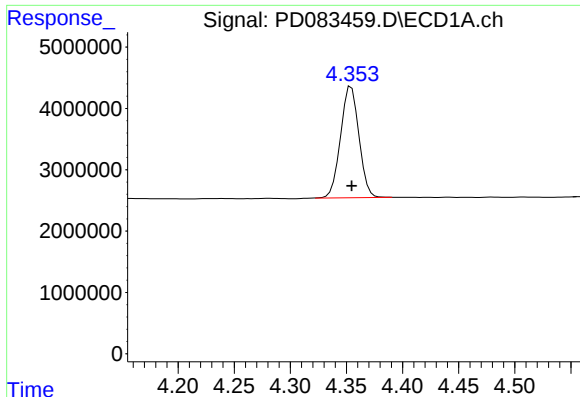


#3 gamma-BHC (Lindane)

R.T.: 4.354 min
Delta R.T.: 0.000 min
Response: 20688082
Conc: 9.67 ng/ml

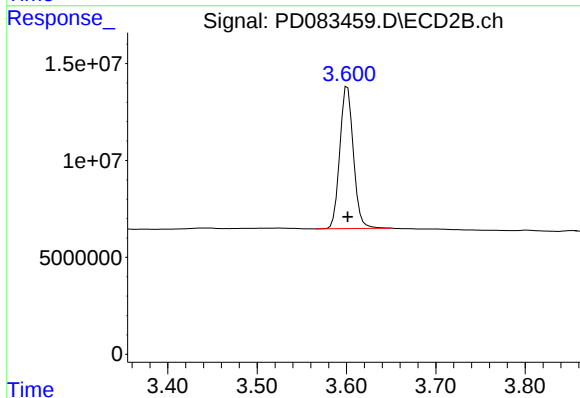


#3 gamma-BHC (Lindane)

R.T.: 3.601 min
Delta R.T.: 0.000 min
Response: 77325065
Conc: 9.88 ng/ml

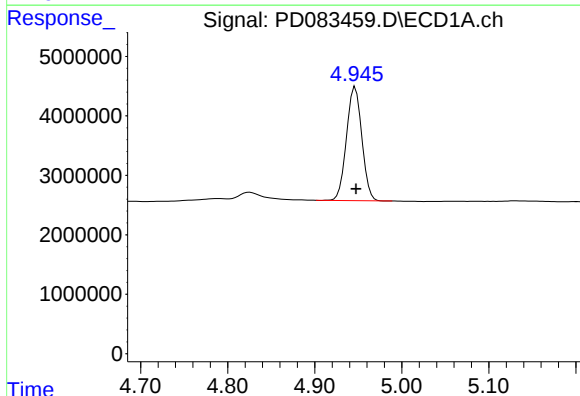


#4 Heptachlor

R.T.: 4.947 min
Delta R.T.: 0.000 min
Response: 23449027
Conc: 9.78 ng/ml

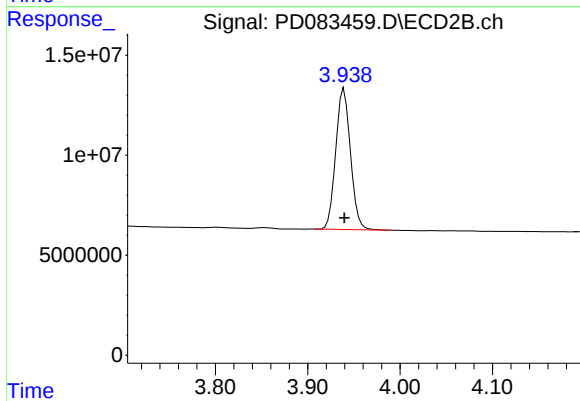


#4 Heptachlor

R.T.: 3.939 min
Delta R.T.: 0.000 min
Response: 78246665
Conc: 9.95 ng/ml

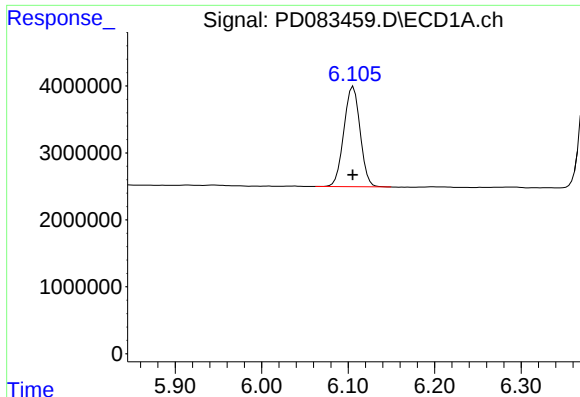


#9 Endosulfan I

R.T.: 6.106 min
Delta R.T.: 0.000 min
Response: 19446919
Conc: 10.00 ng/ml

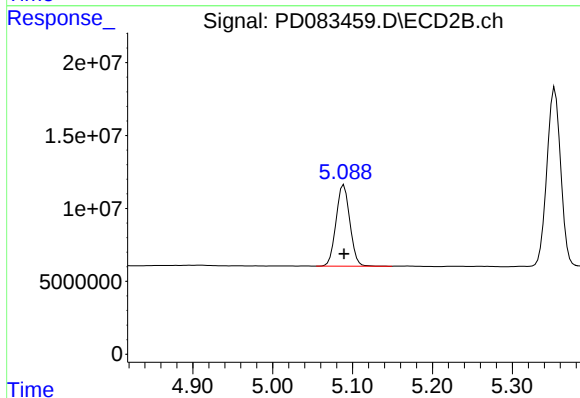


#9 Endosulfan I

R.T.: 5.089 min
Delta R.T.: 0.000 min
Response: 66990524
Conc: 10.07 ng/ml

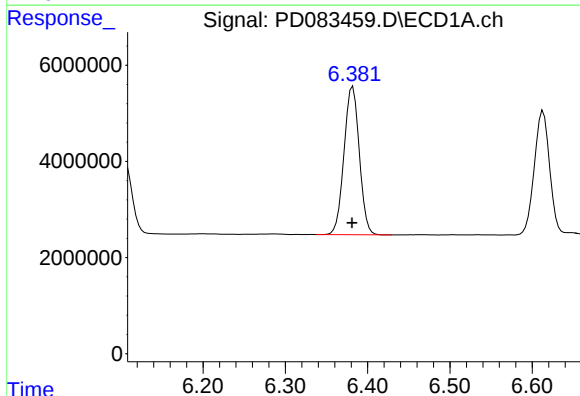


#13 Dieldrin

R.T.: 6.382 min
Delta R.T.: 0.001 min
Response: 39876137
Conc: 19.53 ng/ml

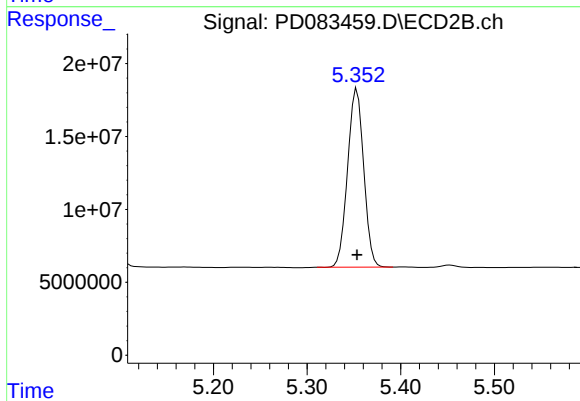


#13 Dieldrin

R.T.: 5.353 min
Delta R.T.: 0.000 min
Response: 146443970
Conc: 19.87 ng/ml

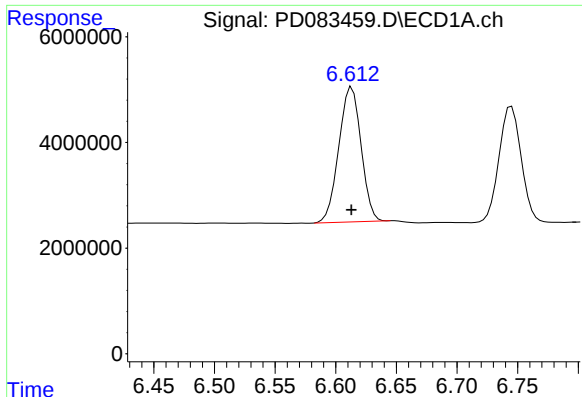


#14 Endrin

R.T.: 6.613 min
Delta R.T.: 0.000 min
Response: 32711279
Conc: 19.46 ng/ml

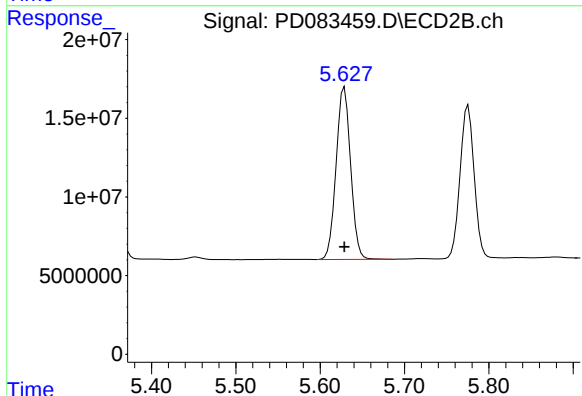


#14 Endrin

R.T.: 5.629 min
Delta R.T.: 0.000 min
Response: 130852563
Conc: 20.04 ng/ml

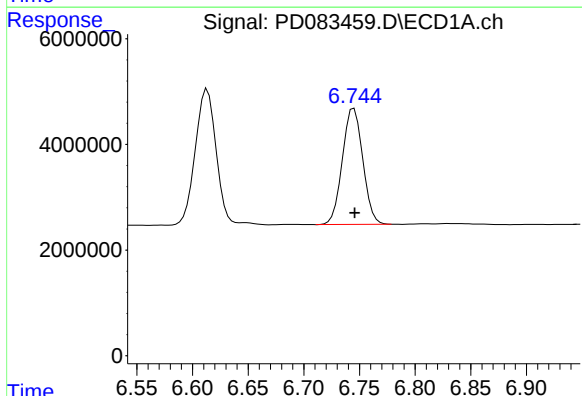


#16 4,4'-DDD

R.T.: 6.745 min
Delta R.T.: 0.000 min
Response: 28061549
Conc: 19.39 ng/ml

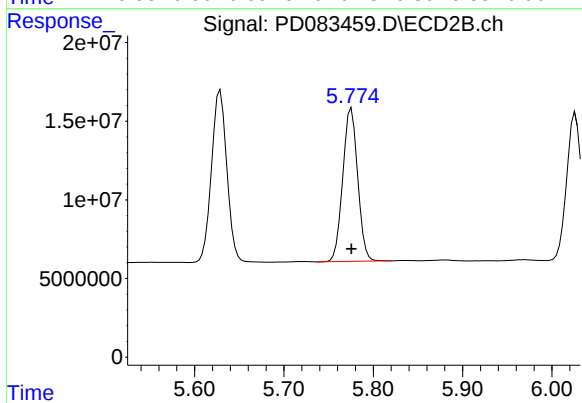


#16 4,4'-DDD

R.T.: 5.775 min
Delta R.T.: 0.000 min
Response: 112926026
Conc: 19.85 ng/ml

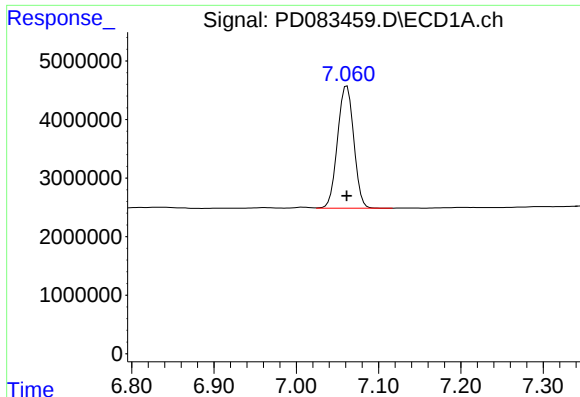


#17 4,4'-DDT

R.T.: 7.061 min
Delta R.T.: 0.000 min
Response: 28677716
Conc: 19.14 ng/ml

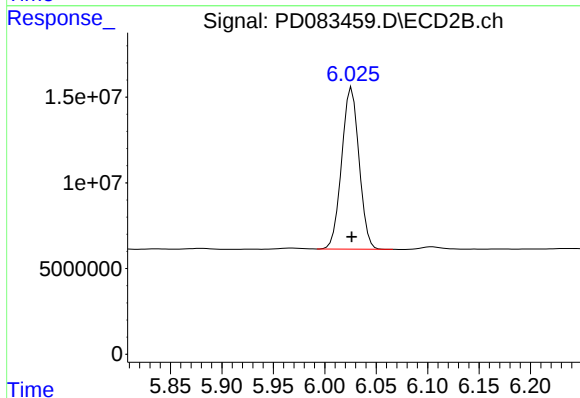


#17 4,4'-DDT

R.T.: 6.026 min
Delta R.T.: 0.000 min
Response: 110769044
Conc: 19.29 ng/ml

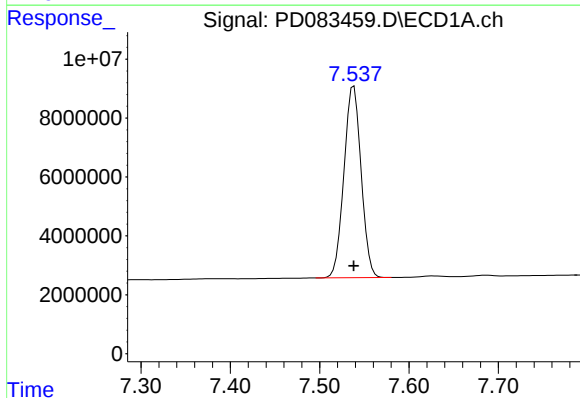


#20 Methoxychlor

R.T.: 7.538 min
Delta R.T.: 0.000 min
Response: 86875768
Conc: 100.38 ng/ml

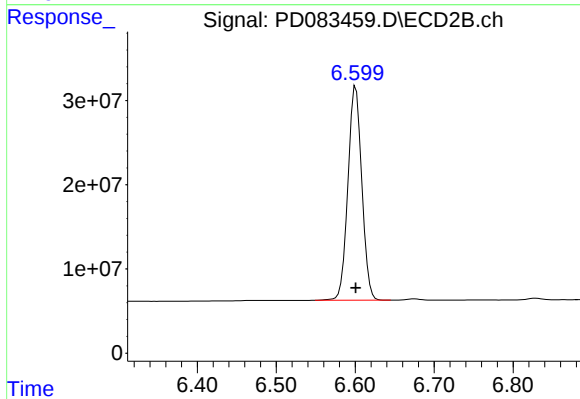


#20 Methoxychlor

R.T.: 6.601 min
Delta R.T.: 0.000 min
Response: 311363891
Conc: 104.90 ng/ml

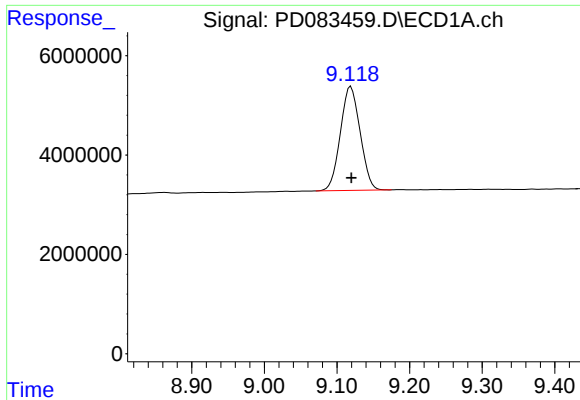

#27 Decachlorobiphenyl

R.T.: 9.119 min
Delta R.T.: 0.000 min
Response: 39601613
Conc: 20.45 ng/ml

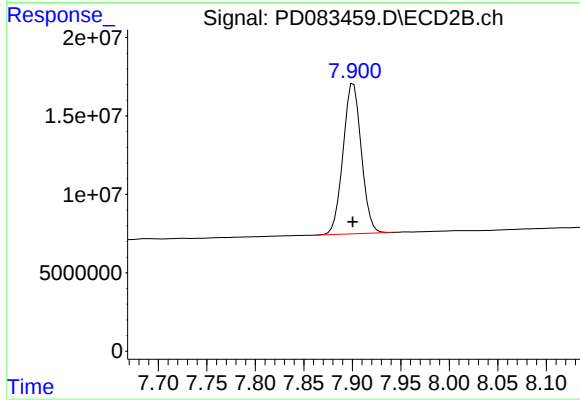

#27 Decachlorobiphenyl

R.T.: 7.901 min
Delta R.T.: 0.000 min
Response: 125342768
Conc: 20.71 ng/ml