

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060724\
 Data File : PD083461.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Jun 2024 18:03
 Operator : AR\AJ
 Sample : INDA301
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 07 03:46:01 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060724CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 07 03:41:46 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.563	2.774	26119112	109.2E6	20.000	20.000
27)	SA Decachlor...	9.120	7.900	77458106	242.1E6	40.000	40.000
Target Compounds							
2)	A alpha-BHC	4.021	3.273	43250586	171.2E6	20.000	20.000
3)	MA gamma-BHC...	4.355	3.601	42785161	156.6E6	20.000	20.000
4)	MA Heptachlor	4.947	3.940	47976211	157.3E6	20.000	20.000
9)	A Endosulfan I	6.105	5.089	38907348	133.1E6	20.000	20.000
13)	MA Dieldrin	6.381	5.353	81668783	294.8E6	40.000	40.000
14)	MA Endrin	6.613	5.629	67230025	261.2E6	40.000	40.000
16)	A 4,4'-DDD	6.746	5.776	57875180	227.6E6	40.000	40.000
17)	MA 4,4'-DDT	7.061	6.026	59943469	229.7E6	40.000	40.000
20)	A Methoxychlor	7.538	6.601	173.1E6	593.6E6	200.000	200.000


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060724\
Data File : PD083461.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Jun 2024 18:03
Operator : AR\AJ
Sample : INDA301
Misc :
ALS Vial : 13 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 07 03:46:01 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060724CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jun 07 03:41:46 2024
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

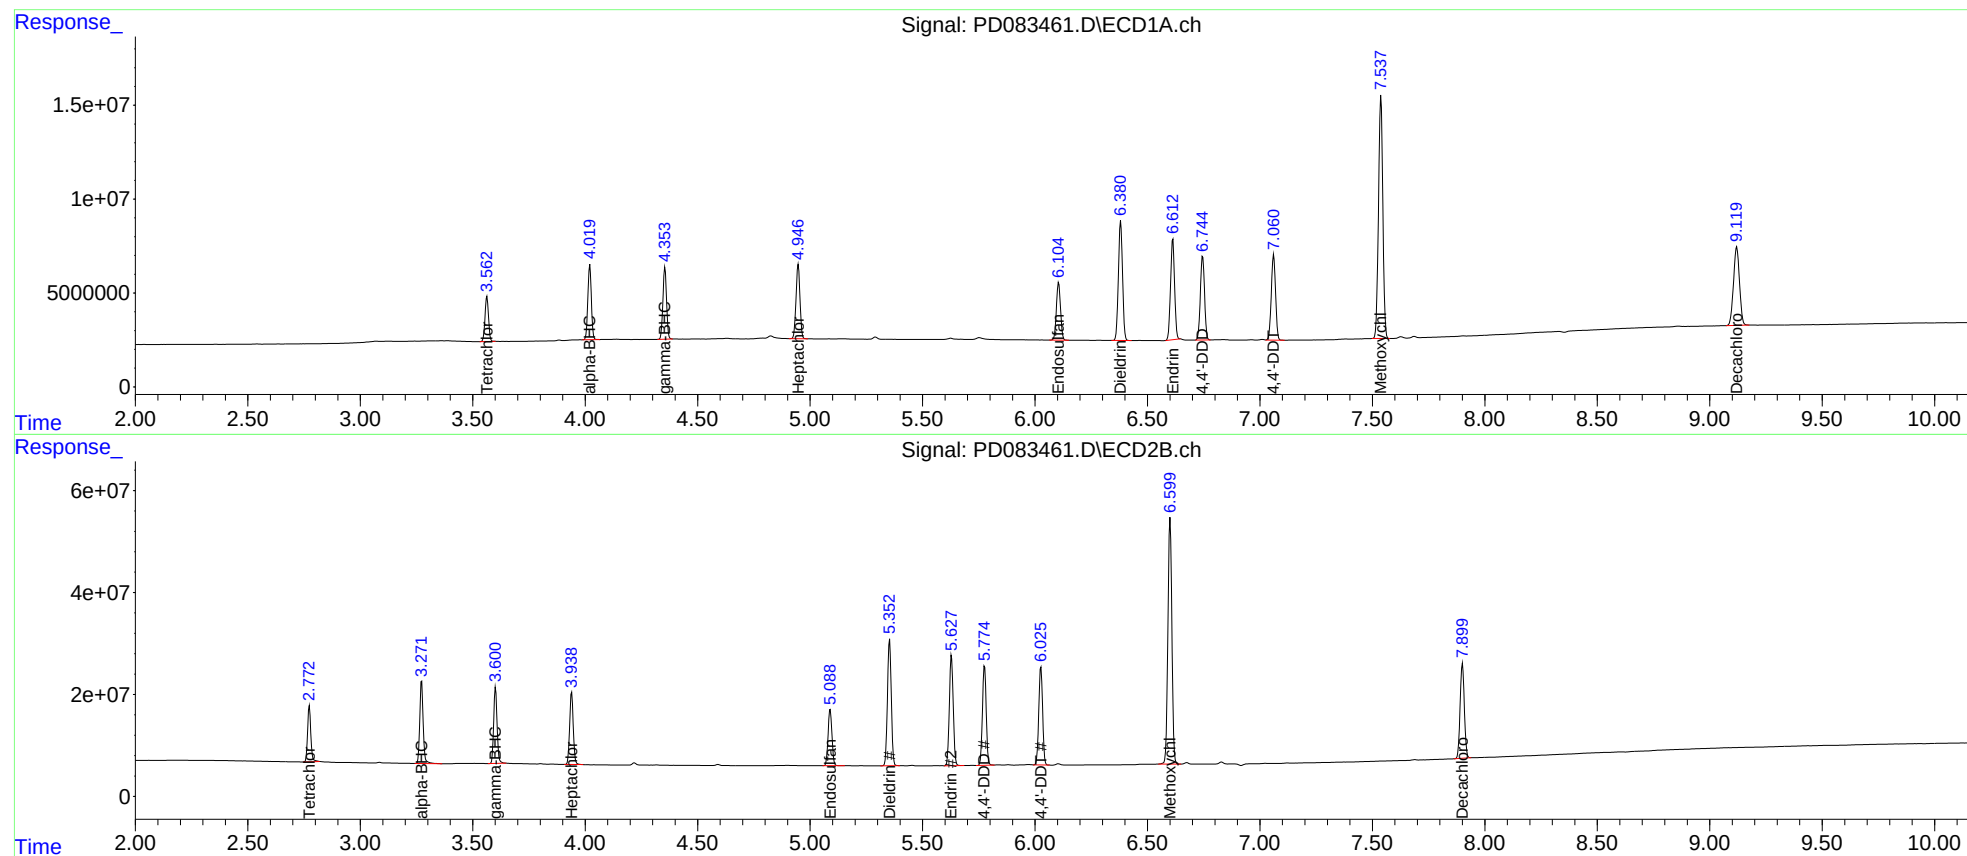

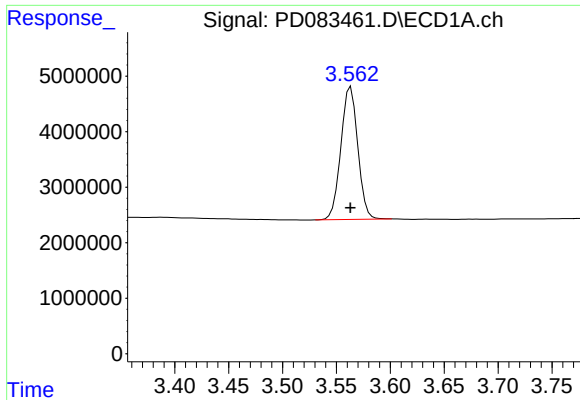


#1 Tetrachloro-m-xylene

R.T.: 3.563 min
Delta R.T.: 0.000 min
Response: 26119112
Conc: 20.00 ng/ml

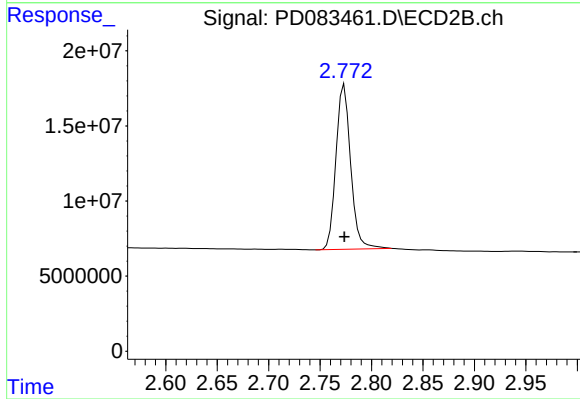


#1 Tetrachloro-m-xylene

R.T.: 2.774 min
Delta R.T.: 0.000 min
Response: 109208177
Conc: 20.00 ng/ml

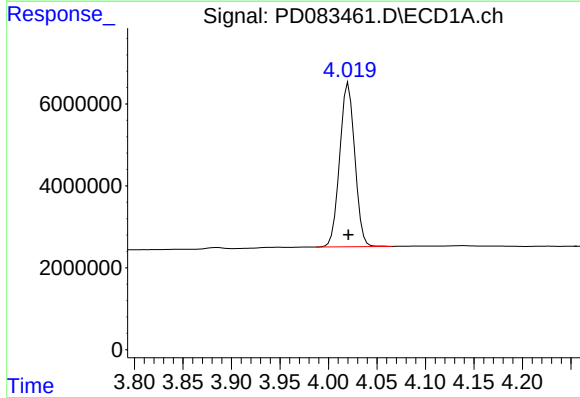


#2 alpha-BHC

R.T.: 4.021 min
Delta R.T.: 0.000 min
Response: 43250586
Conc: 20.00 ng/ml

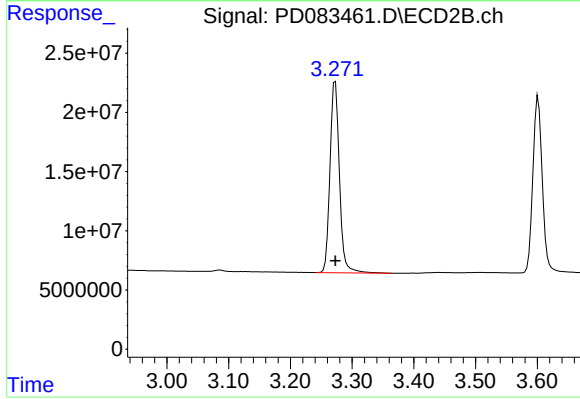


#2 alpha-BHC

R.T.: 3.273 min
Delta R.T.: 0.000 min
Response: 171227090
Conc: 20.00 ng/ml

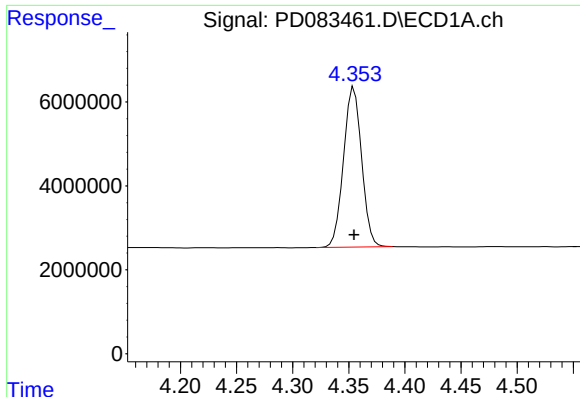


#3 gamma-BHC (Lindane)

R.T.: 4.355 min
Delta R.T.: 0.000 min
Response: 42785161
Conc: 20.00 ng/ml

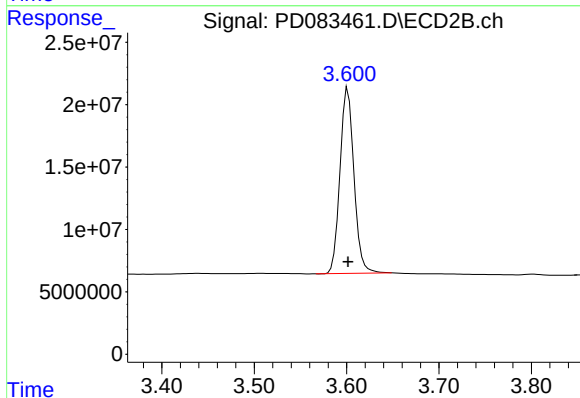


#3 gamma-BHC (Lindane)

R.T.: 3.601 min
Delta R.T.: 0.000 min
Response: 156559256
Conc: 20.00 ng/ml

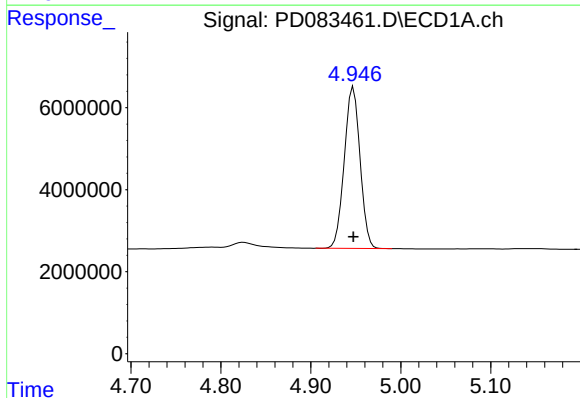


#4 Heptachlor

R.T.: 4.947 min
Delta R.T.: 0.000 min
Response: 47976211
Conc: 20.00 ng/ml

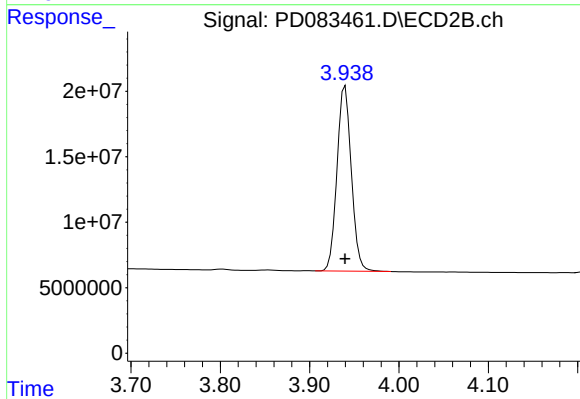


#4 Heptachlor

R.T.: 3.940 min
Delta R.T.: 0.000 min
Response: 157346892
Conc: 20.00 ng/ml

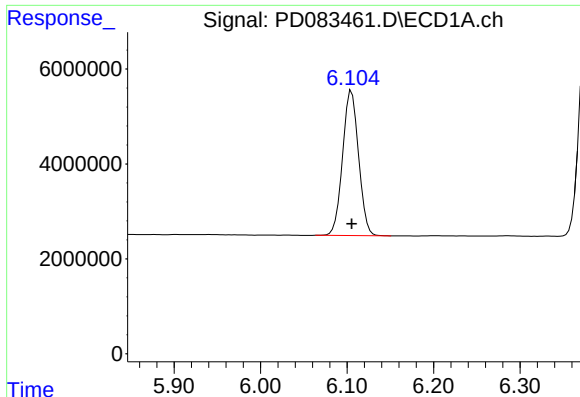


#9 Endosulfan I

R.T.: 6.105 min
Delta R.T.: 0.000 min
Response: 38907348
Conc: 20.00 ng/ml

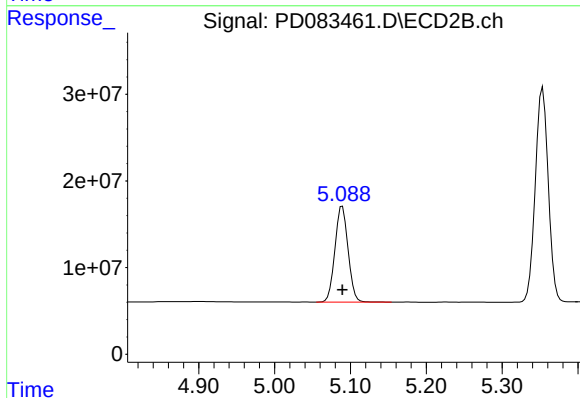


#9 Endosulfan I

R.T.: 5.089 min
Delta R.T.: 0.000 min
Response: 133096935
Conc: 20.00 ng/ml

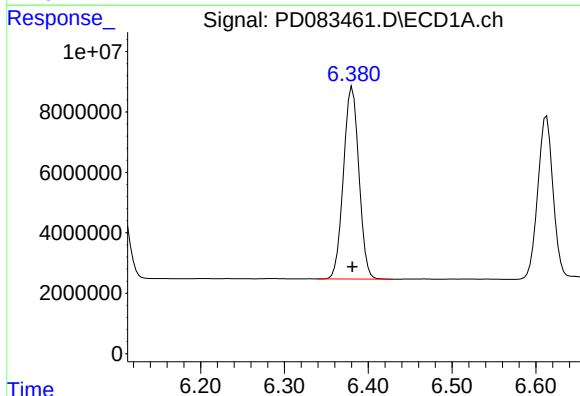


#13 Dieldrin

R.T.: 6.381 min
Delta R.T.: 0.000 min
Response: 81668783
Conc: 40.00 ng/ml

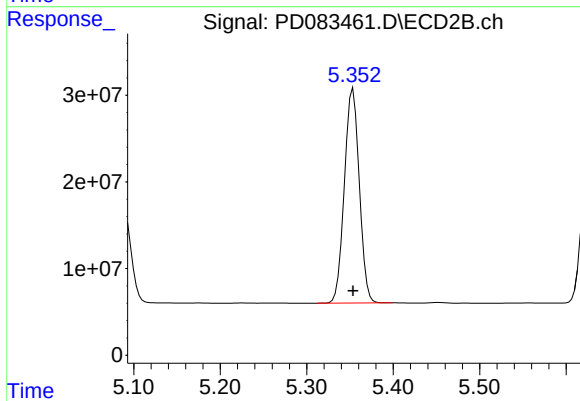


#13 Dieldrin

R.T.: 5.353 min
Delta R.T.: 0.000 min
Response: 294751178
Conc: 40.00 ng/ml

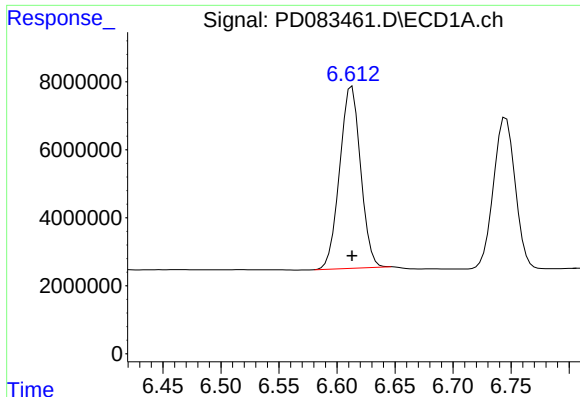


#14 Endrin

R.T.: 6.613 min
Delta R.T.: 0.000 min
Response: 67230025
Conc: 40.00 ng/ml

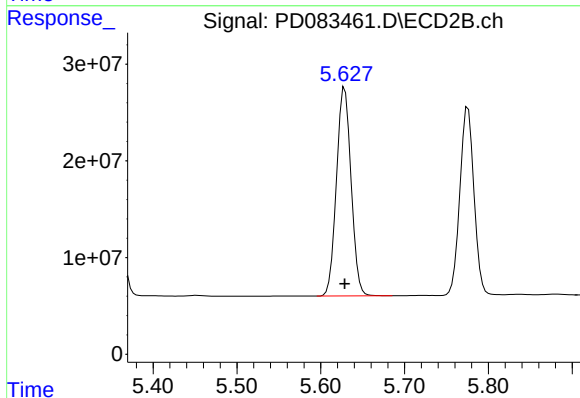


#14 Endrin

R.T.: 5.629 min
Delta R.T.: 0.000 min
Response: 261208809
Conc: 40.00 ng/ml

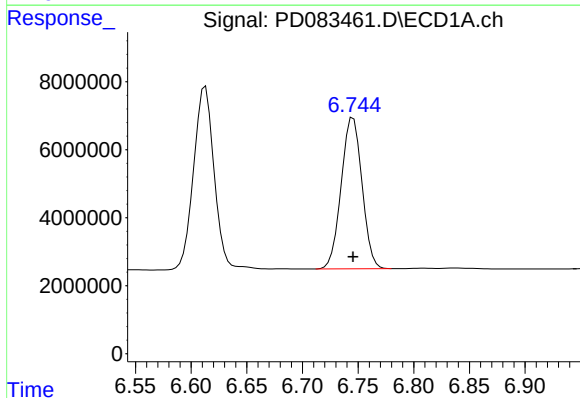


#16 4,4'-DDD

R.T.: 6.746 min
Delta R.T.: 0.000 min
Response: 57875180
Conc: 40.00 ng/ml

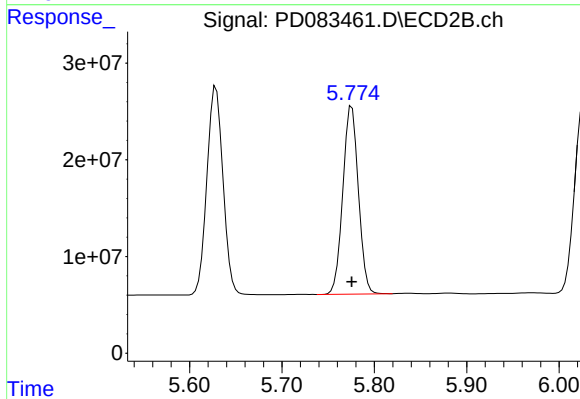


#16 4,4'-DDD

R.T.: 5.776 min
Delta R.T.: 0.000 min
Response: 227566910
Conc: 40.00 ng/ml

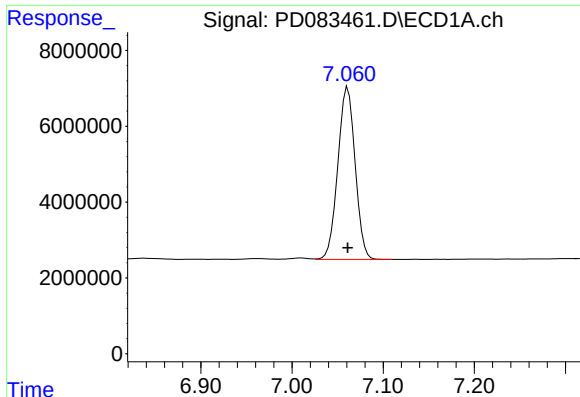


#17 4,4'-DDT

R.T.: 7.061 min
Delta R.T.: 0.000 min
Response: 59943469
Conc: 40.00 ng/ml

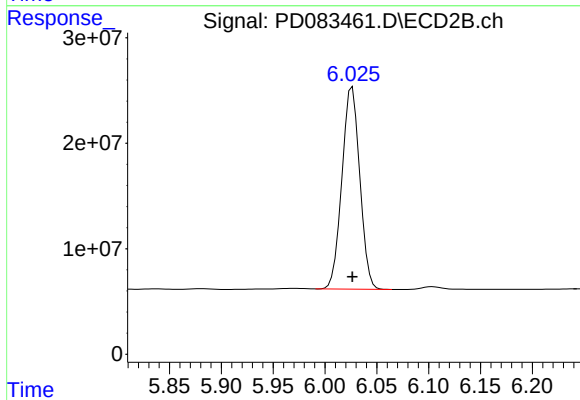


#17 4,4'-DDT

R.T.: 6.026 min
Delta R.T.: 0.000 min
Response: 229707143
Conc: 40.00 ng/ml

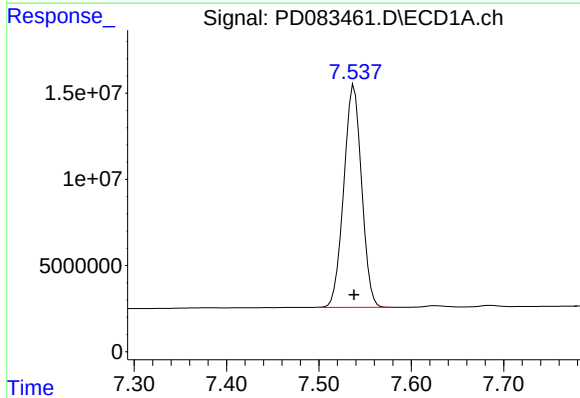


#20 Methoxychlor

R.T.: 7.538 min
Delta R.T.: 0.000 min
Response: 173102143
Conc: 200.00 ng/ml

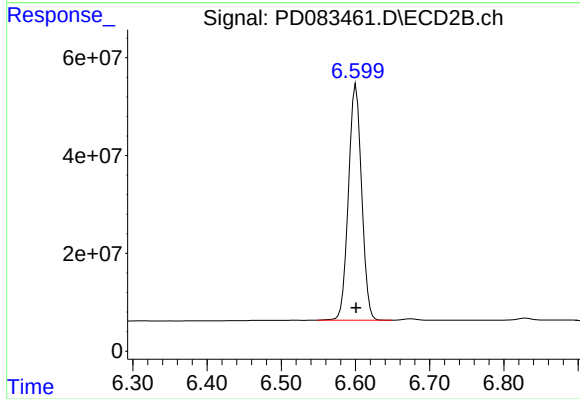


#20 Methoxychlor

R.T.: 6.601 min
Delta R.T.: 0.000 min
Response: 593635385
Conc: 200.00 ng/ml

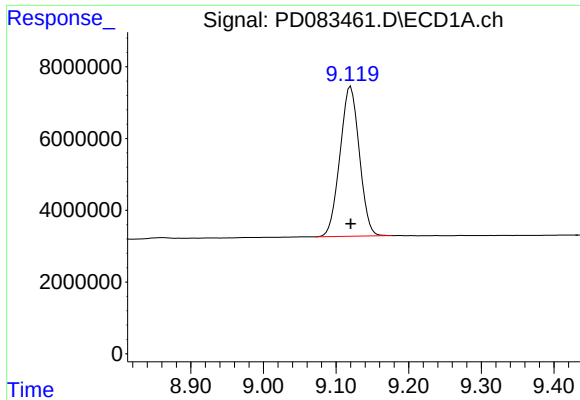

#27 Decachlorobiphenyl

R.T.: 9.120 min
Delta R.T.: 0.000 min
Response: 77458106
Conc: 40.00 ng/ml

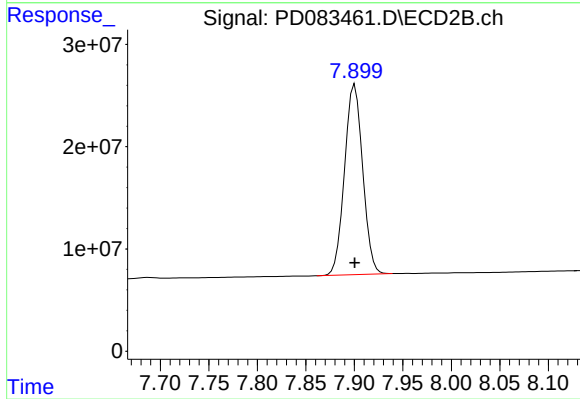

#27 Decachlorobiphenyl

R.T.: 7.900 min
Delta R.T.: 0.000 min
Response: 242066006
Conc: 40.00 ng/ml