

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060724\
 Data File : PD083463.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Jun 2024 18:32
 Operator : AR\AJ
 Sample : INDA401
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 07 03:46:16 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060724CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 07 03:41:46 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.563	2.773	52125807	214.0E6	39.914	39.190
27)	SA Decachlor...	9.121	7.901	152.0E6	472.1E6	78.503	78.017
Target Compounds							
2)	A alpha-BHC	4.021	3.273	92488860	345.3E6	42.769	40.327
3)	MA gamma-BHC...	4.355	3.601	89905950	315.1E6	42.027	40.253
4)	MA Heptachlor	4.947	3.940	99061044	313.6E6	41.296	39.858
9)	A Endosulfan I	6.106	5.090	78507717	261.4E6	40.356	39.283
13)	MA Dieldrin	6.383	5.354	169.3E6	583.6E6	82.900	79.198
14)	MA Endrin	6.613	5.629	137.8E6	516.8E6	81.963	79.140
16)	A 4,4'-DDD	6.746	5.775	120.1E6	454.7E6	83.003	79.928
17)	MA 4,4'-DDT	7.062	6.027	124.5E6	468.8E6	83.076	81.634
20)	A Methoxychlor	7.538	6.601	341.5E6	1104.7E6	394.619	372.191


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060724\
Data File : PD083463.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Jun 2024 18:32
Operator : AR\AJ
Sample : INDA401
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 07 03:46:16 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060724CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jun 07 03:41:46 2024
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

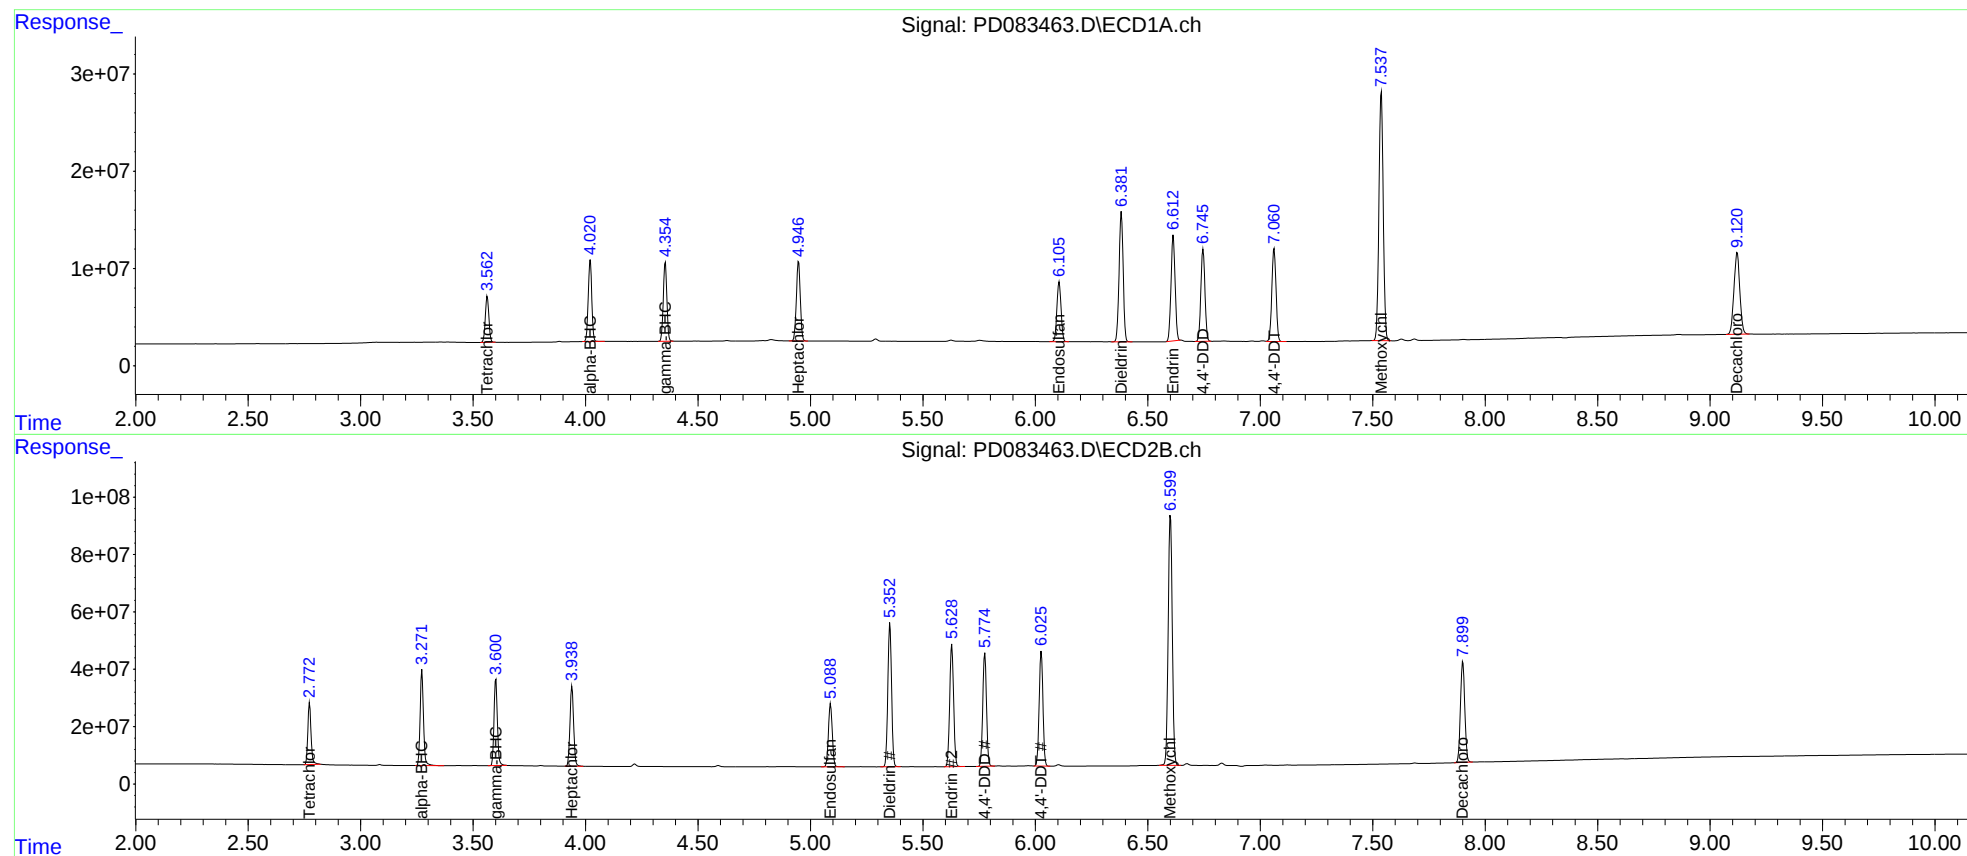

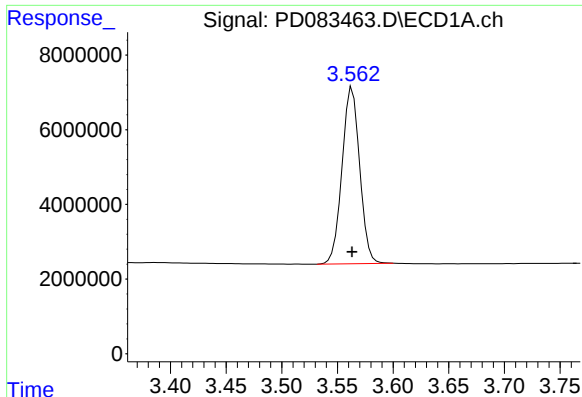


#1 Tetrachloro-m-xylene

R.T.: 3.563 min
Delta R.T.: 0.000 min
Response: 52125807
Conc: 39.91 ng/ml

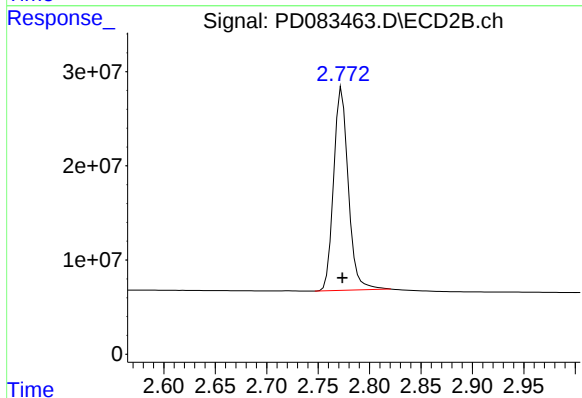


#1 Tetrachloro-m-xylene

R.T.: 2.773 min
Delta R.T.: 0.000 min
Response: 213994723
Conc: 39.19 ng/ml

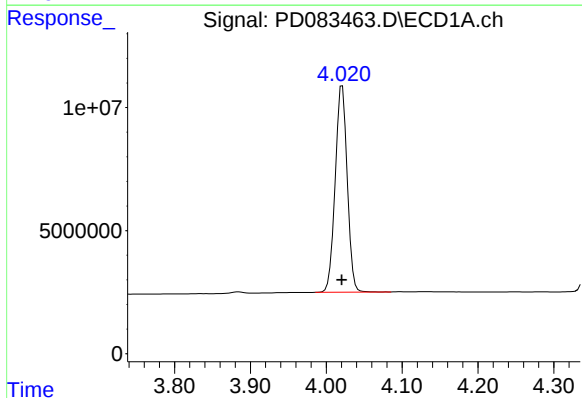


#2 alpha-BHC

R.T.: 4.021 min
Delta R.T.: 0.000 min
Response: 92488860
Conc: 42.77 ng/ml

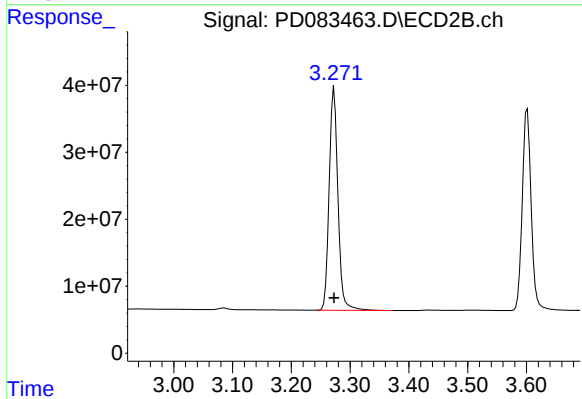


#2 alpha-BHC

R.T.: 3.273 min
Delta R.T.: 0.000 min
Response: 345253915
Conc: 40.33 ng/ml

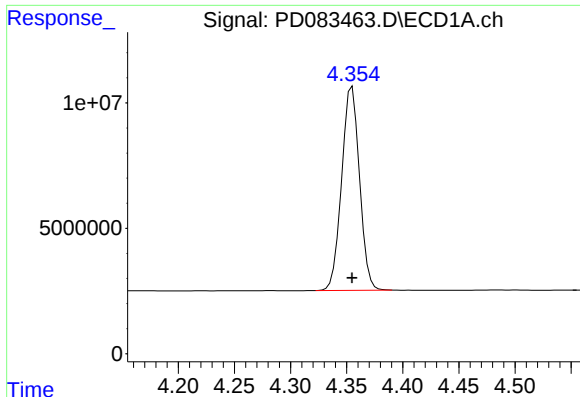


#3 gamma-BHC (Lindane)

R.T.: 4.355 min
Delta R.T.: 0.000 min
Response: 89905950
Conc: 42.03 ng/ml

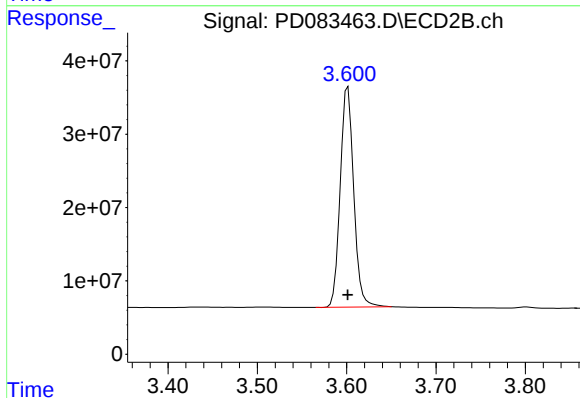


#3 gamma-BHC (Lindane)

R.T.: 3.601 min
Delta R.T.: 0.000 min
Response: 315099520
Conc: 40.25 ng/ml

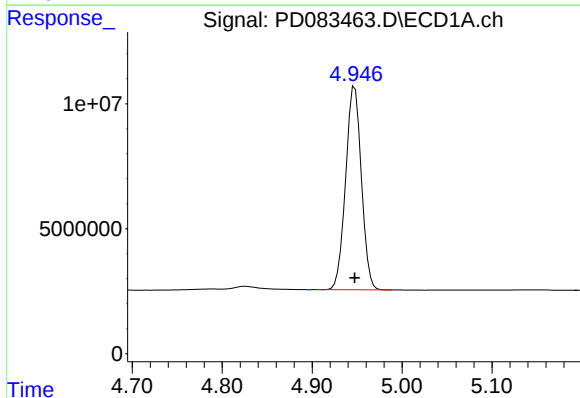


#4 Heptachlor

R.T.: 4.947 min
Delta R.T.: 0.000 min
Response: 99061044
Conc: 41.30 ng/ml

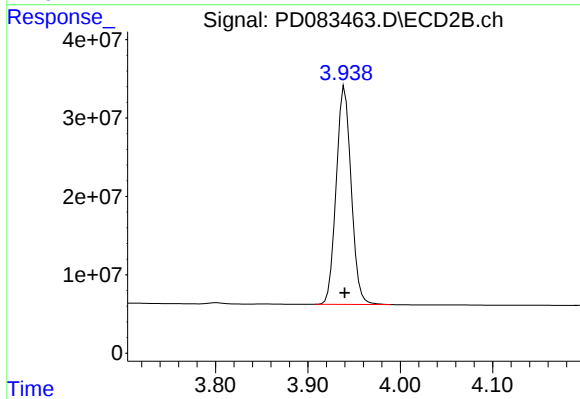


#4 Heptachlor

R.T.: 3.940 min
Delta R.T.: 0.000 min
Response: 313575143
Conc: 39.86 ng/ml

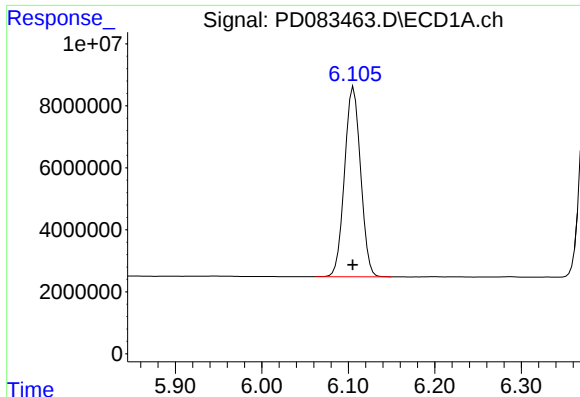


#9 Endosulfan I

R.T.: 6.106 min
Delta R.T.: 0.000 min
Response: 78507717
Conc: 40.36 ng/ml

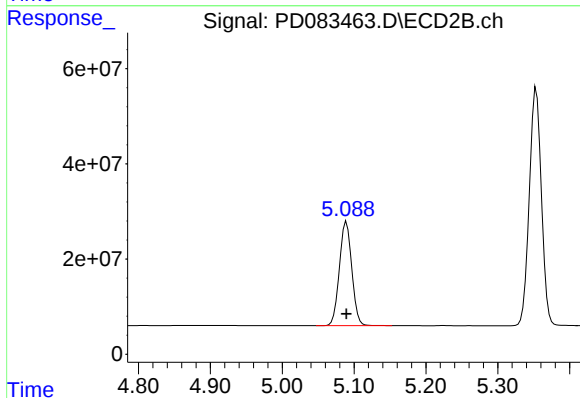


#9 Endosulfan I

R.T.: 5.090 min
Delta R.T.: 0.000 min
Response: 261423683
Conc: 39.28 ng/ml

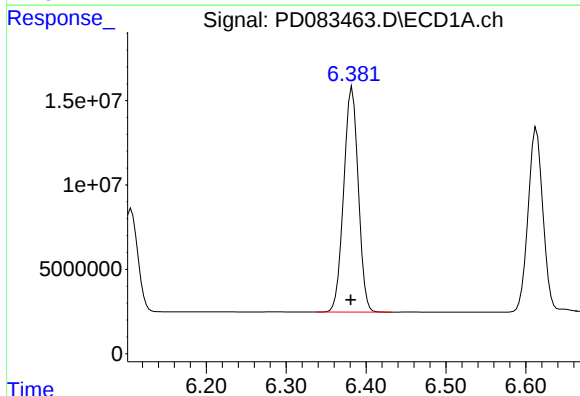


#13 Dieldrin

R.T.: 6.383 min
Delta R.T.: 0.002 min
Response: 169259431
Conc: 82.90 ng/ml

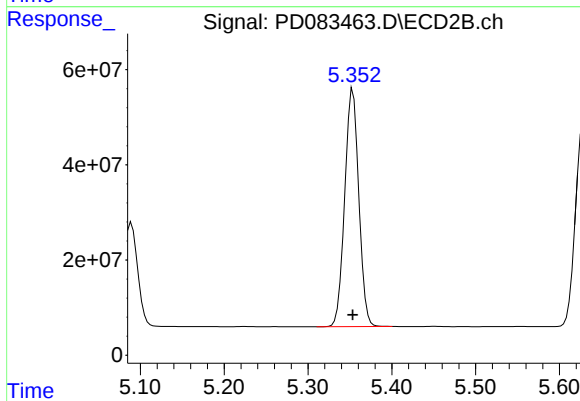


#13 Dieldrin

R.T.: 5.354 min
Delta R.T.: 0.000 min
Response: 583590792
Conc: 79.20 ng/ml

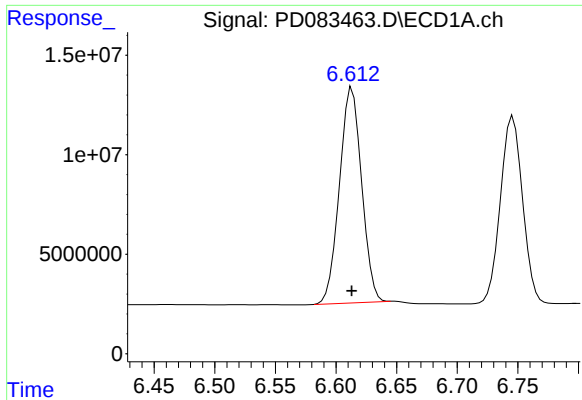


#14 Endrin

R.T.: 6.613 min
Delta R.T.: 0.000 min
Response: 137759232
Conc: 81.96 ng/ml

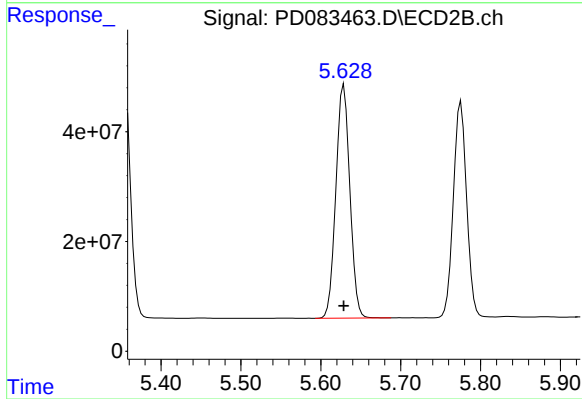


#14 Endrin

R.T.: 5.629 min
Delta R.T.: 0.000 min
Response: 516801447
Conc: 79.14 ng/ml

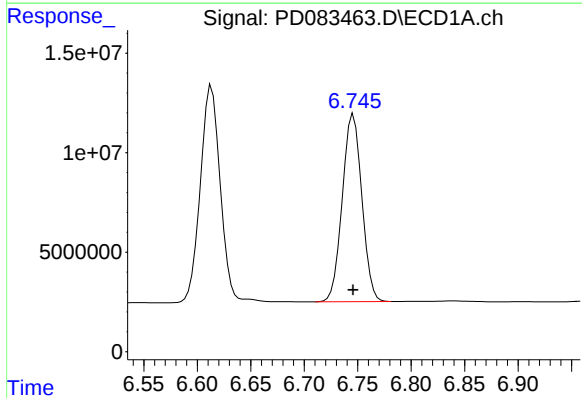


#16 4,4'-DDD

R.T.: 6.746 min
Delta R.T.: 0.000 min
Response: 120095497
Conc: 83.00 ng/ml

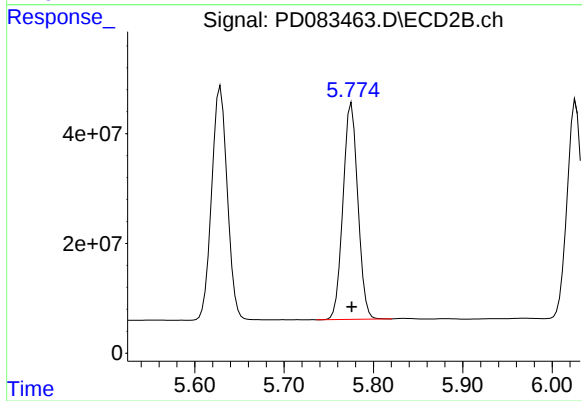


#16 4,4'-DDD

R.T.: 5.775 min
Delta R.T.: 0.000 min
Response: 454721684
Conc: 79.93 ng/ml

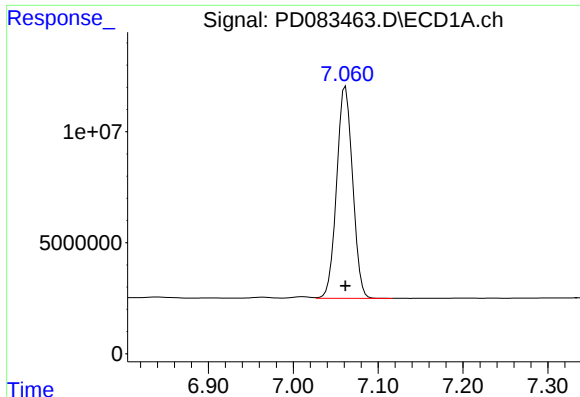


#17 4,4'-DDT

R.T.: 7.062 min
Delta R.T.: 0.000 min
Response: 124496067
Conc: 83.08 ng/ml

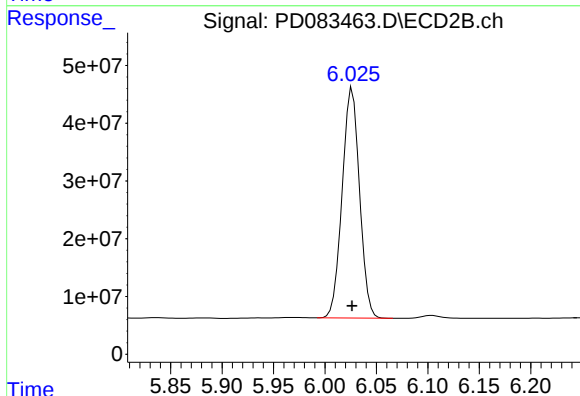


#17 4,4'-DDT

R.T.: 6.027 min
Delta R.T.: 0.000 min
Response: 468795885
Conc: 81.63 ng/ml

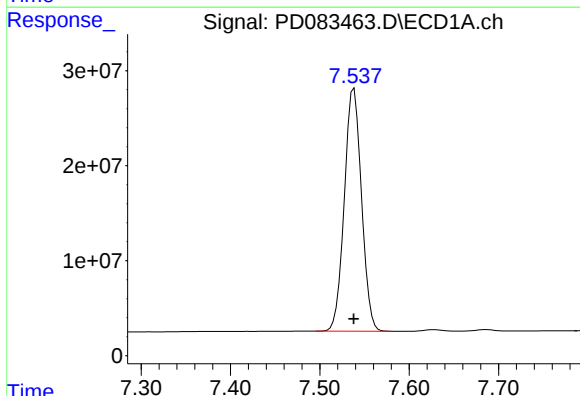


#20 Methoxychlor

R.T.: 7.538 min
Delta R.T.: 0.000 min
Response: 341546738
Conc: 394.62 ng/ml

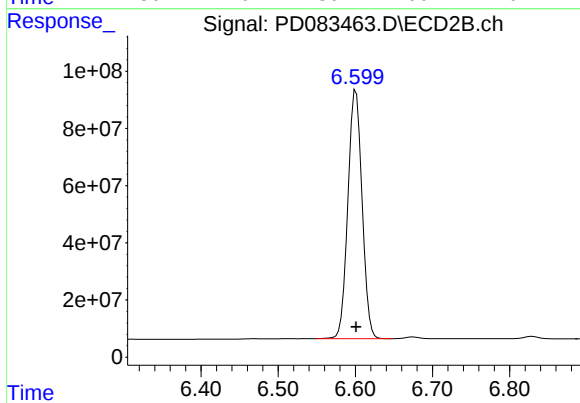

#20 Methoxychlor

R.T.: 6.601 min
Delta R.T.: 0.000 min
Response: 1104727487
Conc: 372.19 ng/ml

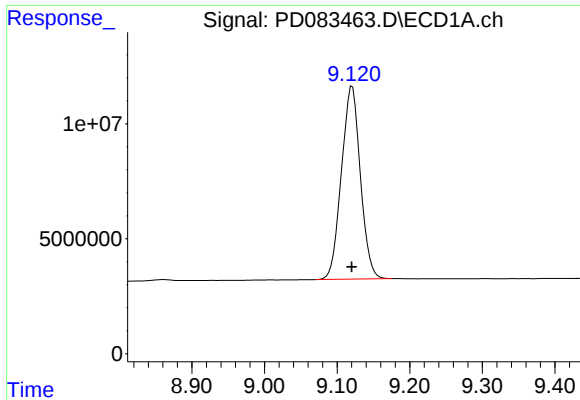


#27 Decachlorobiphenyl

R.T.: 9.121 min

Delta R.T.: 0.000 min

Response: 152017631

Conc: 78.50 ng/ml

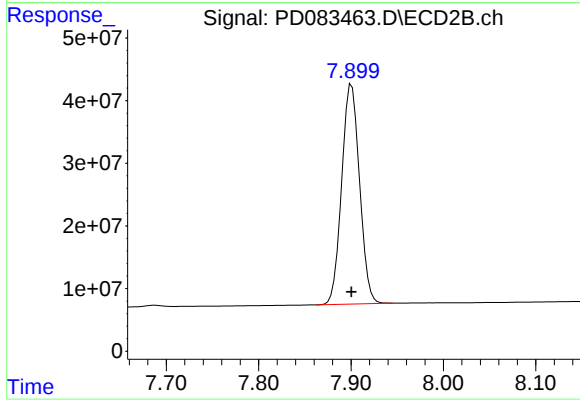

#27 Decachlorobiphenyl

R.T.: 7.901 min

Delta R.T.: 0.000 min

Response: 472130007

Conc: 78.02 ng/ml