

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060724\
 Data File : PD083465.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Jun 2024 18:58
 Operator : AR\AJ
 Sample : INDA501
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 07 03:46:33 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060724CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 07 03:41:46 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.564	2.774	105.3E6	423.4E6	80.613	77.543
27)	SA Decachlor...	9.121	7.902	301.3E6	920.5E6	155.601	152.113
Target Compounds							
2)	A alpha-BHC	4.022	3.274	201.4E6	705.1E6	93.117	82.356
3)	MA gamma-BHC...	4.355	3.602	193.5E6	638.6E6	90.439	81.579
4)	MA Heptachlor	4.948	3.940	208.8E6	628.7E6	87.059	79.918
9)	A Endosulfan I	6.107	5.090	162.5E6	520.0E6	83.529	78.145
13)	MA Dieldrin	6.383	5.354	356.5E6	1156.3E6	174.615	156.917
14)	MA Endrin	6.613	5.630	289.2E6	1014.3E6	172.043	155.319
16)	A 4,4'-DDD	6.747	5.776	256.1E6	907.5E6	176.999	159.515
17)	MA 4,4'-DDT	7.062	6.027	266.4E6	955.1E6	177.785	166.314
20)	A Methoxychlor	7.539	6.602	686.3E6	2021.2E6	792.956	680.966


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060724\
Data File : PD083465.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Jun 2024 18:58
Operator : AR\AJ
Sample : INDA501
Misc :
ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 07 03:46:33 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060724CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jun 07 03:41:46 2024
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

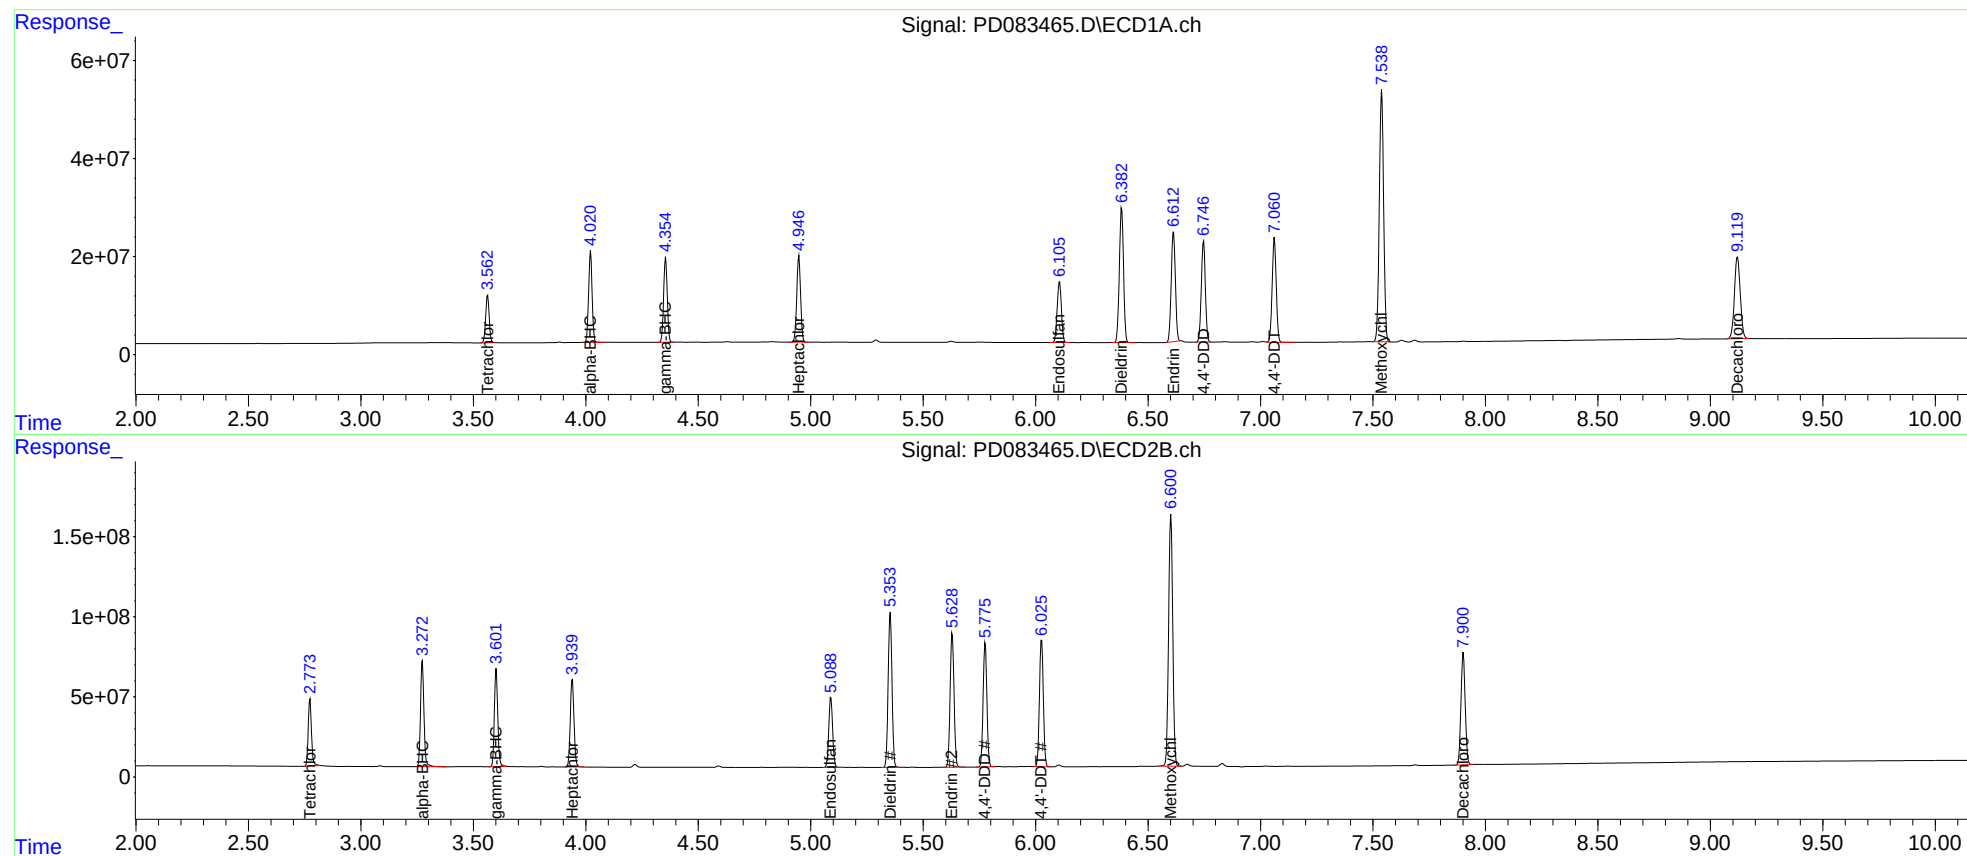

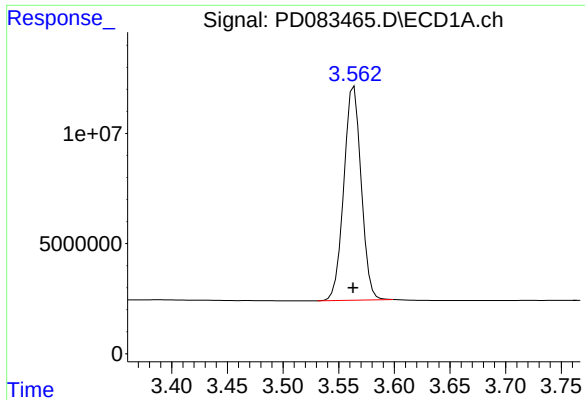


#1 Tetrachloro-m-xylene

R.T.: 3.564 min
Delta R.T.: 0.000 min
Response: 105277018
Conc: 80.61 ng/ml

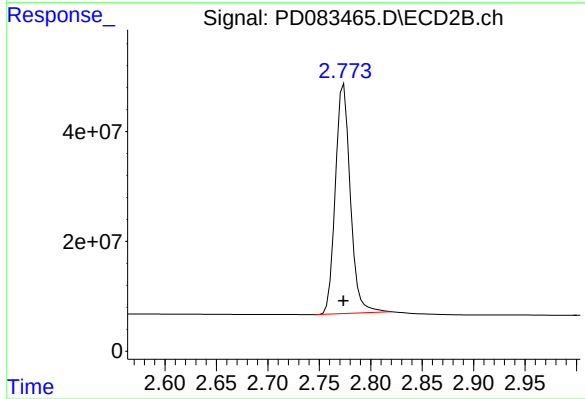


#1 Tetrachloro-m-xylene

R.T.: 2.774 min
Delta R.T.: 0.000 min
Response: 423417853
Conc: 77.54 ng/ml

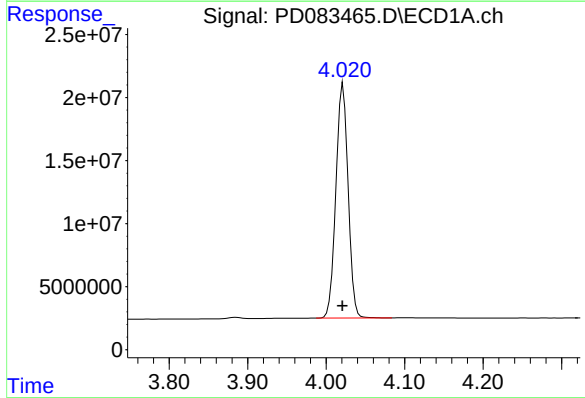


#2 alpha-BHC

R.T.: 4.022 min
Delta R.T.: 0.000 min
Response: 201369083
Conc: 93.12 ng/ml

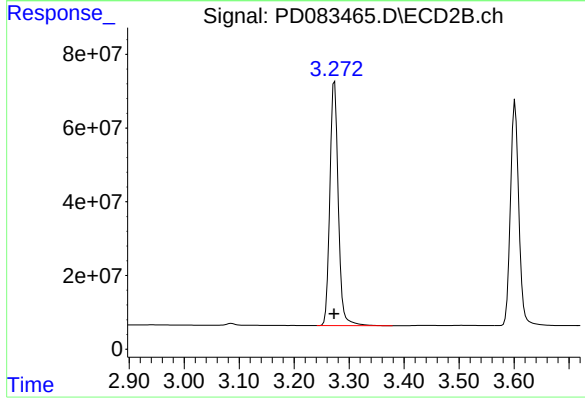


#2 alpha-BHC

R.T.: 3.274 min
Delta R.T.: 0.000 min
Response: 705080653
Conc: 82.36 ng/ml

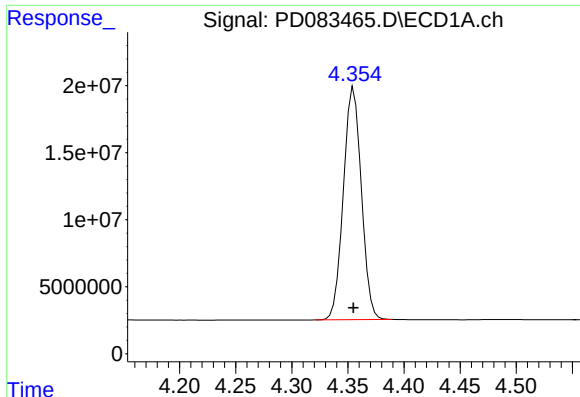


#3 gamma-BHC (Lindane)

R.T.: 4.355 min
Delta R.T.: 0.000 min
Response: 193472526
Conc: 90.44 ng/ml

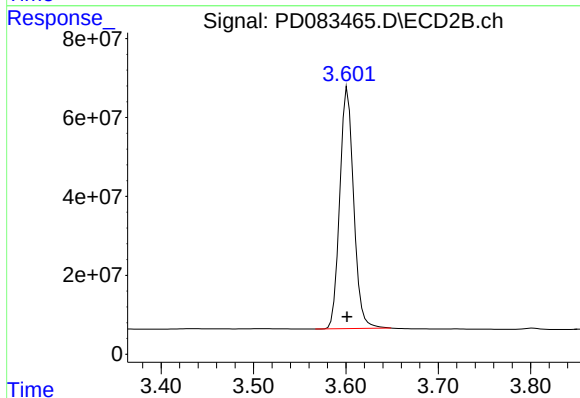


#3 gamma-BHC (Lindane)

R.T.: 3.602 min
Delta R.T.: 0.000 min
Response: 638595805
Conc: 81.58 ng/ml

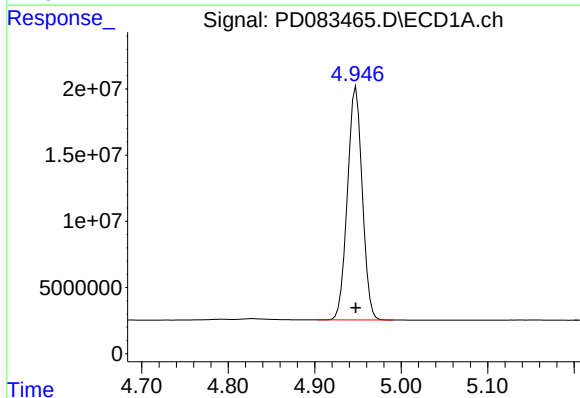


#4 Heptachlor

R.T.: 4.948 min
Delta R.T.: 0.000 min
Response: 208837907
Conc: 87.06 ng/ml

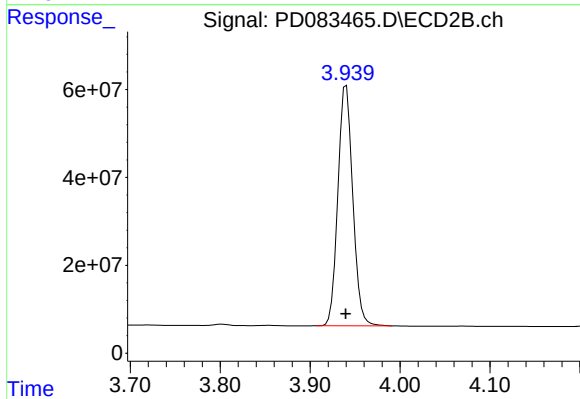


#4 Heptachlor

R.T.: 3.940 min
Delta R.T.: 0.000 min
Response: 628741654
Conc: 79.92 ng/ml

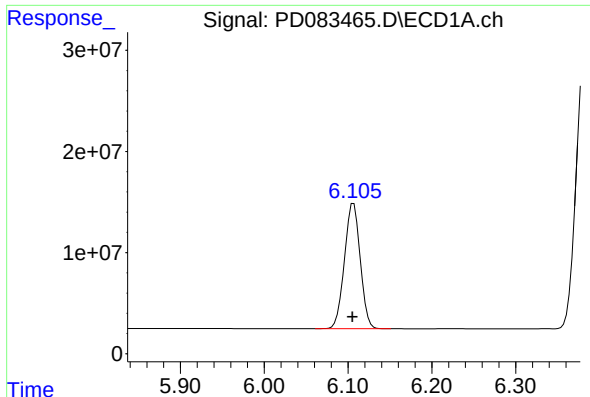


#9 Endosulfan I

R.T.: 6.107 min
Delta R.T.: 0.001 min
Response: 162494955
Conc: 83.53 ng/ml

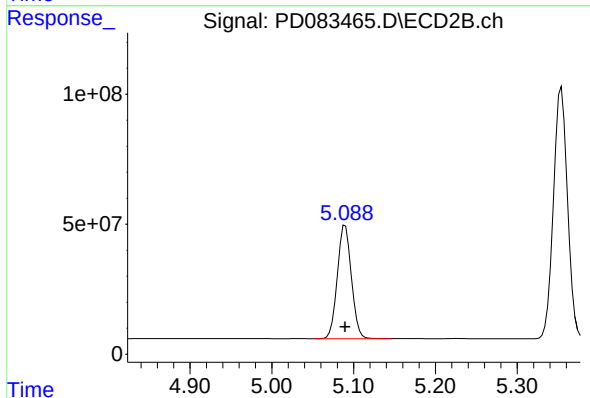


#9 Endosulfan I

R.T.: 5.090 min
Delta R.T.: 0.000 min
Response: 520044516
Conc: 78.15 ng/ml

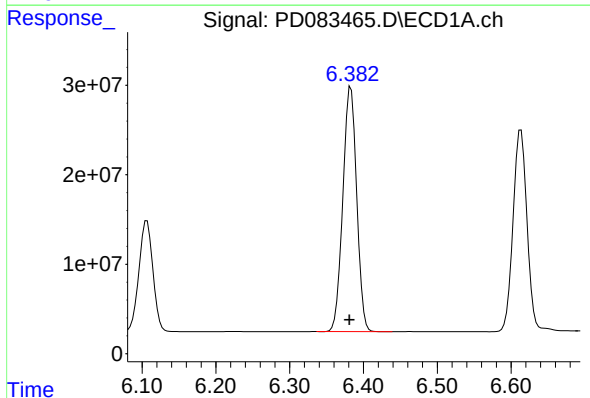


#13 Dieldrin

R.T.: 6.383 min
Delta R.T.: 0.002 min
Response: 356515054
Conc: 174.62 ng/ml

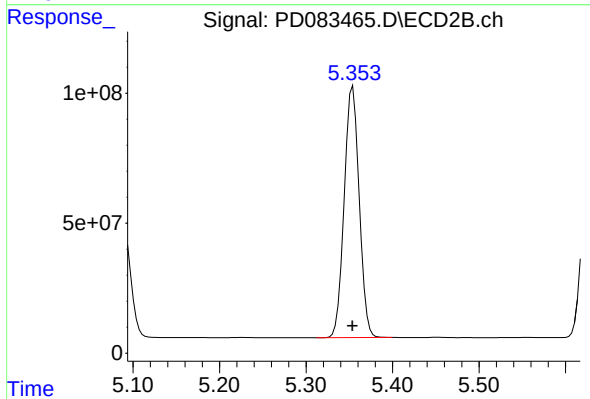


#13 Dieldrin

R.T.: 5.354 min
Delta R.T.: 0.000 min
Response: 1156283386
Conc: 156.92 ng/ml

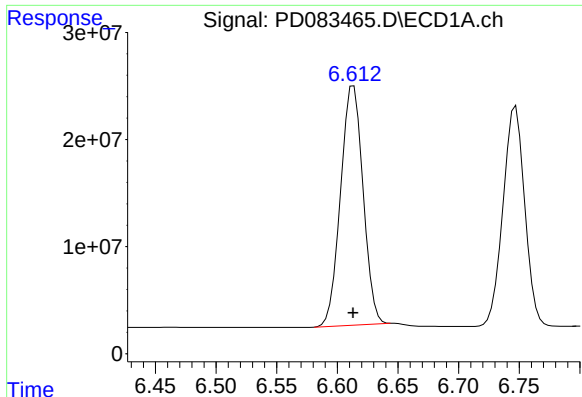


#14 Endrin

R.T.: 6.613 min
Delta R.T.: 0.000 min
Response: 289160775
Conc: 172.04 ng/ml

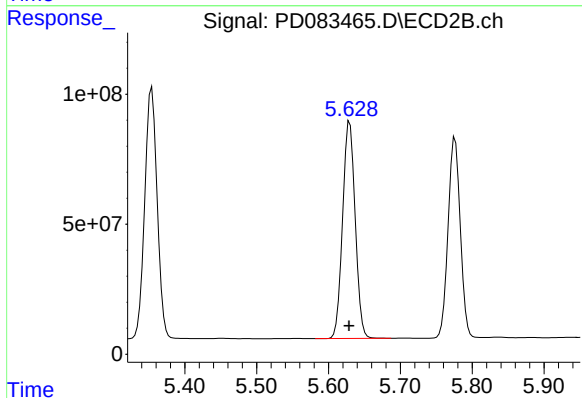


#14 Endrin

R.T.: 5.630 min
Delta R.T.: 0.000 min
Response: 1014266022
Conc: 155.32 ng/ml

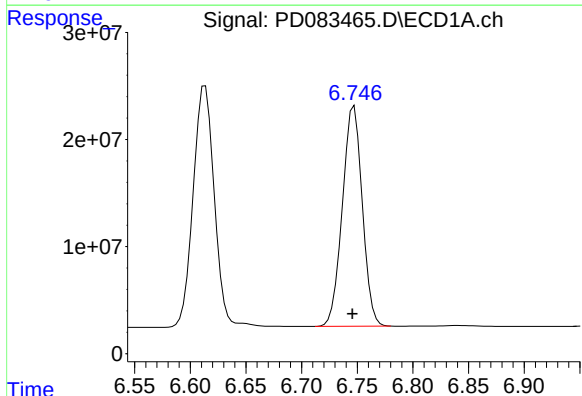


#16 4,4'-DDD

R.T.: 6.747 min
Delta R.T.: 0.002 min
Response: 256096196
Conc: 177.00 ng/ml

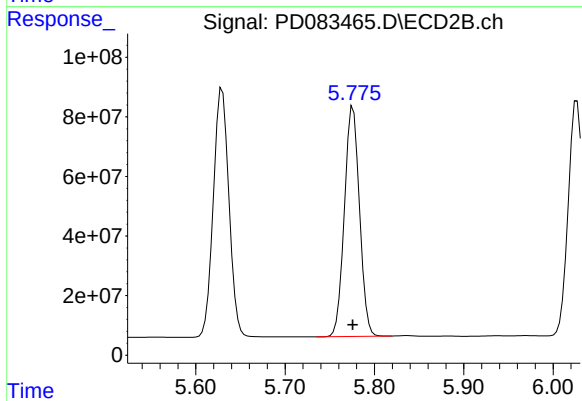


#16 4,4'-DDD

R.T.: 5.776 min
Delta R.T.: 0.000 min
Response: 907508715
Conc: 159.52 ng/ml

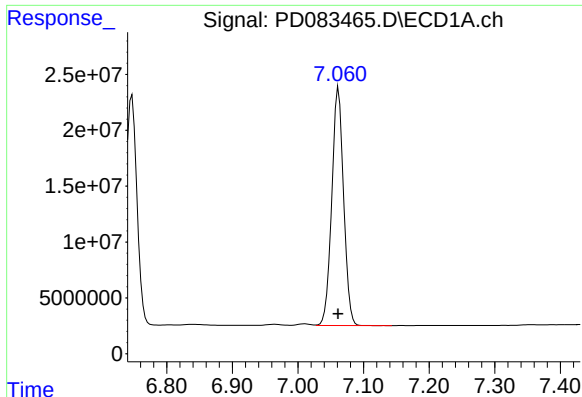


#17 4,4'-DDT

R.T.: 7.062 min
Delta R.T.: 0.000 min
Response: 266426954
Conc: 177.79 ng/ml

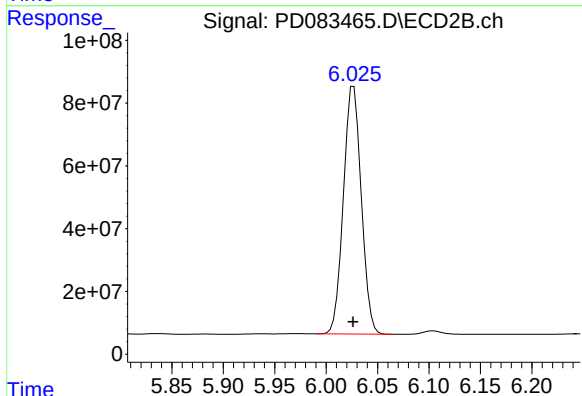


#17 4,4'-DDT

R.T.: 6.027 min
Delta R.T.: 0.000 min
Response: 955089709
Conc: 166.31 ng/ml

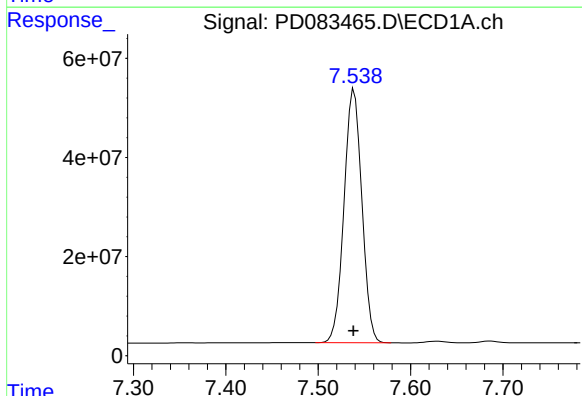


#20 Methoxychlor

R.T.: 7.539 min
Delta R.T.: 0.000 min
Response: 686311813
Conc: 792.96 ng/ml

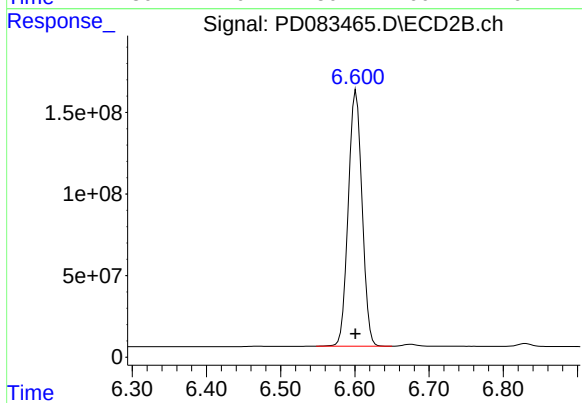


#20 Methoxychlor

R.T.: 6.602 min
Delta R.T.: 0.000 min
Response: 2021226541
Conc: 680.97 ng/ml

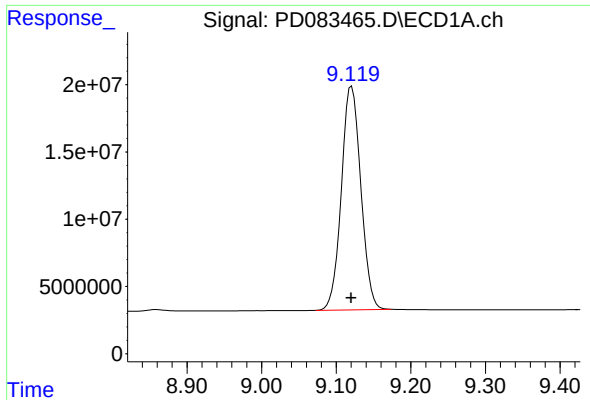

#27 Decachlorobiphenyl

R.T.: 9.121 min
Delta R.T.: 0.000 min
Response: 301314483
Conc: 155.60 ng/ml

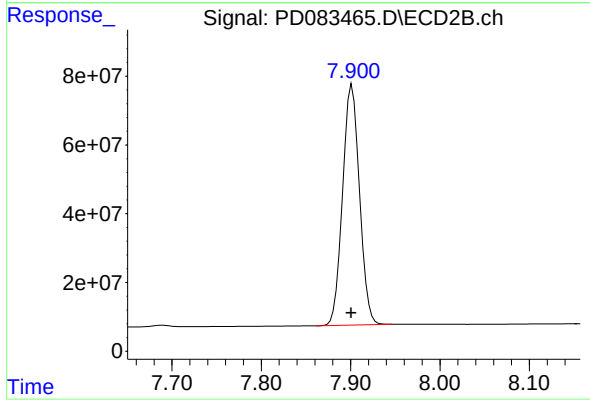

#27 Decachlorobiphenyl

R.T.: 7.902 min
Delta R.T.: 0.001 min
Response: 920535104
Conc: 152.11 ng/ml