

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060724\
 Data File : PD083466.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Jun 2024 19:12
 Operator : AR\AJ
 Sample : INDB501
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 07 02:45:35 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060724CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 07 02:43:54 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.563	2.773	107.1E6	431.8E6	80.501	72.171
27)	SA Decachlor...	9.120	7.901	304.6E6	924.1E6	154.137	139.219
Target Compounds							
5)	MB Aldrin	5.291	4.219	202.2E6	610.4E6	85.272	75.878
6)	B beta-BHC	4.552	3.898	80712668	269.3E6	78.102	71.706
7)	B delta-BHC	4.801	4.128	219.3E6	678.9E6	86.308	75.679
8)	B Heptachlo...	5.718	4.721	177.1E6	559.7E6	85.101	73.461
10)	B trans-Chl...	5.975	4.970	170.3E6	563.7E6	82.908	74.387
11)	B cis-Chlor...	6.055	5.034	171.1E6	565.3E6	81.506	73.663
12)	B 4,4'-DDE	6.227	5.223	347.1E6	1097.8E6	166.759	144.545
15)	B Endosulfa...	6.832	5.923	291.2E6	953.1E6	161.615	140.209
18)	B Endrin al...	6.964	6.103	215.6E6	715.3E6	161.564	139.415
19)	B Endosulfa...	7.200	6.325	274.4E6	922.5E6	159.850	138.156
21)	B Endrin ke...	7.686	6.830	304.8E6	1006.9E6	162.347	138.581


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060724\
Data File : PD083466.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Jun 2024 19:12
Operator : AR\AJ
Sample : INDB501
Misc :
ALS Vial : 18 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 07 02:45:35 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060724CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jun 07 02:43:54 2024
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

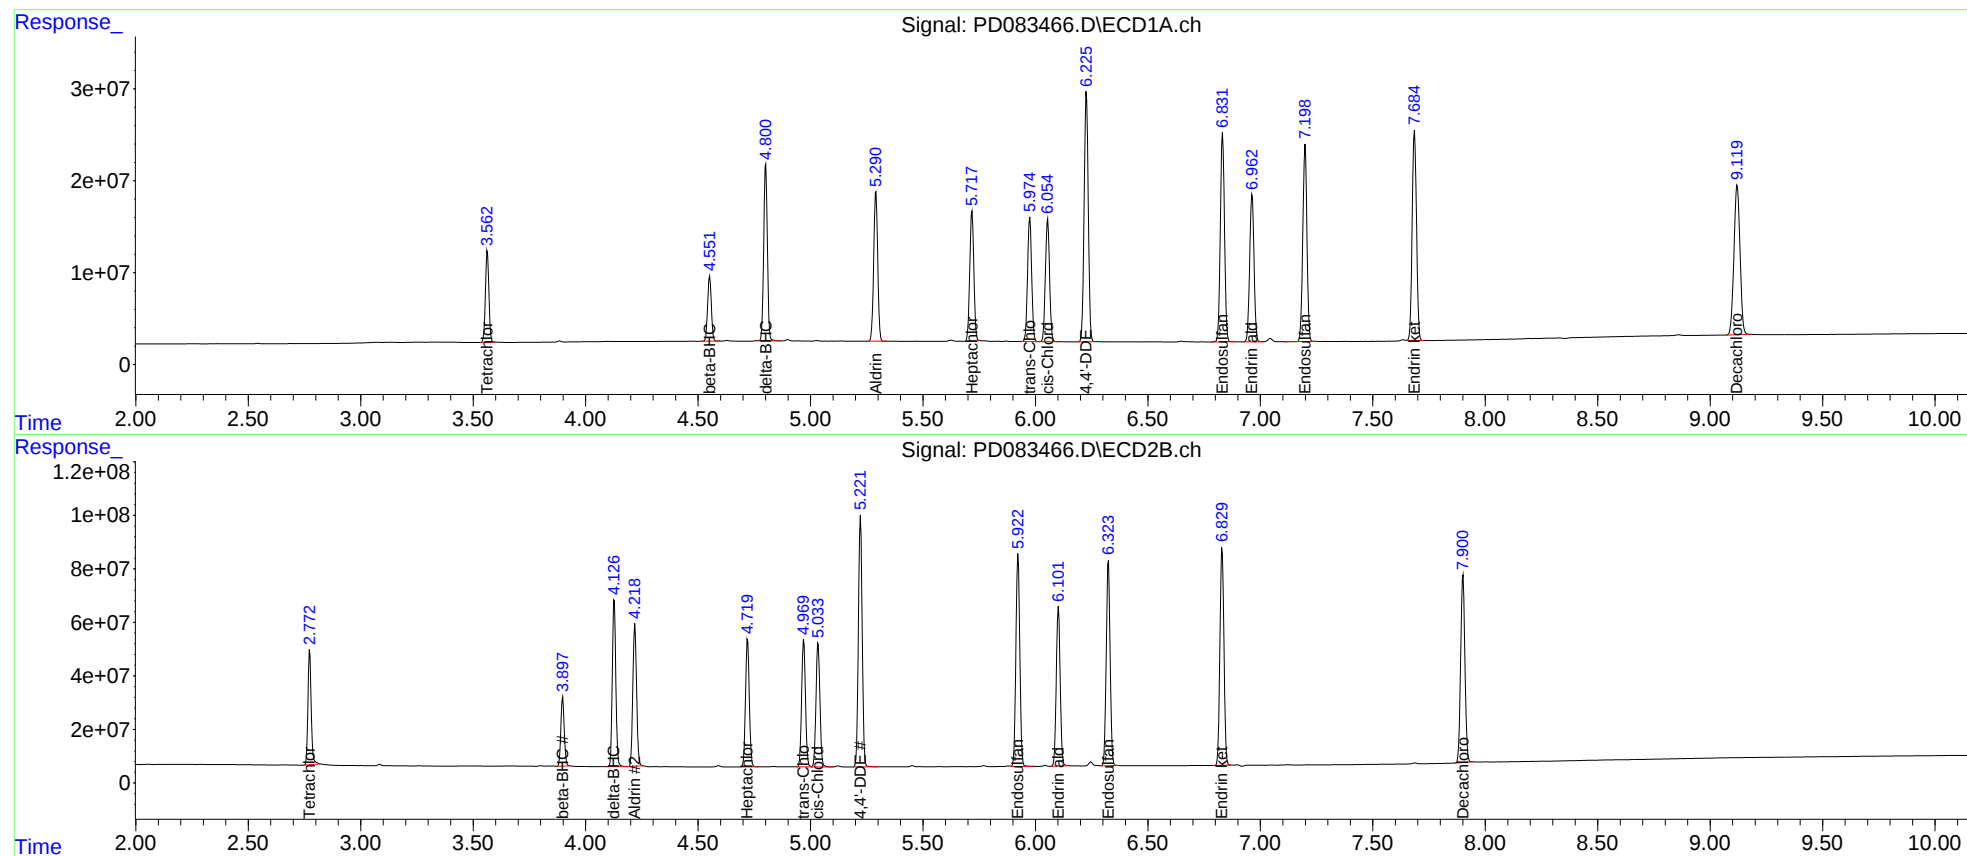

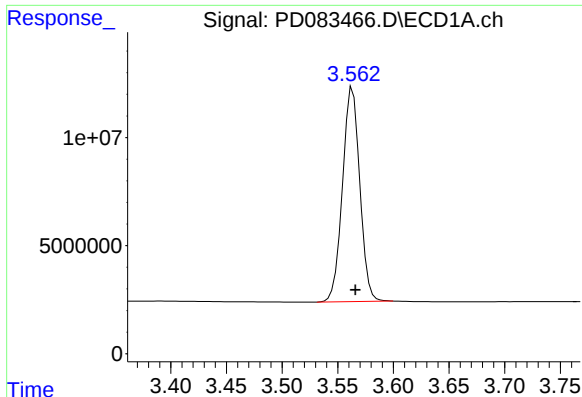


#1 Tetrachloro-m-xylene

R.T.: 3.563 min
Delta R.T.: -0.003 min
Response: 107116806
Conc: 80.50 ng/ml

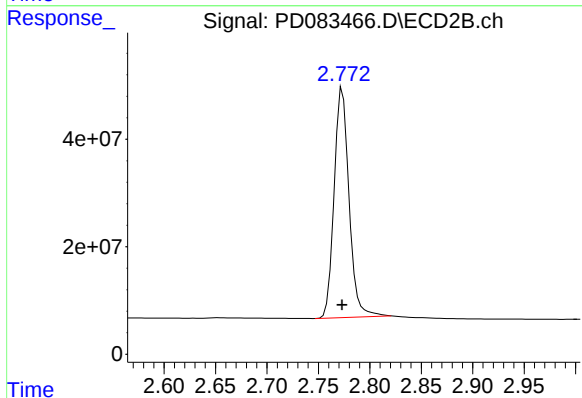


#1 Tetrachloro-m-xylene

R.T.: 2.773 min
Delta R.T.: 0.000 min
Response: 431813549
Conc: 72.17 ng/ml

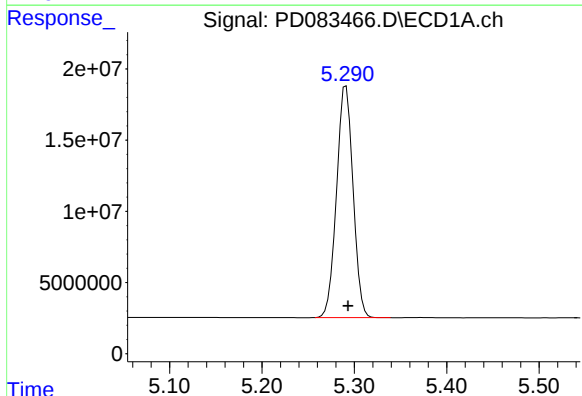


#5 Aldrin

R.T.: 5.291 min
Delta R.T.: -0.002 min
Response: 202169983
Conc: 85.27 ng/ml

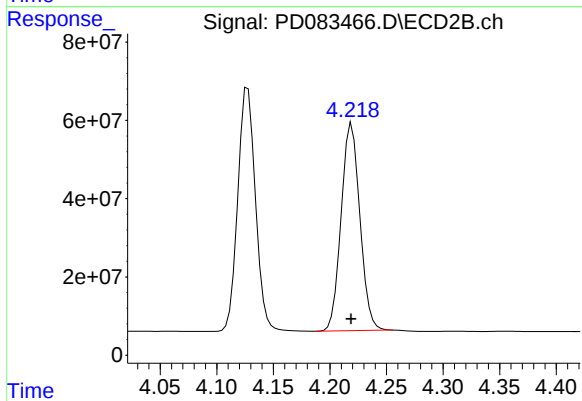


#5 Aldrin

R.T.: 4.219 min
Delta R.T.: 0.000 min
Response: 610375930
Conc: 75.88 ng/ml

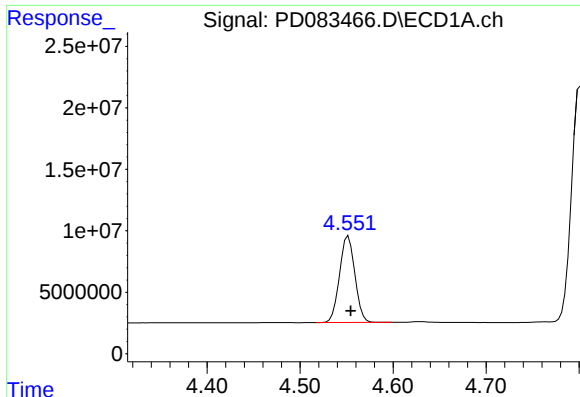


#6 beta-BHC

R.T.: 4.552 min
Delta R.T.: -0.003 min
Response: 80712668
Conc: 78.10 ng/ml

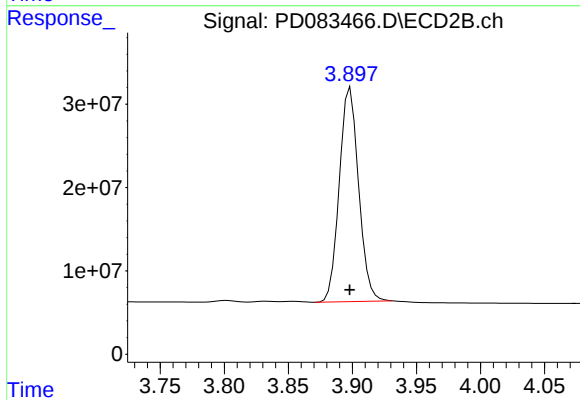


#6 beta-BHC

R.T.: 3.898 min
Delta R.T.: 0.000 min
Response: 269260595
Conc: 71.71 ng/ml

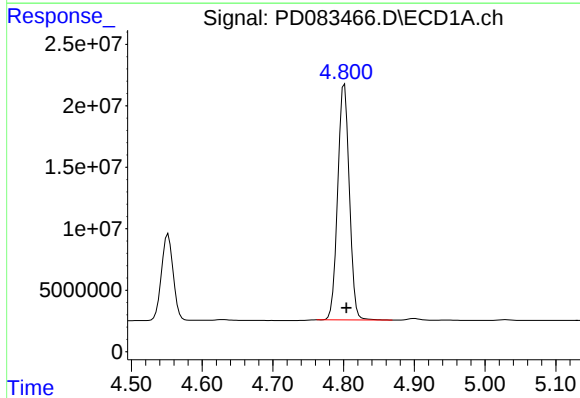


#7 delta-BHC

R.T.: 4.801 min
Delta R.T.: -0.003 min
Response: 219321707
Conc: 86.31 ng/ml

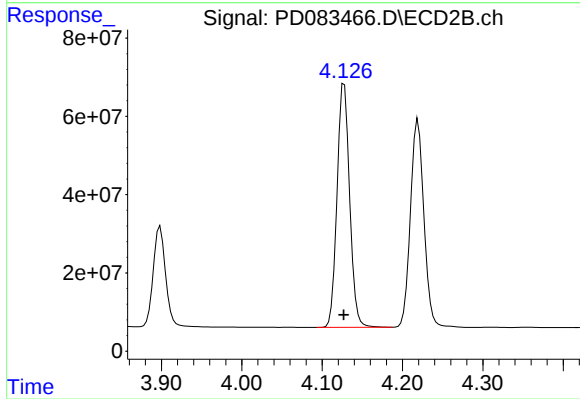


#7 delta-BHC

R.T.: 4.128 min
Delta R.T.: 0.000 min
Response: 678933682
Conc: 75.68 ng/ml

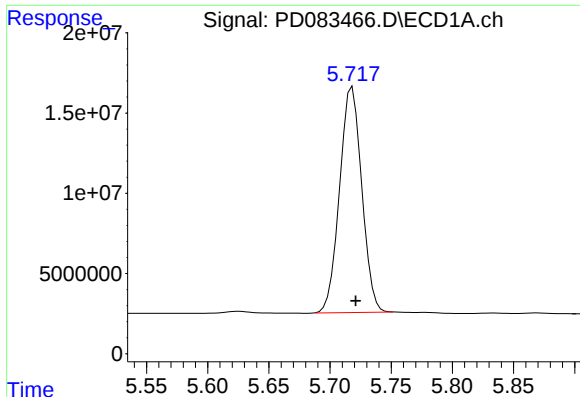


#8 Heptachlor epoxide

R.T.: 5.718 min
Delta R.T.: -0.003 min
Response: 177055876
Conc: 85.10 ng/ml

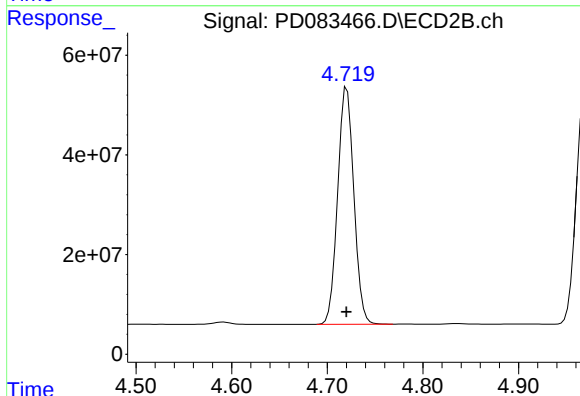


#8 Heptachlor epoxide

R.T.: 4.721 min
Delta R.T.: 0.000 min
Response: 559721009
Conc: 73.46 ng/ml

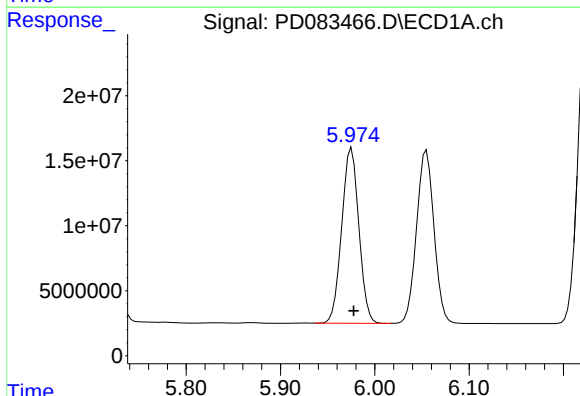


#10 trans-Chlordane

R.T.: 5.975 min
Delta R.T.: -0.003 min
Response: 170262521
Conc: 82.91 ng/ml

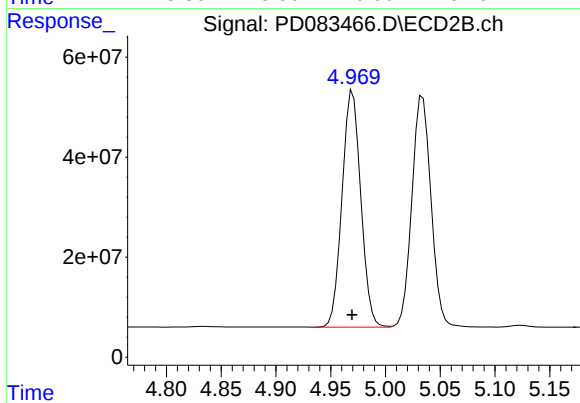


#10 trans-Chlordane

R.T.: 4.970 min
Delta R.T.: 0.000 min
Response: 563721787
Conc: 74.39 ng/ml

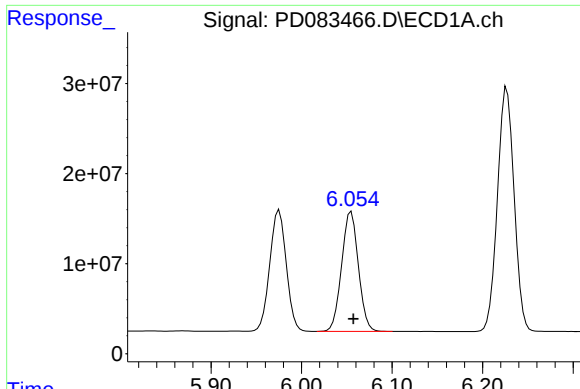


#11 cis-Chlordane

R.T.: 6.055 min
Delta R.T.: -0.003 min
Response: 171066440
Conc: 81.51 ng/ml

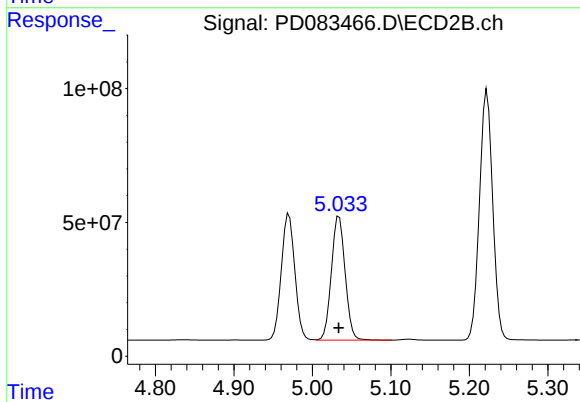


#11 cis-Chlordane

R.T.: 5.034 min
Delta R.T.: 0.000 min
Response: 565335582
Conc: 73.66 ng/ml

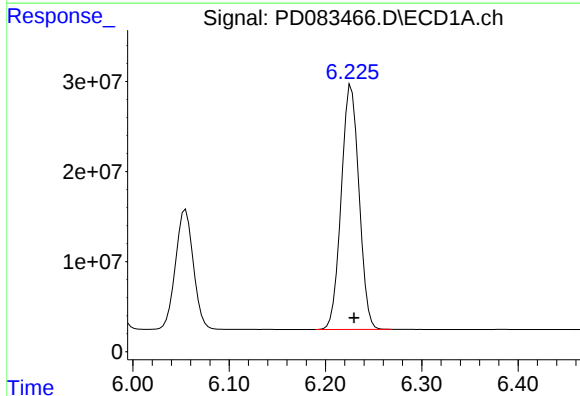


#12 4,4'-DDE

R.T.: 6.227 min
Delta R.T.: -0.003 min
Response: 347131056
Conc: 166.76 ng/ml

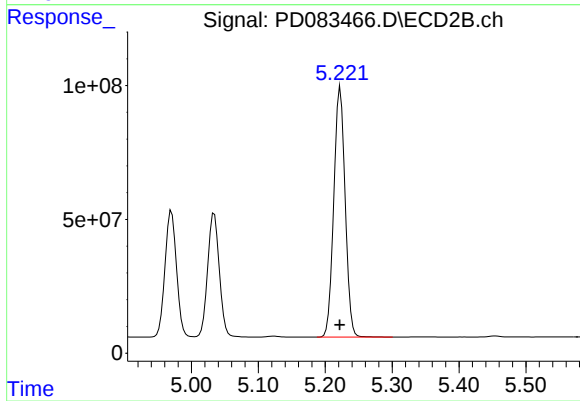


#12 4,4'-DDE

R.T.: 5.223 min
Delta R.T.: 0.000 min
Response: 1097762118
Conc: 144.55 ng/ml

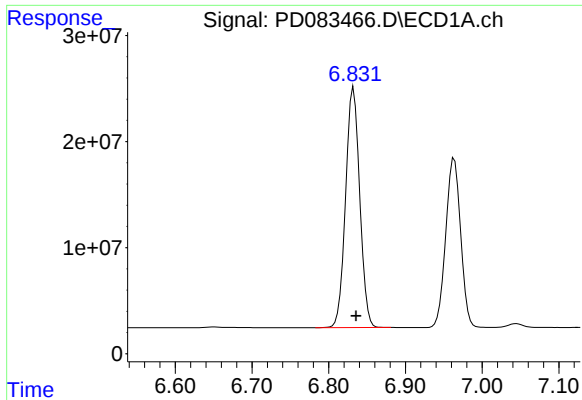


#15 Endosulfan II

R.T.: 6.832 min
Delta R.T.: -0.003 min
Response: 291229733
Conc: 161.62 ng/ml

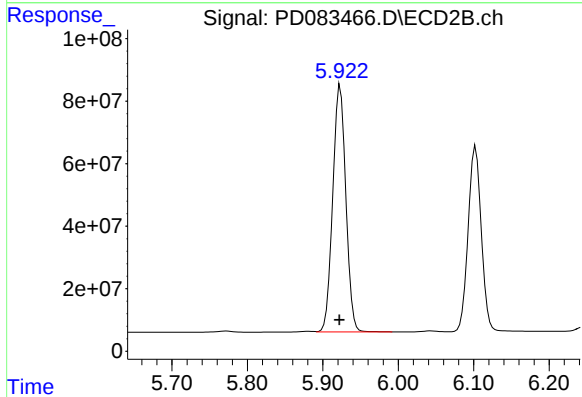


#15 Endosulfan II

R.T.: 5.923 min
Delta R.T.: 0.000 min
Response: 953097136
Conc: 140.21 ng/ml

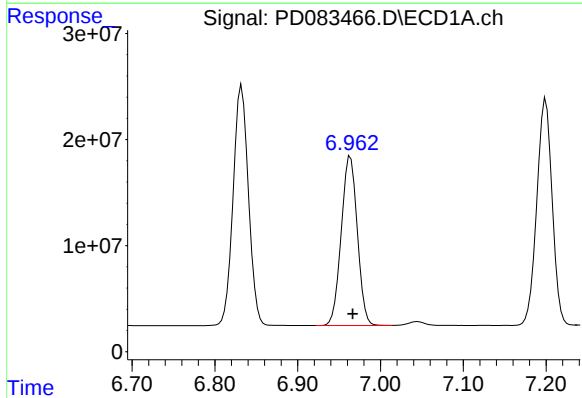


#18 Endrin aldehyde

R.T.: 6.964 min
Delta R.T.: -0.003 min
Response: 215590999
Conc: 161.56 ng/ml

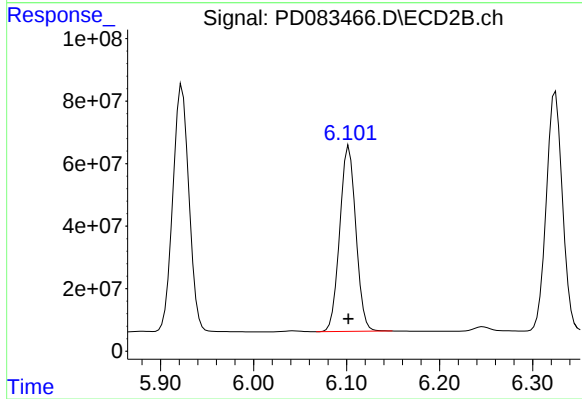


#18 Endrin aldehyde

R.T.: 6.103 min
Delta R.T.: 0.000 min
Response: 715258906
Conc: 139.42 ng/ml

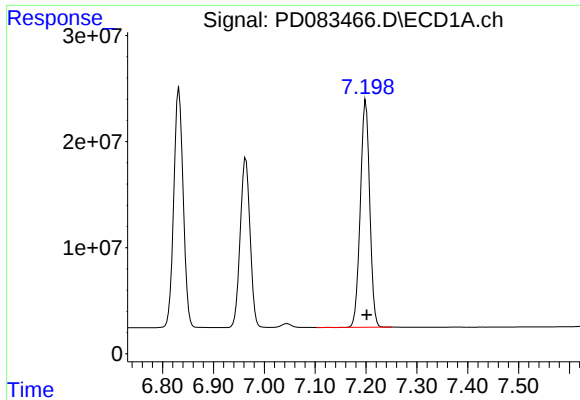


#19 Endosulfan Sulfate

R.T.: 7.200 min
Delta R.T.: -0.002 min
Response: 274385011
Conc: 159.85 ng/ml

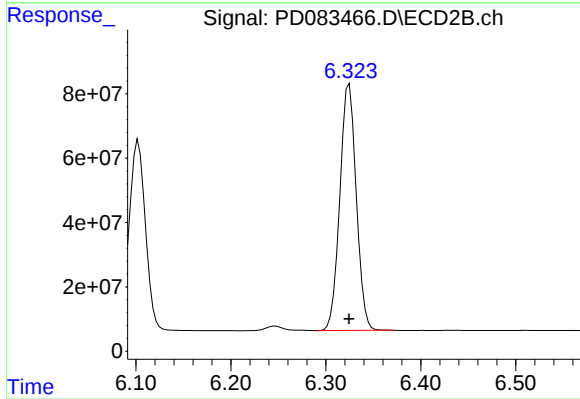


#19 Endosulfan Sulfate

R.T.: 6.325 min
Delta R.T.: 0.000 min
Response: 922460525
Conc: 138.16 ng/ml

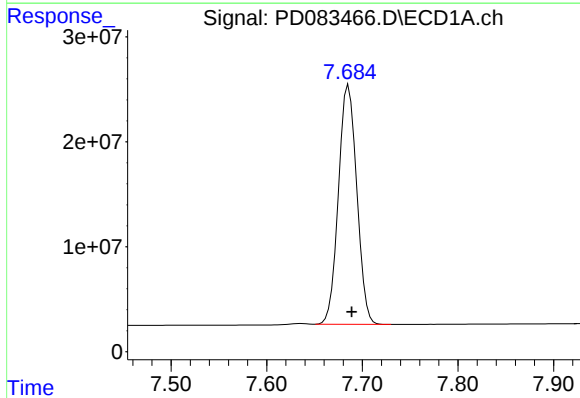


#21 Endrin ketone

R.T.: 7.686 min
Delta R.T.: -0.003 min
Response: 304811615
Conc: 162.35 ng/ml

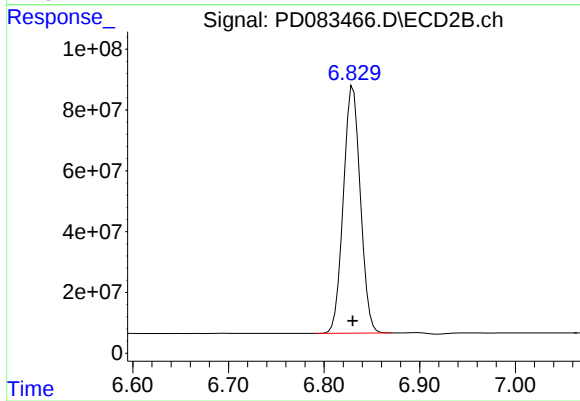


#21 Endrin ketone

R.T.: 6.830 min
Delta R.T.: 0.000 min
Response: 1006922907
Conc: 138.58 ng/ml

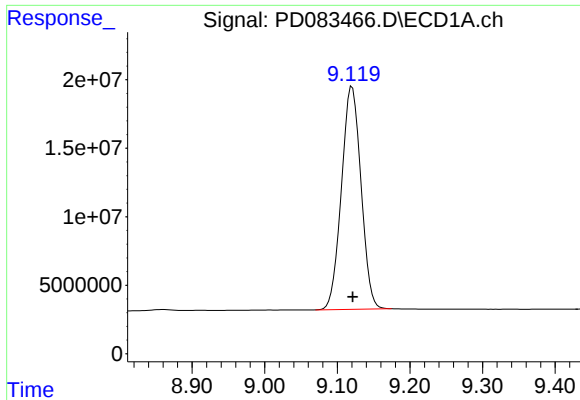

#27 Decachlorobiphenyl

R.T.: 9.120 min
Delta R.T.: 0.000 min
Response: 304641454
Conc: 154.14 ng/ml

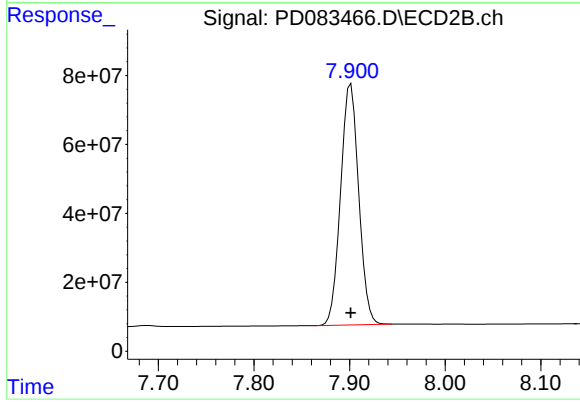

#27 Decachlorobiphenyl

R.T.: 7.901 min
Delta R.T.: 0.000 min
Response: 924125528
Conc: 139.22 ng/ml