

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060724\
 Data File : PD083470.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Jun 2024 20:05
 Operator : AR\AJ
 Sample : PB161345BS
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PLCS345

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 07 10:08:58 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060724CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 07 04:03:14 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.563	2.774	25162217	101.1E6	19.277	18.552
27)	SA Decachlor...	9.119	7.901	39197255	122.6E6	20.158	20.191
Target Compounds							
2)	A alpha-BHC	4.020	3.273	9041994	35820571	4.074	4.202
3)	MA gamma-BHC...	4.355	3.601	9680204	33886521	4.449	4.339
4)	MA Heptachlor	4.947	3.940	11336617	34388100	4.667	4.392
5)	MB Aldrin	5.291	4.219	10761127	33405979	4.530	4.323
6)	B beta-BHC	4.552	3.898	4663400	14534703	4.627	4.073
7)	B delta-BHC	4.800	4.127	9649171	21909677	3.673	2.569 #
8)	B Heptachlo...	5.719	4.720	9386705	33951207	4.545	4.640
9)	A Endosulfan I	6.106	5.090	9581019	31697097	4.899	4.795
10)	B trans-Chl...	5.976	4.970	9722064	33831931	4.775	4.658
11)	B cis-Chlor...	6.055	5.034	10166857	34772650	4.882	4.723
12)	B 4,4'-DDE	6.227	5.221	19658394	63628922	9.478	8.953
13)	MA Dieldrin	6.382	5.353	19137532	67777644	9.255	9.304
14)	MA Endrin	6.613	5.629	15675117	60938003	9.279	9.422
15)	B Endosulfa...	6.833	5.923	17306067	59775417	9.621	9.420
16)	A 4,4'-DDD	6.746	5.775	13344400	52158776	9.107	9.252
17)	MA 4,4'-DDT	7.062	6.026	14033303	49290810	9.315	8.708
18)	B Endrin al...	6.963	6.102	13724419	48567422	10.289	10.139
19)	B Endosulfa...	7.199	6.325	15466028	55045417	9.040	8.909
20)	A Methoxychlor	7.538	6.601	42265277	146.8E6	48.852	50.498
21)	B Endrin ke...	7.686	6.830	18320434	65605279	9.827	9.759

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060724\
Data File : PD083470.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Jun 2024 20:05
Operator : AR\AJ
Sample : PB161345BS
Misc :
ALS Vial : 21 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 07 10:08:58 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060724CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jun 07 04:03:14 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

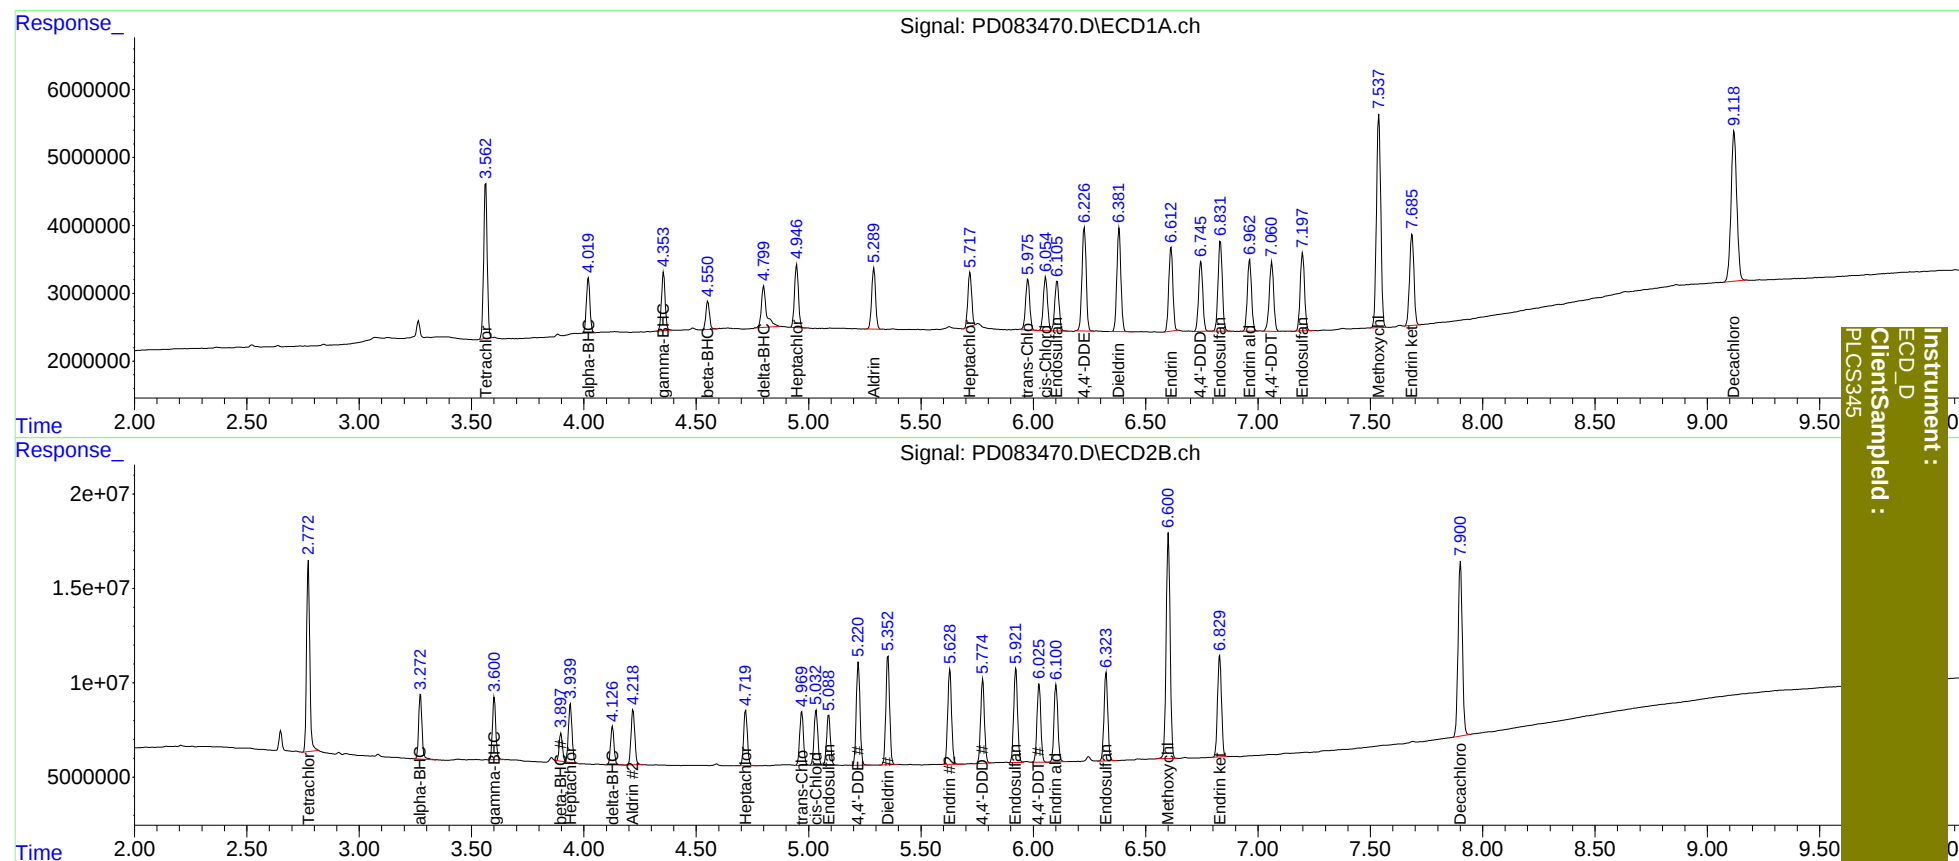

Instrument :
ECD_D
ClientSampled :
PLCS345