

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060724\
 Data File : PD083491.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Jun 2024 03:38
 Operator : AR\AJ
 Sample : P2590-16MSD
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BHBM0MSD

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 06/07/2024
 Supervised By :Ankita Jodhani 06/07/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 07 10:16:28 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060724CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 07 04:03:14 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.561	2.774	8206307	39682349	6.287m	7.280
27)	SA Decachlor...	9.118	7.900	52500672	193.8E6	26.999	31.917
Target Compounds							
2)	A alpha-BHC	4.019	3.273	72127310	263.8E6	32.499m	30.945
3)	MA gamma-BHC...	4.353	3.602	75593237	261.0E6	34.746m	33.419
4)	MA Heptachlor	4.945	3.940	80776828	241.3E6	33.251m	30.817
5)	MB Aldrin	5.290	4.219	73973973	241.9E6	31.137	31.309
6)	B beta-BHC	4.552	3.898	28748574	100.9E6	28.526m	28.277
7)	B delta-BHC	4.801	4.127	76920385	273.4E6	29.281	32.067
8)	B Heptachlo...	5.718	4.720	61823157	229.1E6	29.933	31.316
9)	A Endosulfan I	6.104	5.091	60473317	138.9E6	30.923m	21.010 #
10)	B trans-Chl...	5.973	4.968	63757783	239.1E6	31.313m	32.924m
11)	B cis-Chlor...	6.054	5.033	63800168	251.8E6	30.637	34.195
12)	B 4,4'-DDE	6.226	5.221	97231859	440.7E6	46.878	62.012 #
13)	MA Dieldrin	6.382	5.353	146.1E6	687.2E6	70.671	94.325 #
14)	MA Endrin	6.612	5.629	103.1E6	426.8E6	61.048	65.989
15)	B Endosulfa...	6.832	5.922	109.7E6	404.9E6	60.970	63.809
16)	A 4,4'-DDD	6.745	5.774	97298709	338.7E6	66.401	60.079m
17)	MA 4,4'-DDT	7.060	6.025	112.4E6	365.7E6	74.629	64.608
18)	B Endrin al...	6.963	6.102	77523804	258.6E6	58.118	53.982
19)	B Endosulfa...	7.198	6.324	112.1E6	404.3E6	65.542	65.433
20)	A Methoxychlor	7.539	6.601	260.5E6	827.9E6	301.130	284.862
21)	B Endrin ke...	7.685	6.829	105.5E6	336.5E6	56.613	50.058

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060724\
Data File : PD083491.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Jun 2024 03:38
Operator : AR\AJ
Sample : P2590-16MSD
Misc :
ALS Vial : 39 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 07 10:16:28 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060724CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jun 07 04:03:14 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

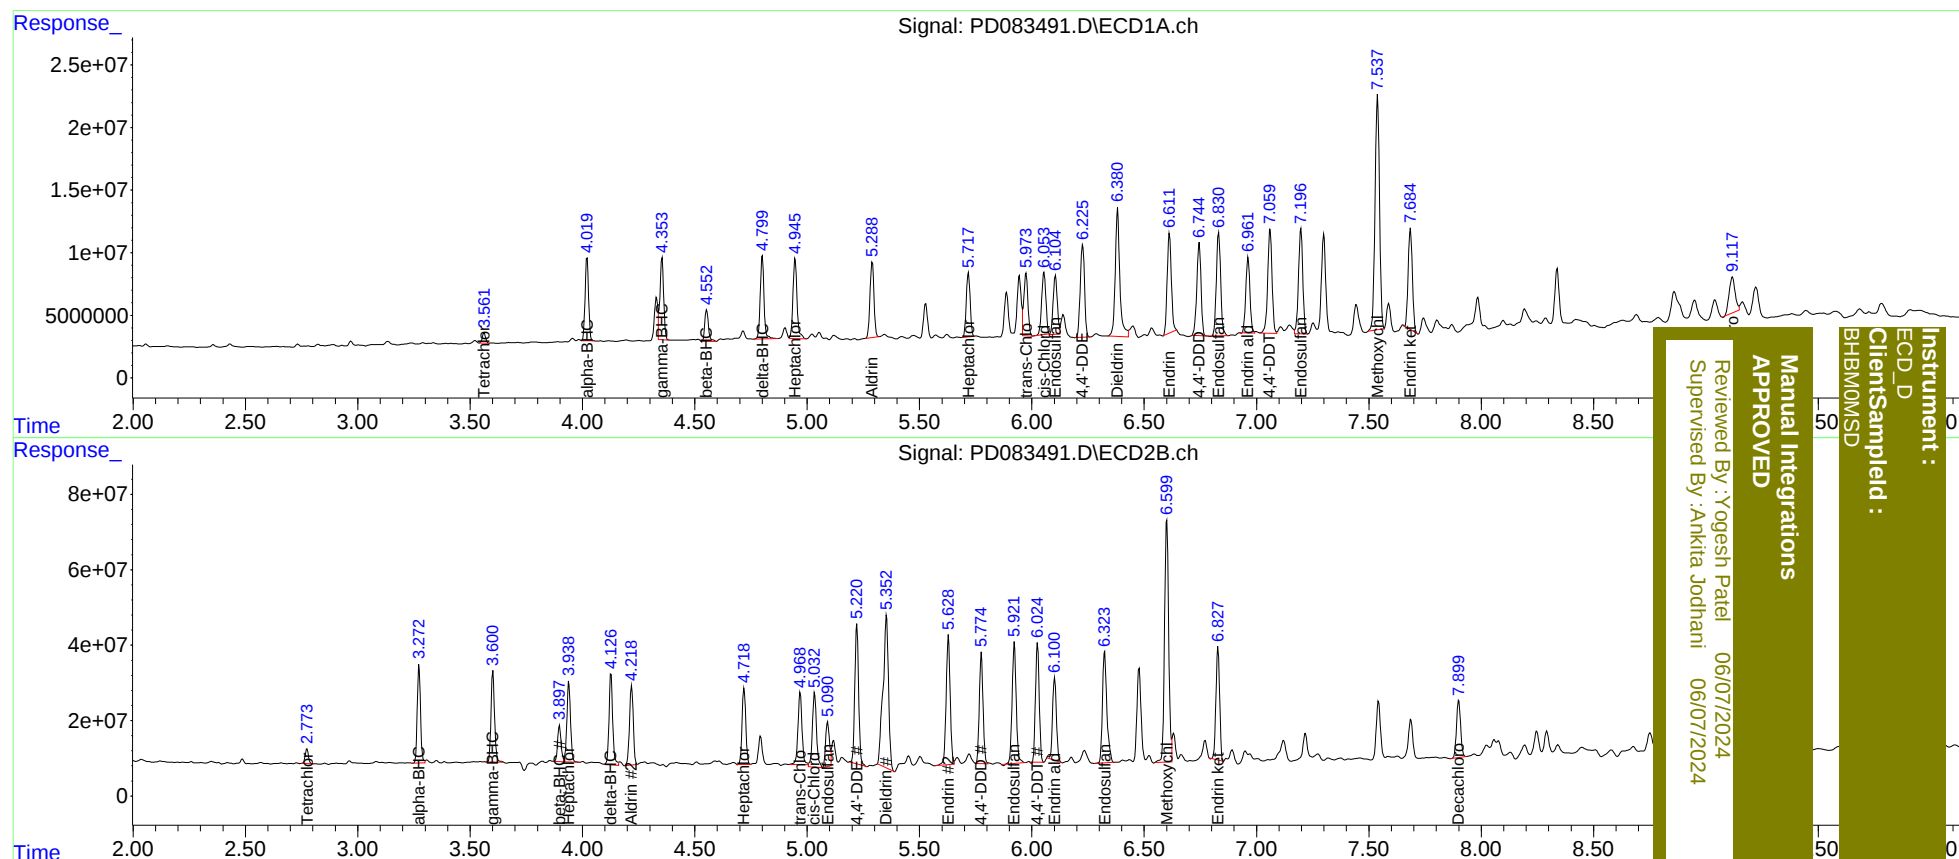

Manual Integrations
APPROVED
Reviewed By : Yogesh Patel 06/07/2024
Supervised By : Ankita Jodhani 06/07/2024

Instrument :
ECD_D
Client Sampled :
BHMOMSD