

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060821\
 Data File : PD063652.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jun 2021 21:35
 Operator : AR\AJ
 Sample : M2634-04
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 R44-STONE-2

Manual Integrations
 APPROVED

Ankita
 6/9/2021 1:41:34 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 09 01:53:10 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060221.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 03 01:33:41 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.442	3.971	10876953	79597763	7.861	5.941m
28)	SA Decachlor...	8.195	9.025	19789153	184.1E6	12.583	13.323
Target Compounds							
12)	B 4,4'-DDE	5.598	6.305	1155338	12955686	0.664m	0.713m
17)	MA 4,4'-DDT	6.353	7.093	4879270	20053123	3.377m	1.332 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060821\
Data File : PD063652.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Jun 2021 21:35
Operator : AR\AJ
Sample : M2634-04
Misc :
ALS Vial : 40 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampled :
R44-STONE-2


Manual Integrations
APPROVED

Ankita
6/9/2021 1:41:34 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 09 01:53:10 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060221.M
Quant Title : GC Extractables
QLast Update : Thu Jun 03 01:33:41 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

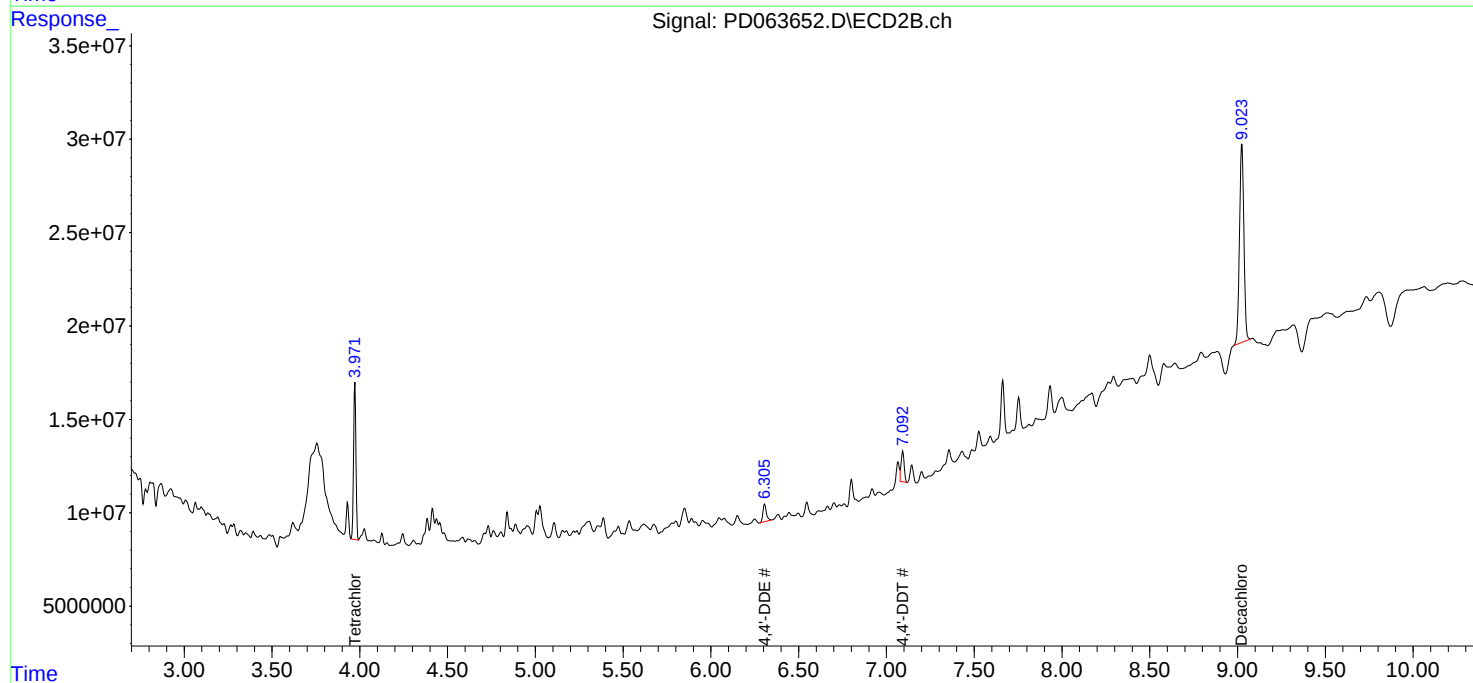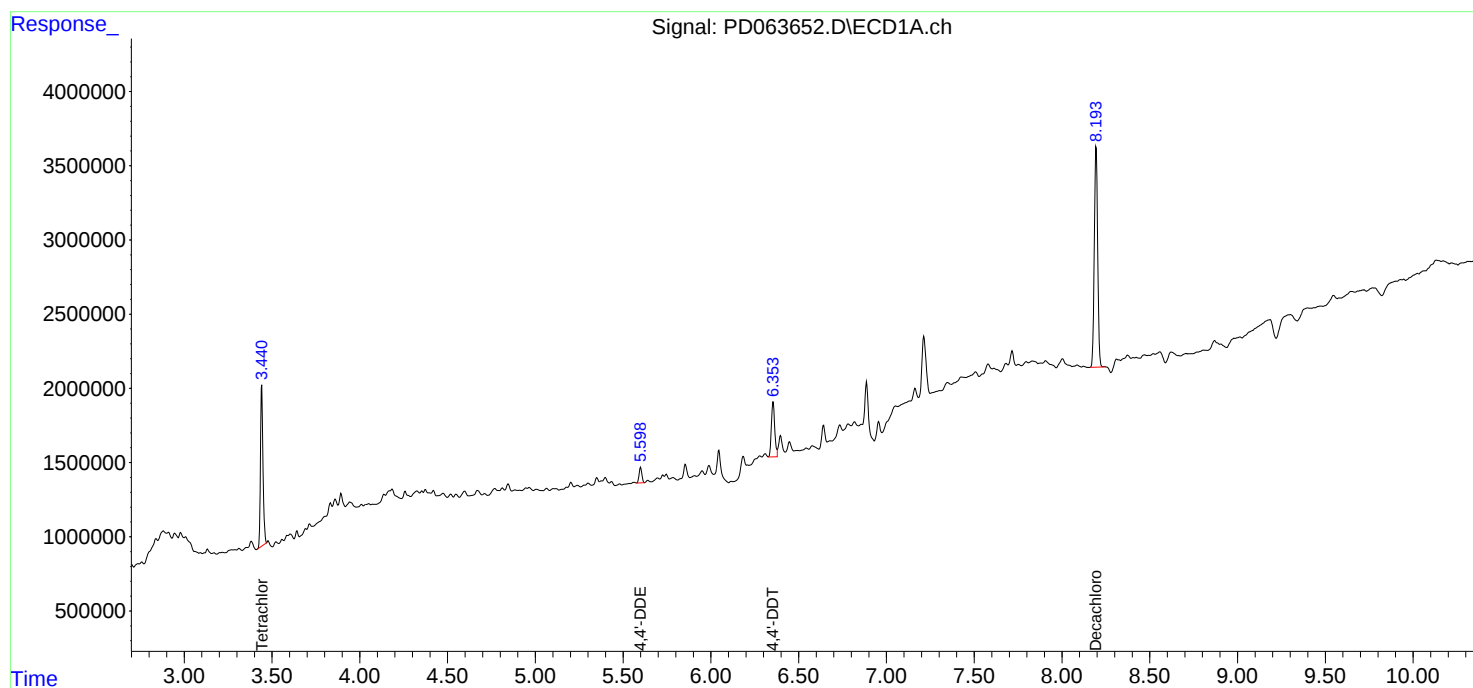

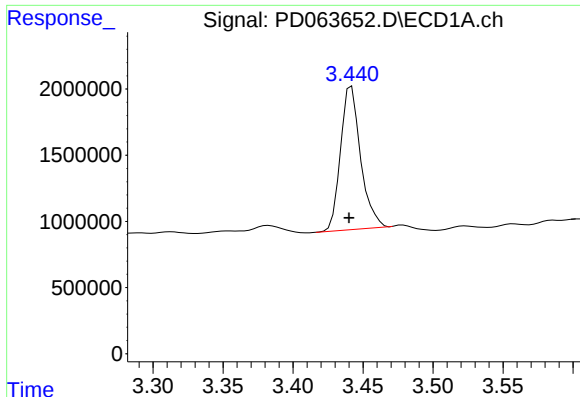


#1 Tetrachloro-m-xylene

R.T.: 3.442 min
Delta R.T.: 0.002 min
Response: 10876953
Conc: 7.86 ng/ml

Instrument :
ECD_D
ClientSampleId :
R44-STONE-2


Manual Integrations
APPROVED

Ankita
6/9/2021 1:41:34 PM

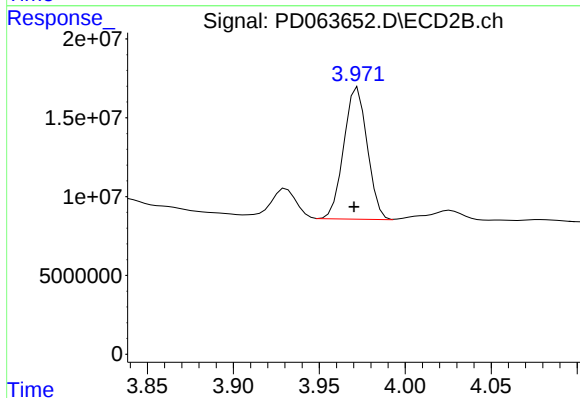


#1 Tetrachloro-m-xylene

R.T.: 3.971 min
Delta R.T.: 0.000 min
Response: 79597763
Conc: 5.94 ng/ml m

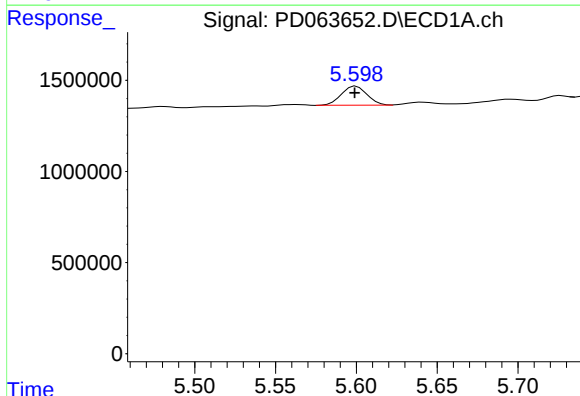


#12 4,4'-DDE

R.T.: 5.598 min
Delta R.T.: 0.000 min
Response: 1155338
Conc: 0.66 ng/ml m

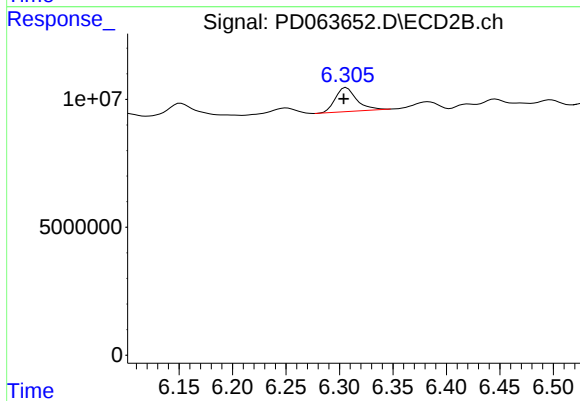

#12 4,4'-DDE

R.T.: 6.305 min
Delta R.T.: 0.001 min
Response: 12955686
Conc: 0.71 ng/ml m

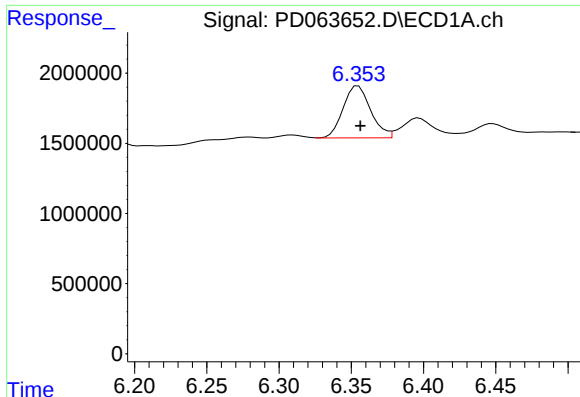


#17 4,4'-DDT

R.T.: 6.353 min
Delta R.T.: -0.003 min
Response: 4879270
Conc: 3.38 ng/ml m

Instrument :
ECD_D
ClientSampleId :
R44-STONE-2


Manual Integrations
APPROVED

Ankita
6/9/2021 1:41:34 PM

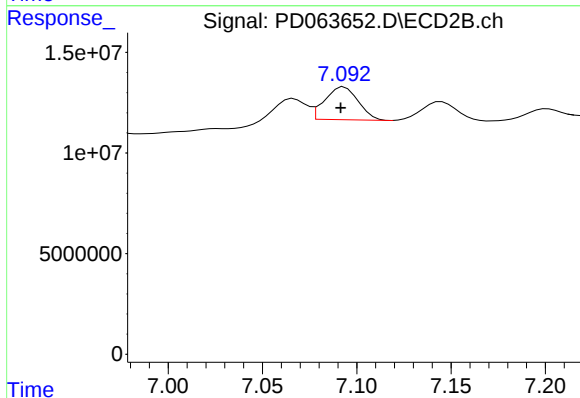


#17 4,4'-DDT

R.T.: 7.093 min
Delta R.T.: 0.002 min
Response: 20053123
Conc: 1.33 ng/ml

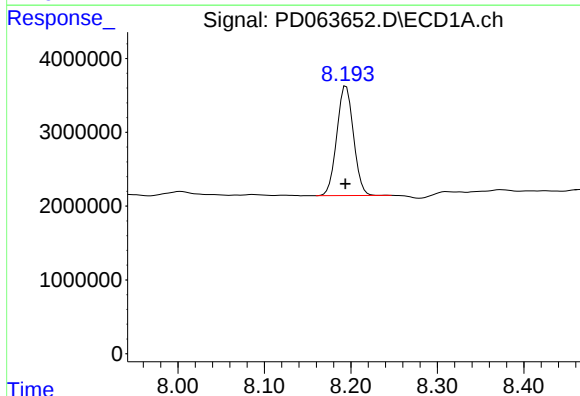

#28 Decachlorobiphenyl

R.T.: 8.195 min
Delta R.T.: 0.000 min
Response: 19789153
Conc: 12.58 ng/ml

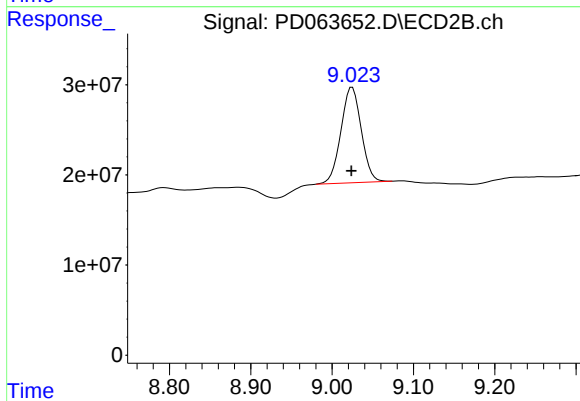

#28 Decachlorobiphenyl

R.T.: 9.025 min
Delta R.T.: 0.001 min
Response: 184098701
Conc: 13.32 ng/ml