

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060822\
 Data File : PD070185.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jun 2022 08:51
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 08 12:30:48 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060622.M
 Quant Title : GC Extractables
 QLast Update : Wed Jun 08 02:48:31 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
8) B	Heptachlo...	0.000	6.067	0 80236869	N.D.	9.739 #
9) A	Endosulfan I	0.000	6.458	0 18840352	N.D.	1.779 #
10) B	gamma-Chl...	0.000	6.340f	0 85291281	N.D.	7.421 #
14) MA	Endrin	6.001	0.000	699687 0	0.581	N.D. #
25)	Chlordane-3	0.000	6.340f	0 85291281	N.D.	58.202 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060822\
Data File : PD070185.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Jun 2022 08:51
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 08 12:30:48 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060622.M
Quant Title : GC Extractables
QLast Update : Wed Jun 08 02:48:31 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

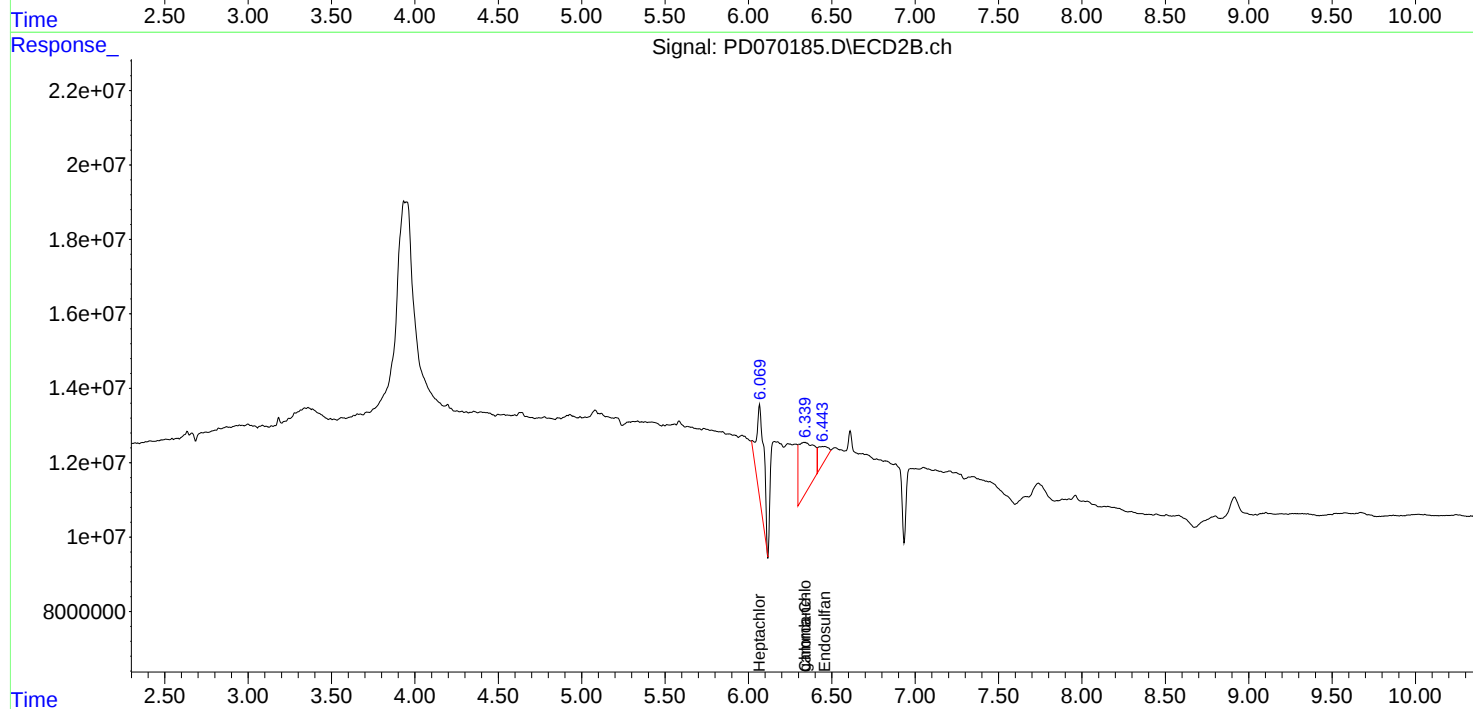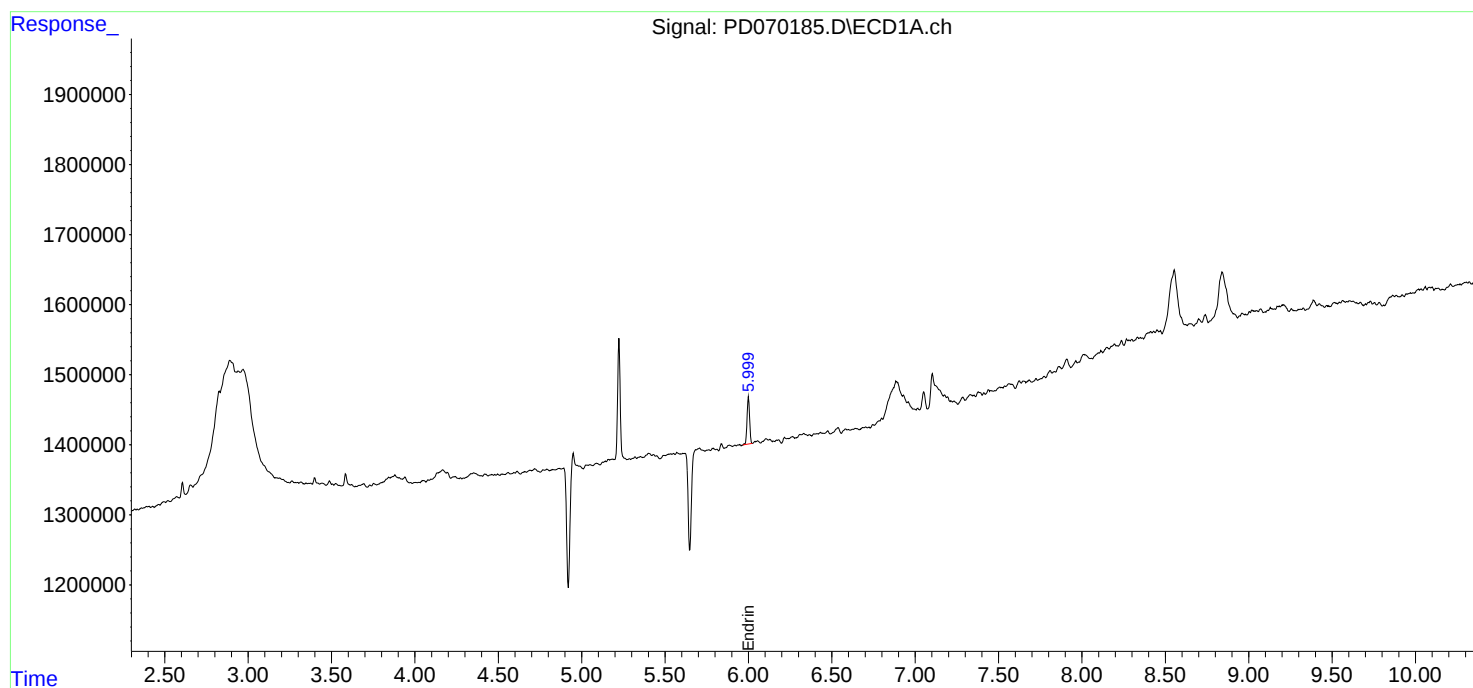


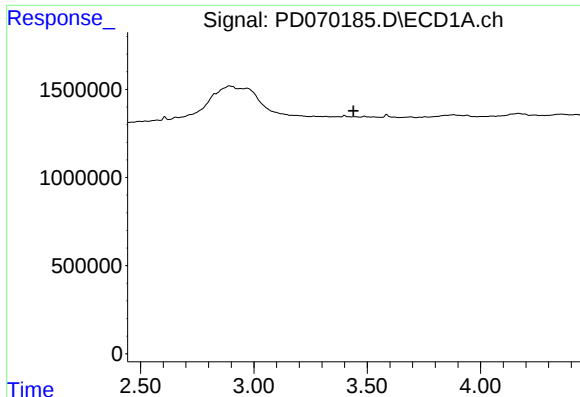

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.440 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

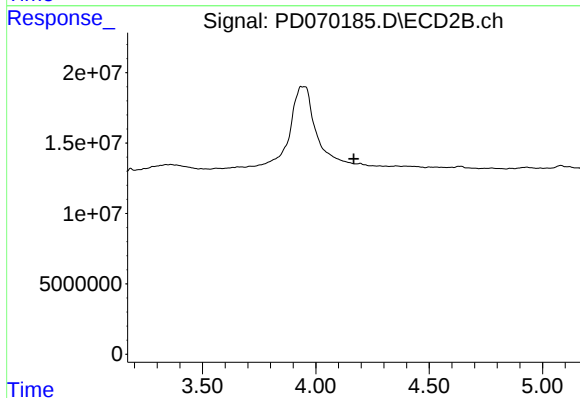


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 4.167 min
Response: 0
Conc: N.D.

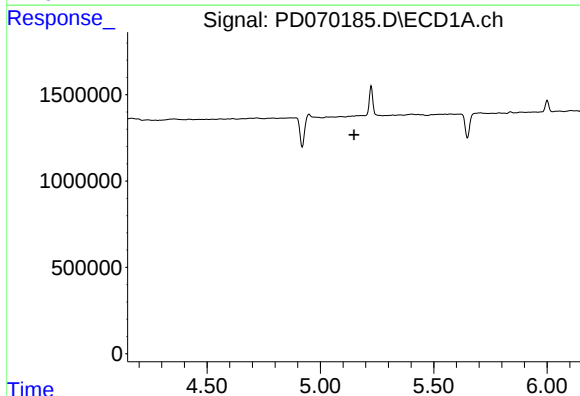


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.149 min
Response: 0
Conc: N.D.

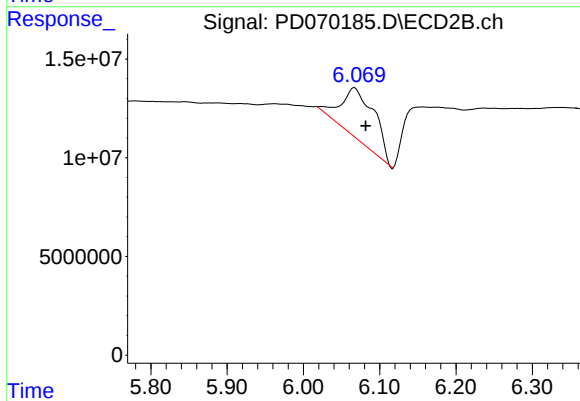

#8 Heptachlor epoxide


R.T.: 6.067 min
Delta R.T.: -0.014 min
Response: 80236869
Conc: 9.74 ng/ml

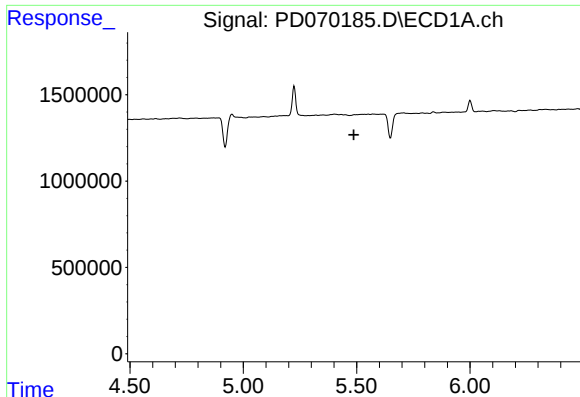

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 5.487 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

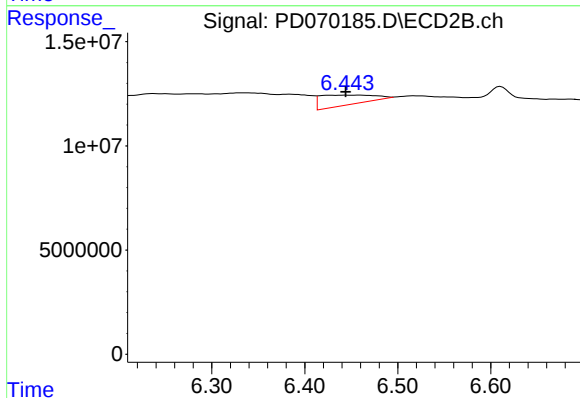


#9 Endosulfan I

R.T.: 6.458 min
Delta R.T.: 0.014 min
Response: 18840352
Conc: 1.78 ng/ml

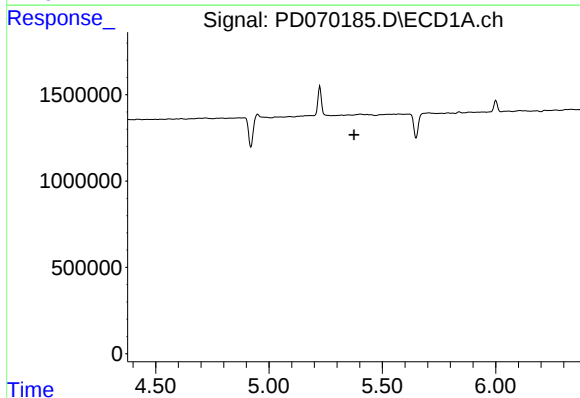


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.375 min
Response: 0
Conc: N.D.

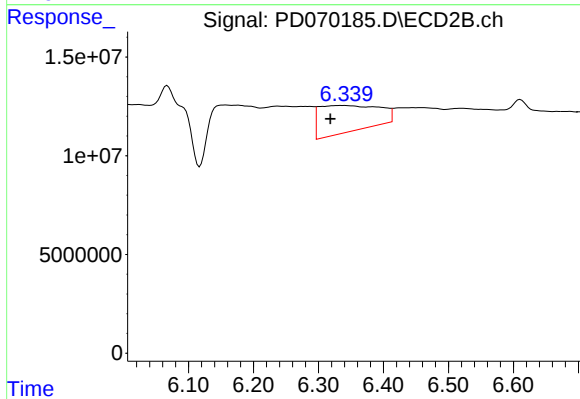

#10 gamma-Chlordane


R.T.: 6.340 min
Delta R.T.: 0.022 min
Response: 85291281
Conc: 7.42 ng/ml

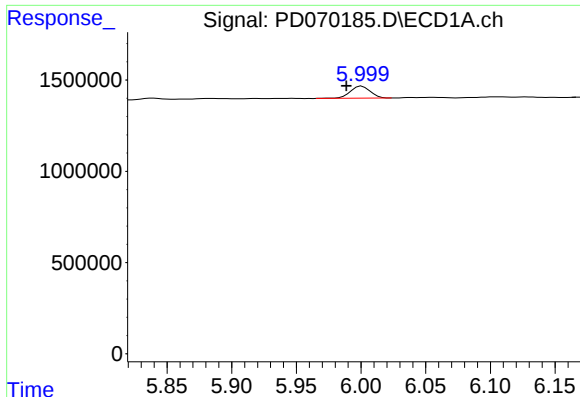

#14 Endrin


R.T.: 6.001 min
Delta R.T.: 0.012 min
Response: 699687
Conc: 0.58 ng/ml

Instrument :
ECD_D
ClientSampleId :

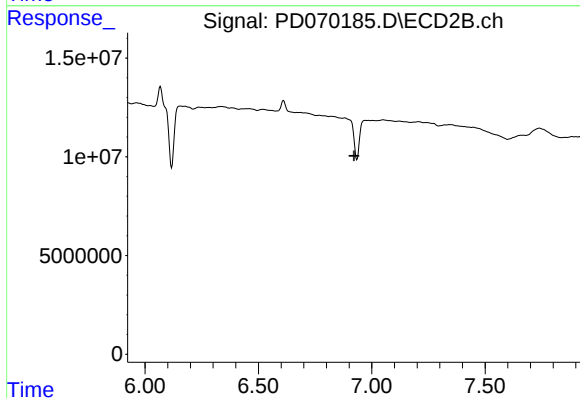


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.922 min
Response: 0
Conc: N.D.

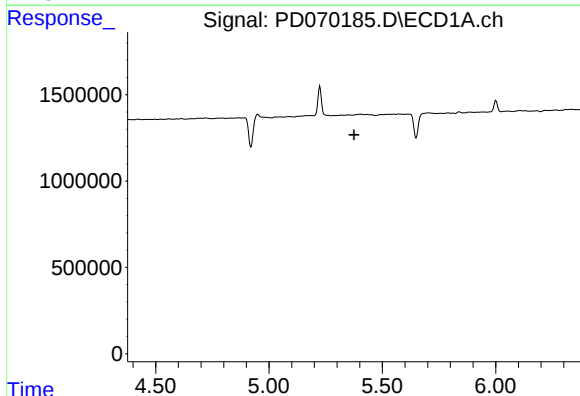


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.375 min
Response: 0
Conc: N.D.

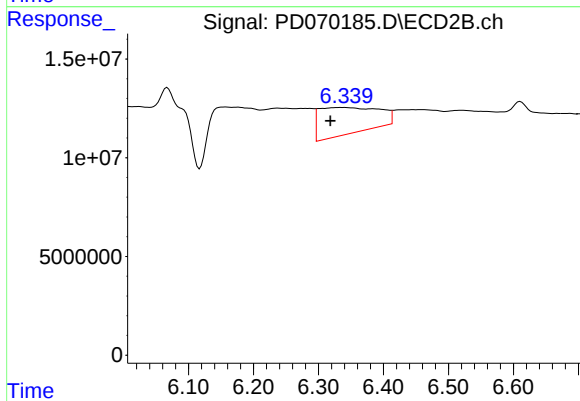

#25 Chlordane-3


R.T.: 6.340 min
Delta R.T.: 0.022 min
Response: 85291281
Conc: 58.20 ng/ml

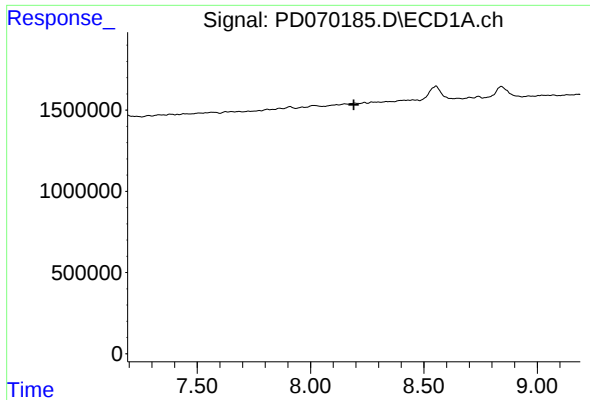

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.191 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

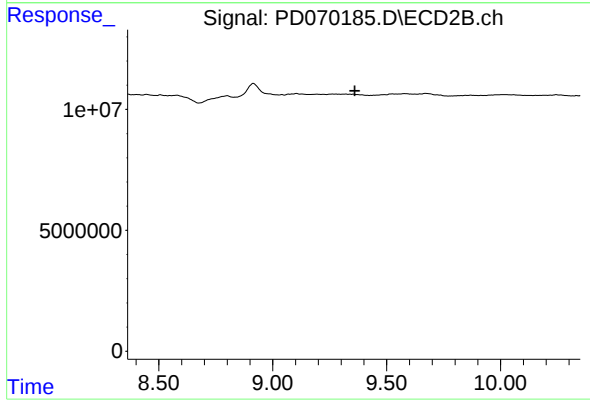

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.360 min
Response: 0
Conc: N.D.