

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060822\
 Data File : PD070197.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jun 2022 12:19
 Operator : AR\AJ
 Sample : N3194-04
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 08 12:32:13 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060622.M
 Quant Title : GC Extractables
 QLast Update : Wed Jun 08 02:48:31 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.441	4.169	21369701	203.2E6	19.684	20.819
28)	SA Decachlor...	8.192	9.362	19664523	114.6E6	17.682	18.632
Target Compounds							
9)	A Endosulfan I	5.515f	0.000	703363	0	0.537	N.D. #
17)	MA 4,4'-DDT	6.351	0.000	730616	0	0.689	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060822\
Data File : PD070197.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Jun 2022 12:19
Operator : AR\AJ
Sample : N3194-04
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 08 12:32:13 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060622.M
Quant Title : GC Extractables
QLast Update : Wed Jun 08 02:48:31 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

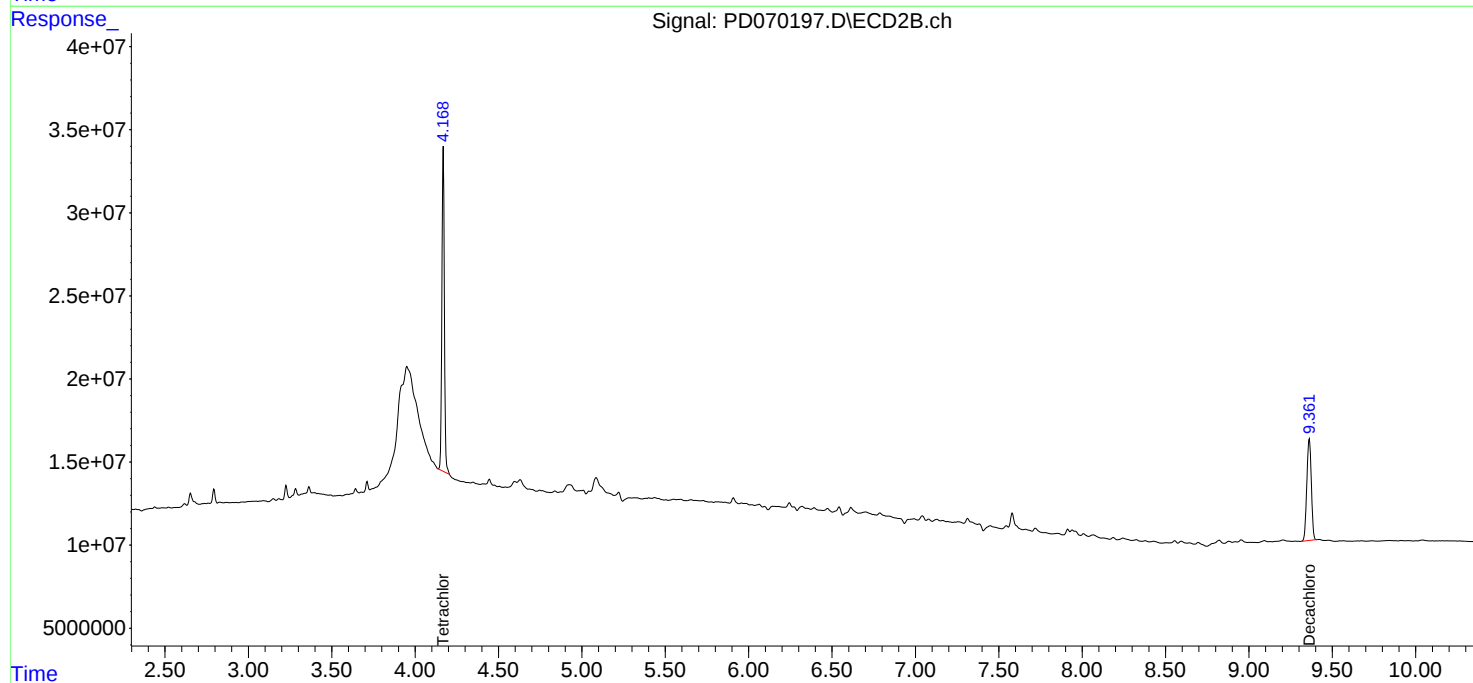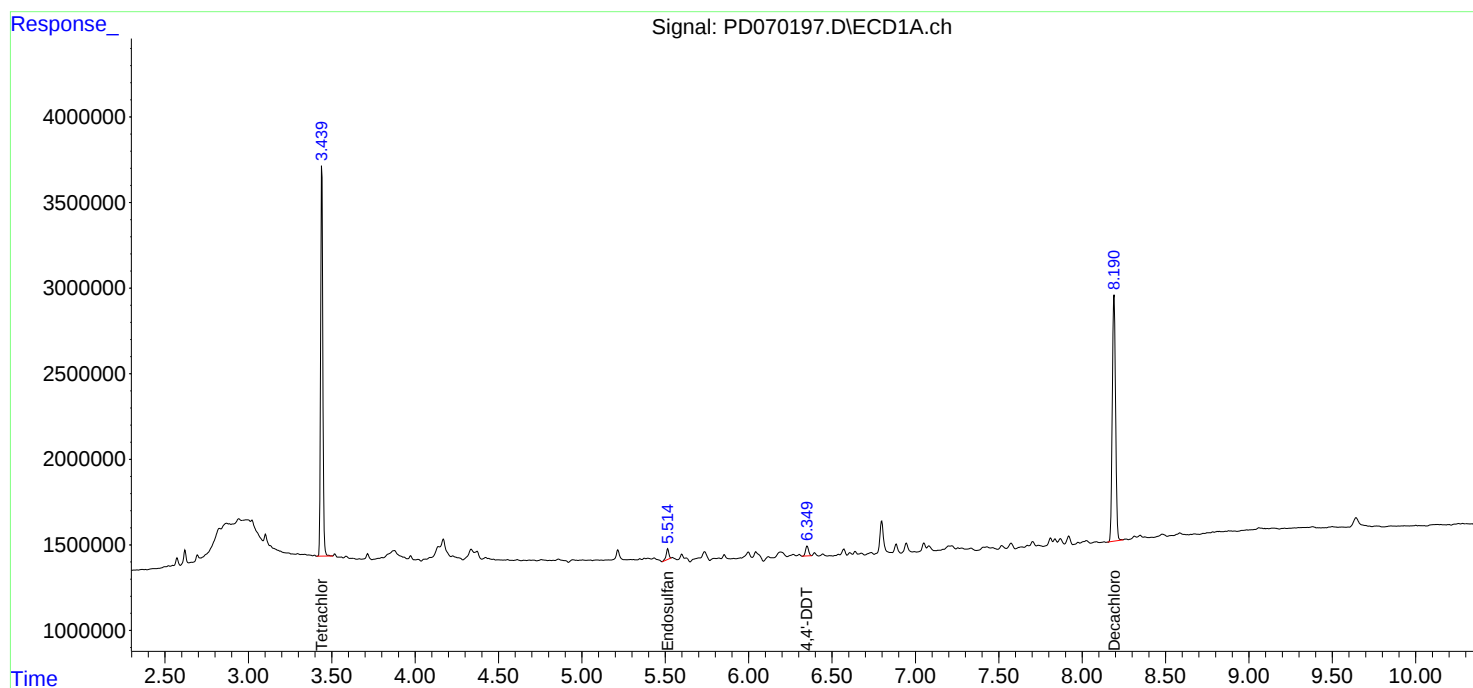


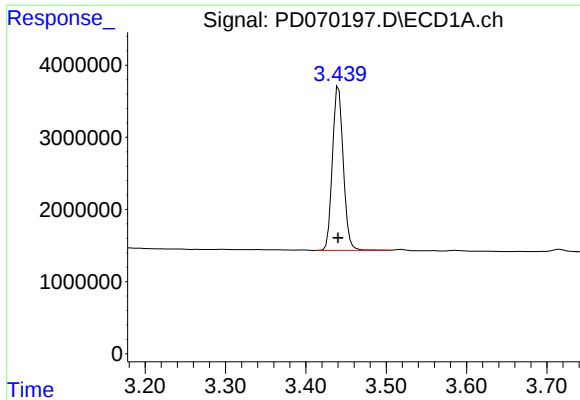

#1 Tetrachloro-m-xylene


R.T.: 3.441 min
Delta R.T.: 0.000 min
Response: 21369701
Conc: 19.68 ng/ml

Instrument :
ECD_D
ClientSampleId :

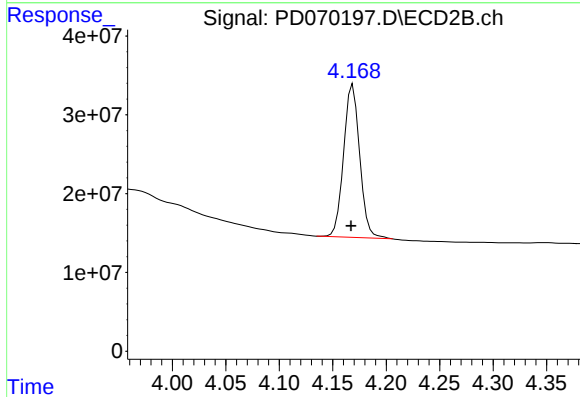


#1 Tetrachloro-m-xylene

R.T.: 4.169 min
Delta R.T.: 0.002 min
Response: 203220362
Conc: 20.82 ng/ml

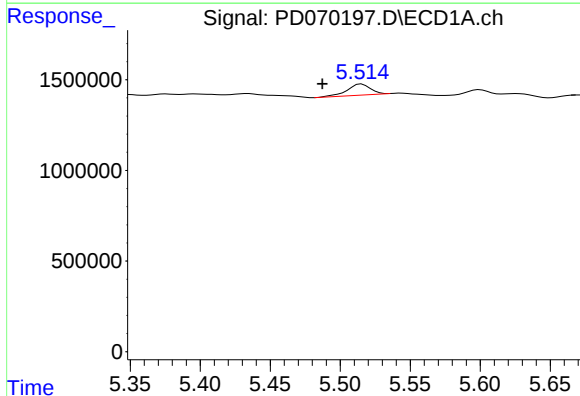


#9 Endosulfan I

R.T.: 5.515 min
Delta R.T.: 0.028 min
Response: 703363
Conc: 0.54 ng/ml

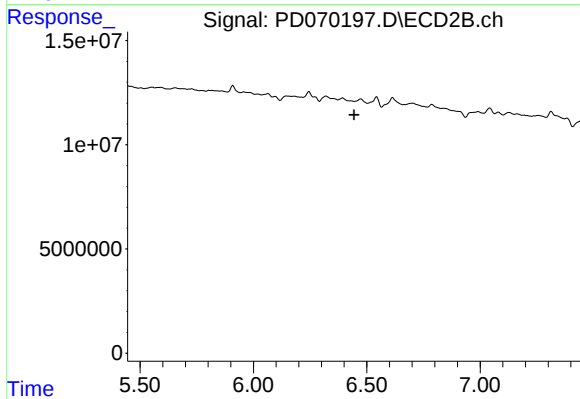

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 6.444 min
Response: 0
Conc: N.D.

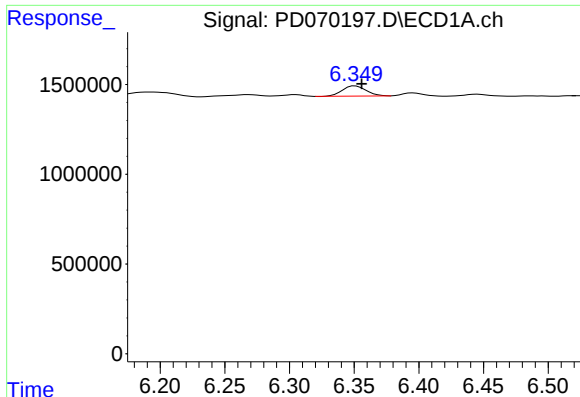

#17 4,4'-DDT


R.T.: 6.351 min
Delta R.T.: -0.005 min
Response: 730616
Conc: 0.69 ng/ml

Instrument :
ECD_D
ClientSampleId :

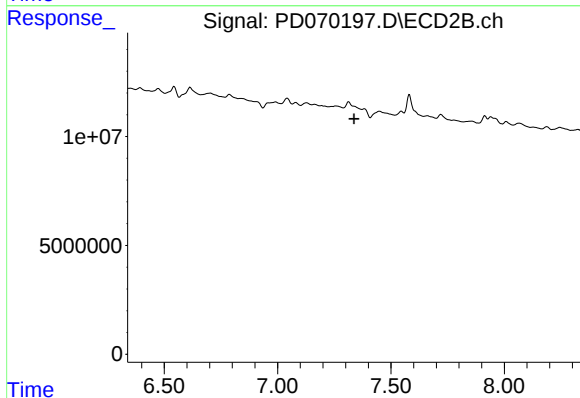


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 7.337 min
Response: 0
Conc: N.D.

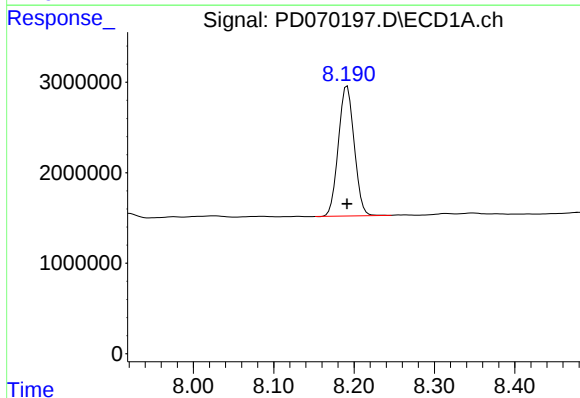

#28 Decachlorobiphenyl

R.T.: 8.192 min
Delta R.T.: 0.000 min
Response: 19664523
Conc: 17.68 ng/ml

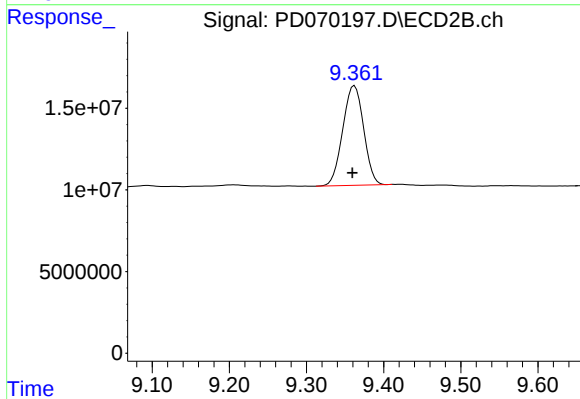

#28 Decachlorobiphenyl

R.T.: 9.362 min
Delta R.T.: 0.003 min
Response: 114595474
Conc: 18.63 ng/ml