

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060822\
 Data File : PD070200.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jun 2022 13:01
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 08 13:37:04 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060622.M
 Quant Title : GC Extractables
 QLast Update : Wed Jun 08 02:48:31 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.441	4.168	22238993	208.1E6	20.484	21.316
28)	SA Decachlor...	8.192	9.361	23317161	135.4E6	20.967	22.019
Target Compounds							
8)	B Heptachlo...	0.000	6.068	0	61152510	N.D.	7.423 #
10)	B gamma-Chl...	0.000	6.330	0	33939311	N.D.	2.953 #
14)	MA Endrin	6.000	0.000	668841	0	0.555	N.D. #
23)	Chlordane-1	4.336f	0.000	1408176	0	35.341	N.D. #
25)	Chlordane-3	0.000	6.330	0	33939311	N.D.	23.160 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060822\
Data File : PD070200.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Jun 2022 13:01
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 08 13:37:04 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060622.M
Quant Title : GC Extractables
QLast Update : Wed Jun 08 02:48:31 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

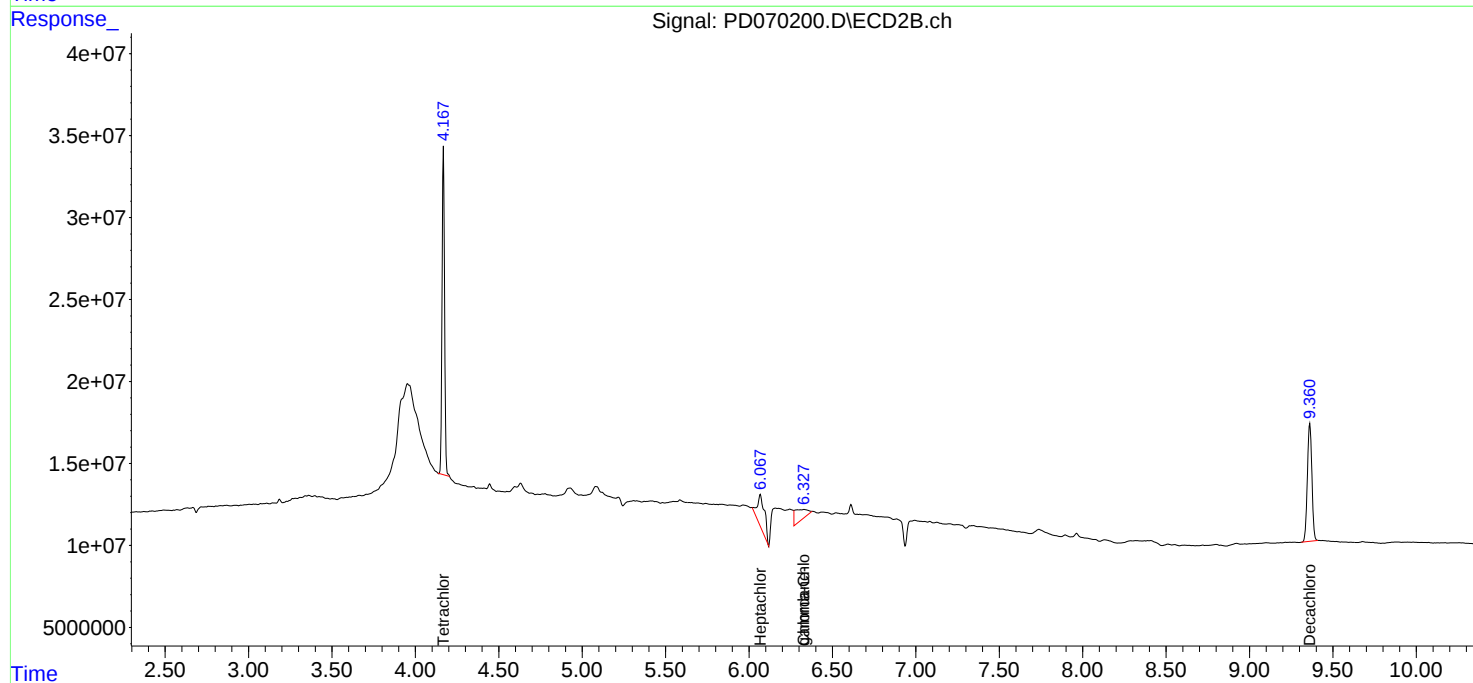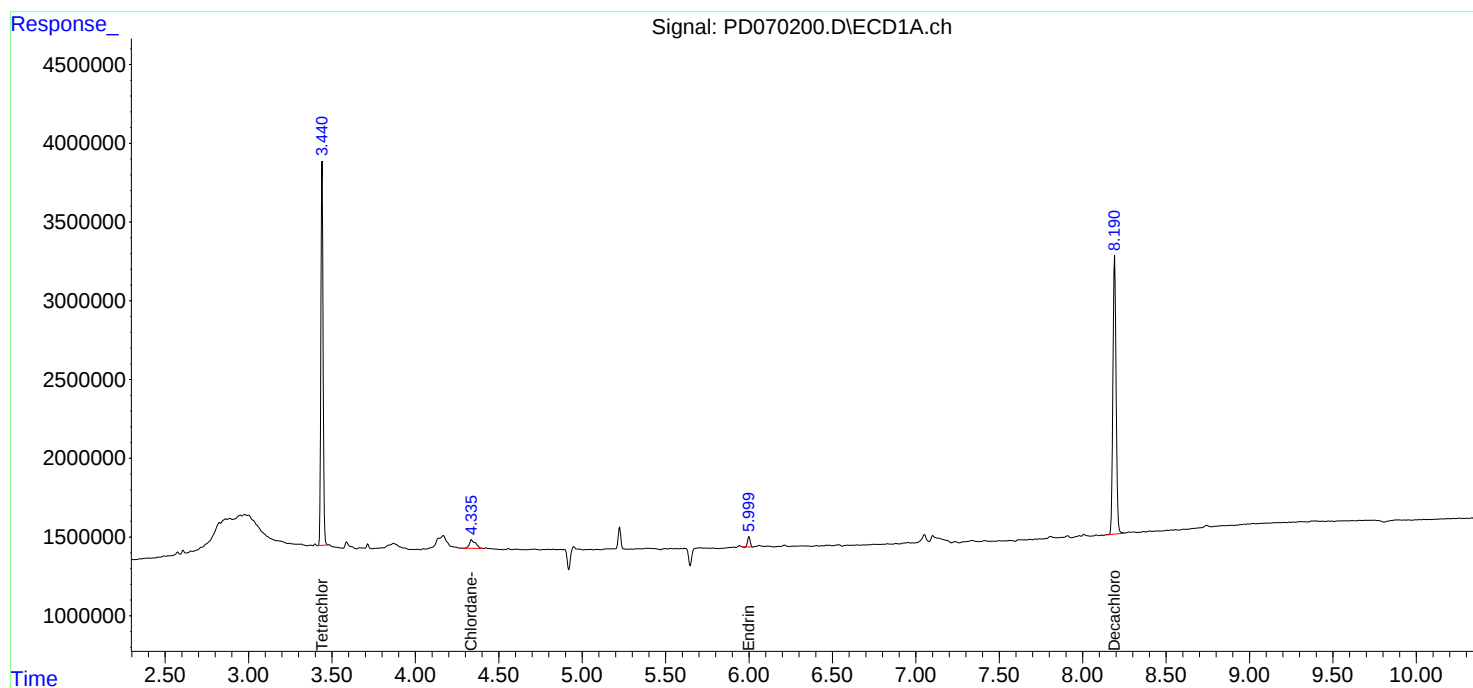


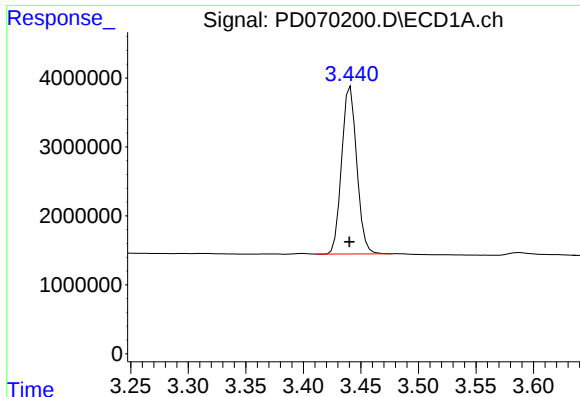

#1 Tetrachloro-m-xylene


R.T.: 3.441 min
Delta R.T.: 0.000 min
Response: 22238993
Conc: 20.48 ng/ml

Instrument :
ECD_D
ClientSampleId :

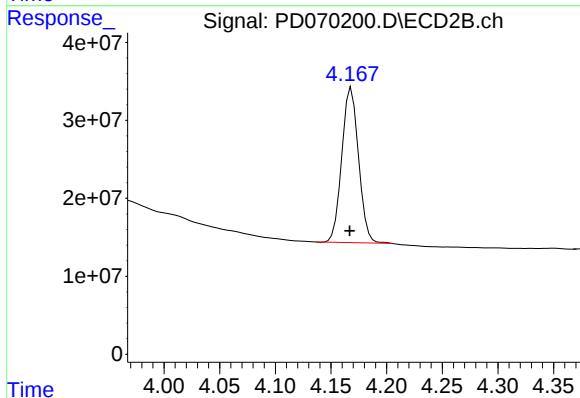


#1 Tetrachloro-m-xylene

R.T.: 4.168 min
Delta R.T.: 0.001 min
Response: 208076655
Conc: 21.32 ng/ml

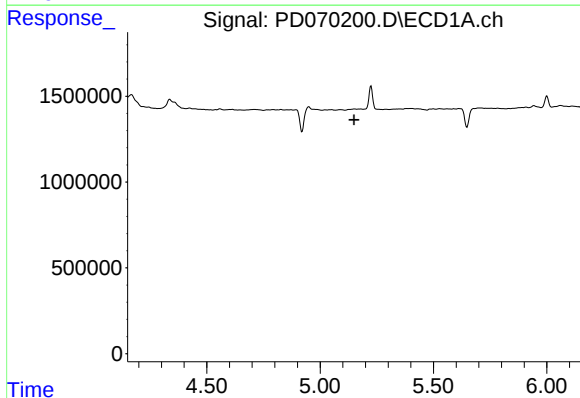


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.149 min
Response: 0
Conc: N.D.

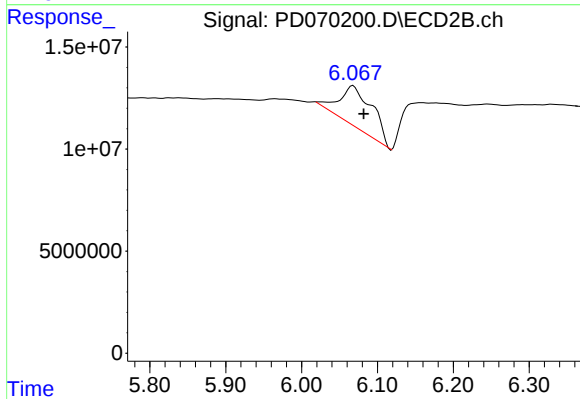

#8 Heptachlor epoxide


R.T.: 6.068 min
Delta R.T.: -0.014 min
Response: 61152510
Conc: 7.42 ng/ml

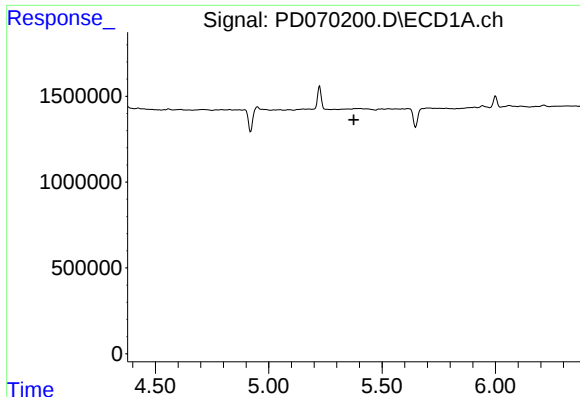

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.375 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

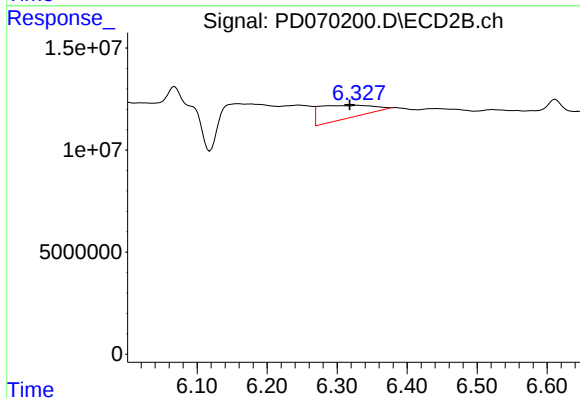


#10 gamma-Chlordane

R.T.: 6.330 min
Delta R.T.: 0.012 min
Response: 33939311
Conc: 2.95 ng/ml

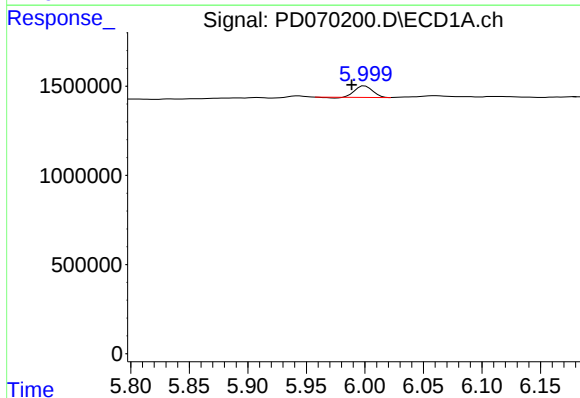


#14 Endrin

R.T.: 6.000 min
Delta R.T.: 0.011 min
Response: 668841
Conc: 0.56 ng/ml

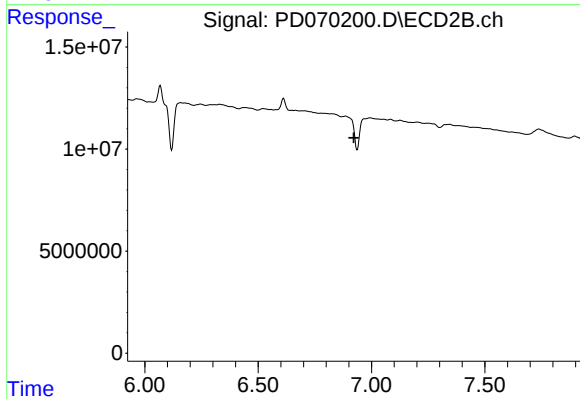

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.922 min
Response: 0
Conc: N.D.

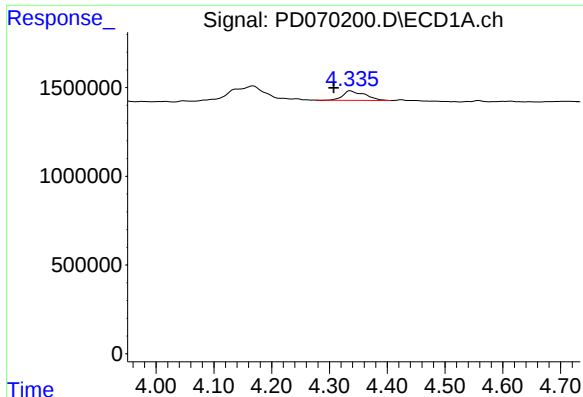

#23 Chlordane-1


R.T.: 4.336 min
Delta R.T.: 0.029 min
Response: 1408176
Conc: 35.34 ng/ml

Instrument :
ECD_D
ClientSampleId :

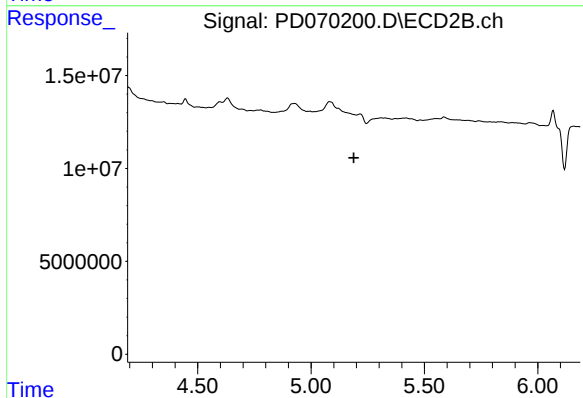


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.189 min
Response: 0
Conc: N.D.

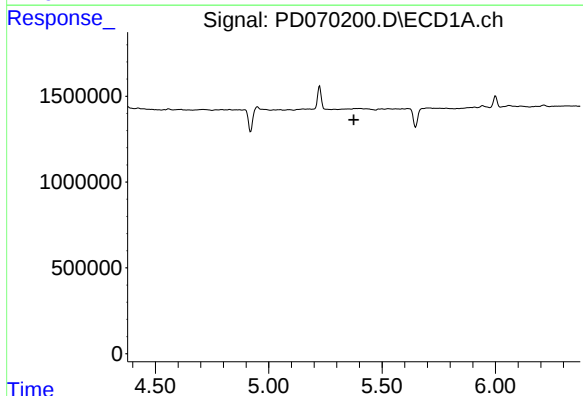


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.375 min
Response: 0
Conc: N.D.

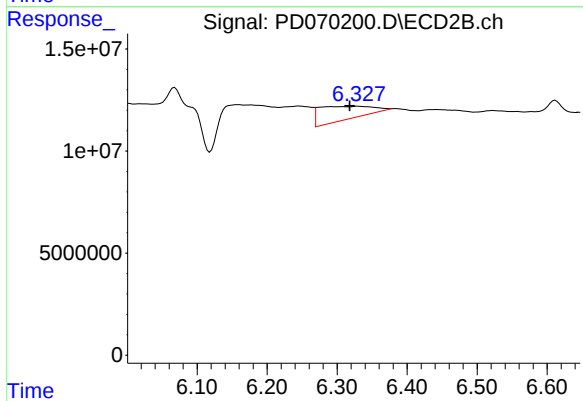

#25 Chlordane-3


R.T.: 6.330 min
Delta R.T.: 0.012 min
Response: 33939311
Conc: 23.16 ng/ml

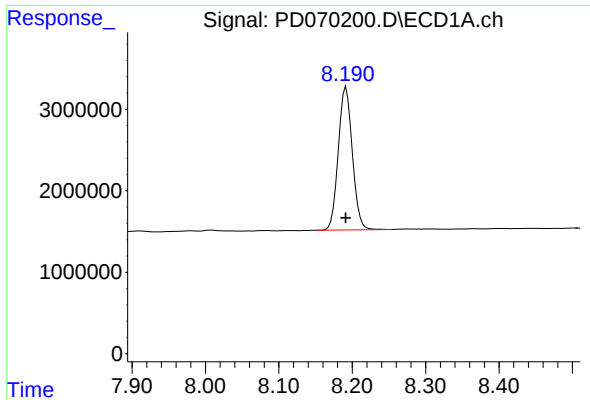

#28 Decachlorobiphenyl

R.T.: 8.192 min
Delta R.T.: 0.000 min
Response: 23317161
Conc: 20.97 ng/ml

Instrument :
ECD_D
ClientSampleId :

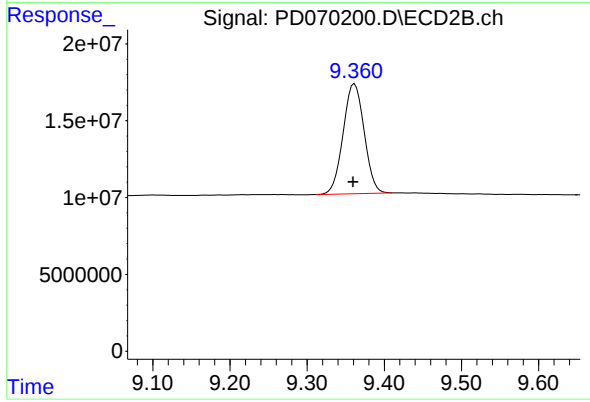

#28 Decachlorobiphenyl

R.T.: 9.361 min
Delta R.T.: 0.002 min
Response: 135427945
Conc: 22.02 ng/ml