

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060822\
 Data File : PD070207.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jun 2022 15:02
 Operator : AR\AJ
 Sample : N3209-07
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 08 23:29:39 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060622.M
 Quant Title : GC Extractables
 QLast Update : Wed Jun 08 02:48:31 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	0.000	4.169	0	53330997	N.D.	5.463 #
28)	SA Decachlor...	8.193	9.364	8523695	51650953	7.664	8.398
Target Compounds							
2)	A alpha-BHC	3.860f	0.000	7748444	0	4.737	N.D. #
5)	MB Aldrin	4.699	5.675f	422.9E6	8112.4E6	287.565	634.181 #
11)	B alpha-Chl...	5.435	0.000	530.2E6	0	382.891	N.D. #
12)	B 4,4'-DDE	0.000	6.543	0	14081428	N.D.	1.343 #
16)	A 4,4'-DDD	0.000	7.036	0	12545501	N.D.	1.492 #
23)	Chlordane-1	0.000	5.196	0	5620617	N.D.	13.908 #
24)	Chlordane-2	0.000	5.675	0	8112.4E6	N.D.	17844.657 #
26)	Chlordane-4	5.435	0.000	530.2E6	0	4899.227	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060822\
Data File : PD070207.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Jun 2022 15:02
Operator : AR\AJ
Sample : N3209-07
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 08 23:29:39 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060622.M
Quant Title : GC Extractables
QLast Update : Wed Jun 08 02:48:31 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

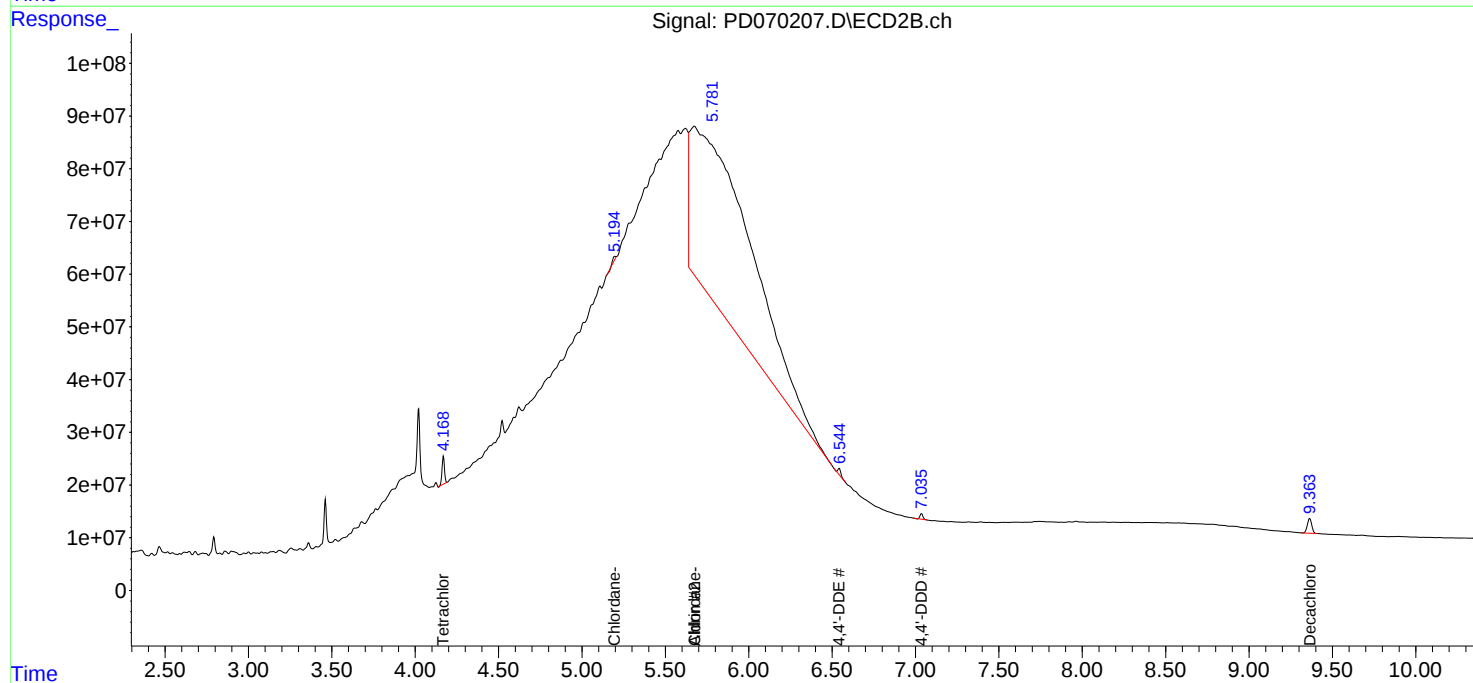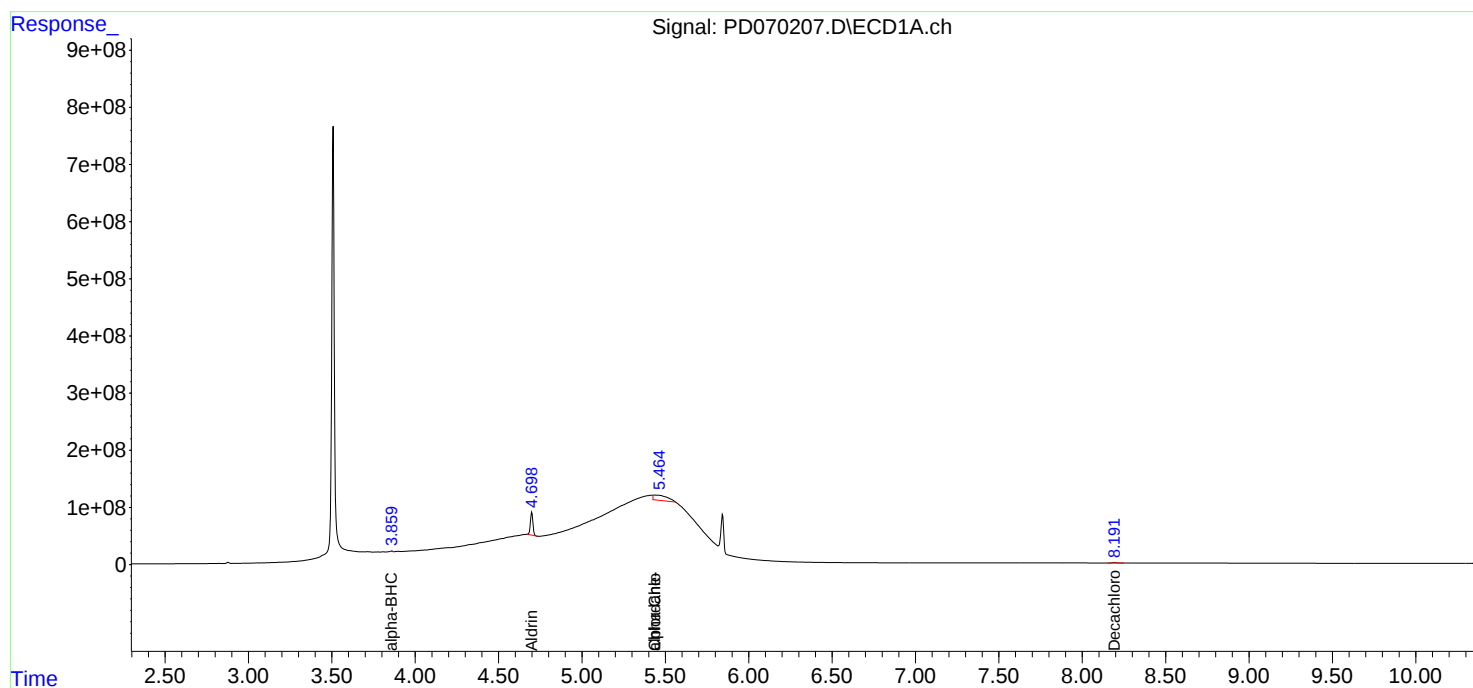


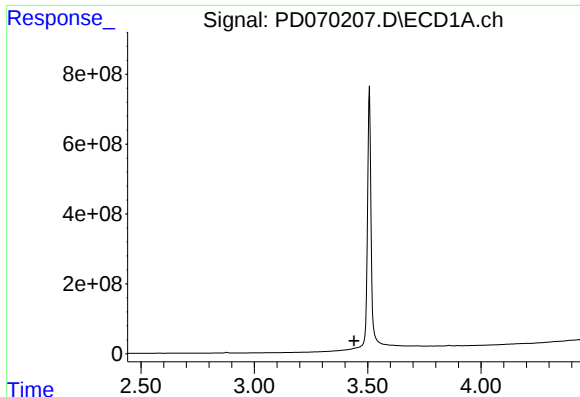

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T.: 3.440 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

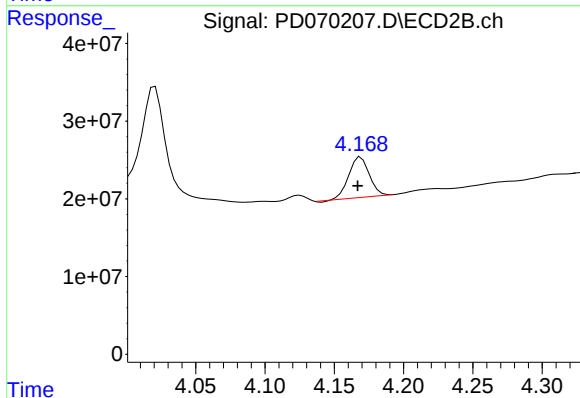


#1 Tetrachloro-m-xylene

R.T.: 4.169 min
Delta R.T.: 0.002 min
Response: 53330997
Conc: 5.46 ng/ml

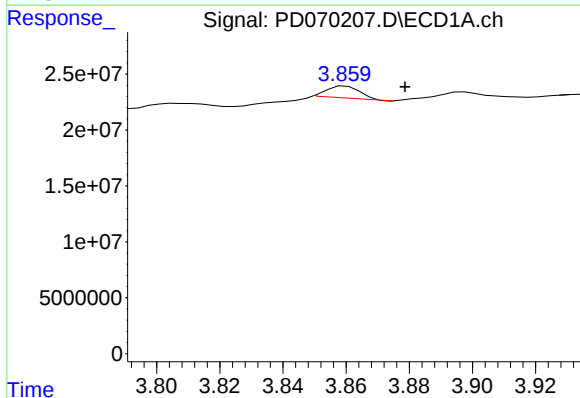


#2 alpha-BHC

R.T.: 3.860 min
Delta R.T.: -0.019 min
Response: 7748444
Conc: 4.74 ng/ml

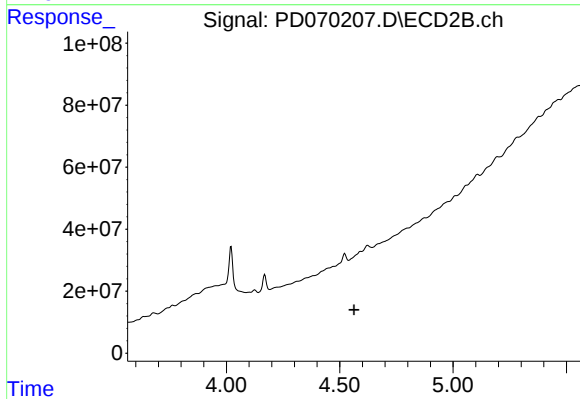

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T.: 4.563 min
Response: 0
Conc: N.D.

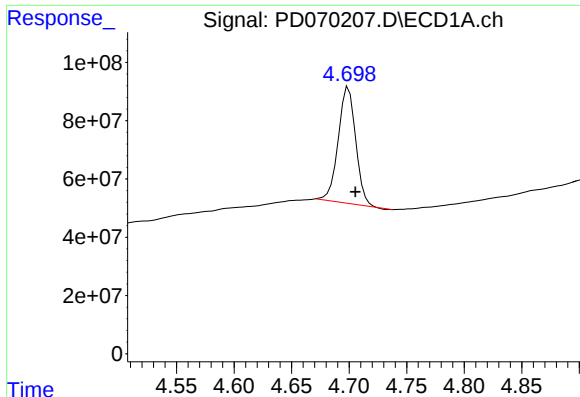

#5 Aldrin


R.T.: 4.699 min
Delta R.T.: -0.006 min
Response: 422919544
Conc: 287.57 ng/ml

Instrument :
ECD_D
ClientSampleId :

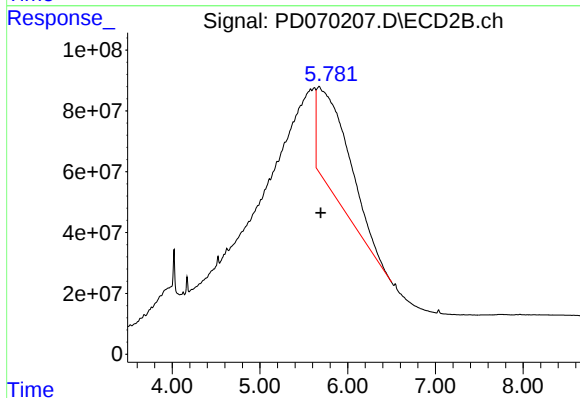


#5 Aldrin

R.T.: 5.675 min
Delta R.T.: -0.018 min
Response: 8112367748
Conc: 634.18 ng/ml

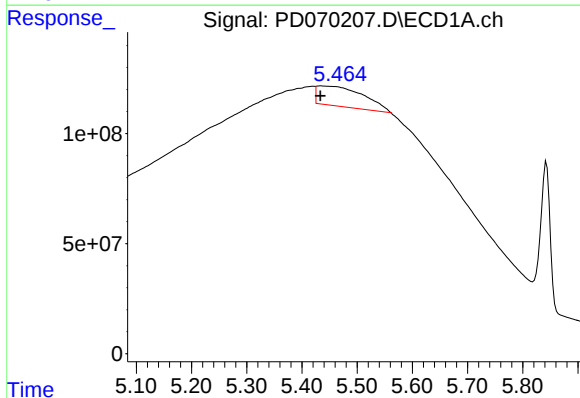


#11 alpha-Chlordane

R.T.: 5.435 min
Delta R.T.: 0.001 min
Response: 530168400
Conc: 382.89 ng/ml

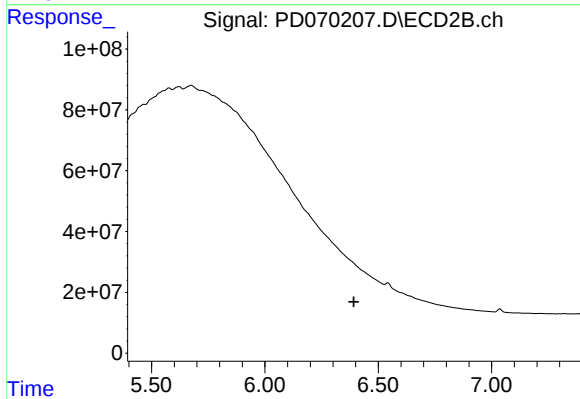

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.393 min
Response: 0
Conc: N.D.

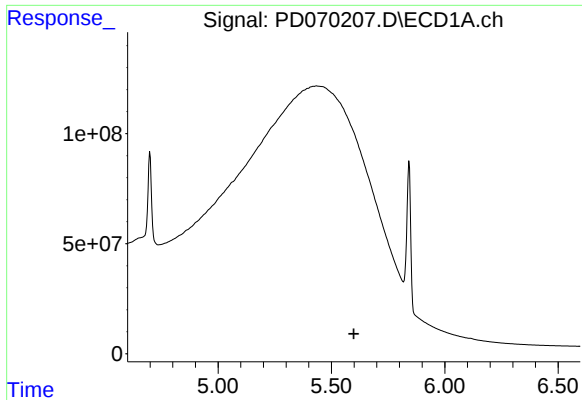

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T.: 5.599 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

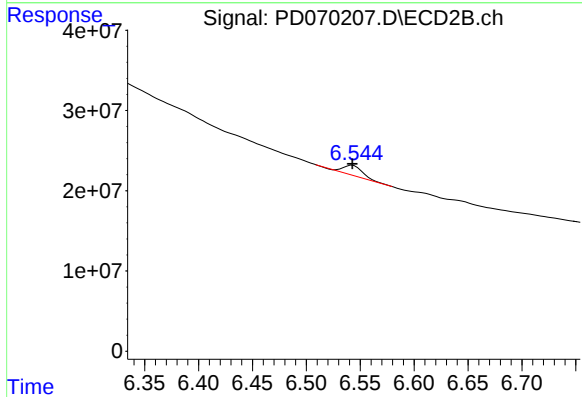


#12 4,4'-DDE

R.T.: 6.543 min
Delta R.T.: 0.000 min
Response: 14081428
Conc: 1.34 ng/ml

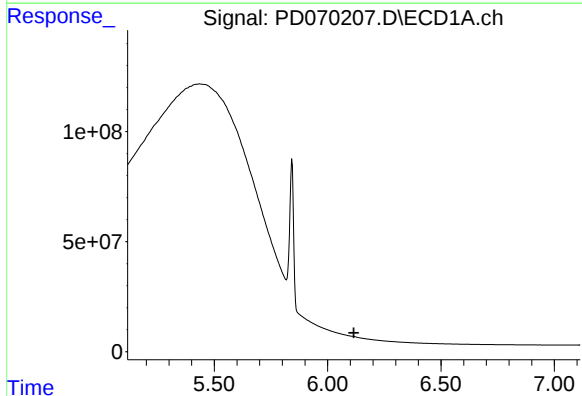


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T.: 6.115 min
Response: 0
Conc: N.D.

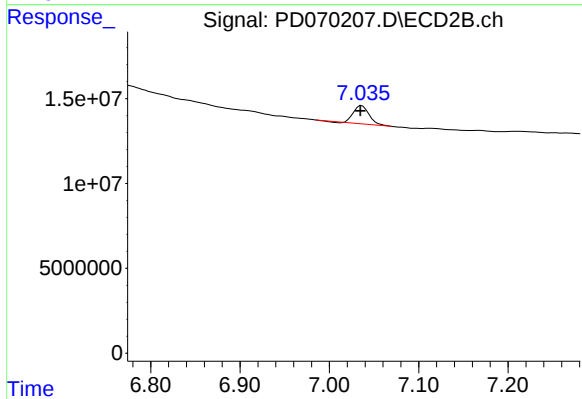

#16 4,4'-DDD


R.T.: 7.036 min
Delta R.T.: 0.002 min
Response: 12545501
Conc: 1.49 ng/ml

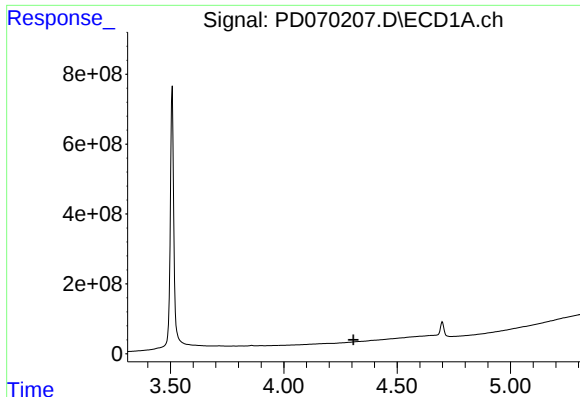

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 4.308 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

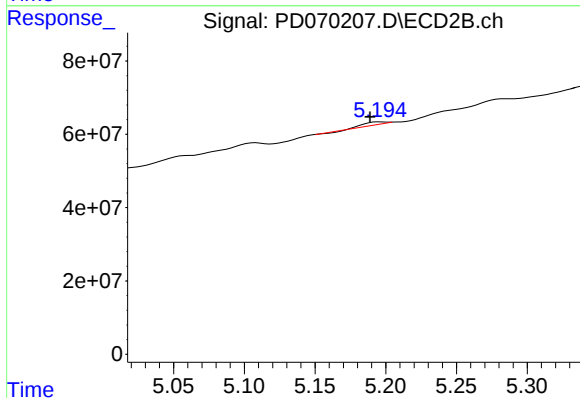


#23 Chlordane-1

R.T.: 5.196 min
Delta R.T.: 0.007 min
Response: 5620617
Conc: 13.91 ng/ml

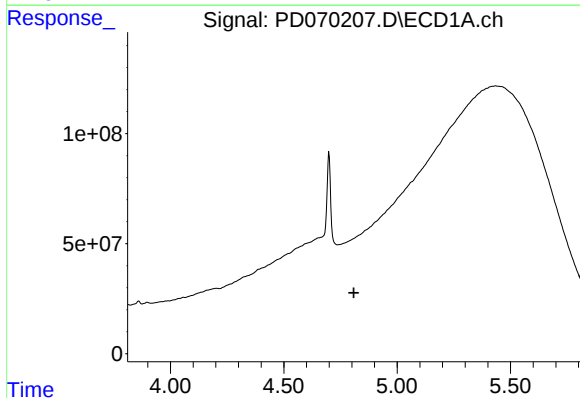


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 4.808 min
Response: 0
Conc: N.D.

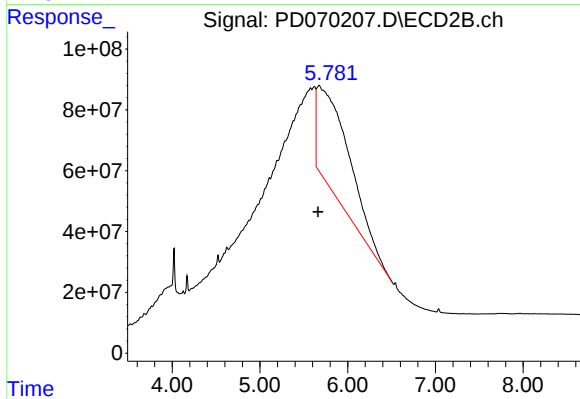

#24 Chlordane-2


R.T.: 5.675 min
Delta R.T.: 0.013 min
Response: 8112367748
Conc: 17844.66 ng/ml

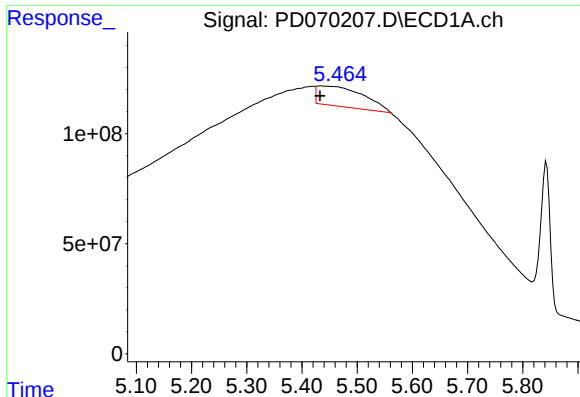

#26 Chlordane-4


R.T.: 5.435 min
Delta R.T.: 0.002 min
Response: 530168400
Conc: 4899.23 ng/m

Instrument :
ECD_D
ClientSampleId :

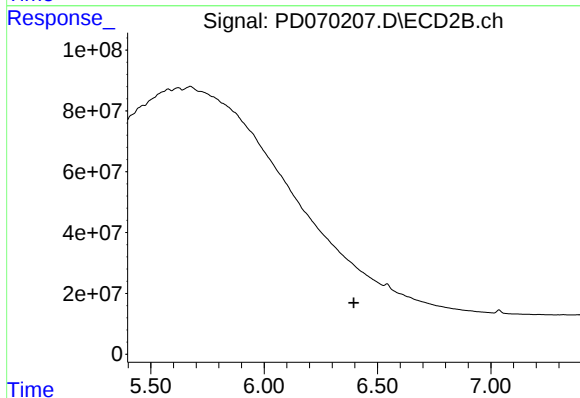


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 6.395 min
Response: 0
Conc: N.D.

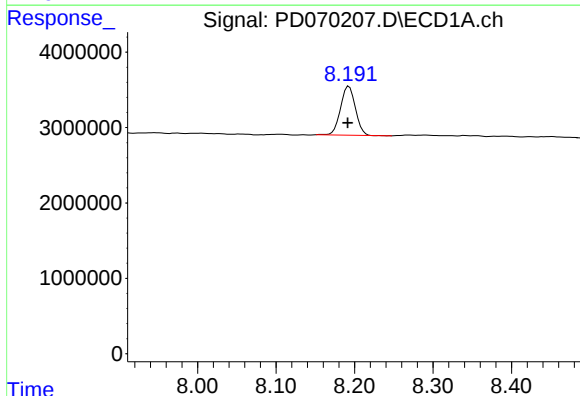

#28 Decachlorobiphenyl

R.T.: 8.193 min
Delta R.T.: 0.002 min
Response: 8523695
Conc: 7.66 ng/ml

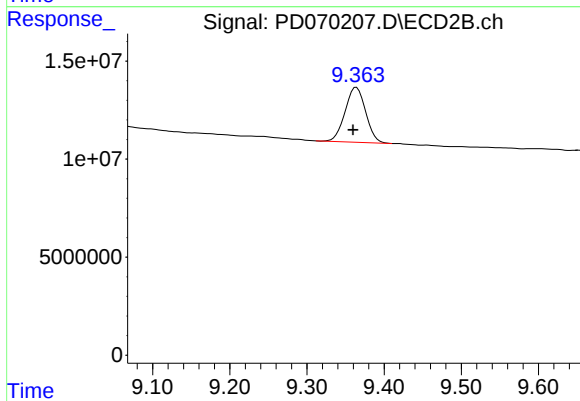

#28 Decachlorobiphenyl

R.T.: 9.364 min
Delta R.T.: 0.004 min
Response: 51650953
Conc: 8.40 ng/ml