

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060822\
 Data File : PD070216.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jun 2022 18:11
 Operator : AR\AJ
 Sample : N3209-06
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 08 23:35:25 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060622.M
 Quant Title : GC Extractables
 QLast Update : Wed Jun 08 02:48:31 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.441	4.170	20788927	197.2E6	19.149	20.206
28)	SA Decachlor...	8.192	9.363	22405090	125.9E6	20.146	20.468
Target Compounds							
10)	B gamma-Chl...	0.000	6.319	0 17525105	N.D.	1.525	#
25)	Chlordane-3	0.000	6.319	0 17525105	N.D.	11.959	#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060822\
Data File : PD070216.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Jun 2022 18:11
Operator : AR\AJ
Sample : N3209-06
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 08 23:35:25 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060622.M
Quant Title : GC Extractables
QLast Update : Wed Jun 08 02:48:31 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

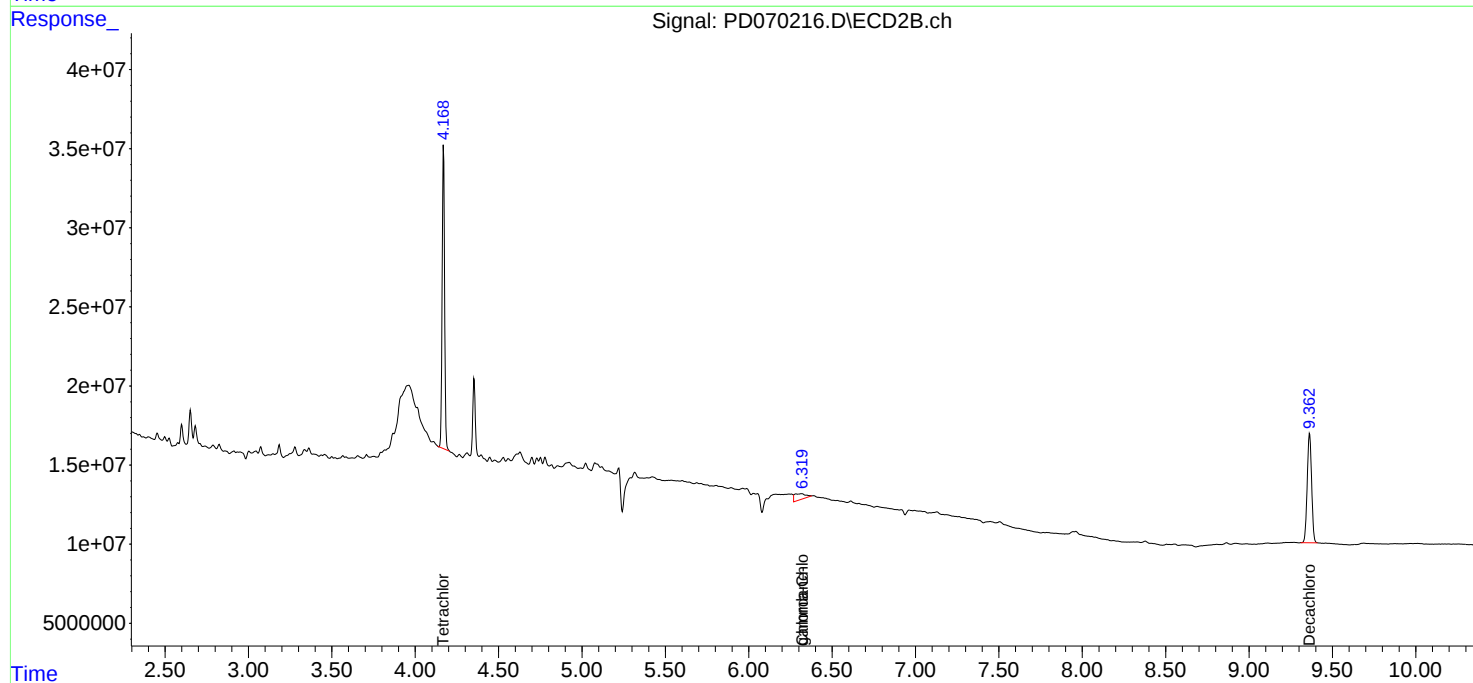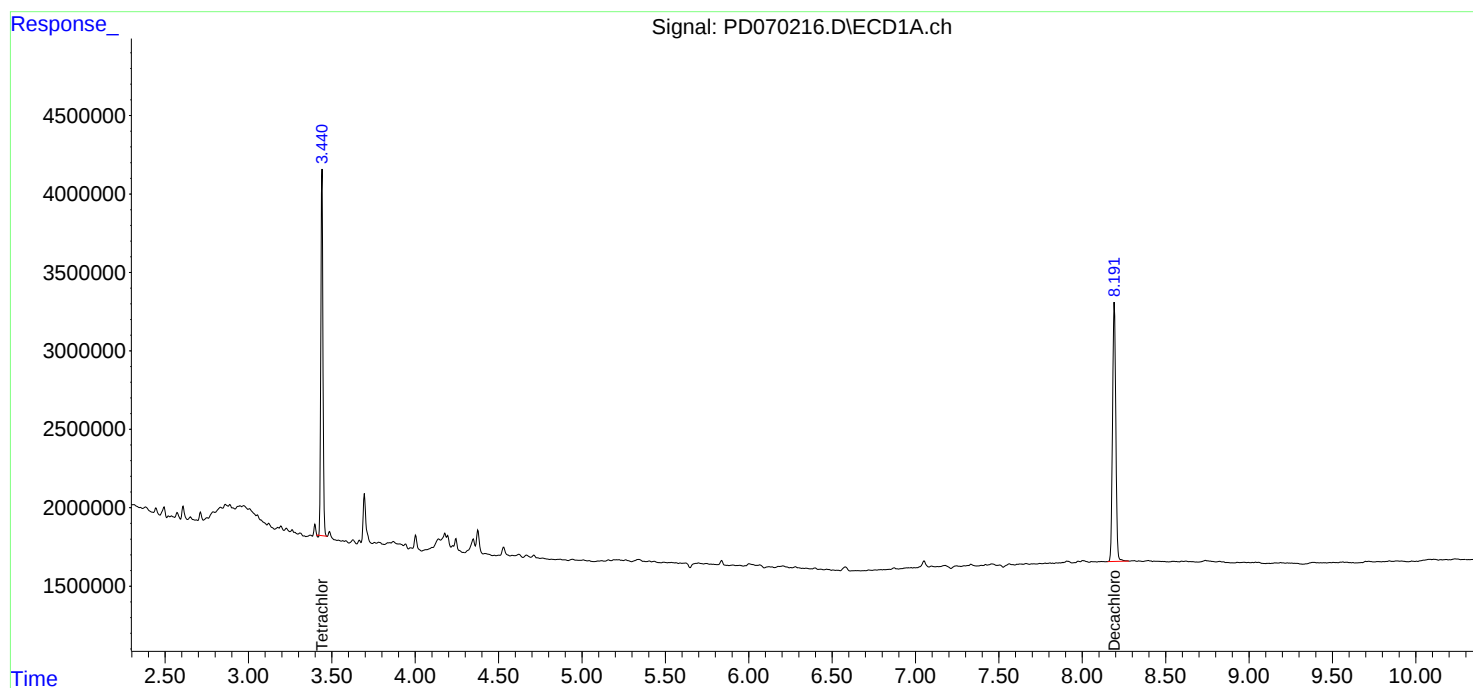


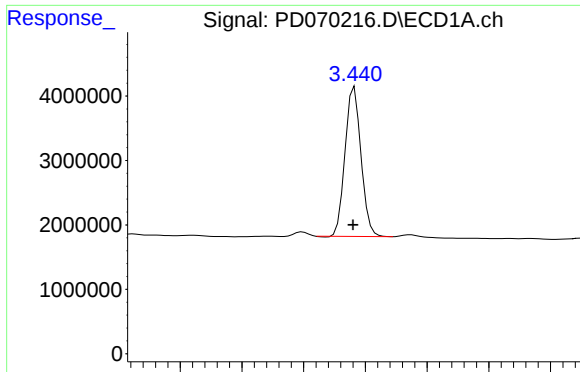

#1 Tetrachloro-m-xylene


R.T.: 3.441 min
Delta R.T.: 0.001 min
Response: 20788927
Conc: 19.15 ng/ml

Instrument :
ECD_D
ClientSampleId :

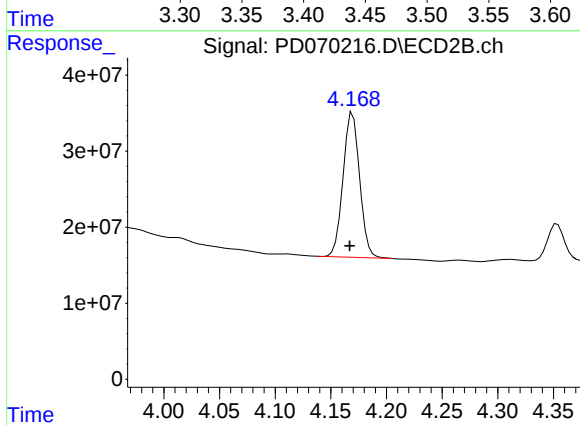


#1 Tetrachloro-m-xylene

R.T.: 4.170 min
Delta R.T.: 0.003 min
Response: 197238976
Conc: 20.21 ng/ml

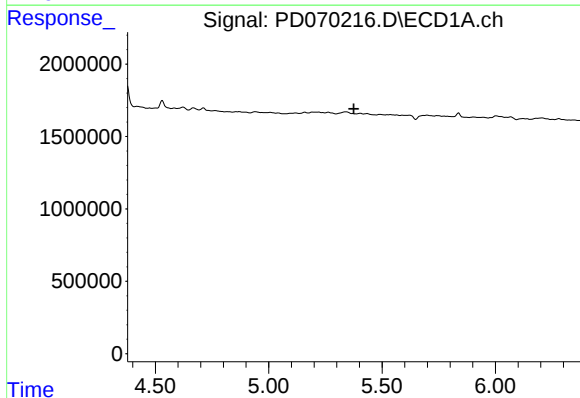


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.375 min
Response: 0
Conc: N.D.

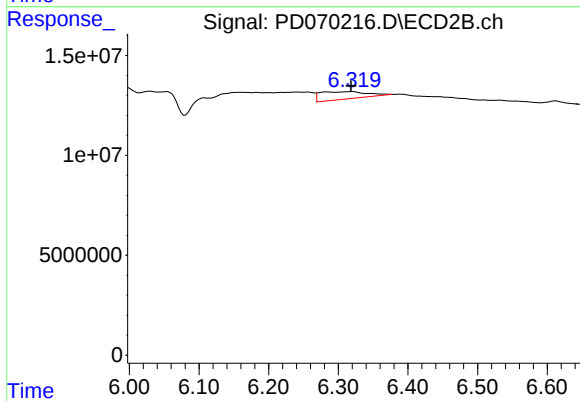

#10 gamma-Chlordane


R.T.: 6.319 min
Delta R.T.: 0.001 min
Response: 17525105
Conc: 1.52 ng/ml

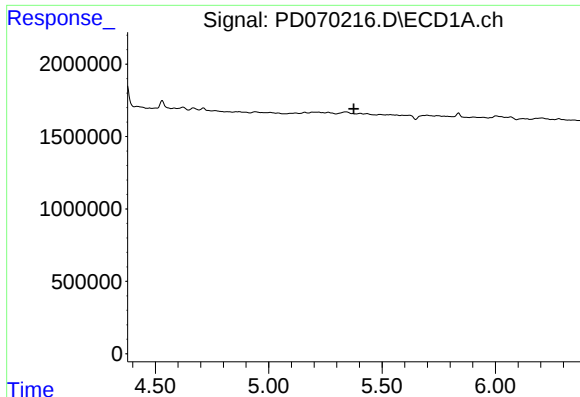

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.375 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

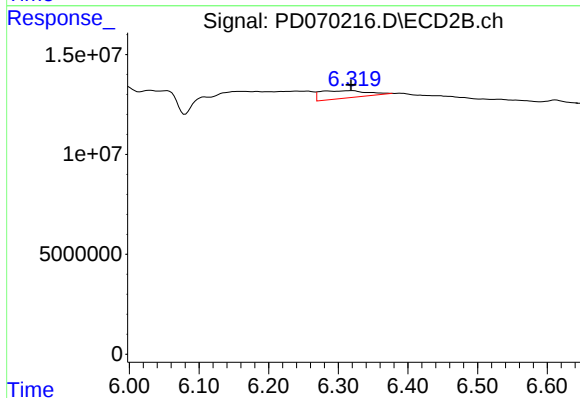


#25 Chlordane-3

R.T.: 6.319 min
Delta R.T.: 0.001 min
Response: 17525105
Conc: 11.96 ng/ml

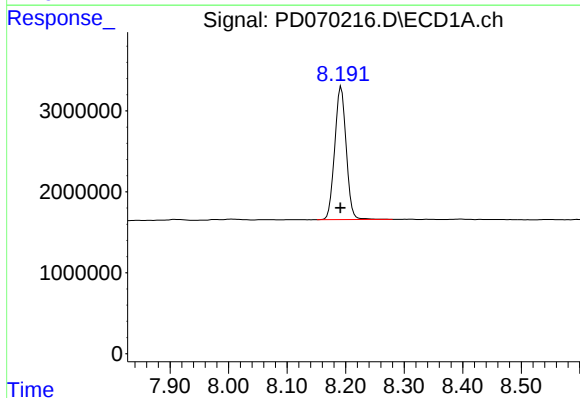

#28 Decachlorobiphenyl

R.T.: 8.192 min
Delta R.T.: 0.001 min
Response: 22405090
Conc: 20.15 ng/ml

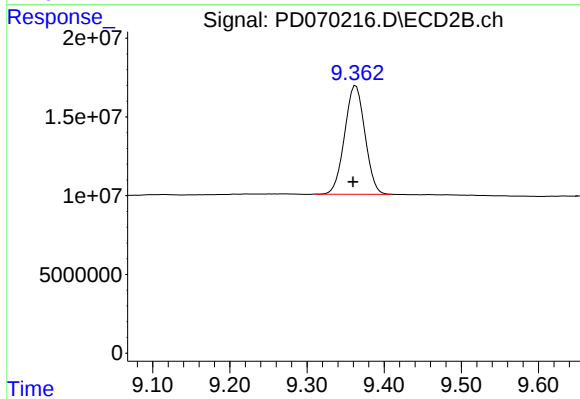

#28 Decachlorobiphenyl

R.T.: 9.363 min
Delta R.T.: 0.004 min
Response: 125891477
Conc: 20.47 ng/ml