

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060824\
 Data File : PD083513.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Jun 2024 13:32
 Operator : AR\AJ
 Sample : P2590-11
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BHBL7

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 06/10/2024
 Supervised By : Ankita Jodhani 06/10/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 07 21:34:26 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060724CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 07 04:03:14 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.562	2.772	4603415	29016934	3.527m	5.323m#
2) SA Decachlor...	9.108	7.900	13668333	60599123	7.029m	9.980 #
Target Compounds						
9) A Endosulfan I	6.139	5.116	29774516	113.7E6	15.225m	17.197m
13) MA Dieldrin	6.403	5.361	11137879	67253696	5.387	9.232m#
16) A 4,4'-DDD	6.733	5.777	15508698	29391727	10.584m	5.214m#
17) MA 4,4'-DDT	7.062	6.024	12571194	52409608	8.345m	9.259m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060824\
Data File : PD083513.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Jun 2024 13:32
Operator : AR\AJ
Sample : P2590-11
Misc :
ALS Vial : 13 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 07 21:34:26 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060724CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jun 07 04:03:14 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

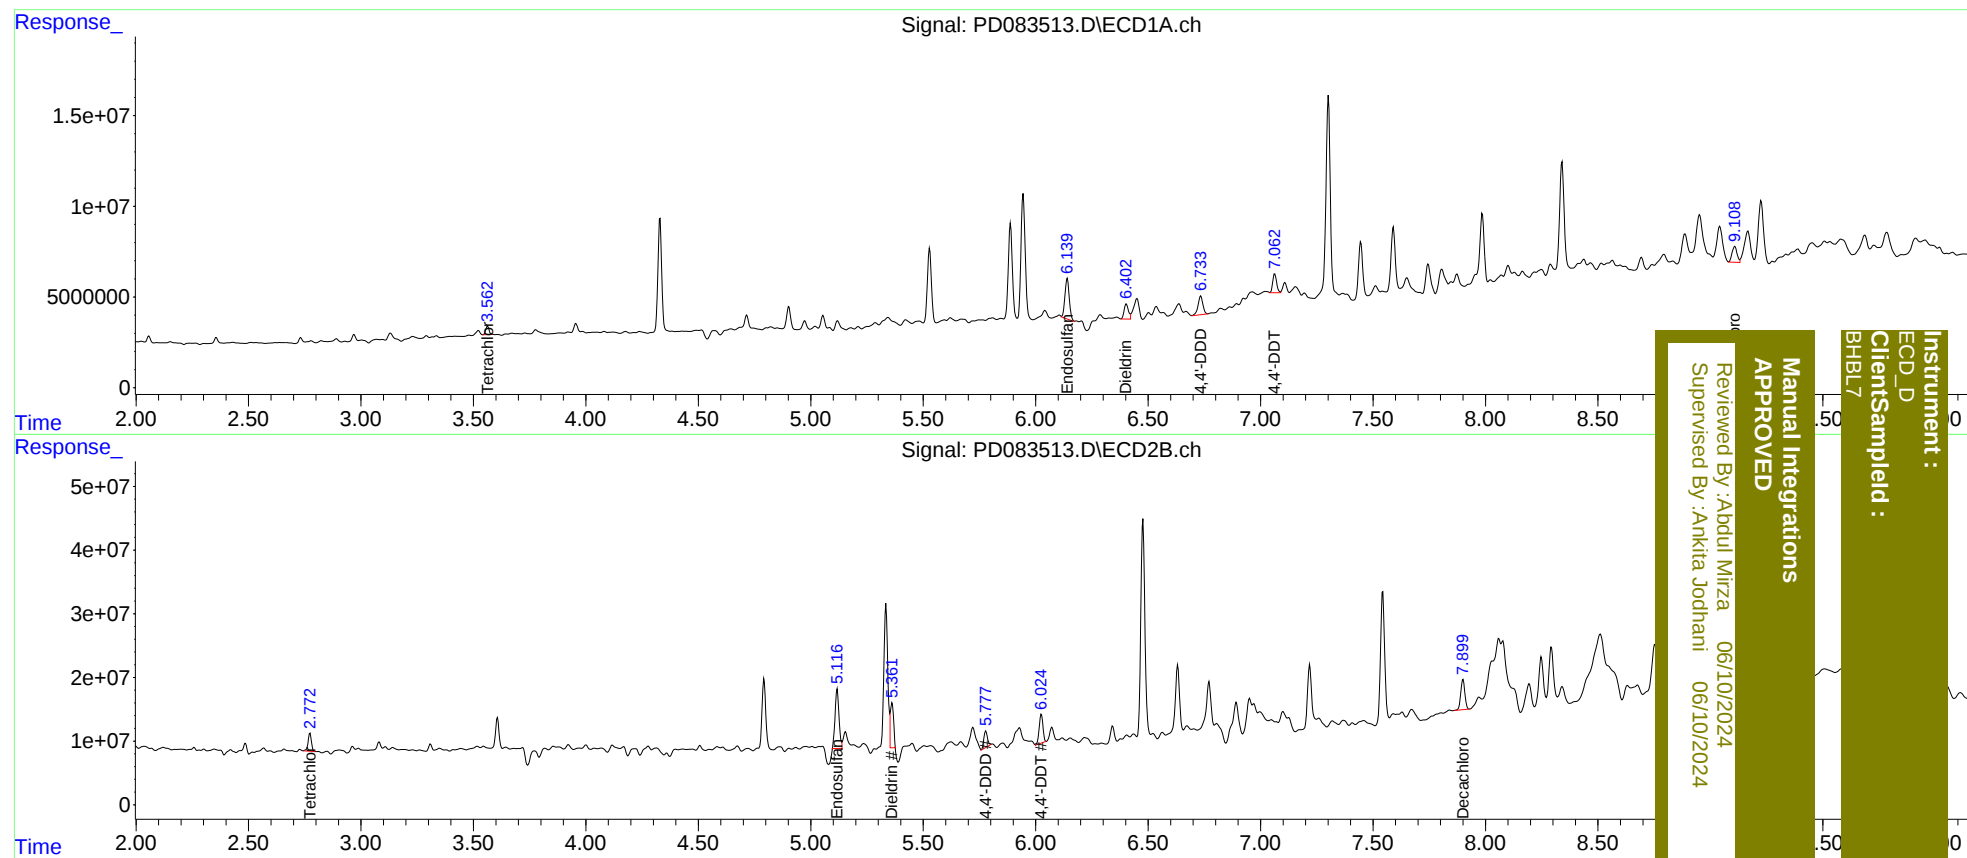

Reviewed By: Abdul Mirza 06/10/2024
Supervised By: Ankita Jodhani 06/10/2024

Manual Integrations
APPROVED

Instrument :
ECD_D
ClientSampled :
BHL7