

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060824\
 Data File : PD083538.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jun 2024 03:34
 Operator : AR\AJ
 Sample : P2634-14DL 10X
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BHBX8DL

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 06/10/2024
 Supervised By :Ankita Jodhani 06/10/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 08 07:40:11 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060724CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 07 04:03:14 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.561	2.773	1059605	7250085	0.812m	1.330 #
2) SA Decachlor...	9.105	7.899	3496025	20342880	1.798m	3.350 #
Target Compounds						
9) A Endosulfan I	6.138	5.115	3349261	16409636	1.713m	2.482m#
13) MA Dieldrin	6.401	5.358	2359222	15448279	1.141m	2.121m#
16) A 4,4'-DDD	6.745	5.774	207.6E6	779.2E6	141.657	138.210
17) MA 4,4'-DDT	7.061	6.022	2579104	11779187	1.712	2.081m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060824\
Data File : PD083538.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Jun 2024 03:34
Operator : AR\AJ
Sample : P2634-14DL 10X
Misc :
ALS Vial : 36 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 08 07:40:11 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060724CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jun 07 04:03:14 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

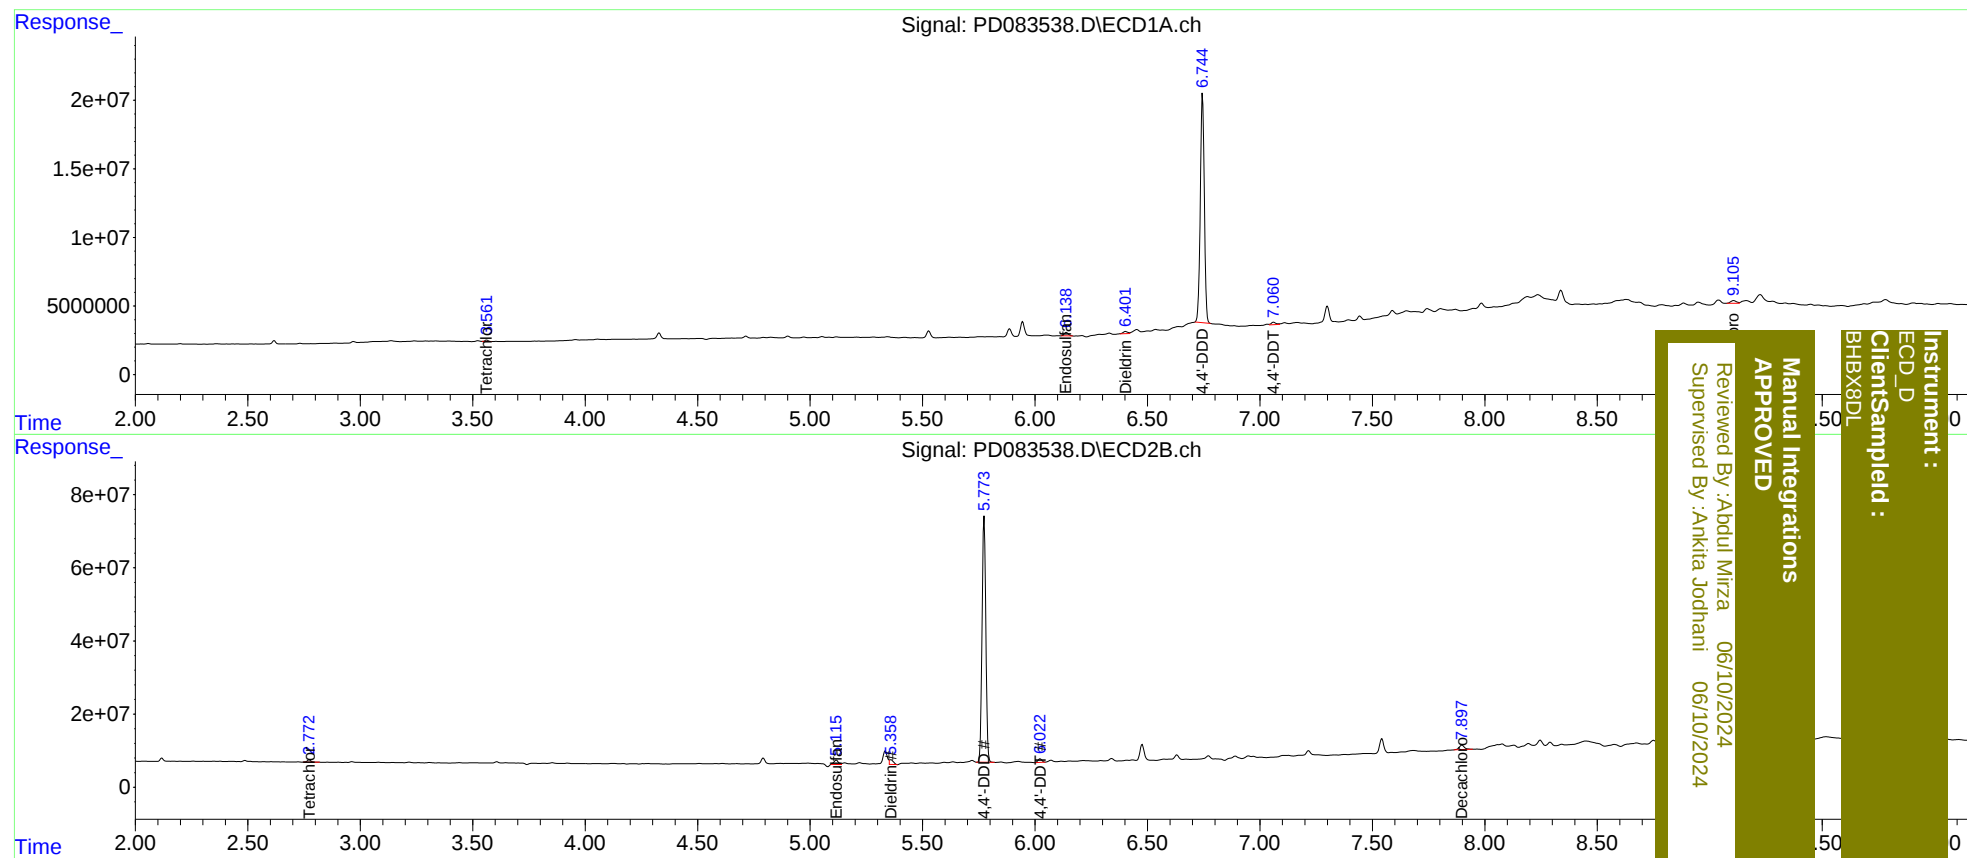

Instrument :
ECD_D
ClientSampled :
BHBX8DL

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 06/10/2024
Supervised By :Ankita Jodhani 06/10/2024