

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060824\
 Data File : PD083548.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jun 2024 07:07
 Operator : AR\AJ
 Sample : P2623-03MSD
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BHBQ8MSD

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 06/10/2024
 Supervised By :Ankita Jodhani 06/10/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 09 05:38:23 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060724CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 07 04:03:14 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.582	2.772	139.9E6	53239373	107.193	9.767m#
27)	SA Decachlor...	9.104	7.898	100.8E6	176.1E6	51.827m	29.005m#
Target Compounds							
2)	A alpha-BHC	4.020	3.271	97979391	360.9E6	44.148	42.331m
3)	MA gamma-BHC...	4.354	3.602	91232444	485.8E6	41.935	62.205m#
4)	MA Heptachlor	4.947	3.937	120.0E6	313.6E6	49.402	40.049m
5)	MB Aldrin	5.290	4.218	108.2E6	371.3E6	45.545	48.050
6)	B beta-BHC	4.553	3.896	36045733	128.5E6	35.767	36.008m
7)	B delta-BHC	4.801	4.125	103.7E6	355.5E6	39.476	41.687m
8)	B Heptachlo...	5.718	4.719	87066463	359.4E6	42.155	49.122
9)	A Endosulfan I	6.105	5.090	92533500	134.1E6	47.317	20.281m#
10)	B trans-Chl...	5.975	4.967	91555856	305.8E6	44.965	42.099m
11)	B cis-Chlor...	6.054	5.031	119.1E6	279.8E6	57.211	38.003m#
12)	B 4,4'-DDE	6.226	5.219	169.3E6	732.8E6	81.615	103.120m#
13)	MA Dieldrin	6.382	5.350	265.2E6	772.7E6	128.273	106.062
14)	MA Endrin	6.611	5.628	157.0E6	646.3E6	92.922m	99.937
15)	B Endosulfa...	6.831	5.920	147.7E6	542.1E6	82.117m	85.437m
16)	A 4,4'-DDD	6.743	5.775	153.3E6	504.8E6	104.592m	89.542
17)	MA 4,4'-DDT	7.061	6.025	261.2E6	815.7E6	173.421	144.094
18)	B Endrin al...	6.963	6.101	107.4E6	390.3E6	80.508	81.470
19)	B Endosulfa...	7.198	6.324	139.3E6	551.4E6	81.428	89.254
20)	A Methoxychlor	7.538	6.600	365.6E6	996.9E6	422.557	342.993
21)	B Endrin ke...	7.685	6.828	163.7E6	459.0E6	87.808	68.272

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060824\
Data File : PD083548.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Jun 2024 07:07
Operator : AR\AJ
Sample : P2623-03MSD
Misc :
ALS Vial : 41 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 09 05:38:23 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060724CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jun 07 04:03:14 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

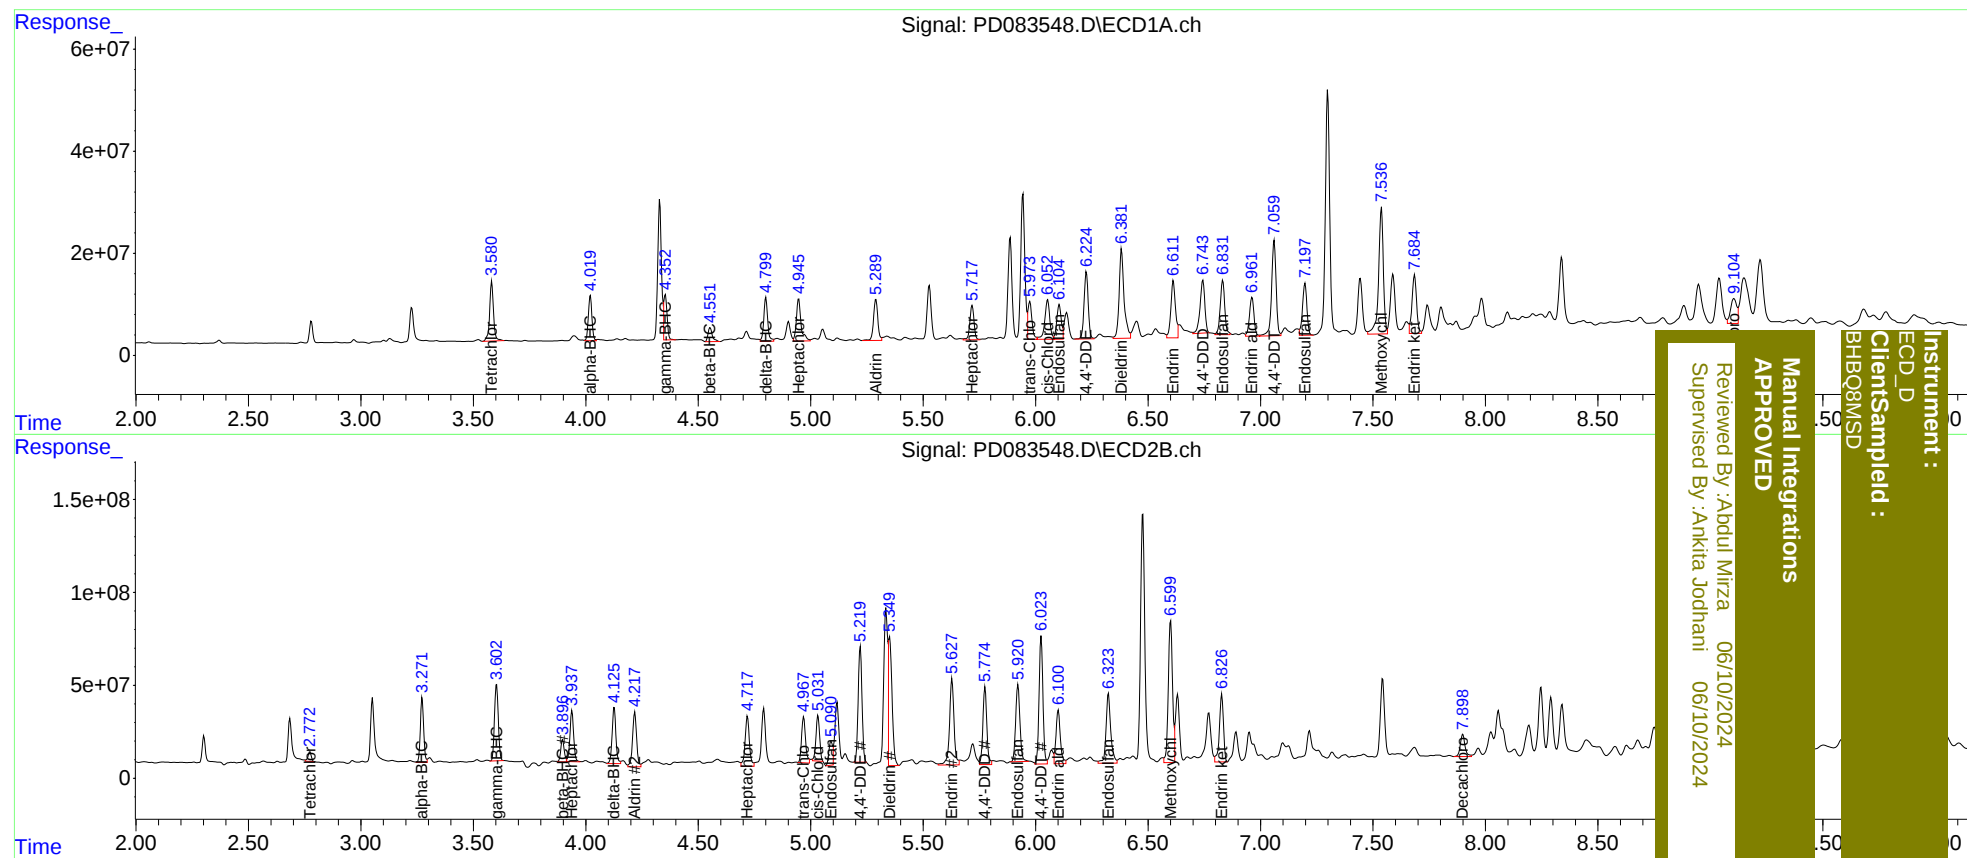

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 06/10/2024
Supervised By: Ankita Jodhani 06/10/2024

Instrument :
ECD_D
Client Sampled :
BHB08MSD