

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060921\
 Data File : PD063680.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Jun 2021 15:45
 Operator : AR\AJ
 Sample : M2647-01
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 SU-01-060821

Manual Integrations
 APPROVED

Ankita
 6/10/2021 3:19:46 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 10 07:32:33 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060221.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 03 01:33:41 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.439	3.969	9451444	79286669	6.830	5.918m
28) SA Decachlor...	8.195	9.026	8874998	88308872	5.643	6.391
Target Compounds						
12) B 4,4'-DDE	5.597	6.297	1936151	25019279	1.114m	1.377m
17) MA 4,4'-DDT	6.355	7.093	1444681	14337493	1.000m	0.953

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060921\
Data File : PD063680.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Jun 2021 15:45
Operator : AR\AJ
Sample : M2647-01
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
SU-01-060821


Manual Integrations
APPROVED

Ankita
6/10/2021 3:19:46 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 10 07:32:33 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060221.M
Quant Title : GC Extractables
QLast Update : Thu Jun 03 01:33:41 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

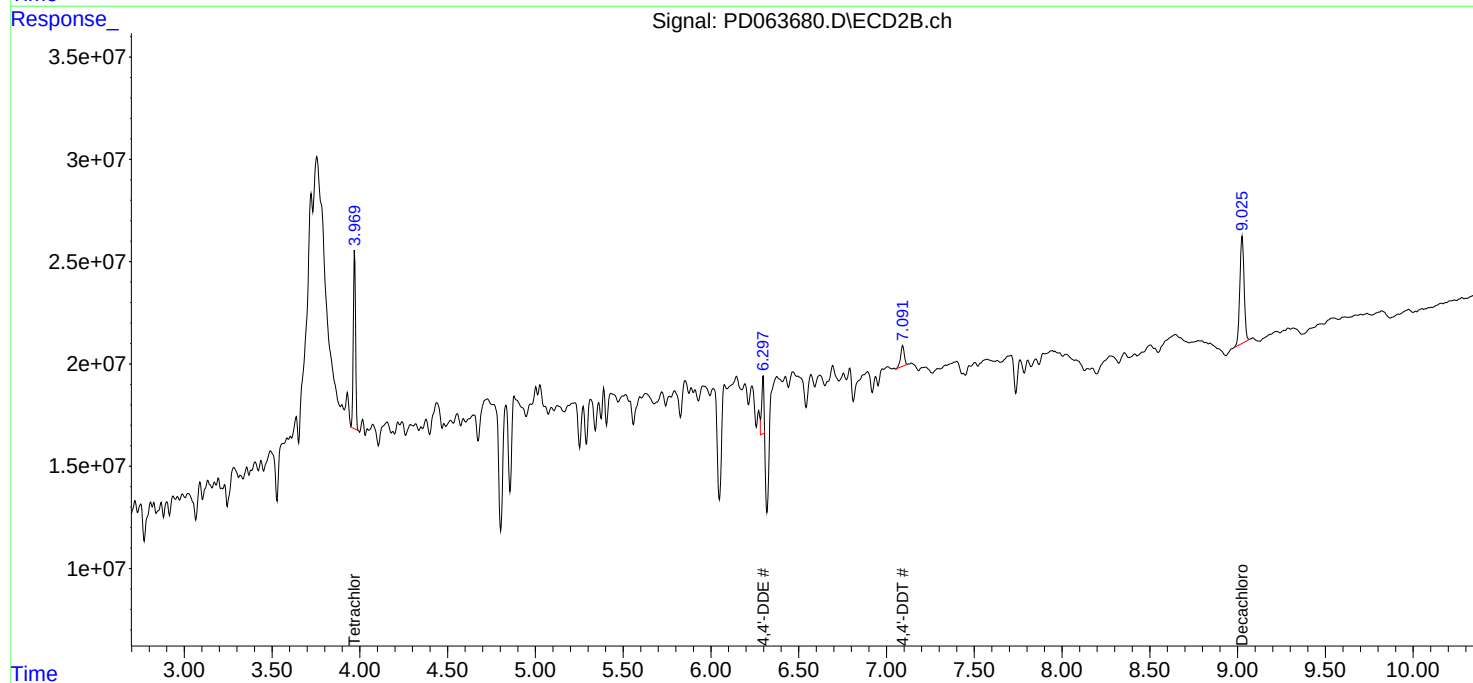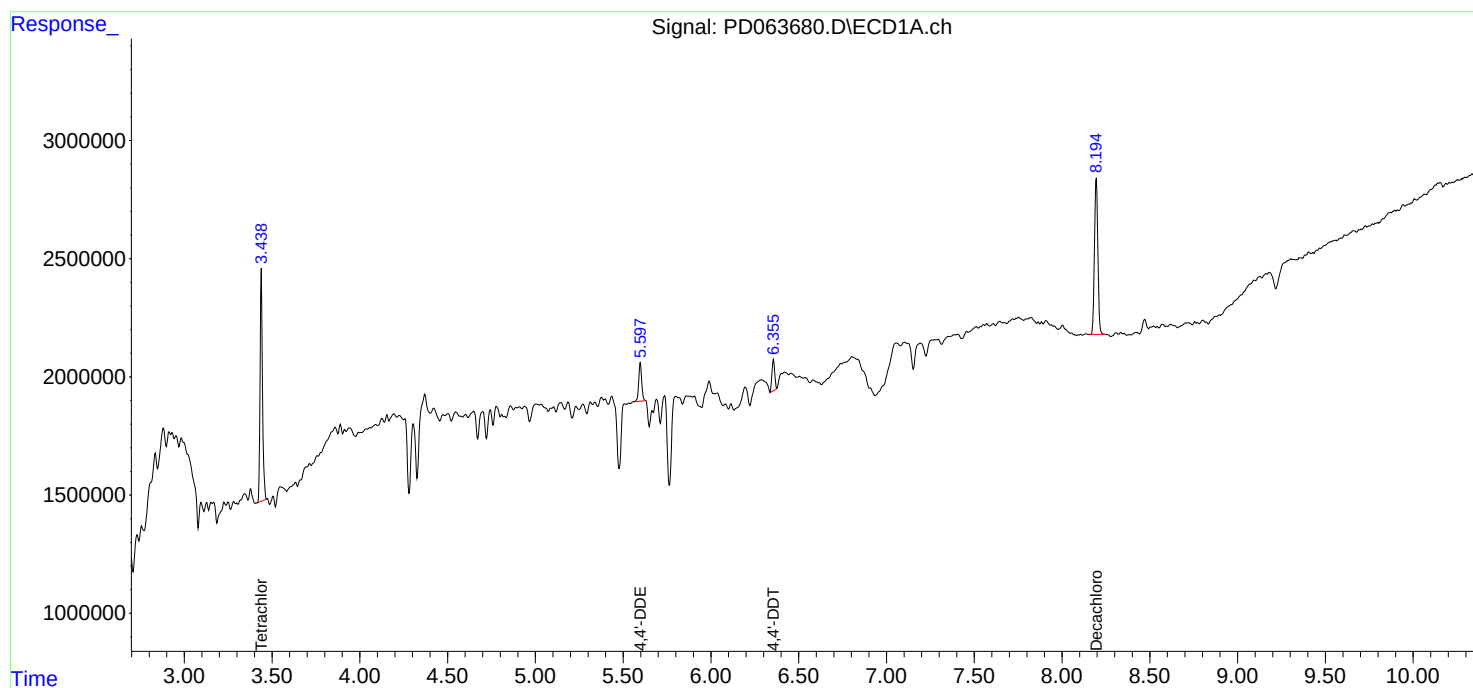

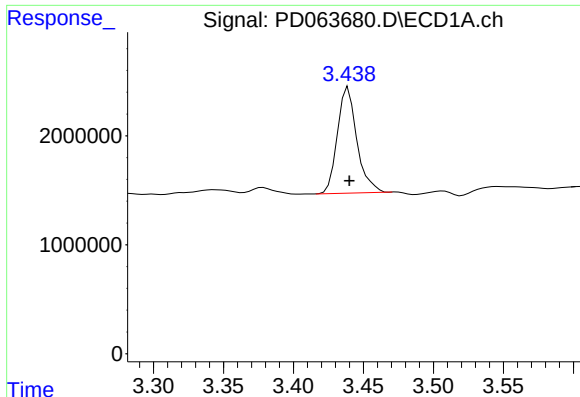


#1 Tetrachloro-m-xylene

R.T.: 3.439 min
Delta R.T.: 0.000 min
Response: 9451444
Conc: 6.83 ng/ml

Instrument :
ECD_D
ClientSampleId :
SU-01-060821


Manual Integrations
APPROVED

Ankita
6/10/2021 3:19:46 PM

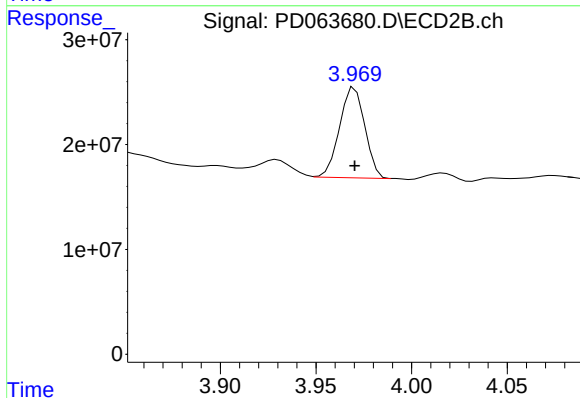


#1 Tetrachloro-m-xylene

R.T.: 3.969 min
Delta R.T.: -0.001 min
Response: 79286669
Conc: 5.92 ng/ml m

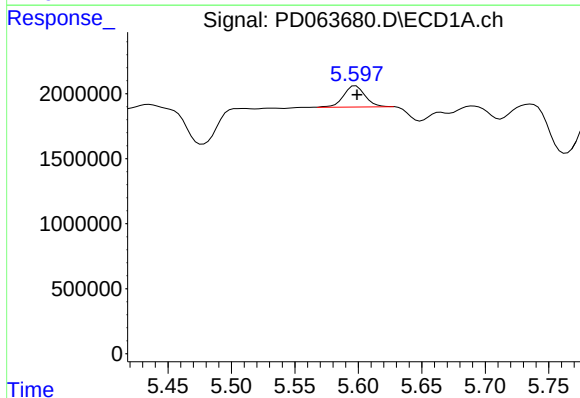


#12 4,4'-DDE

R.T.: 5.597 min
Delta R.T.: -0.002 min
Response: 1936151
Conc: 1.11 ng/ml m

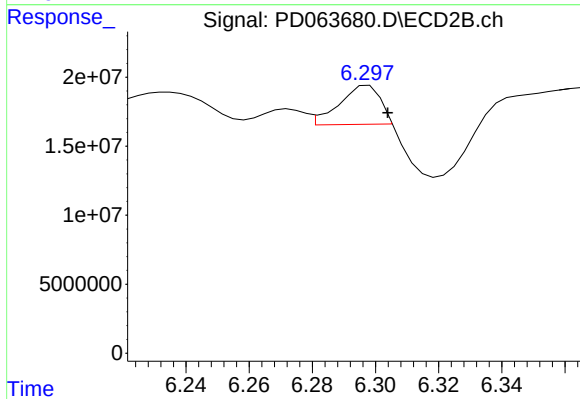

#12 4,4'-DDE

R.T.: 6.297 min
Delta R.T.: -0.007 min
Response: 25019279
Conc: 1.38 ng/ml m

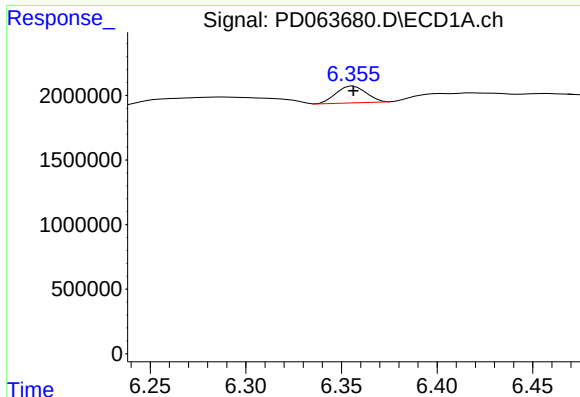


#17 4,4'-DDT

R.T.: 6.355 min
Delta R.T.: -0.001 min
Response: 1444681
Conc: 1.00 ng/ml m

Instrument :
ECD_D
ClientSampleId :
SU-01-060821


Manual Integrations
APPROVED

Ankita
6/10/2021 3:19:46 PM

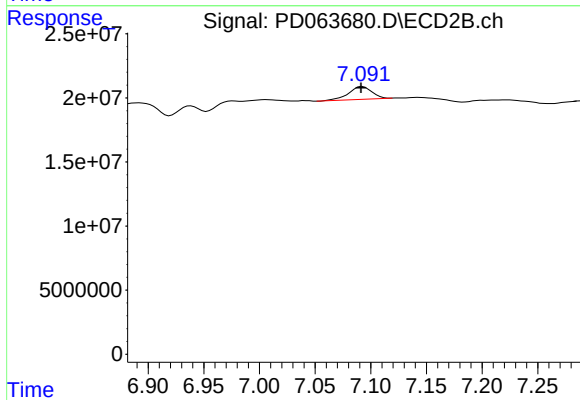


#17 4,4'-DDT

R.T.: 7.093 min
Delta R.T.: 0.001 min
Response: 14337493
Conc: 0.95 ng/ml

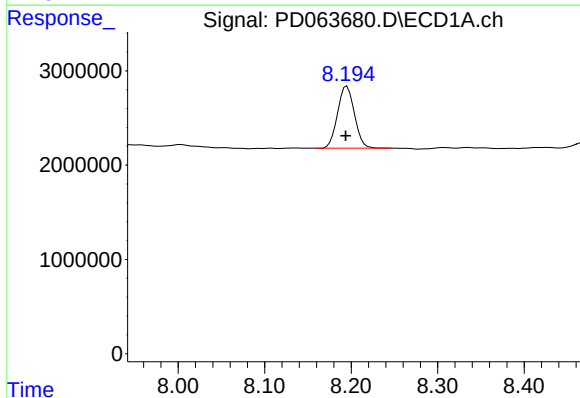

#28 Decachlorobiphenyl

R.T.: 8.195 min
Delta R.T.: 0.001 min
Response: 8874998
Conc: 5.64 ng/ml

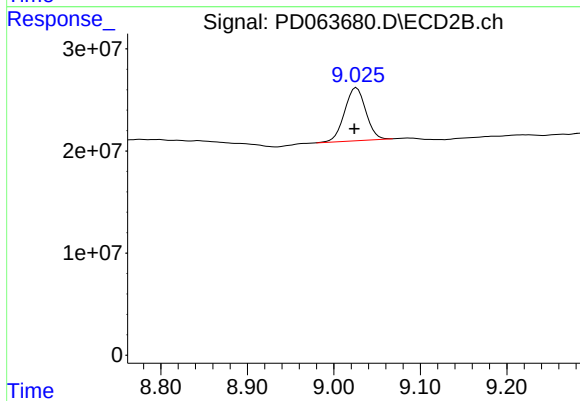

#28 Decachlorobiphenyl

R.T.: 9.026 min
Delta R.T.: 0.002 min
Response: 88308872
Conc: 6.39 ng/ml