

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060921\
 Data File : PD063702.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Jun 2021 21:44
 Operator : AR\AJ
 Sample : M2651-02
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 17-B2(0-5)

Manual Integrations
 APPROVED

Ankita
 6/10/2021 3:19:50 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 10 07:42:27 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060221.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 03 01:33:41 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.439	3.971	16915618	180.5E6	12.225	13.471
28)	SA Decachlor...	8.194	9.025	18029437	161.8E6	11.464	11.709
Target Compounds							
11)	B alpha-Chl...	5.436	6.148	2006620	17556858	1.135m	0.988
12)	B 4,4'-DDE	5.597	6.299	1178045	28619967	0.678m	1.575m#
14)	MA Endrin	5.984	6.663	1365179	41327668	0.858m	2.689 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060921\
Data File : PD063702.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Jun 2021 21:44
Operator : AR\AJ
Sample : M2651-02
Misc :
ALS Vial : 32 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
17-B2(0-5)


Manual Integrations
APPROVED

Ankita
6/10/2021 3:19:50 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 10 07:42:27 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060221.M
Quant Title : GC Extractables
QLast Update : Thu Jun 03 01:33:41 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

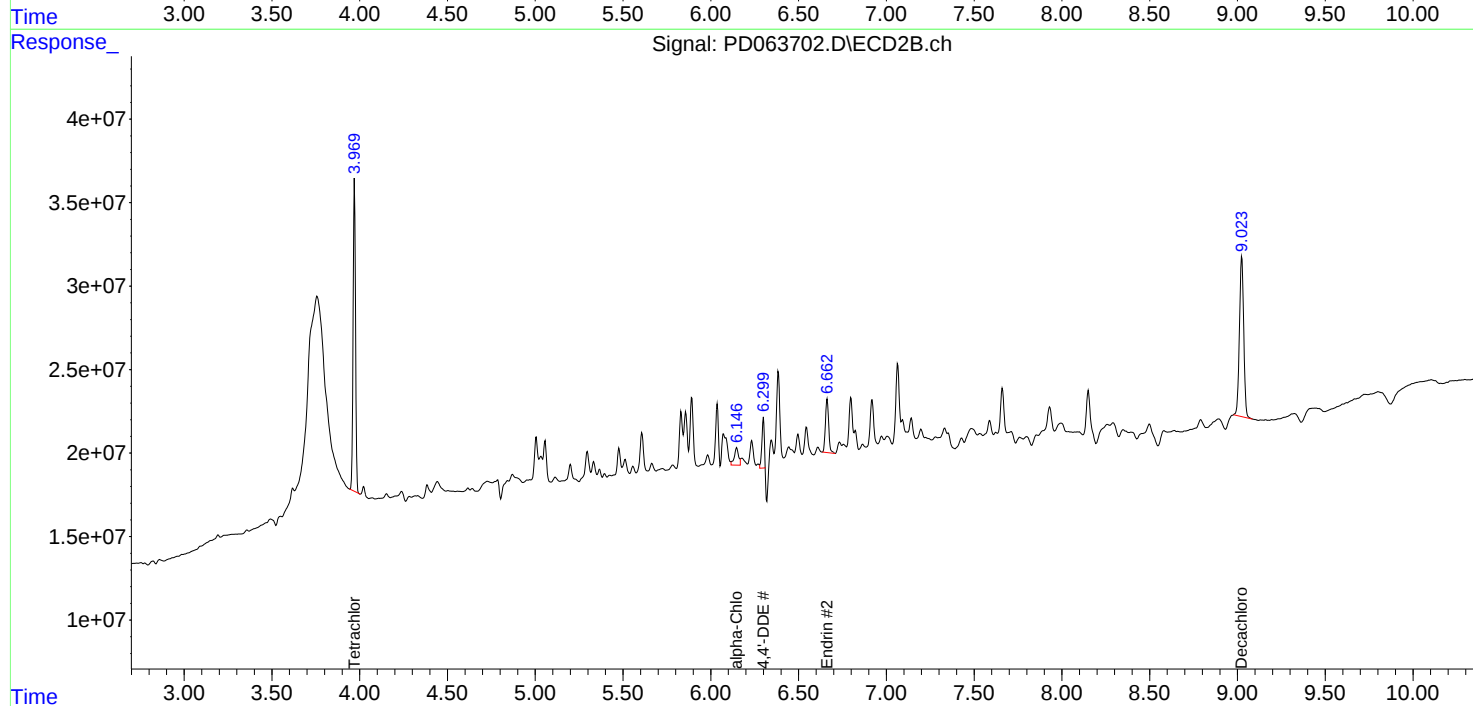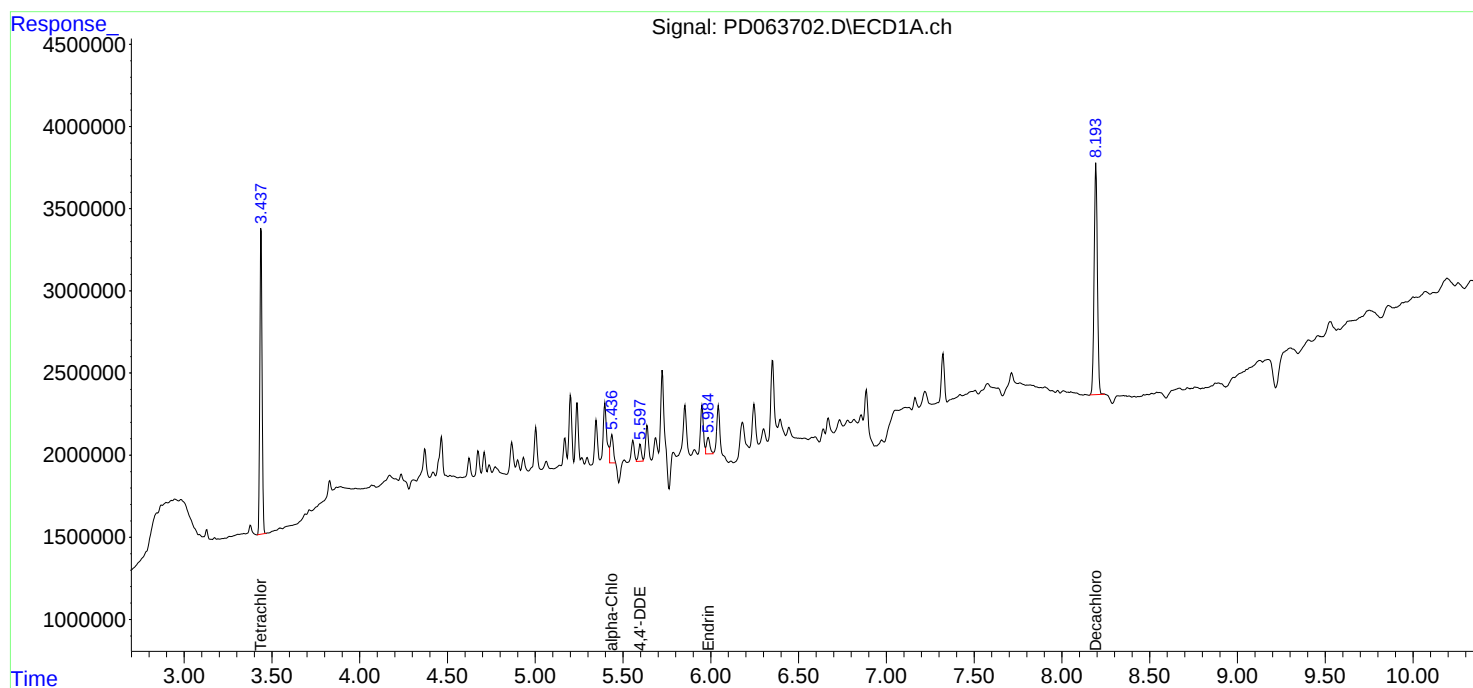

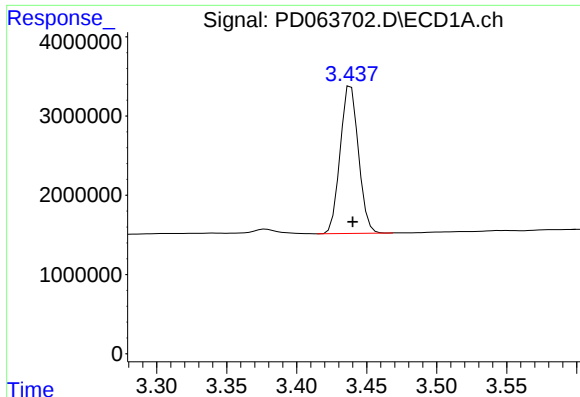


#1 Tetrachloro-m-xylene

R.T.: 3.439 min
Delta R.T.: -0.001 min
Response: 16915618
Conc: 12.22 ng/ml

Instrument :
ECD_D
ClientSampleId :
17-B2(0-5)


Manual Integrations
APPROVED

Ankita
6/10/2021 3:19:50 PM

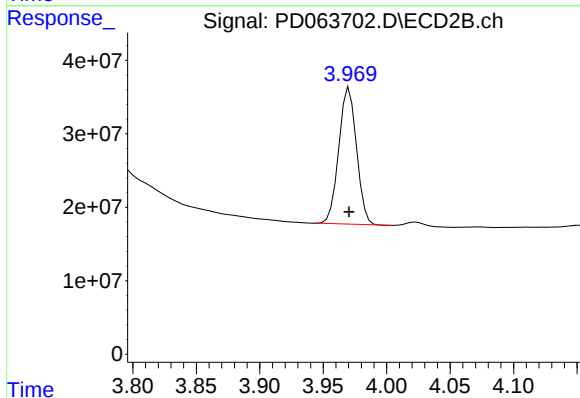


#1 Tetrachloro-m-xylene

R.T.: 3.971 min
Delta R.T.: 0.000 min
Response: 180491775
Conc: 13.47 ng/ml

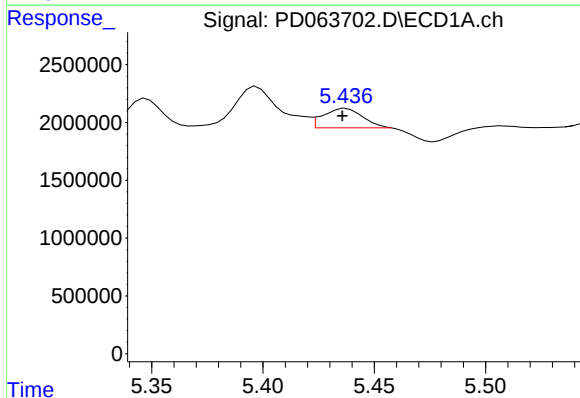


#11 alpha-Chlordane

R.T.: 5.436 min
Delta R.T.: 0.000 min
Response: 2006620
Conc: 1.13 ng/ml m

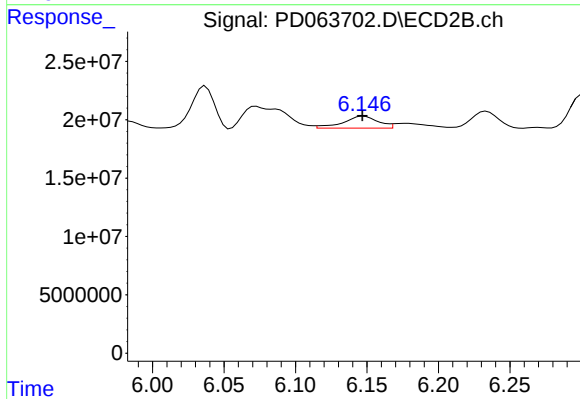

#11 alpha-Chlordane

R.T.: 6.148 min
Delta R.T.: 0.001 min
Response: 17556858
Conc: 0.99 ng/ml

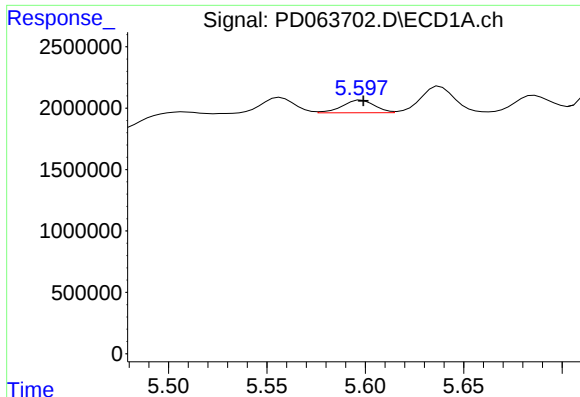


#12 4,4'-DDE

R.T.: 5.597 min
Delta R.T.: -0.002 min
Response: 1178045
Conc: 0.68 ng/ml m

Instrument :
ECD_D
ClientSampleId :
17-B2(0-5)


Manual Integrations
APPROVED

Ankita
6/10/2021 3:19:50 PM

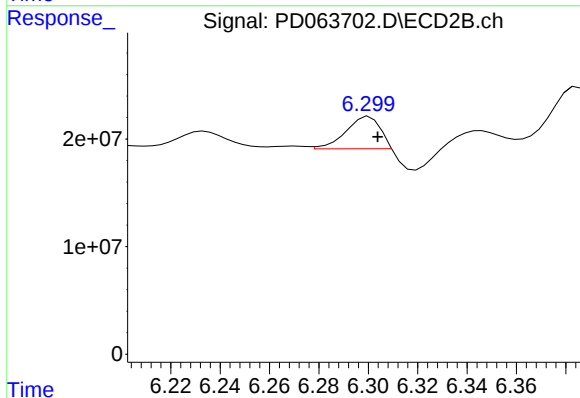


#12 4,4'-DDE

R.T.: 6.299 min
Delta R.T.: -0.005 min
Response: 28619967
Conc: 1.57 ng/ml m

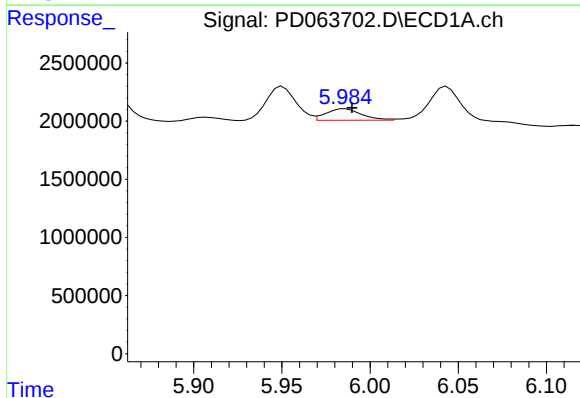


#14 Endrin

R.T.: 5.984 min
Delta R.T.: -0.005 min
Response: 1365179
Conc: 0.86 ng/ml m

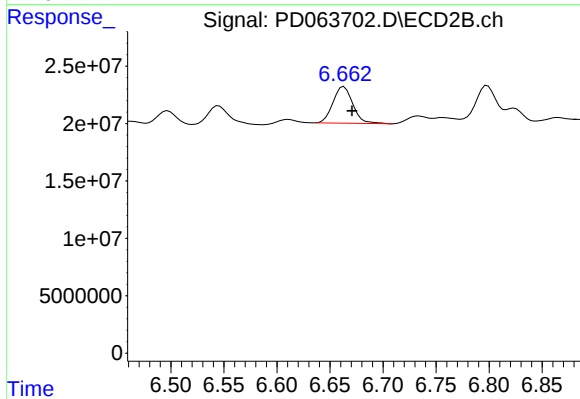

#14 Endrin

R.T.: 6.663 min
Delta R.T.: -0.008 min
Response: 41327668
Conc: 2.69 ng/ml

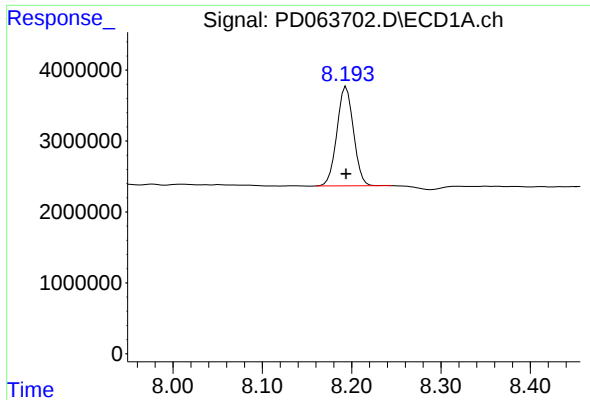


#28 Decachlorobiphenyl

R.T.: 8.194 min
Delta R.T.: 0.000 min
Response: 18029437
Conc: 11.46 ng/ml

Instrument :
ECD_D
ClientSampleId :
17-B2(0-5)

Manual Integrations
APPROVED

Ankita
6/10/2021 3:19:50 PM

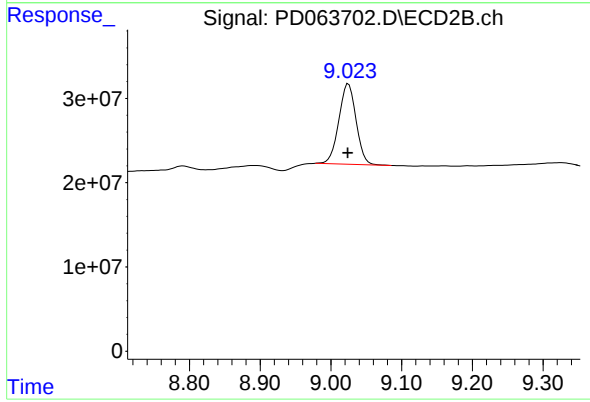

#28 Decachlorobiphenyl

R.T.: 9.025 min
Delta R.T.: 0.001 min
Response: 161807666
Conc: 11.71 ng/ml