

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060921\
 Data File : PD063703.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Jun 2021 21:58
 Operator : AR\AJ
 Sample : M2651-03
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 DEP-CRANE-PAD-EXCAVATION

Manual Integrations
 APPROVED

Ankita
 6/10/2021 3:19:51 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 10 07:42:57 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060221.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 03 01:33:41 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.438	3.971	15648080	165.9E6	11.309	12.381
28)	SA Decachlor...	8.193	9.024	17415246	168.5E6	11.073	12.193
Target Compounds							
12)	B 4,4'-DDE	5.597	6.302	5468830	135.1E6	3.145m	7.433 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060921\
Data File : PD063703.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Jun 2021 21:58
Operator : AR\AJ
Sample : M2651-03
Misc :
ALS Vial : 33 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
DEP-CRANE-PAD-EXCAVATION


Manual Integrations
APPROVED

Ankita
6/10/2021 3:19:51 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 10 07:42:57 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060221.M
Quant Title : GC Extractables
QLast Update : Thu Jun 03 01:33:41 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

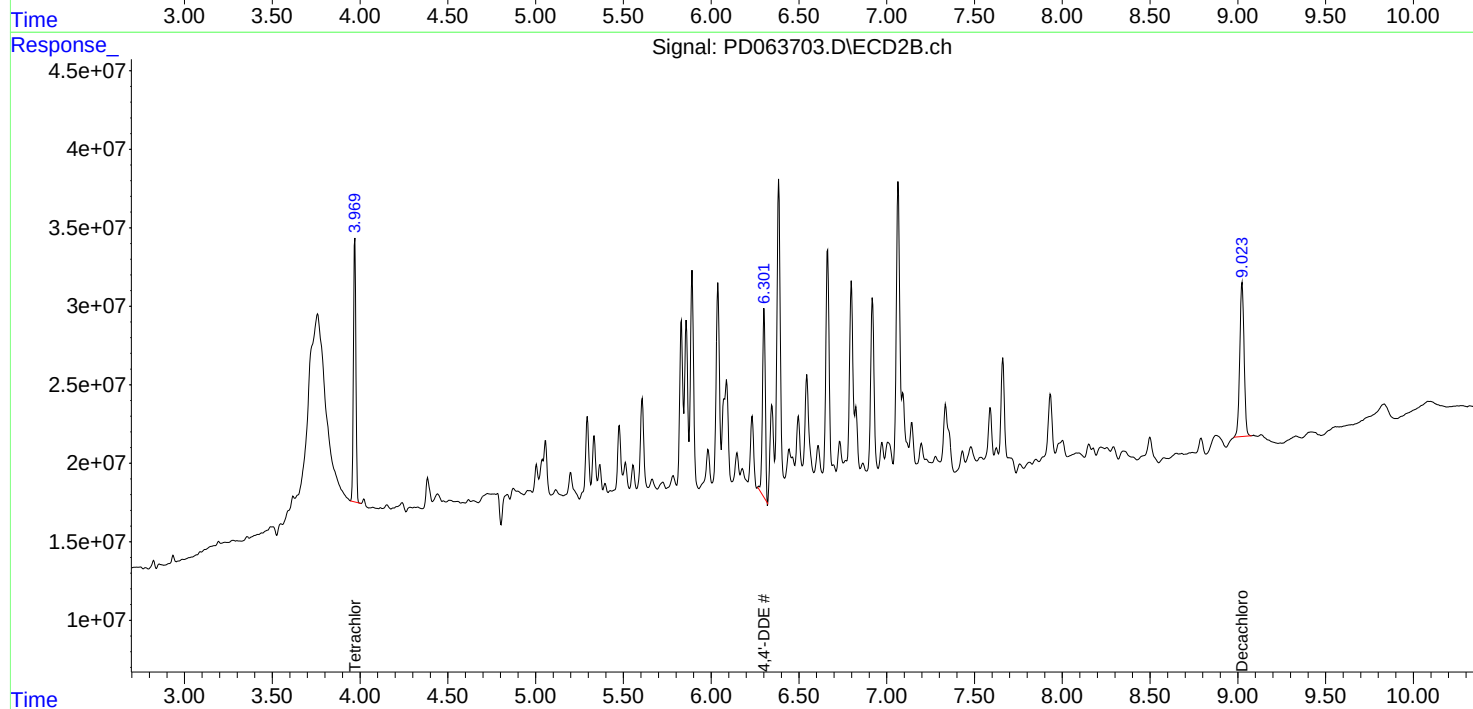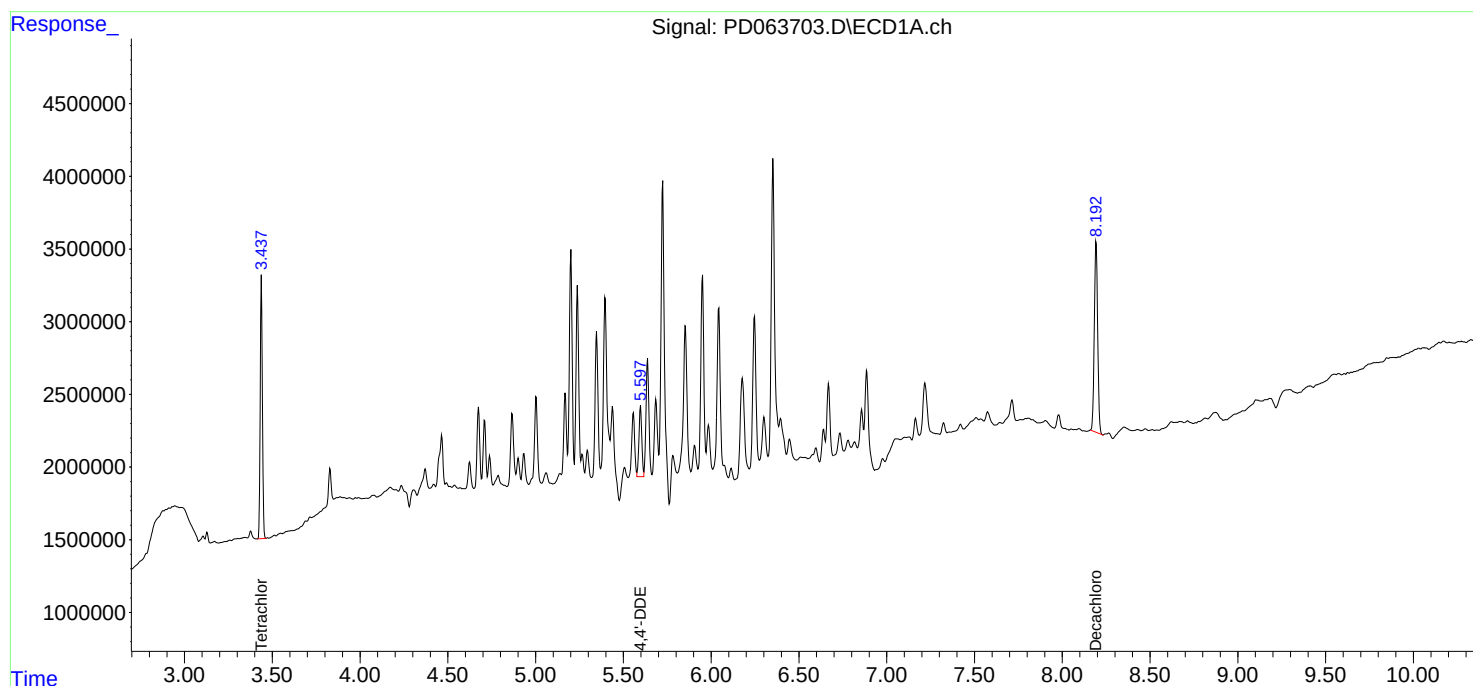

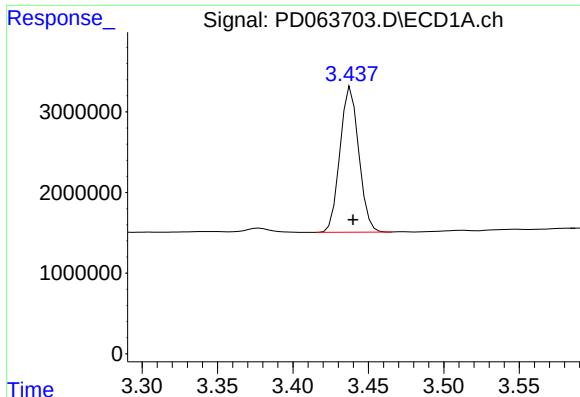


#1 Tetrachloro-m-xylene

R.T.: 3.438 min
Delta R.T.: -0.002 min
Response: 15648080
Conc: 11.31 ng/ml

Instrument :
ECD_D
ClientSampleId :
DEP-CRANE-PAD-EXCAVATION


Manual Integrations
APPROVED

Ankita
6/10/2021 3:19:51 PM

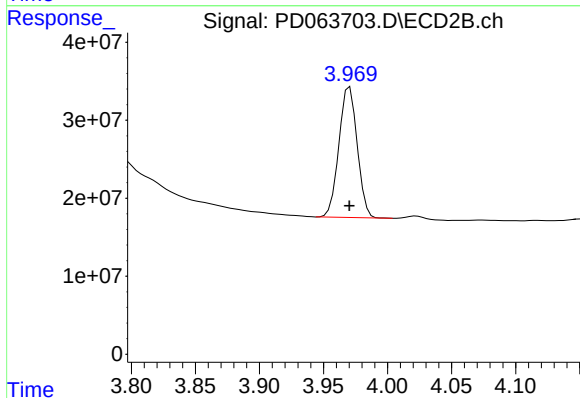


#1 Tetrachloro-m-xylene

R.T.: 3.971 min
Delta R.T.: 0.000 min
Response: 165891225
Conc: 12.38 ng/ml

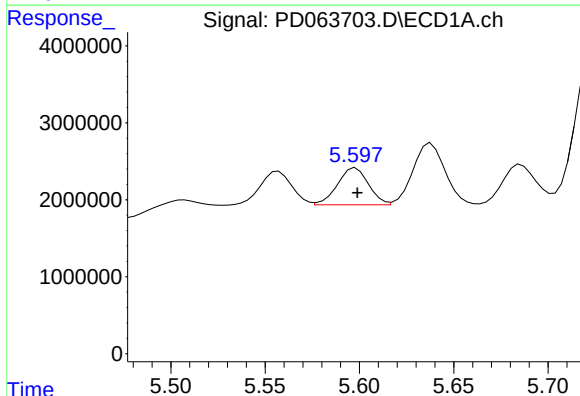


#12 4,4'-DDE

R.T.: 5.597 min
Delta R.T.: -0.002 min
Response: 5468830
Conc: 3.15 ng/ml m

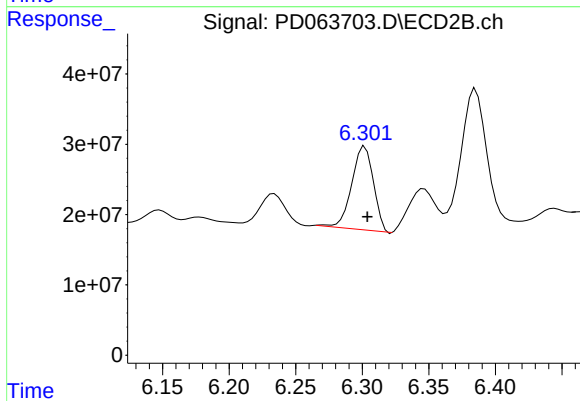

#12 4,4'-DDE

R.T.: 6.302 min
Delta R.T.: -0.002 min
Response: 135077470
Conc: 7.43 ng/ml

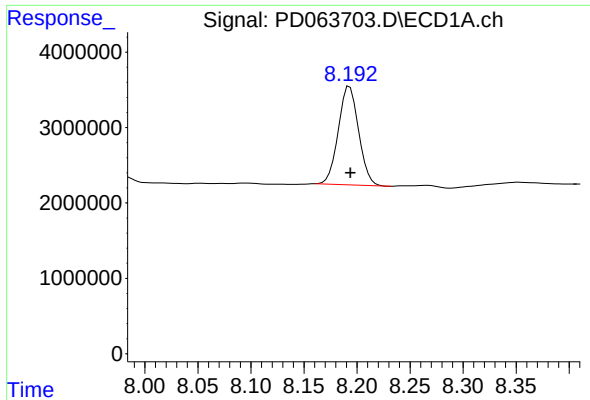


#28 Decachlorobiphenyl

R.T.: 8.193 min
Delta R.T.: 0.000 min
Response: 17415246
Conc: 11.07 ng/ml

Instrument :
ECD_D
ClientSampleId :
DEP-CRANE-PAD-EXCAVATION

Manual Integrations
APPROVED

Ankita
6/10/2021 3:19:51 PM

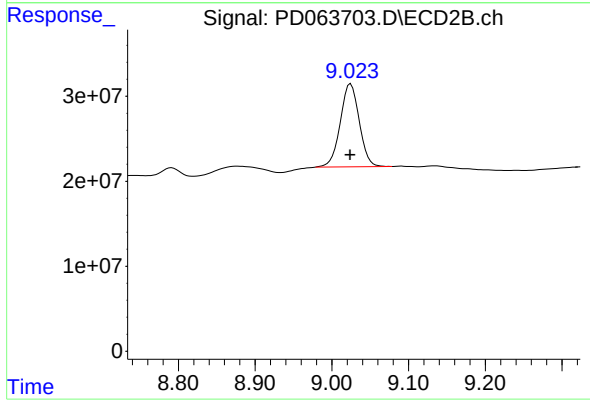

#28 Decachlorobiphenyl

R.T.: 9.024 min
Delta R.T.: 0.000 min
Response: 168483239
Conc: 12.19 ng/ml