

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060921\
 Data File : PD063704.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Jun 2021 22:11
 Operator : AR\AJ
 Sample : M2651-04
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 17-B6(0-4)

Manual Integrations
 APPROVED

Ankita
 6/10/2021 3:19:53 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 10 07:43:27 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060221.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 03 01:33:41 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.438	3.970	15823298	166.1E6	11.435	12.395
28) SA Decachlor...	8.193	9.024	19192408	169.9E6	12.203	12.295
Target Compounds						
12) B 4,4'-DDE	5.598	6.301	1106779	20360814	0.637	1.120 #
17) MA 4,4'-DDT	6.352	7.090	3479079	15430771	2.408m	1.025m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060921\
Data File : PD063704.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Jun 2021 22:11
Operator : AR\AJ
Sample : M2651-04
Misc :
ALS Vial : 34 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
17-B6(0-4)


Manual Integrations
APPROVED

Ankita
6/10/2021 3:19:53 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 10 07:43:27 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060221.M
Quant Title : GC Extractables
QLast Update : Thu Jun 03 01:33:41 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

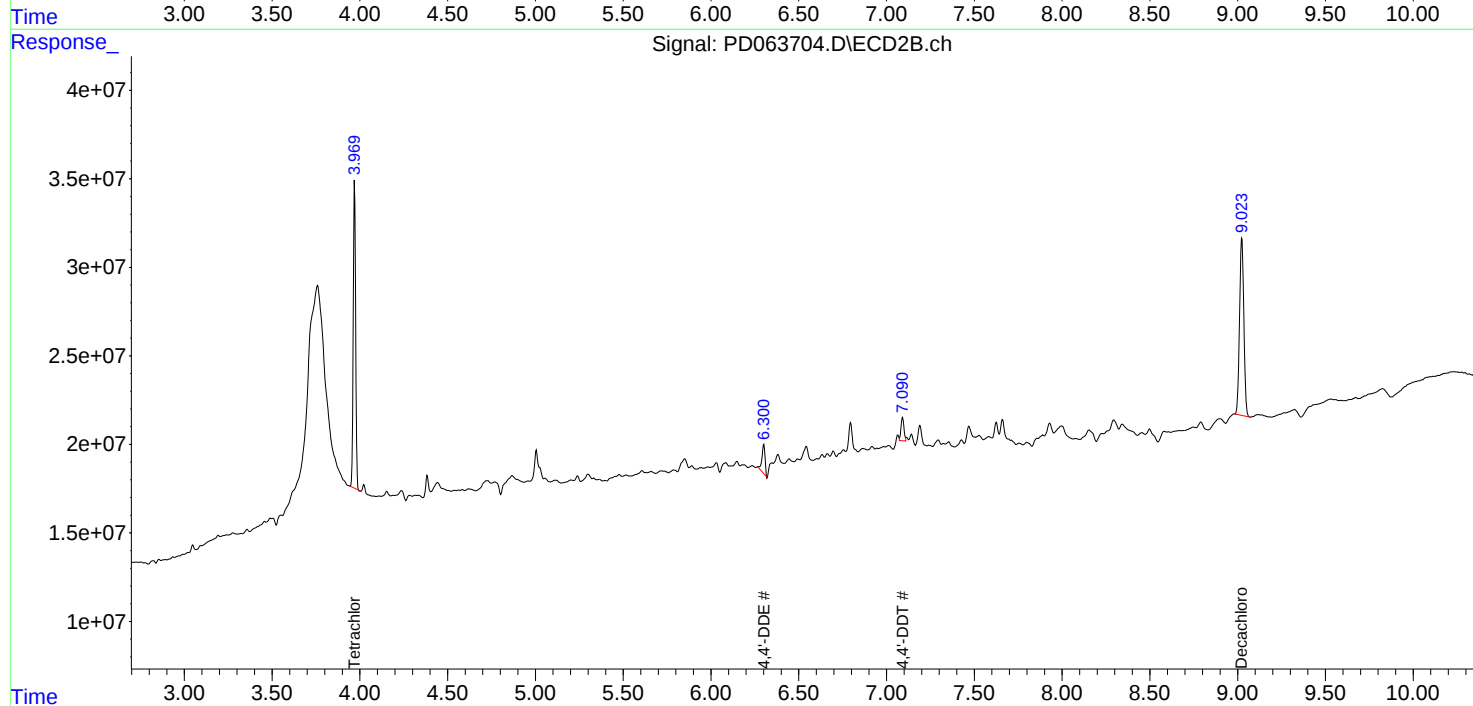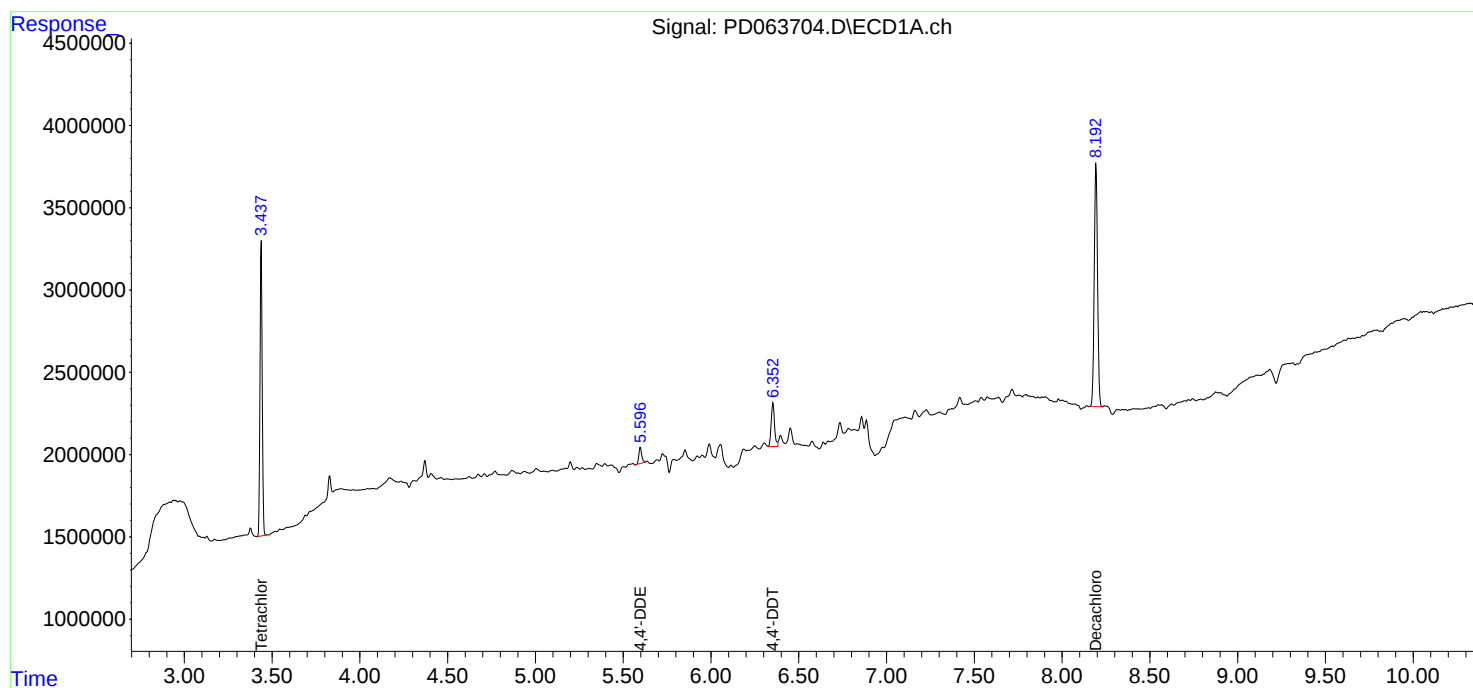

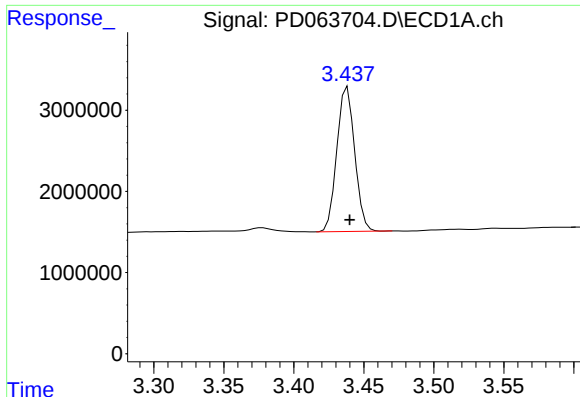


#1 Tetrachloro-m-xylene

R.T.: 3.438 min
Delta R.T.: -0.002 min
Response: 15823298
Conc: 11.44 ng/ml

Instrument :
ECD_D
ClientSampleId :
17-B6(0-4)


Manual Integrations
APPROVED

Ankita
6/10/2021 3:19:53 PM

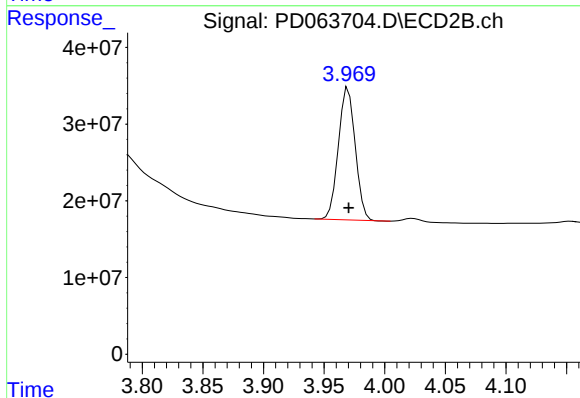


#1 Tetrachloro-m-xylene

R.T.: 3.970 min
Delta R.T.: 0.000 min
Response: 166079482
Conc: 12.40 ng/ml

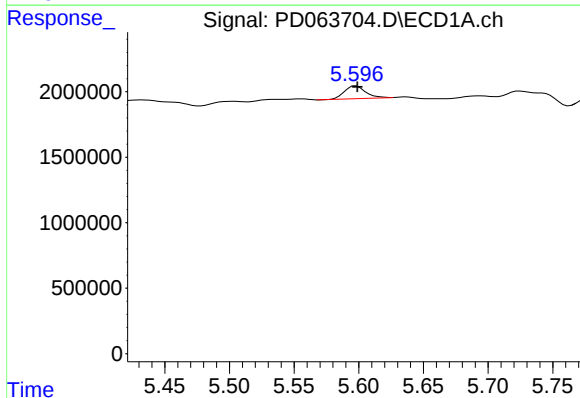


#12 4,4'-DDE

R.T.: 5.598 min
Delta R.T.: -0.001 min
Response: 1106779
Conc: 0.64 ng/ml

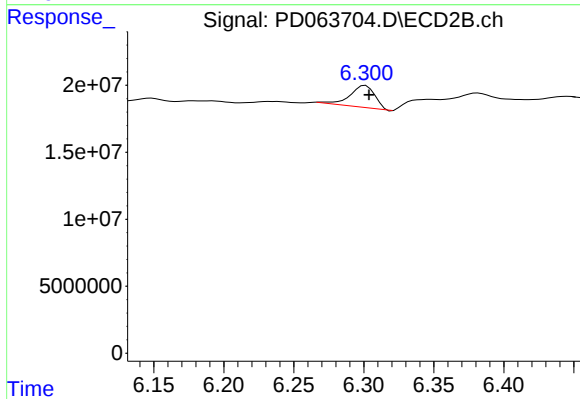

#12 4,4'-DDE

R.T.: 6.301 min
Delta R.T.: -0.003 min
Response: 20360814
Conc: 1.12 ng/ml

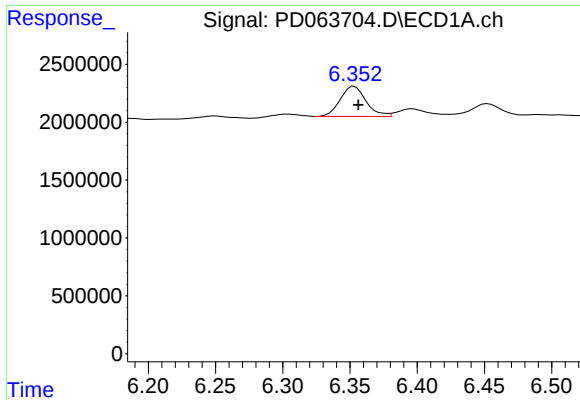


#17 4,4'-DDT

R.T.: 6.352 min
Delta R.T.: -0.004 min
Response: 3479079
Conc: 2.41 ng/ml m

Instrument :
ECD_D
ClientSampleId :
17-B6(0-4)


Manual Integrations
APPROVED

Ankita
6/10/2021 3:19:53 PM

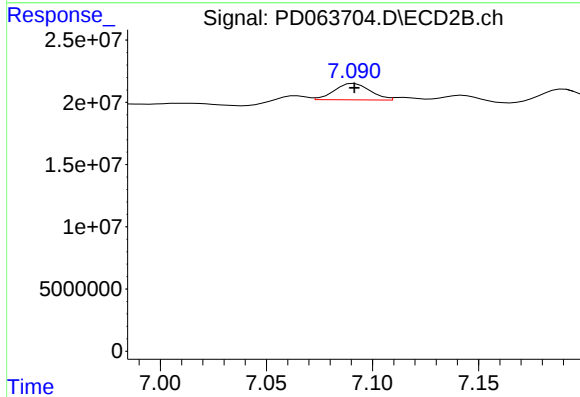


#17 4,4'-DDT

R.T.: 7.090 min
Delta R.T.: -0.001 min
Response: 15430771
Conc: 1.03 ng/ml m

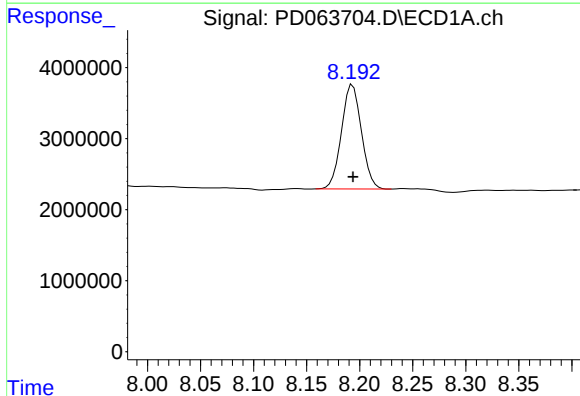

#28 Decachlorobiphenyl

R.T.: 8.193 min
Delta R.T.: 0.000 min
Response: 19192408
Conc: 12.20 ng/ml

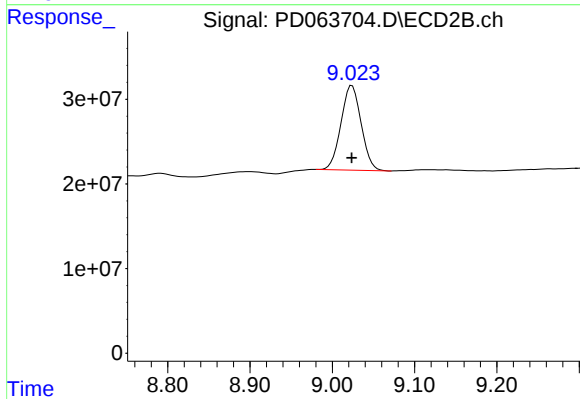

#28 Decachlorobiphenyl

R.T.: 9.024 min
Delta R.T.: 0.000 min
Response: 169905719
Conc: 12.30 ng/ml