

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060921\
 Data File : PD063705.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Jun 2021 22:25
 Operator : AR\AJ
 Sample : M2651-05
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 17-B6(4-8)

Manual Integrations
 APPROVED

Ankita
 6/10/2021 3:19:56 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 10 07:43:55 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060221.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 03 01:33:41 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.438	3.970	16794317	177.4E6	12.137	13.240
28)	SA Decachlor...	8.193	9.023	17308033	147.3E6	11.005	10.662
Target Compounds							
17)	MA 4,4'-DDT	6.351	7.089	1505720	11694328	1.042m	0.777m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060921\
Data File : PD063705.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Jun 2021 22:25
Operator : AR\AJ
Sample : M2651-05
Misc :
ALS Vial : 35 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
17-B6(4-8)


Manual Integrations
APPROVED

Ankita
6/10/2021 3:19:56 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 10 07:43:55 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060221.M
Quant Title : GC Extractables
QLast Update : Thu Jun 03 01:33:41 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

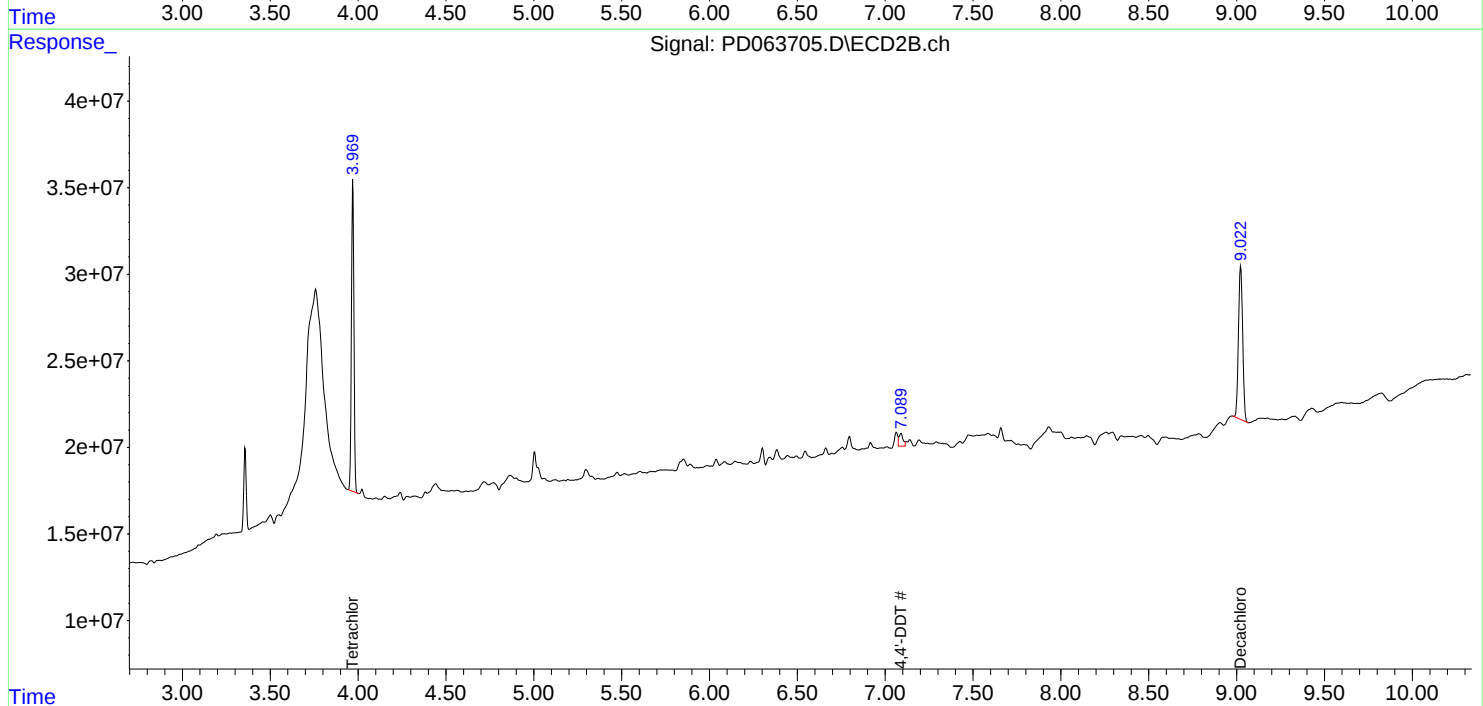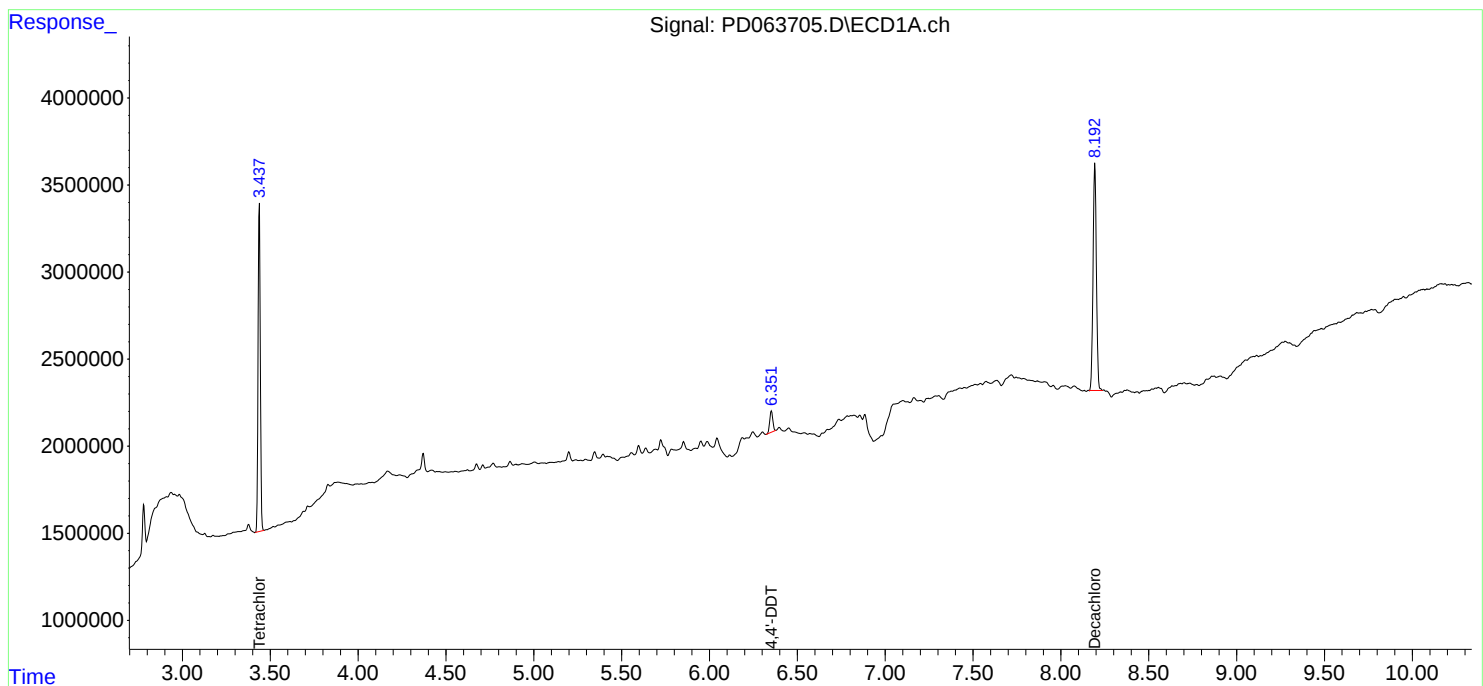

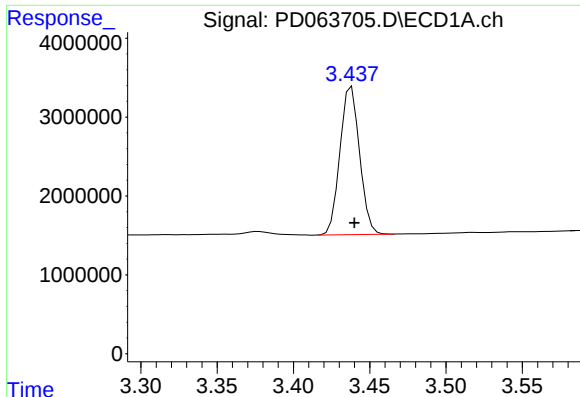


#1 Tetrachloro-m-xylene

R.T.: 3.438 min
Delta R.T.: -0.002 min
Response: 16794317
Conc: 12.14 ng/ml

Instrument :
ECD_D
ClientSampleId :
17-B6(4-8)


Manual Integrations
APPROVED

Ankita
6/10/2021 3:19:56 PM

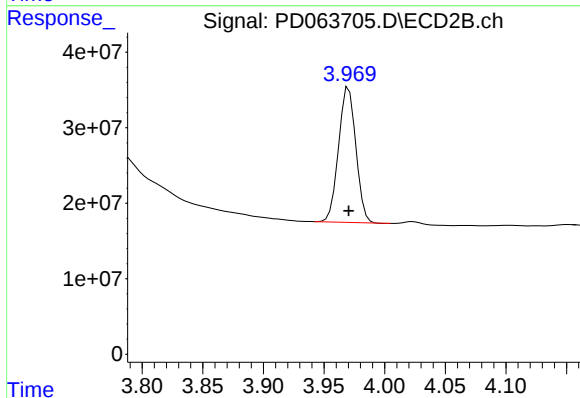


#1 Tetrachloro-m-xylene

R.T.: 3.970 min
Delta R.T.: 0.000 min
Response: 177403006
Conc: 13.24 ng/ml

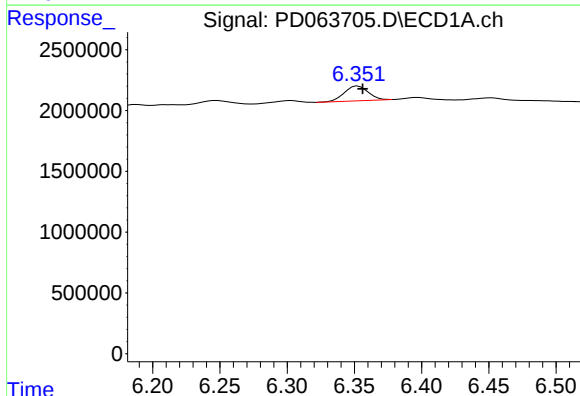


#17 4,4'-DDT

R.T.: 6.351 min
Delta R.T.: -0.005 min
Response: 1505720
Conc: 1.04 ng/ml m

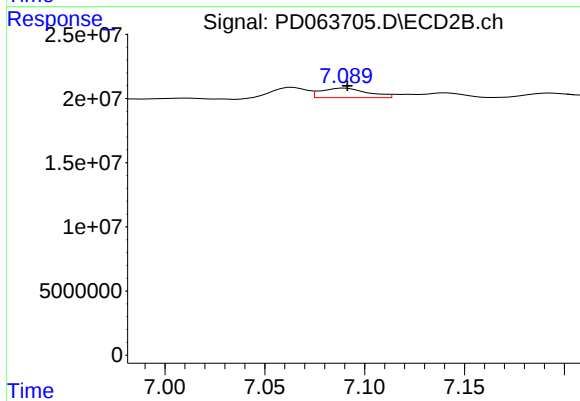

#17 4,4'-DDT

R.T.: 7.089 min
Delta R.T.: -0.002 min
Response: 11694328
Conc: 0.78 ng/ml m

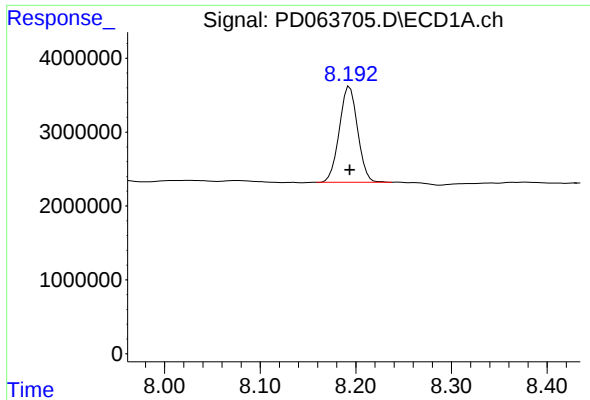


#28 Decachlorobiphenyl

R.T.: 8.193 min
Delta R.T.: 0.000 min
Response: 17308033
Conc: 11.01 ng/ml

Instrument :
ECD_D
ClientSampleId :
17-B6(4-8)

Manual Integrations
APPROVED

Ankita
6/10/2021 3:19:56 PM

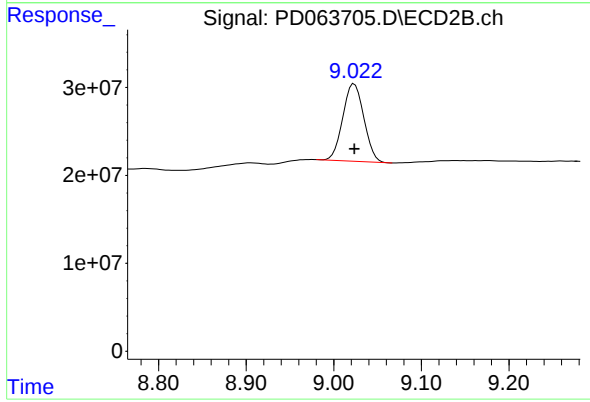

#28 Decachlorobiphenyl

R.T.: 9.023 min
Delta R.T.: 0.000 min
Response: 147330118
Conc: 10.66 ng/ml