

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060922\
 Data File : PD070226.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Jun 2022 09:00
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 09 14:23:17 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060622.M
 Quant Title : GC Extractables
 QLast Update : Wed Jun 08 02:48:31 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
8) B	Heptachlo...	5.147	6.069	2542590	143.6E6	1.854 17.428 #
10) B	gamma-Chl...	0.000	6.292f	0	36445341	N.D. 3.171 #
14) MA	Endrin	6.013f	0.000	714999	0	0.594 N.D. #
17) MA	4,4'-DDT	0.000	7.362f	0	10638865	N.D. 1.240 #
18) B	Endrin al...	0.000	7.240	0	13141436	N.D. 1.915 #
19) B	Endosulfa...	0.000	7.485	0	12116085	N.D. 1.455 #
20) A	Methoxychlor	0.000	7.776	0	18818524	N.D. 4.463 #
25)	Chlordane-3	0.000	6.292f	0	36445341	N.D. 24.870 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060922\
Data File : PD070226.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Jun 2022 09:00
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 09 14:23:17 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060622.M
Quant Title : GC Extractables
QLast Update : Wed Jun 08 02:48:31 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

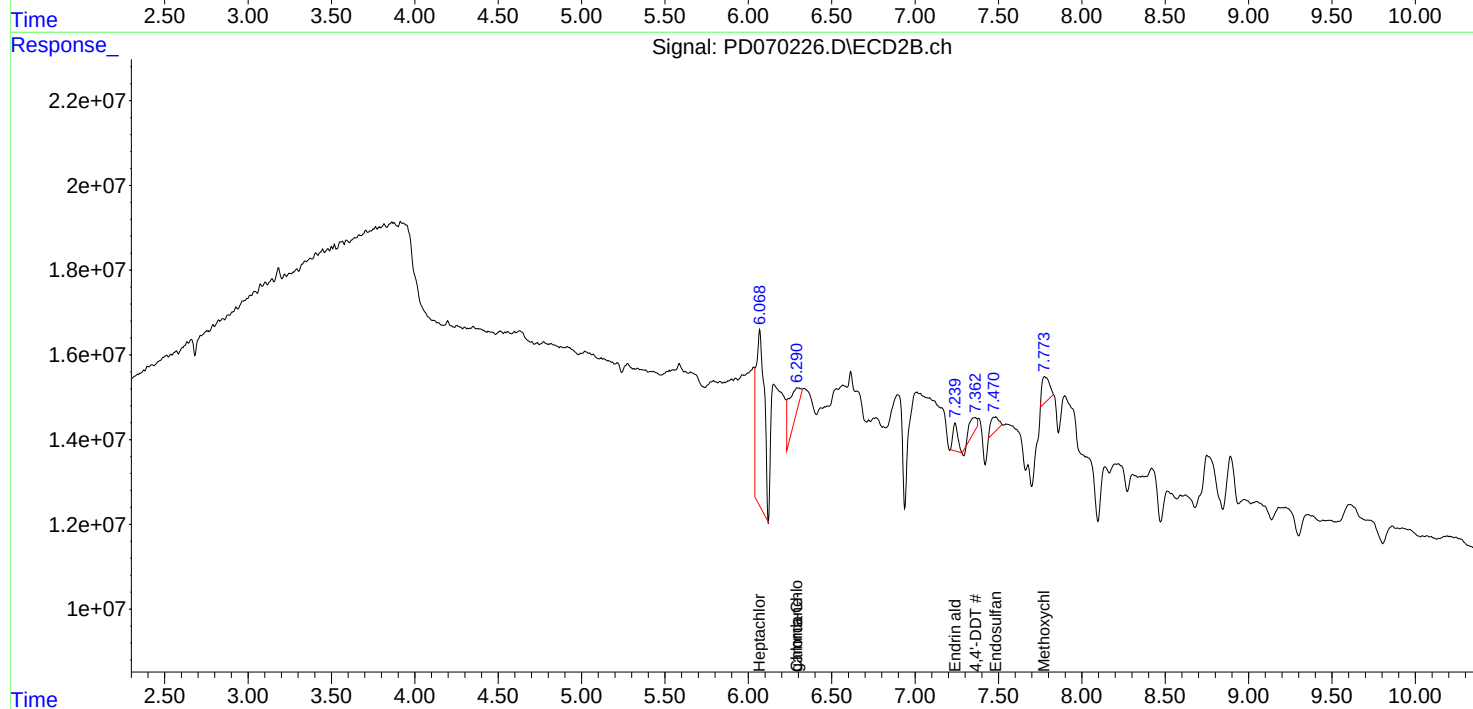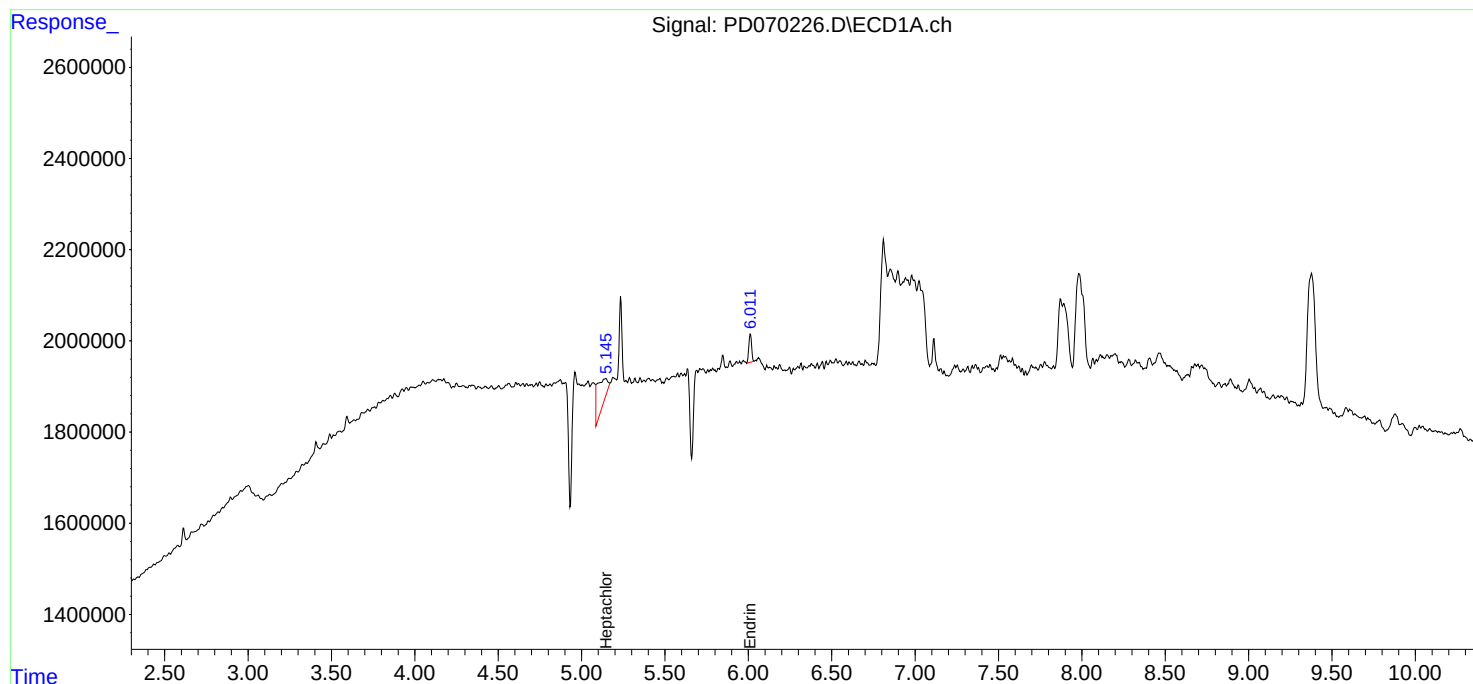


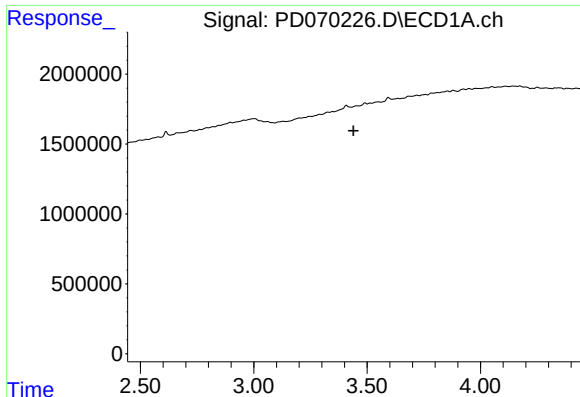

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T.: 3.440 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

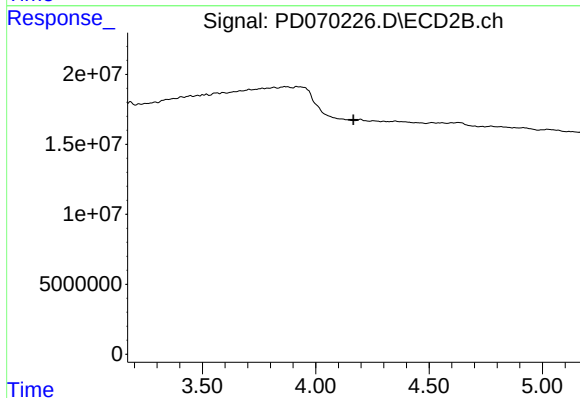


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T.: 4.167 min
Response: 0
Conc: N.D.

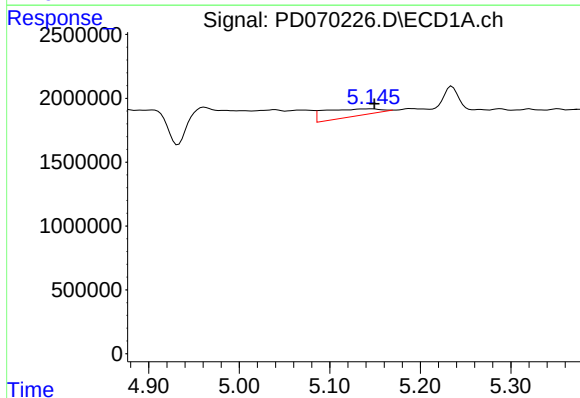


#8 Heptachlor epoxide

R.T.: 5.147 min
Delta R.T.: -0.003 min
Response: 2542590
Conc: 1.85 ng/ml

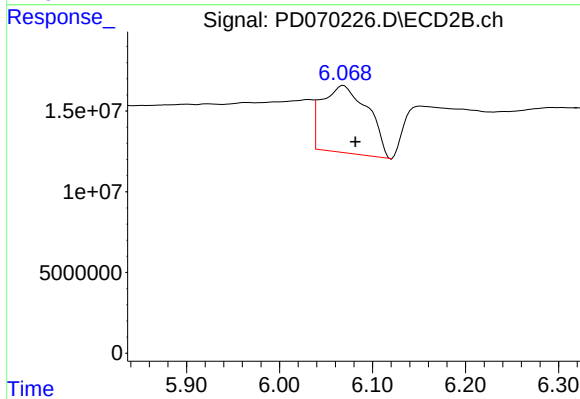

#8 Heptachlor epoxide


R.T.: 6.069 min
Delta R.T.: -0.013 min
Response: 143577679
Conc: 17.43 ng/ml

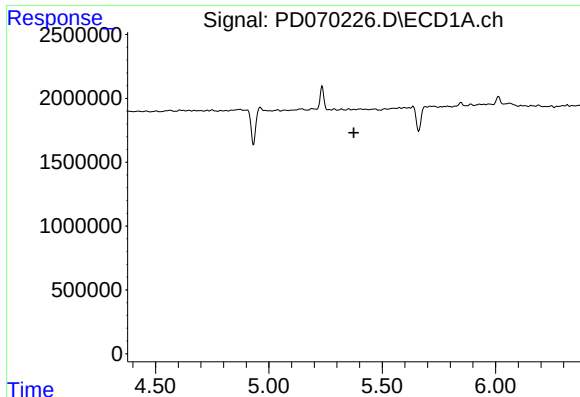

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.375 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

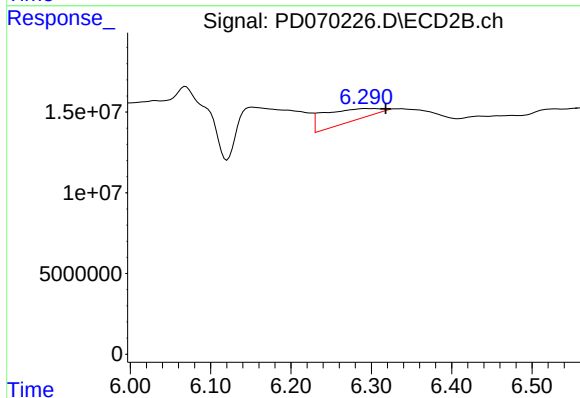


#10 gamma-Chlordane

R.T.: 6.292 min
Delta R.T.: -0.026 min
Response: 36445341
Conc: 3.17 ng/ml

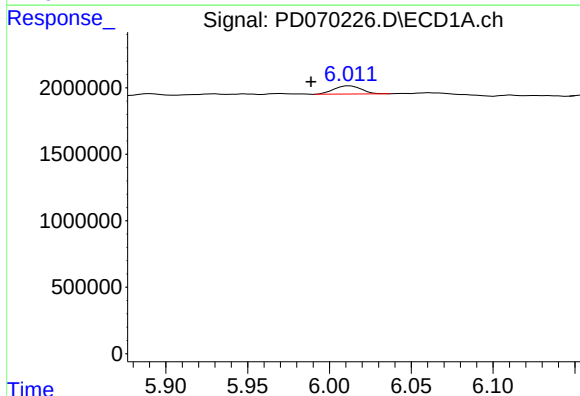


#14 Endrin

R.T.: 6.013 min
Delta R.T.: 0.024 min
Response: 714999
Conc: 0.59 ng/ml

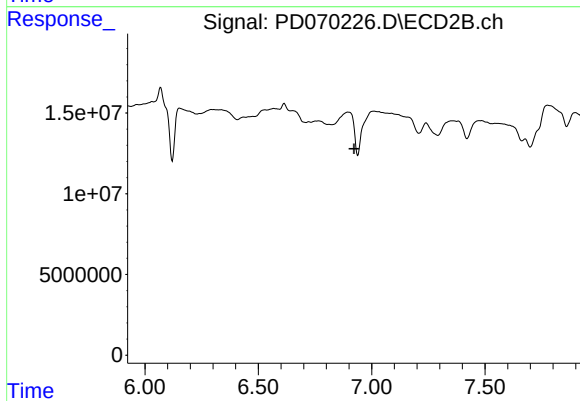

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.922 min
Response: 0
Conc: N.D.

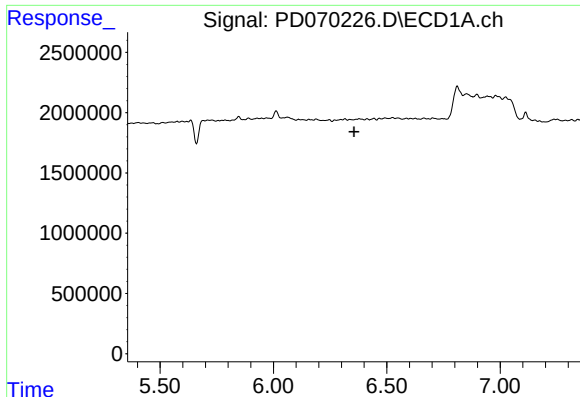

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 6.356 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

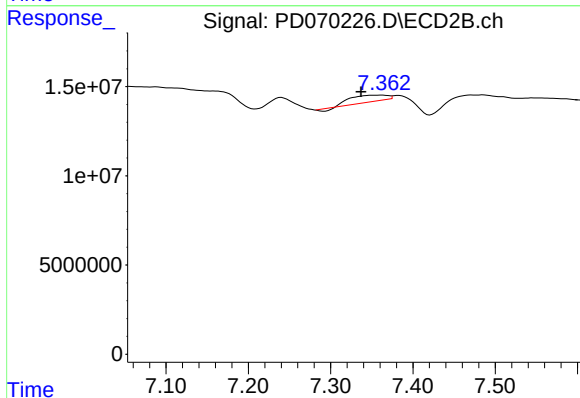


#17 4,4'-DDT

R.T.: 7.362 min
Delta R.T.: 0.025 min
Response: 10638865
Conc: 1.24 ng/ml

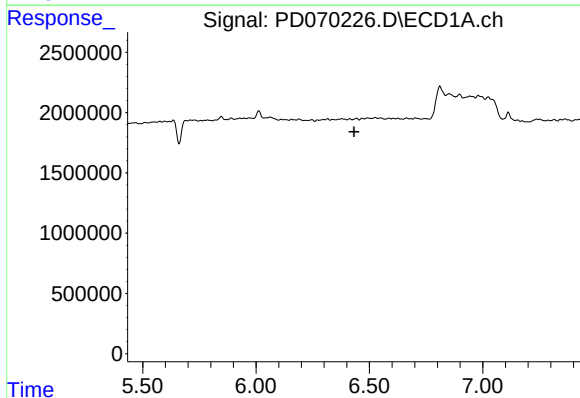


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T.: 6.432 min
Response: 0
Conc: N.D.

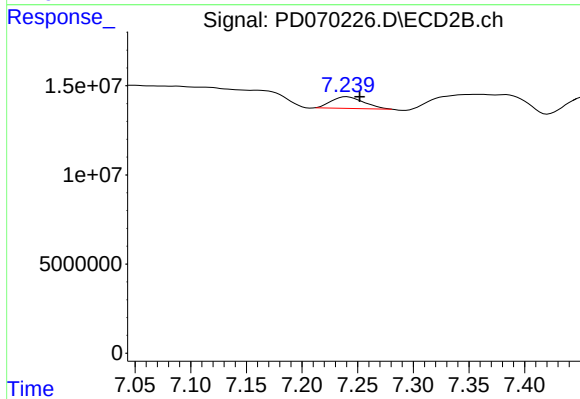

#18 Endrin aldehyde


R.T.: 7.240 min
Delta R.T.: -0.012 min
Response: 13141436
Conc: 1.91 ng/ml

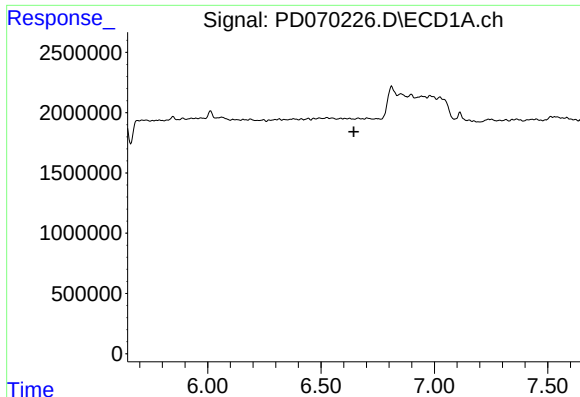

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T.: 6.645 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

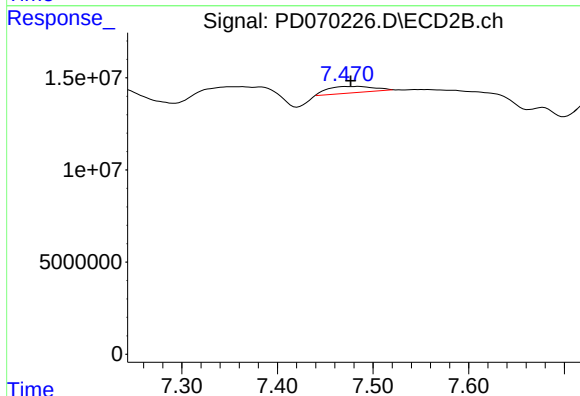


#19 Endosulfan Sulfate

R.T.: 7.485 min
Delta R.T.: 0.009 min
Response: 12116085
Conc: 1.45 ng/ml

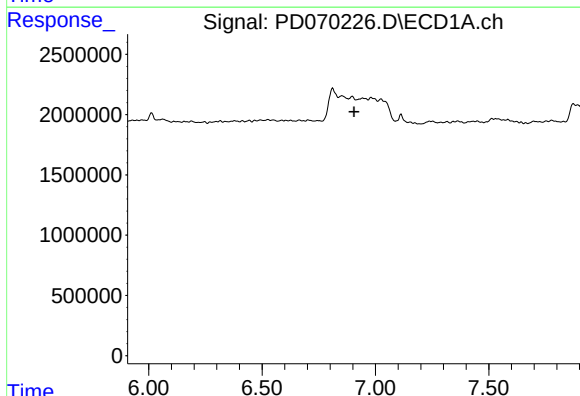


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T.: 6.905 min
Response: 0
Conc: N.D.

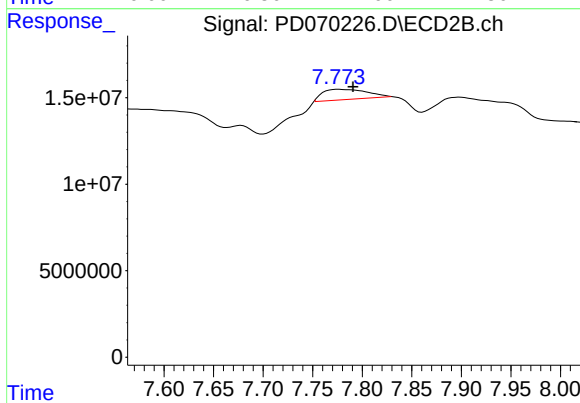

#20 Methoxychlor


R.T.: 7.776 min
Delta R.T.: -0.014 min
Response: 18818524
Conc: 4.46 ng/ml

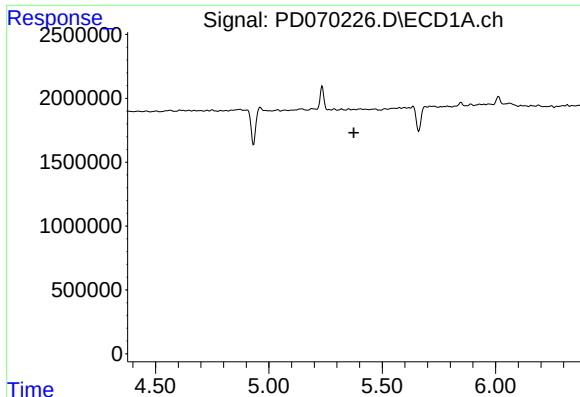

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.375 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

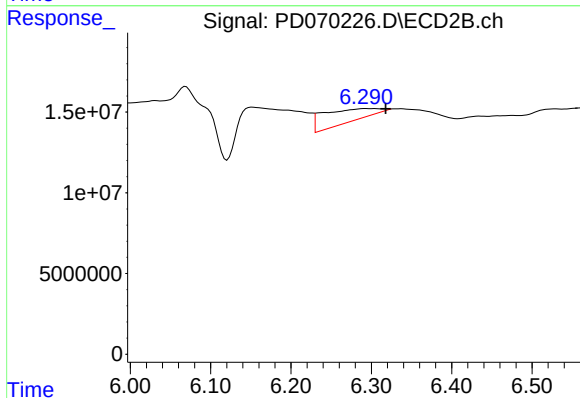


#25 Chlordane-3

R.T.: 6.292 min
Delta R.T.: -0.026 min
Response: 36445341
Conc: 24.87 ng/ml

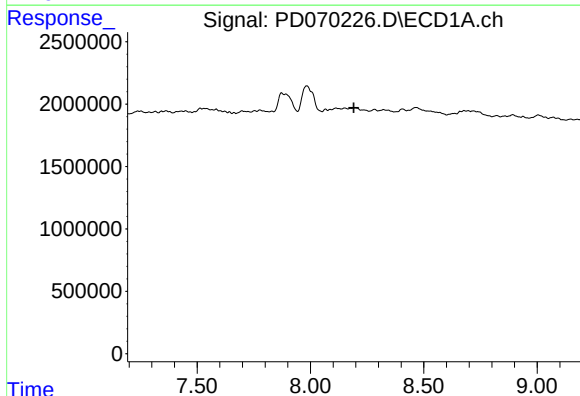

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T.: 8.191 min
Response: 0
Conc: N.D.

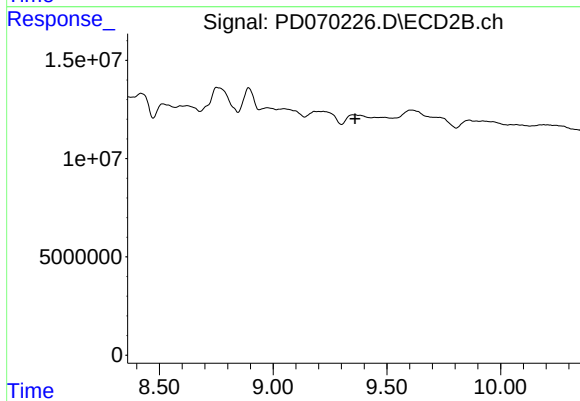

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T.: 9.360 min
Response: 0
Conc: N.D.