

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060922\
 Data File : PD070232.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Jun 2022 12:48
 Operator : AR\AJ
 Sample : N3209-06
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 09 14:24:22 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060622.M
 Quant Title : GC Extractables
 QLast Update : Wed Jun 08 02:48:31 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.441	4.169	11289793	81483143	10.399	8.348
28)	SA Decachlor...	8.194	9.365	12948838	82540593	11.643	13.420
Target Compounds							
16)	A 4,4'-DDD	0.000	7.046	0	7678171	N.D.	0.913 #
20)	A Methoxychlor	6.887f	0.000	927758	0	1.505	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060922\
Data File : PD070232.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Jun 2022 12:48
Operator : AR\AJ
Sample : N3209-06
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 09 14:24:22 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060622.M
Quant Title : GC Extractables
QLast Update : Wed Jun 08 02:48:31 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

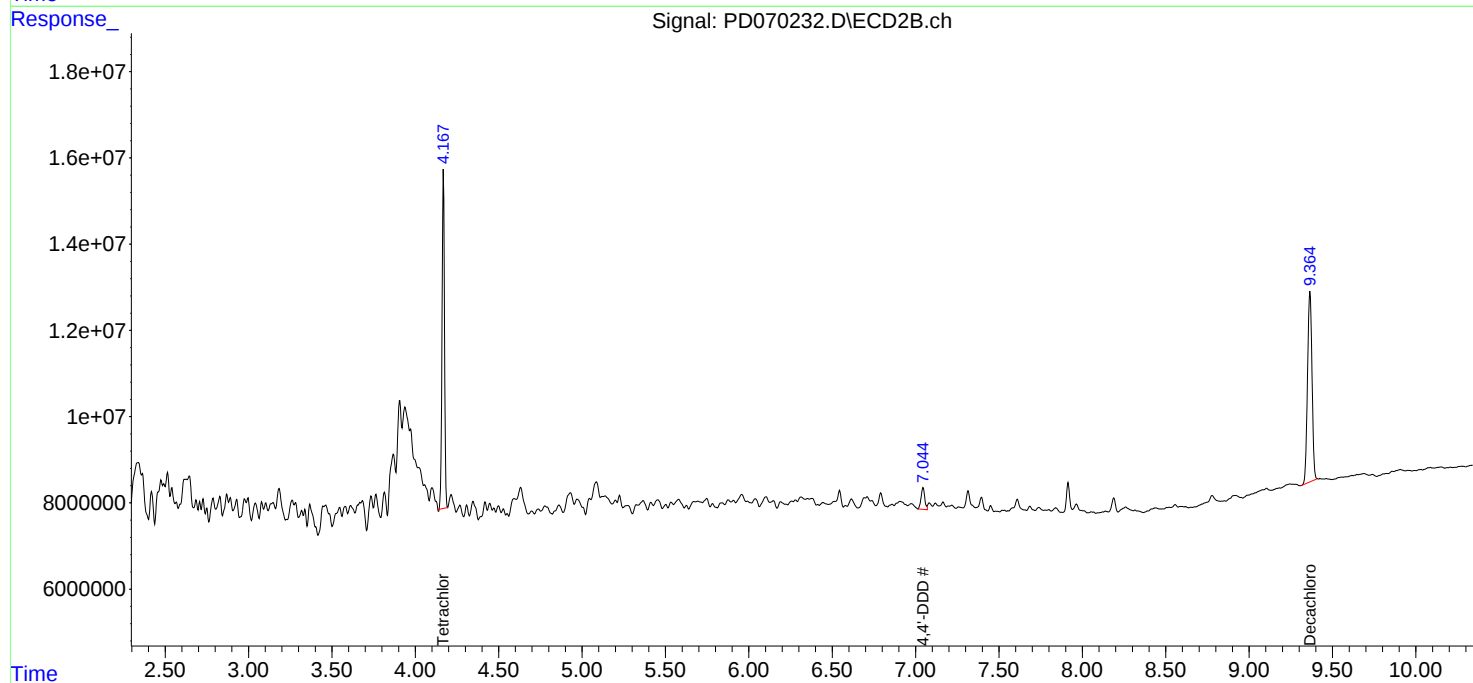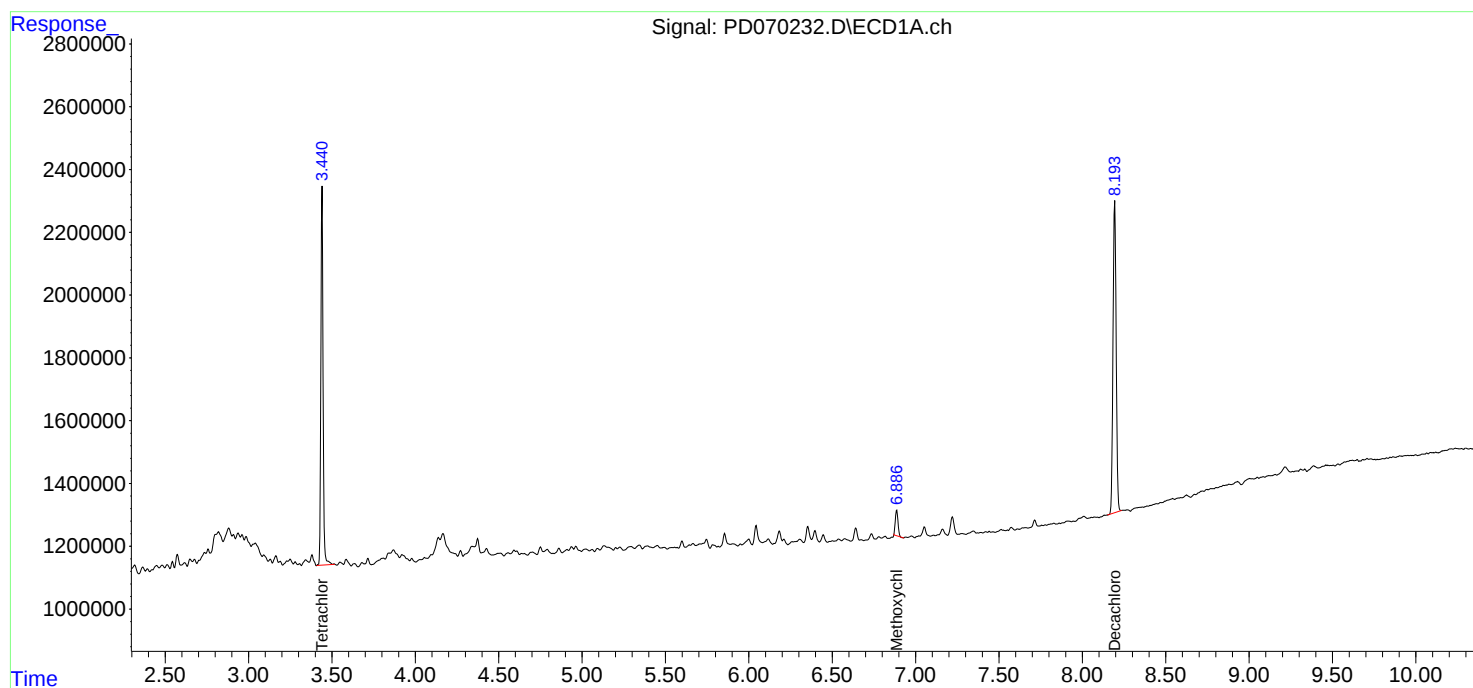


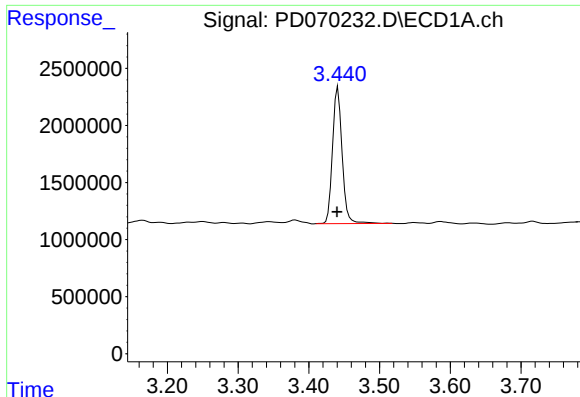

#1 Tetrachloro-m-xylene


R.T.: 3.441 min
Delta R.T.: 0.001 min
Response: 11289793
Conc: 10.40 ng/ml

Instrument :
ECD_D
ClientSampleId :

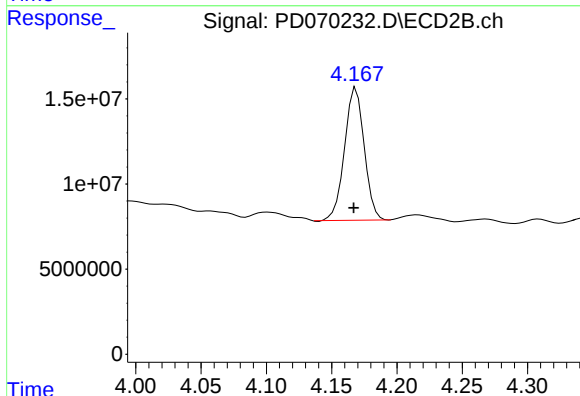


#1 Tetrachloro-m-xylene

R.T.: 4.169 min
Delta R.T.: 0.002 min
Response: 81483143
Conc: 8.35 ng/ml

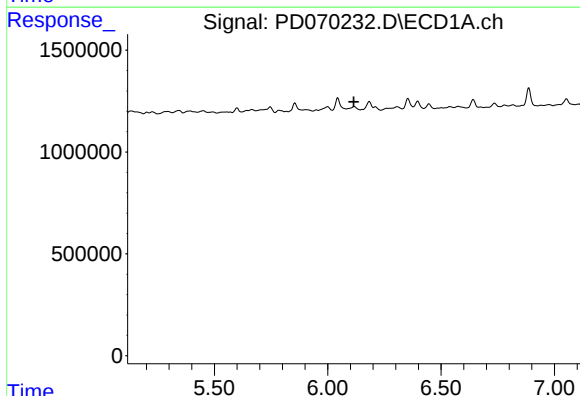


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 6.115 min
Response: 0
Conc: N.D.

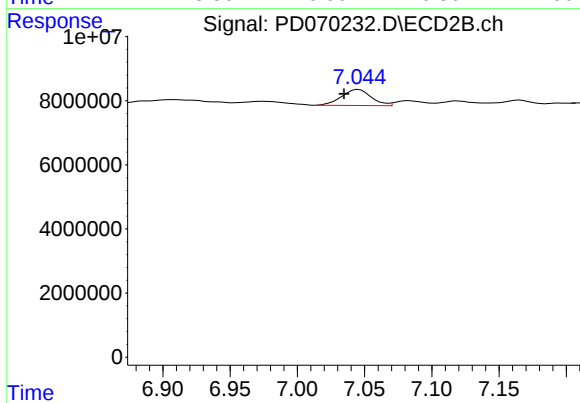

#16 4,4'-DDD


R.T.: 7.046 min
Delta R.T.: 0.011 min
Response: 7678171
Conc: 0.91 ng/ml

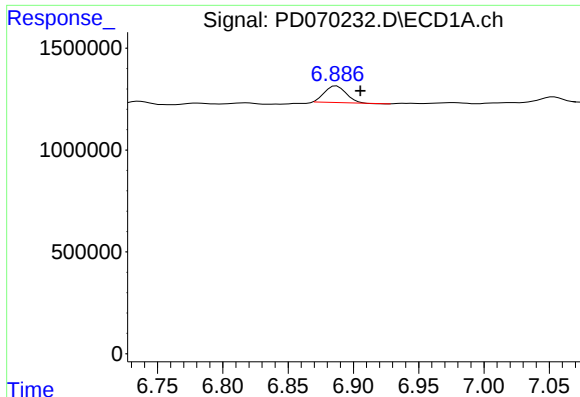

#20 Methoxychlor


R.T.: 6.887 min
Delta R.T.: -0.018 min
Response: 927758
Conc: 1.50 ng/ml

Instrument :
ECD_D
ClientSampleId :

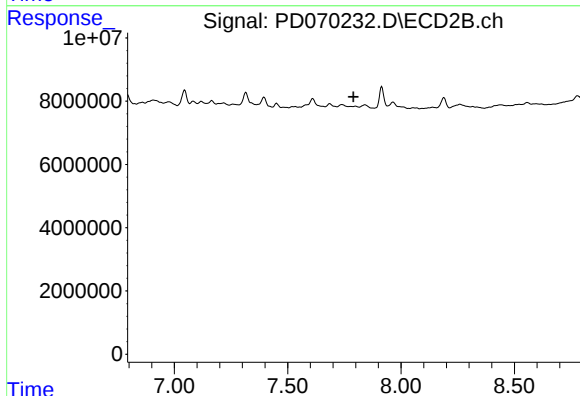


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T.: 7.791 min
Response: 0
Conc: N.D.

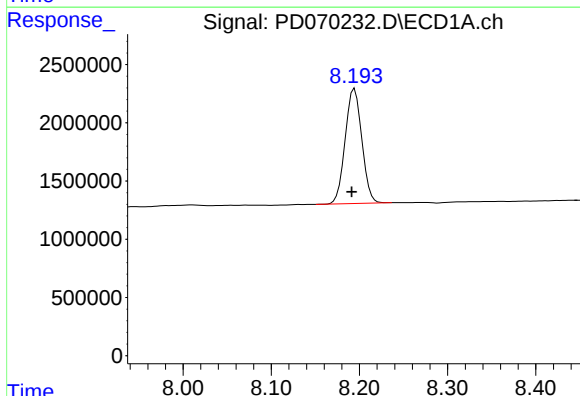

#28 Decachlorobiphenyl

R.T.: 8.194 min
Delta R.T.: 0.003 min
Response: 12948838
Conc: 11.64 ng/ml

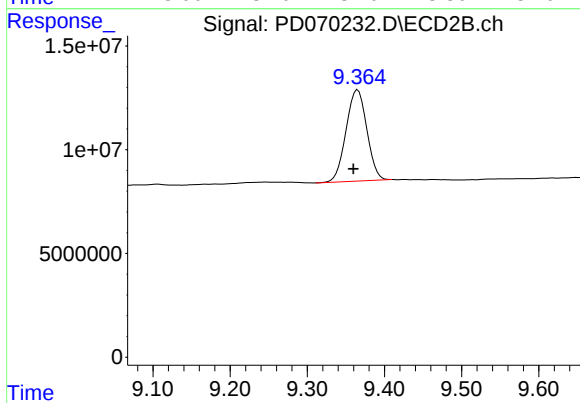

#28 Decachlorobiphenyl

R.T.: 9.365 min
Delta R.T.: 0.006 min
Response: 82540593
Conc: 13.42 ng/ml