

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060922\
 Data File : PD070233.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Jun 2022 13:02
 Operator : AR\AJ
 Sample : N3209-09
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 09 14:24:29 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060622.M
 Quant Title : GC Extractables
 QLast Update : Wed Jun 08 02:48:31 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.441	4.169	9802148	73354372	9.029	7.515
2) SA Decachlor...	8.195	9.366	9917252	63423455	8.918	10.312
Target Compounds						
16) A 4,4'-DDD	0.000	7.045	0	8361672	N.D.	0.994 #
17) MA 4,4'-DDT	6.355	7.316f	799018	8664698	0.753	1.010 #
19) B Endosulfa...	6.642	0.000	585170	0	0.494	N.D. #
20) A Methoxychlor	6.888f	0.000	1411839	0	2.290	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060922\
Data File : PD070233.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Jun 2022 13:02
Operator : AR\AJ
Sample : N3209-09
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 09 14:24:29 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060622.M
Quant Title : GC Extractables
QLast Update : Wed Jun 08 02:48:31 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

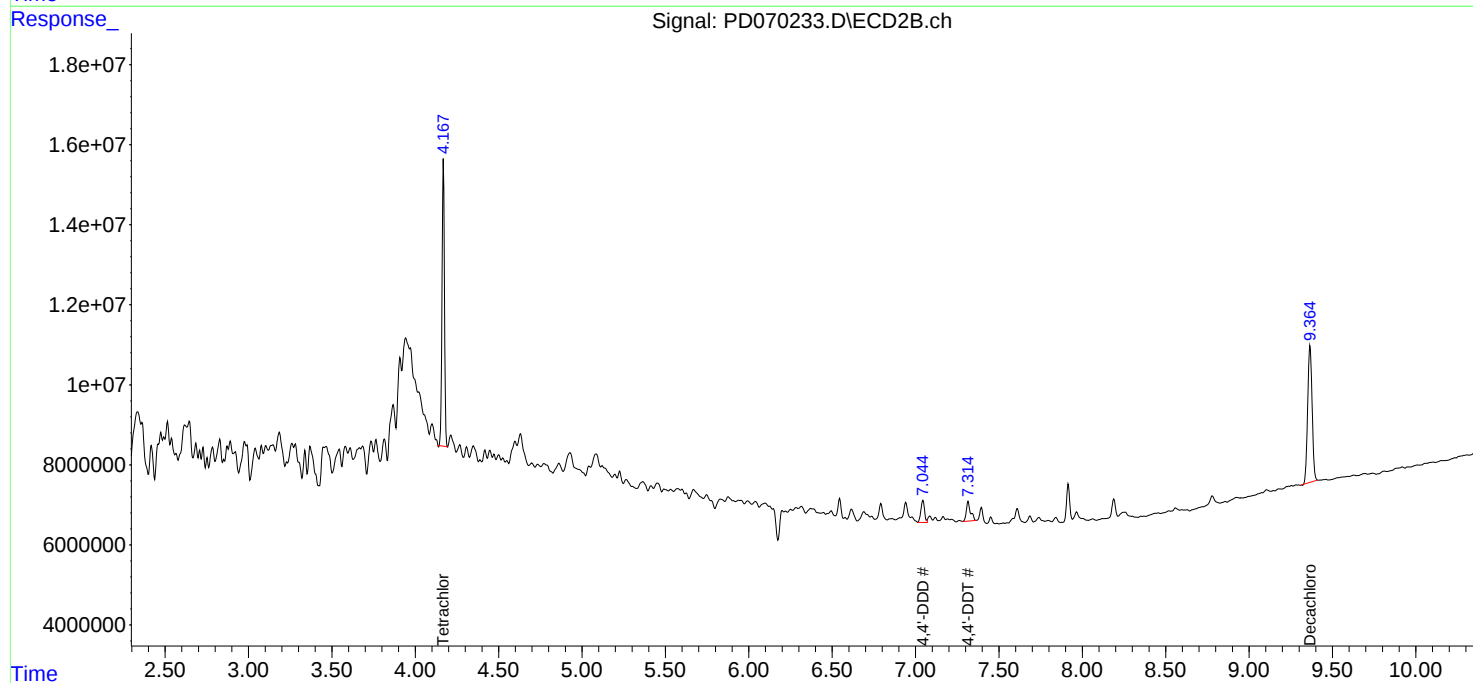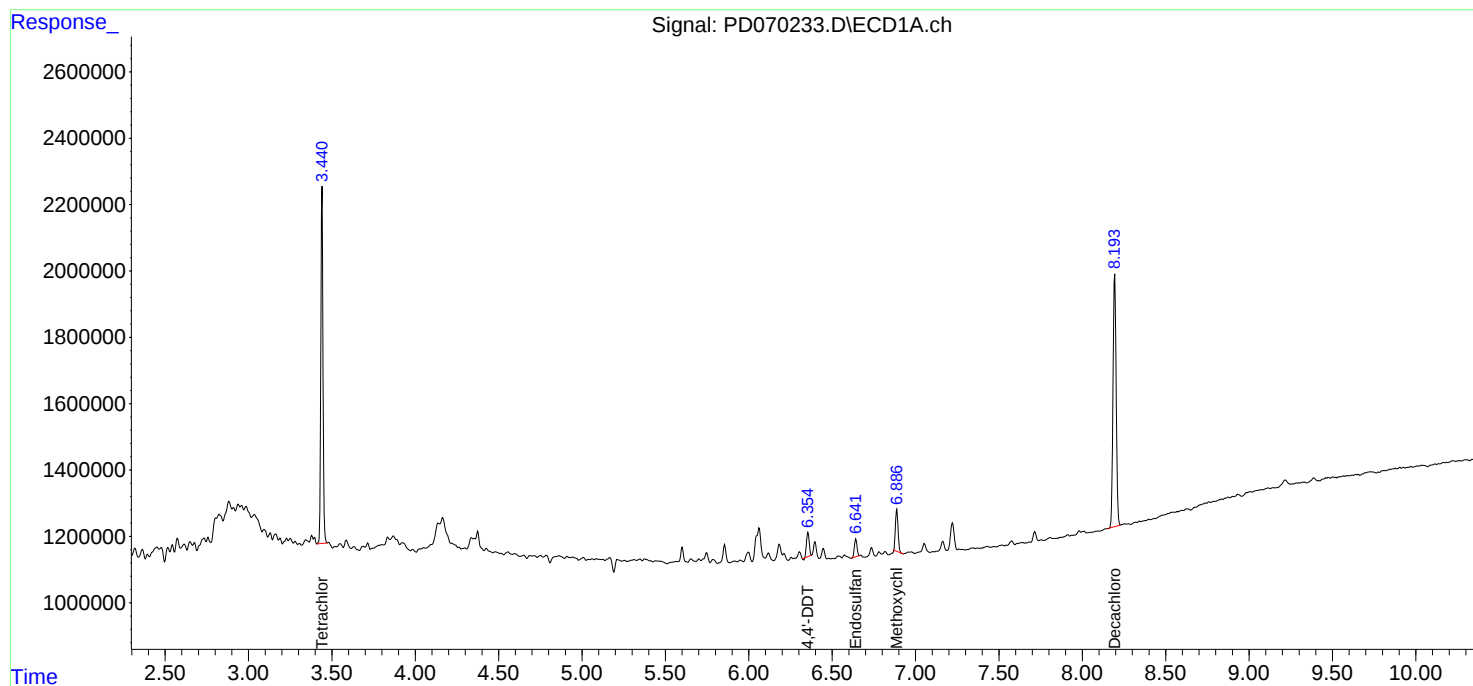


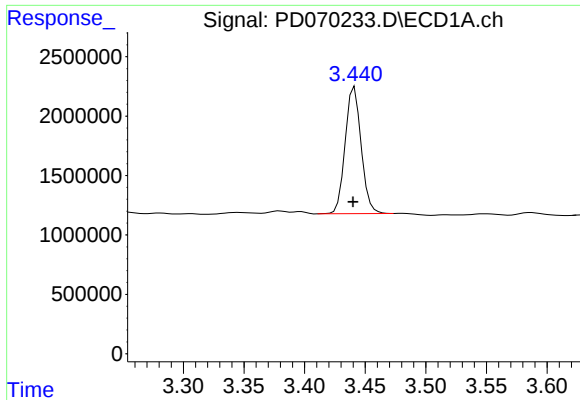

#1 Tetrachloro-m-xylene


R.T.: 3.441 min
Delta R.T.: 0.001 min
Response: 9802148
Conc: 9.03 ng/ml

Instrument :
ECD_D
ClientSampleId :

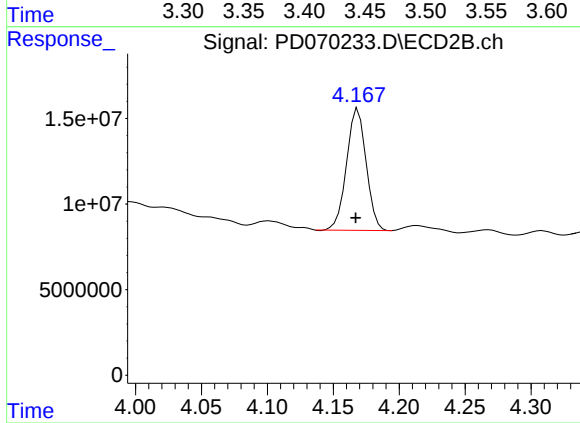


#1 Tetrachloro-m-xylene

R.T.: 4.169 min
Delta R.T.: 0.002 min
Response: 73354372
Conc: 7.51 ng/ml

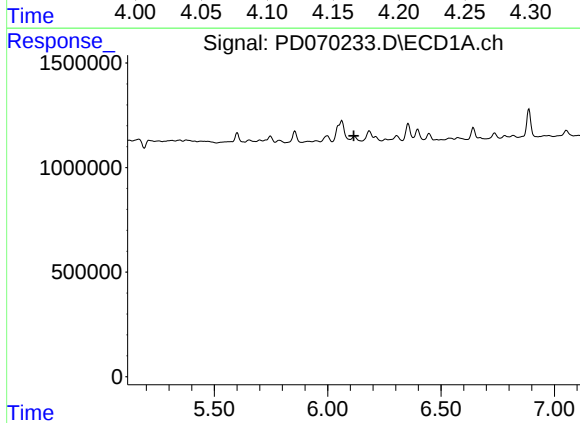


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 6.115 min
Response: 0
Conc: N.D.

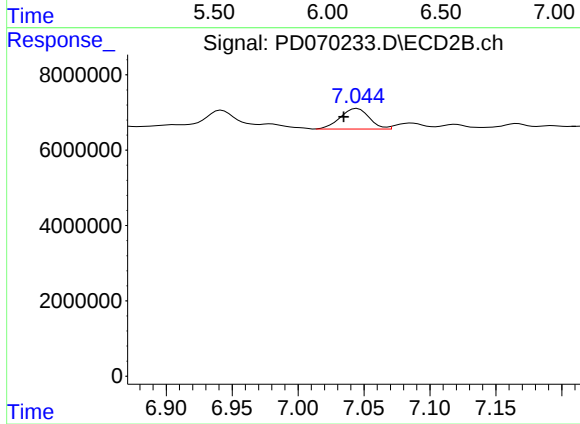

#16 4,4'-DDD


R.T.: 7.045 min
Delta R.T.: 0.010 min
Response: 8361672
Conc: 0.99 ng/ml

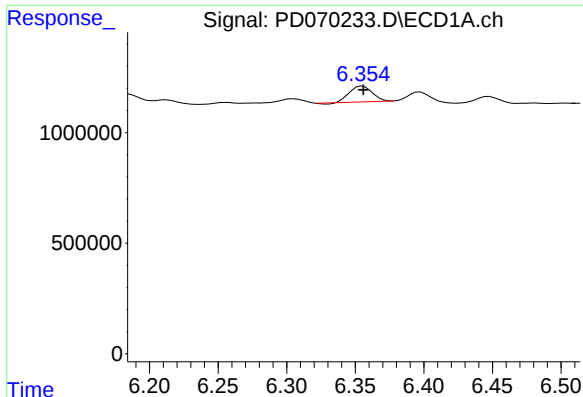

#17 4,4'-DDT


R.T.: 6.355 min
Delta R.T.: 0.000 min
Response: 799018
Conc: 0.75 ng/ml

Instrument :
ECD_D
ClientSampleId :

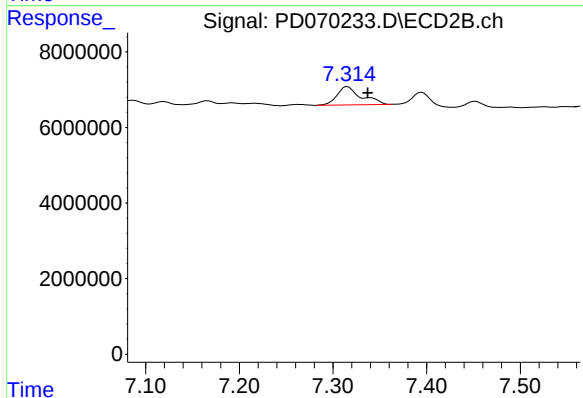


#17 4,4'-DDT

R.T.: 7.316 min
Delta R.T.: -0.021 min
Response: 8664698
Conc: 1.01 ng/ml

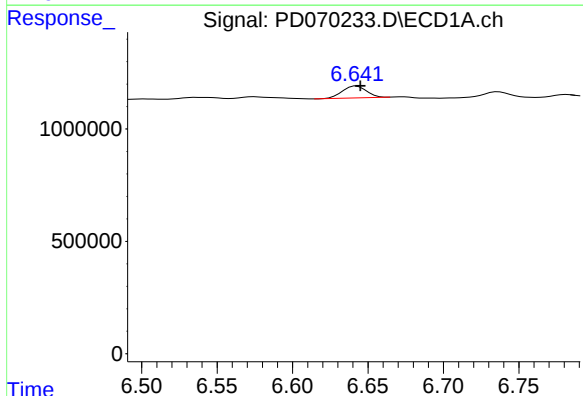


#19 Endosulfan Sulfate

R.T.: 6.642 min
Delta R.T.: -0.002 min
Response: 585170
Conc: 0.49 ng/ml

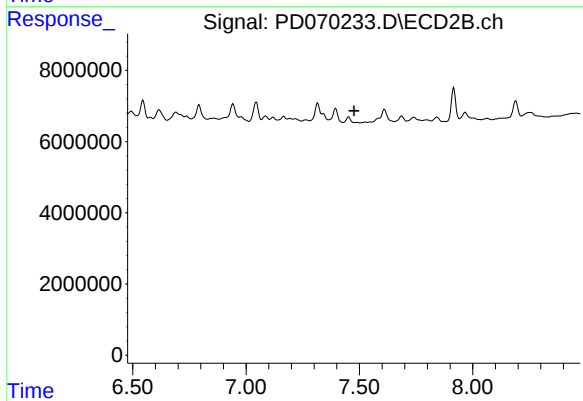

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T.: 7.477 min
Response: 0
Conc: N.D.

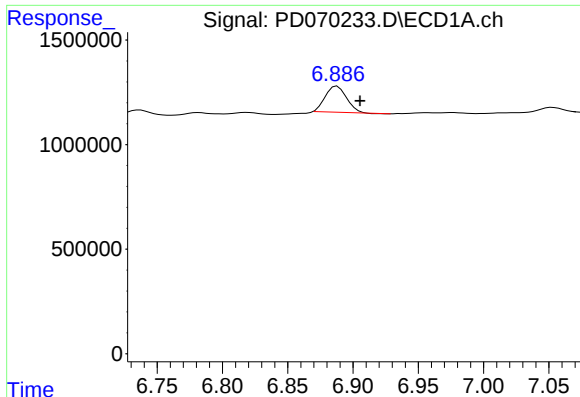

#20 Methoxychlor


R.T.: 6.888 min
Delta R.T.: -0.018 min
Response: 1411839
Conc: 2.29 ng/ml

Instrument :
ECD_D
ClientSampleId :

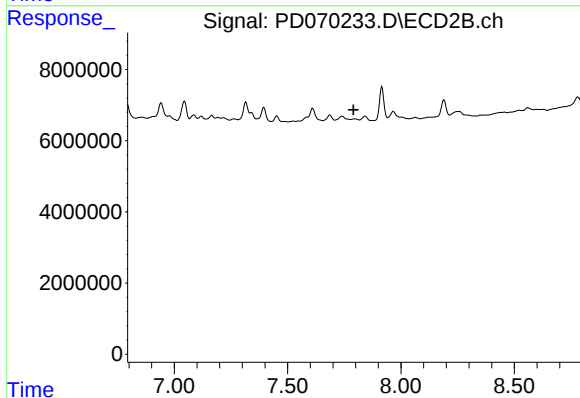


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 7.791 min
Response: 0
Conc: N.D.

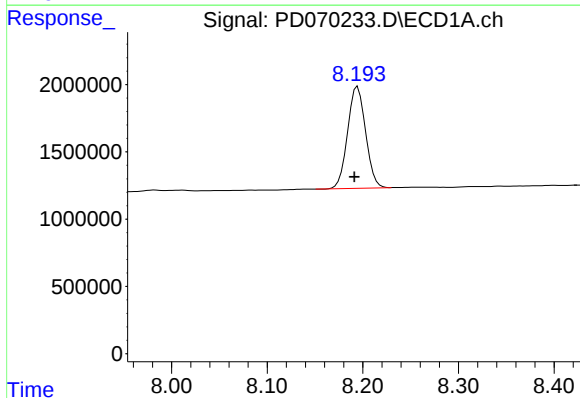

#28 Decachlorobiphenyl

R.T.: 8.195 min
Delta R.T.: 0.003 min
Response: 9917252
Conc: 8.92 ng/ml

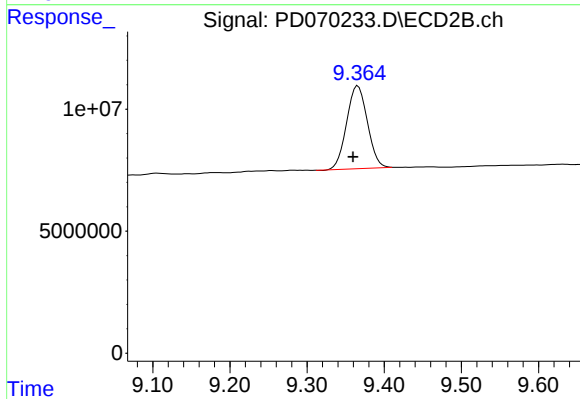

#28 Decachlorobiphenyl

R.T.: 9.366 min
Delta R.T.: 0.006 min
Response: 63423455
Conc: 10.31 ng/ml