

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060922\
 Data File : PD070236.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Jun 2022 13:45
 Operator : AR\AJ
 Sample : N3225-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 09 14:24:51 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060622.M
 Quant Title : GC Extractables
 QLast Update : Wed Jun 08 02:48:31 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.441	4.169	11308290	93807173	10.416	9.610
28)	SA Decachlor...	8.193	9.365	10236751	59667723	9.205	9.701
Target Compounds							
2)	A alpha-BHC	3.873	0.000	1604006	0	0.981	N.D. #
10)	B gamma-Chl...	5.397f	0.000	1830410	0	1.317	N.D. #
11)	B alpha-Chl...	5.436	6.397	1164833	13580447	0.841	1.201 #
12)	B 4,4'-DDE	5.601	6.545	5369486	37795484	4.293	3.605
14)	MA Endrin	5.994	0.000	738598	0	0.613	N.D. #
17)	MA 4,4'-DDT	6.357	7.339	3308265	21481798	3.118	2.503
23)	Chlordane-1	4.311	0.000	963684	0	24.186	N.D. #
25)	Chlordane-3	5.397f	0.000	1830410	0	14.365	N.D. #
26)	Chlordane-4	5.436	6.397	1164833	13580447	10.764	7.971 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060922\
Data File : PD070236.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Jun 2022 13:45
Operator : AR\AJ
Sample : N3225-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 09 14:24:51 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060622.M
Quant Title : GC Extractables
QLast Update : Wed Jun 08 02:48:31 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

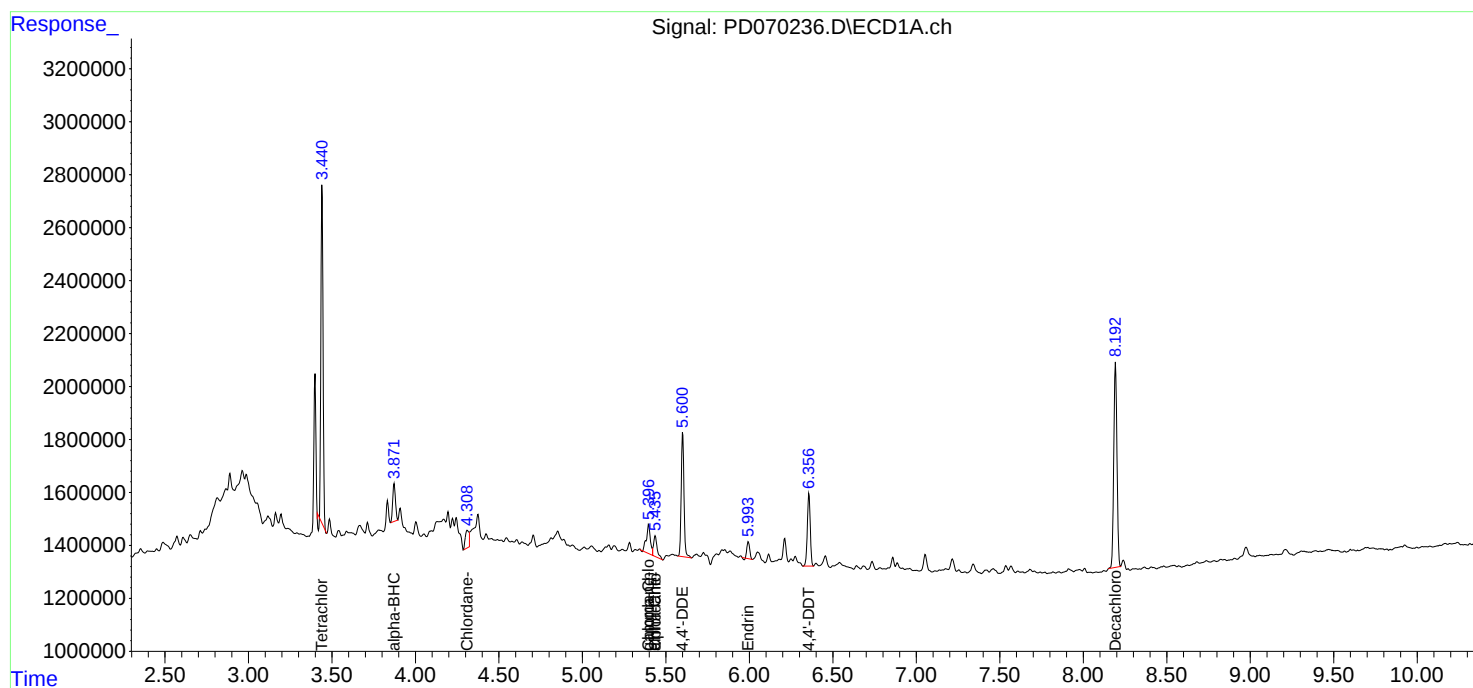


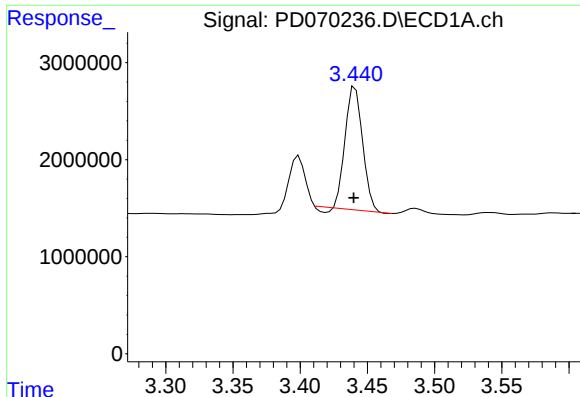

#1 Tetrachloro-m-xylene


R.T.: 3.441 min
Delta R.T.: 0.000 min
Response: 11308290
Conc: 10.42 ng/ml

Instrument :
ECD_D
ClientSampleId :

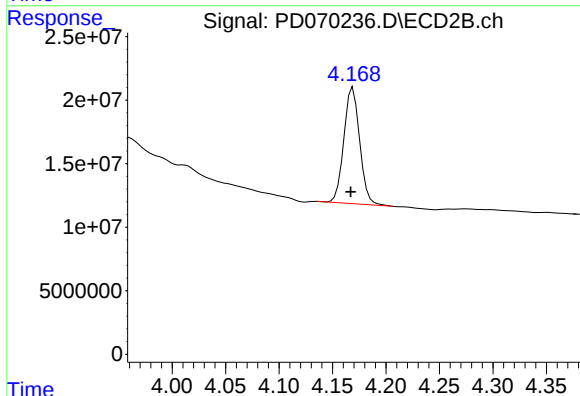


#1 Tetrachloro-m-xylene

R.T.: 4.169 min
Delta R.T.: 0.002 min
Response: 93807173
Conc: 9.61 ng/ml

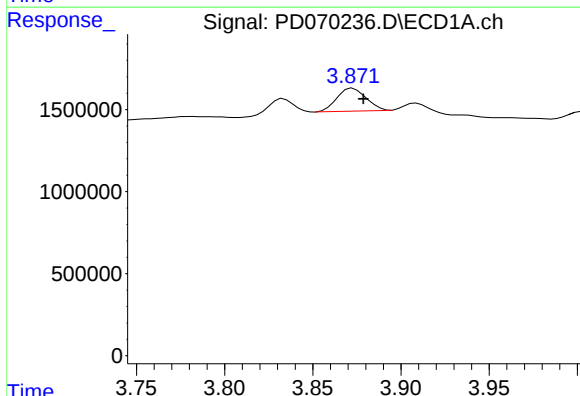


#2 alpha-BHC

R.T.: 3.873 min
Delta R.T.: -0.006 min
Response: 1604006
Conc: 0.98 ng/ml

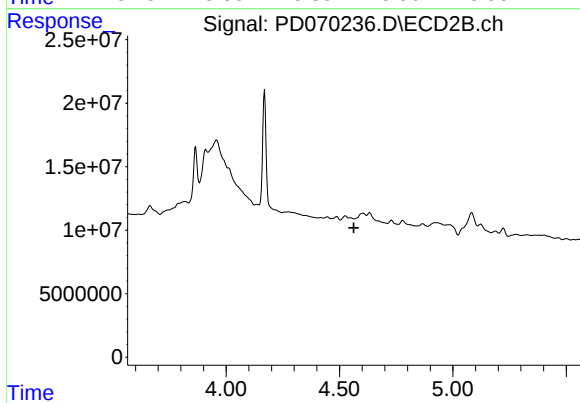

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.563 min
Response: 0
Conc: N.D.

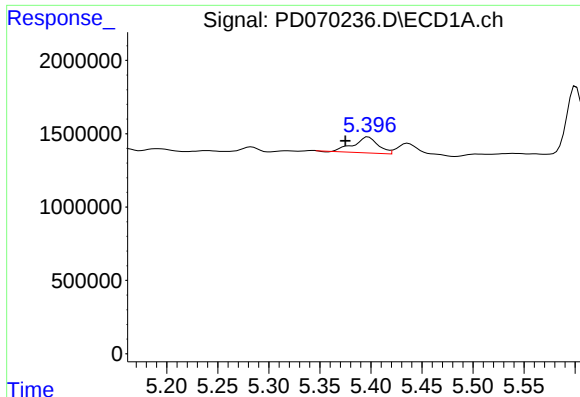

#10 gamma-Chlordane


R.T.: 5.397 min
Delta R.T.: 0.022 min
Response: 1830410
Conc: 1.32 ng/ml

Instrument :
ECD_D
ClientSampleId :

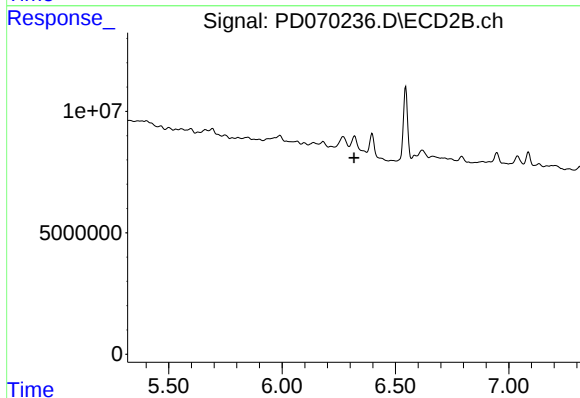


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.318 min
Response: 0
Conc: N.D.

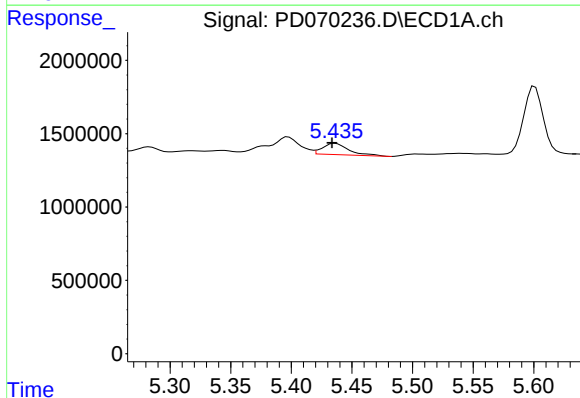


#11 alpha-Chlordane

R.T.: 5.436 min
Delta R.T.: 0.003 min
Response: 1164833
Conc: 0.84 ng/ml

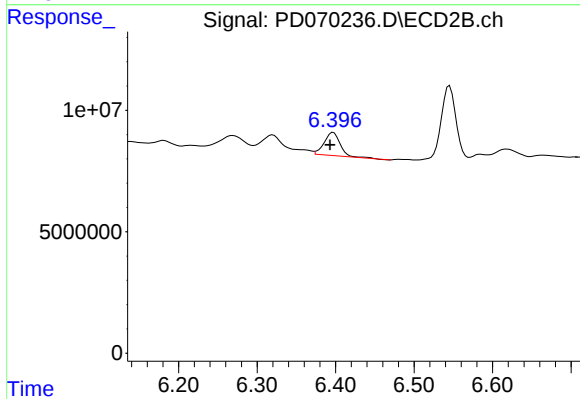

#11 alpha-Chlordane


R.T.: 6.397 min
Delta R.T.: 0.004 min
Response: 13580447
Conc: 1.20 ng/ml

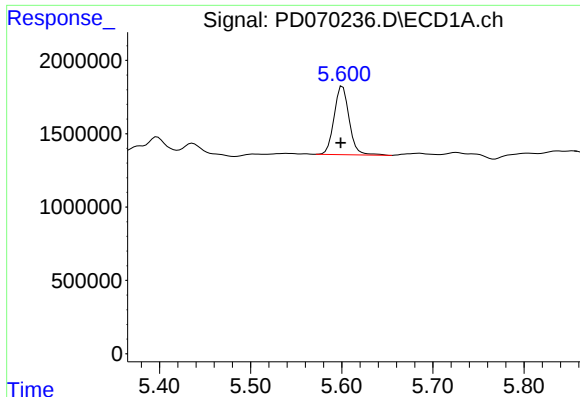

#12 4,4'-DDE


R.T.: 5.601 min
Delta R.T.: 0.002 min
Response: 5369486
Conc: 4.29 ng/ml

Instrument :
ECD_D
ClientSampleId :

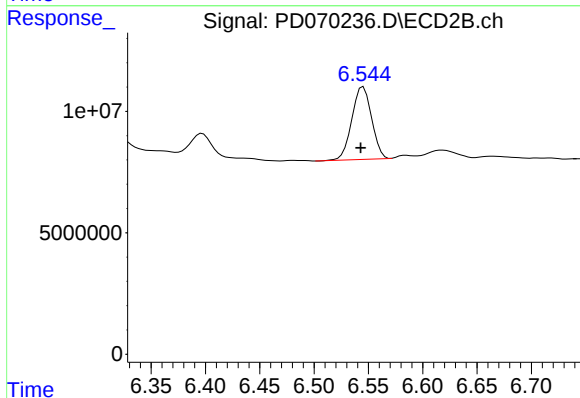


#12 4,4'-DDE

R.T.: 6.545 min
Delta R.T.: 0.002 min
Response: 37795484
Conc: 3.60 ng/ml

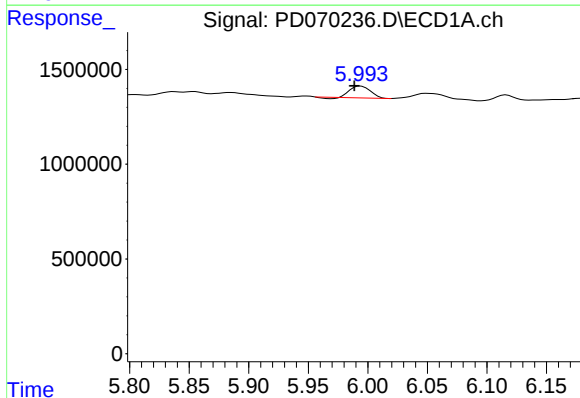


#14 Endrin

R.T.: 5.994 min
Delta R.T.: 0.005 min
Response: 738598
Conc: 0.61 ng/ml

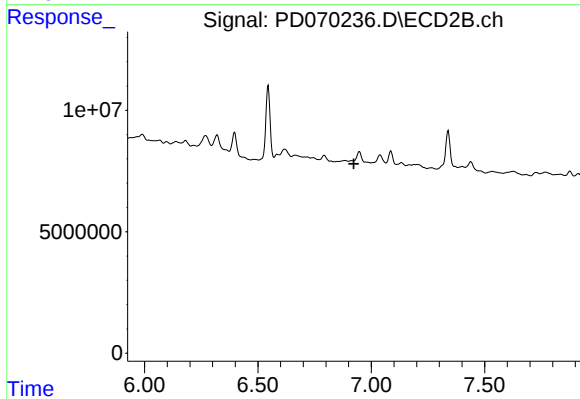

#14 Endrin


R.T.: 0.000 min
Exp R.T. : 6.922 min
Response: 0
Conc: N.D.

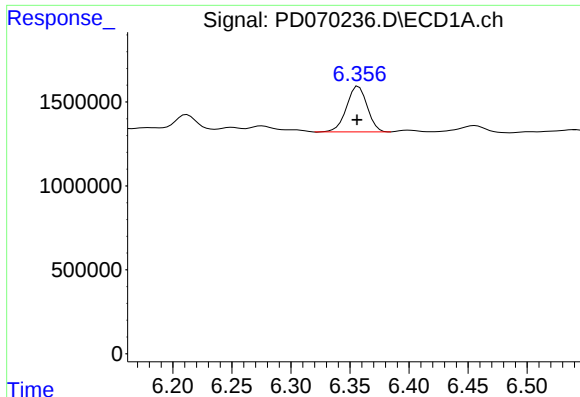

#17 4,4'-DDT


R.T.: 6.357 min
Delta R.T.: 0.001 min
Response: 3308265
Conc: 3.12 ng/ml

Instrument :
ECD_D
ClientSampleId :

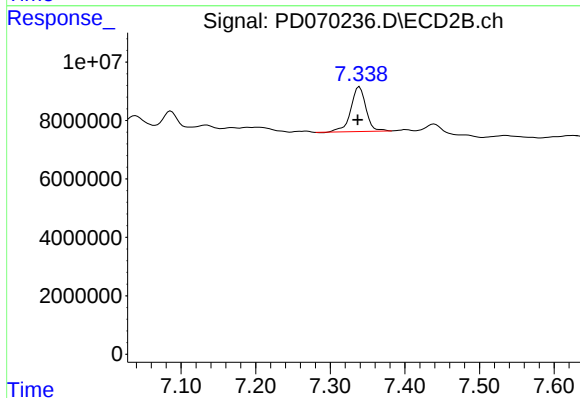


#17 4,4'-DDT

R.T.: 7.339 min
Delta R.T.: 0.002 min
Response: 21481798
Conc: 2.50 ng/ml

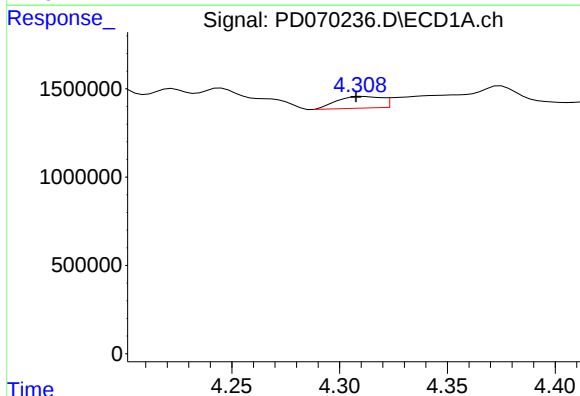


#23 Chlordane-1

R.T.: 4.311 min
Delta R.T.: 0.004 min
Response: 963684
Conc: 24.19 ng/ml

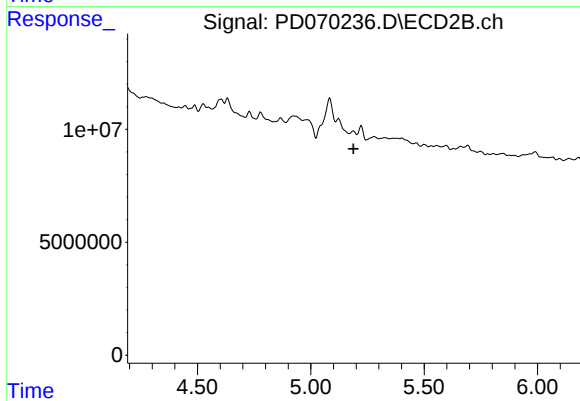

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 5.189 min
Response: 0
Conc: N.D.

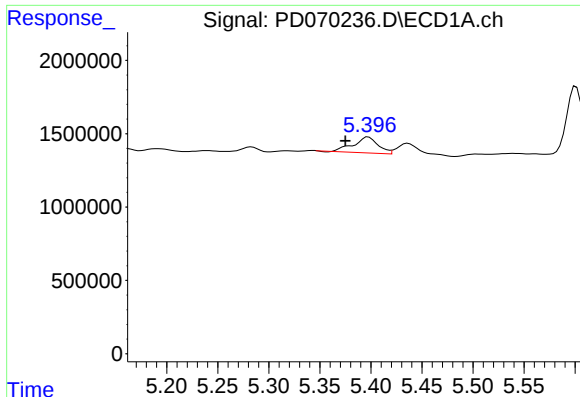

#25 Chlordane-3


R.T.: 5.397 min
Delta R.T.: 0.022 min
Response: 1830410
Conc: 14.36 ng/ml

Instrument :
ECD_D
ClientSampleId :

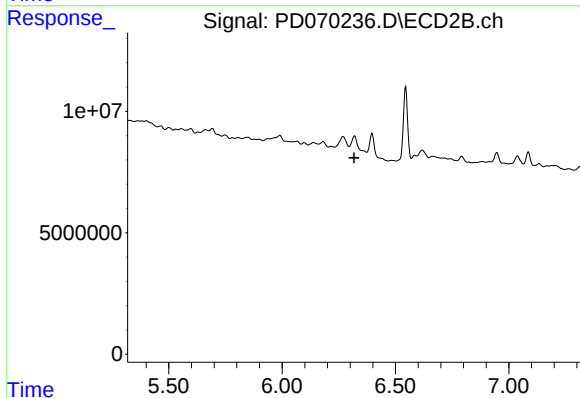


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 6.318 min
Response: 0
Conc: N.D.

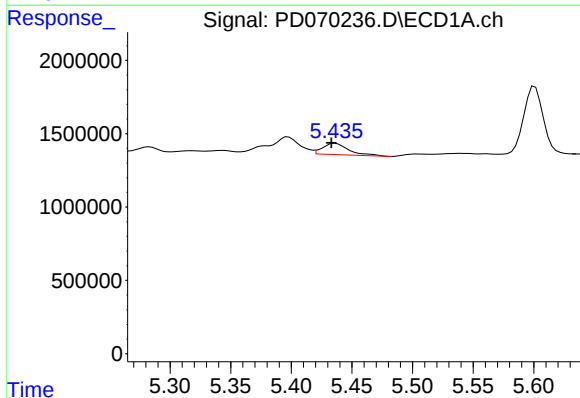


#26 Chlordane-4

R.T.: 5.436 min
Delta R.T.: 0.003 min
Response: 1164833
Conc: 10.76 ng/ml

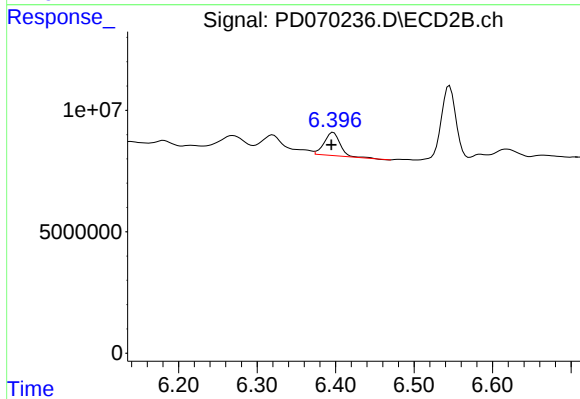

#26 Chlordane-4


R.T.: 6.397 min
Delta R.T.: 0.002 min
Response: 13580447
Conc: 7.97 ng/ml

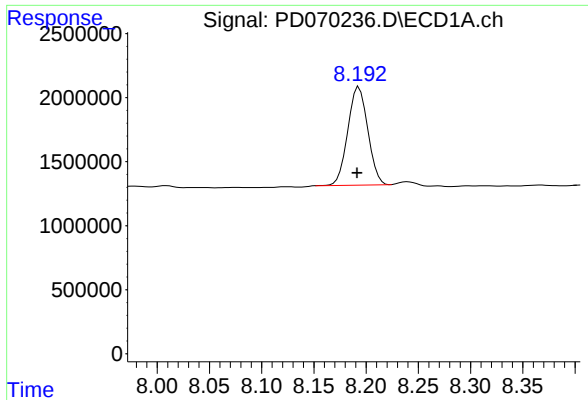

#28 Decachlorobiphenyl

R.T.: 8.193 min
Delta R.T.: 0.002 min
Response: 10236751
Conc: 9.20 ng/ml

Instrument :
ECD_D
ClientSampleId :

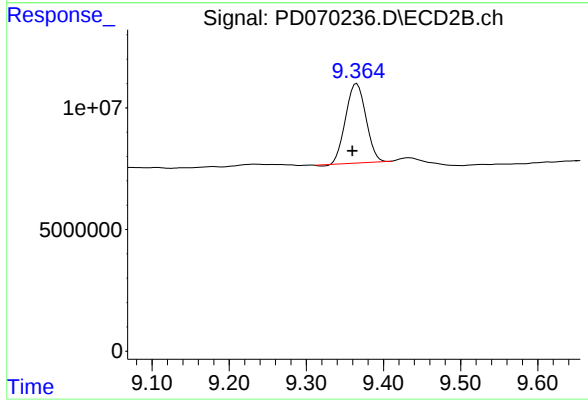

#28 Decachlorobiphenyl

R.T.: 9.365 min
Delta R.T.: 0.006 min
Response: 59667723
Conc: 9.70 ng/ml