

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060922\
 Data File : PD070243.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Jun 2022 15:46
 Operator : AR\AJ
 Sample : N3209-01
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 09 16:41:21 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060622.M
 Quant Title : GC Extractables
 QLast Update : Wed Jun 08 02:48:31 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.447	4.169	10007303	67768546	9.218	6.943
28)	SA Decachlor...	8.201	9.367	11851796	73127848	10.657	11.890
Target Compounds							
12)	B 4,4'-DDE	5.607	6.547	2292552	22619309	1.833	2.157
13)	MA Dieldrin	5.755f	6.693	1582736	7796867	1.175	0.713 #
14)	MA Endrin	6.005f	0.000	883143	0	0.733	N.D. #
16)	A 4,4'-DDD	6.124	7.043	1988875	32815488	1.831	3.902 #
17)	MA 4,4'-DDT	6.360	7.316f	2225863	20992029	2.098	2.446
18)	B Endrin al...	6.453f	0.000	960729	0	1.038	N.D. #
19)	B Endosulfa...	6.648	0.000	1722085	0	1.455	N.D. #
20)	A Methoxychlor	6.894	0.000	4198310	0	6.810	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060922\
Data File : PD070243.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Jun 2022 15:46
Operator : AR\AJ
Sample : N3209-01
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 09 16:41:21 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060622.M
Quant Title : GC Extractables
QLast Update : Wed Jun 08 02:48:31 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

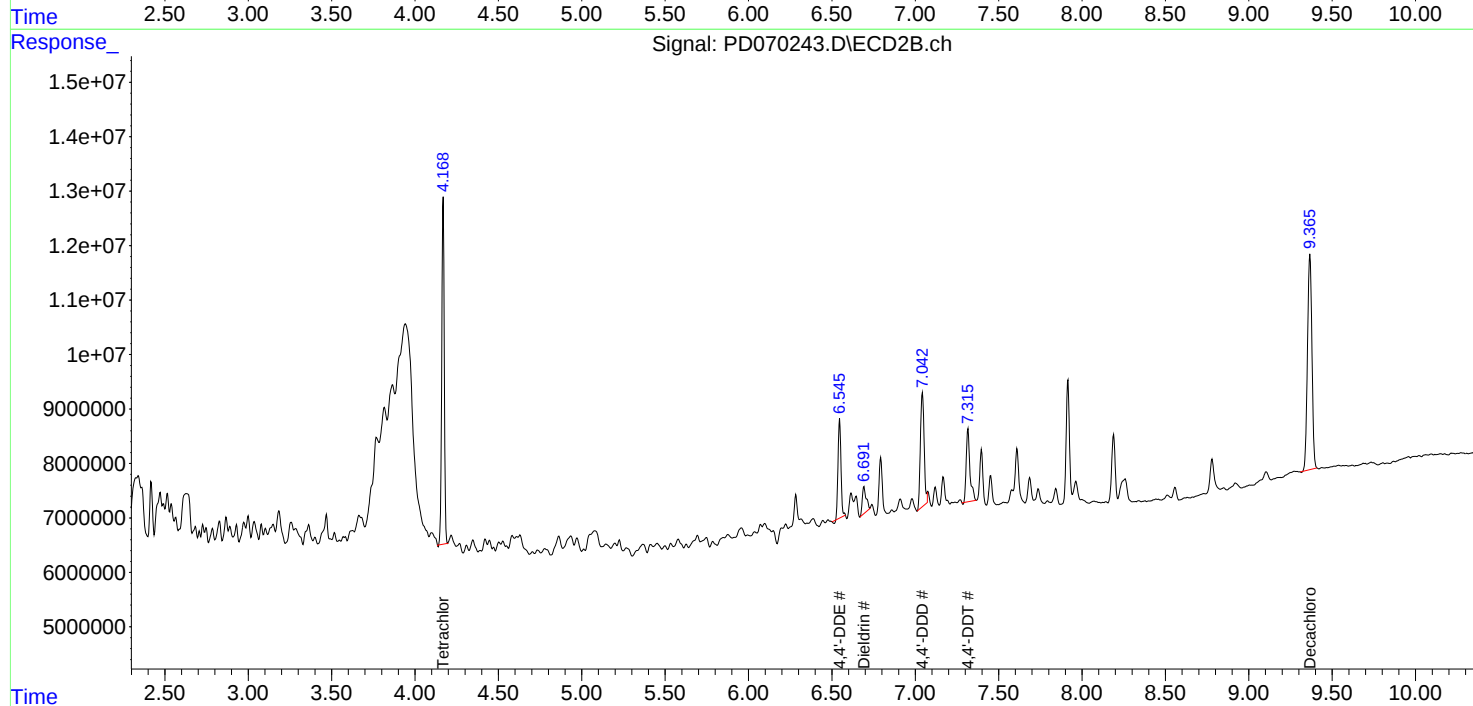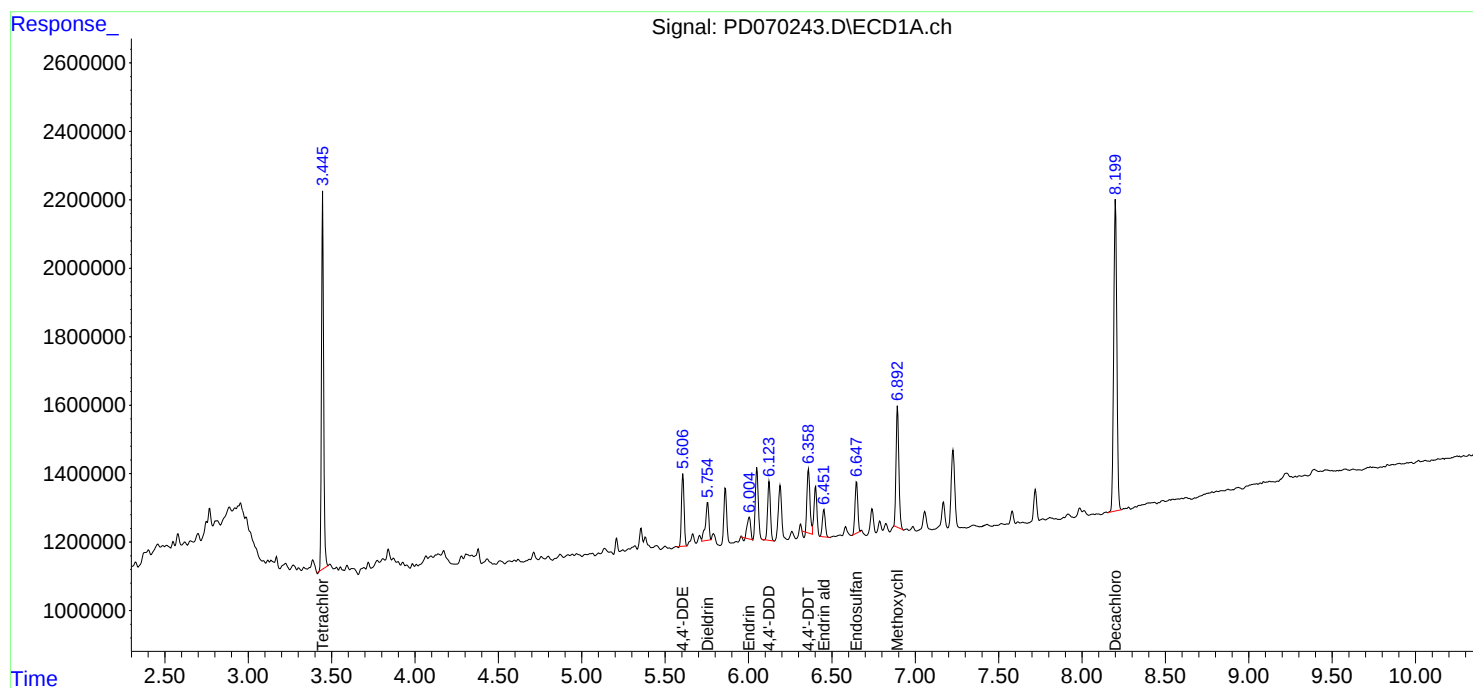


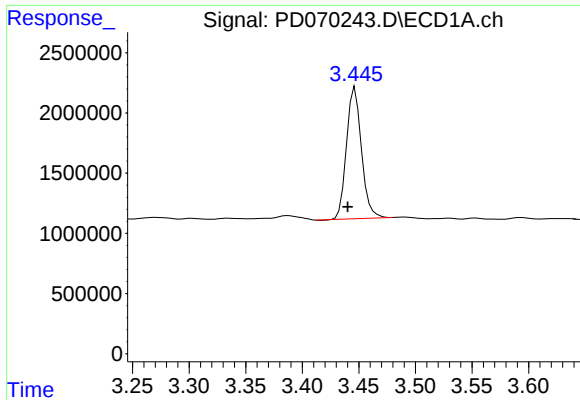

#1 Tetrachloro-m-xylene


R.T.: 3.447 min
Delta R.T.: 0.007 min
Response: 10007303
Conc: 9.22 ng/ml

Instrument :
ECD_D
ClientSampleId :

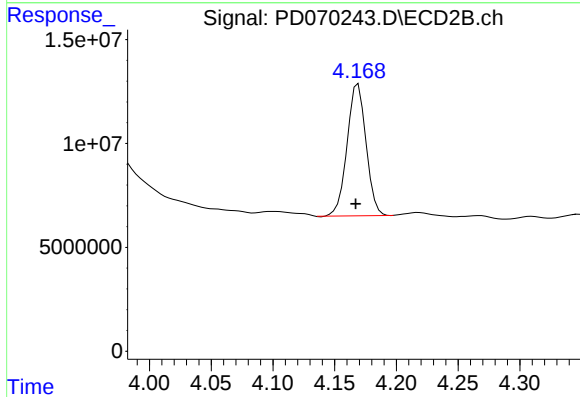


#1 Tetrachloro-m-xylene

R.T.: 4.169 min
Delta R.T.: 0.002 min
Response: 67768546
Conc: 6.94 ng/ml

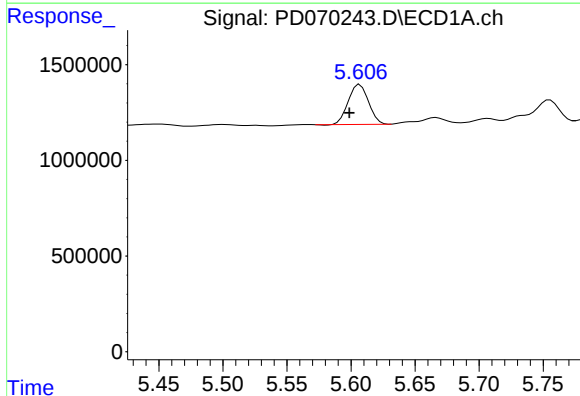


#12 4,4'-DDE

R.T.: 5.607 min
Delta R.T.: 0.008 min
Response: 2292552
Conc: 1.83 ng/ml

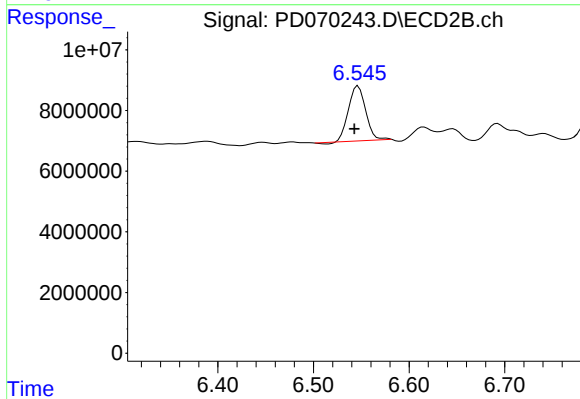

#12 4,4'-DDE


R.T.: 6.547 min
Delta R.T.: 0.004 min
Response: 22619309
Conc: 2.16 ng/ml

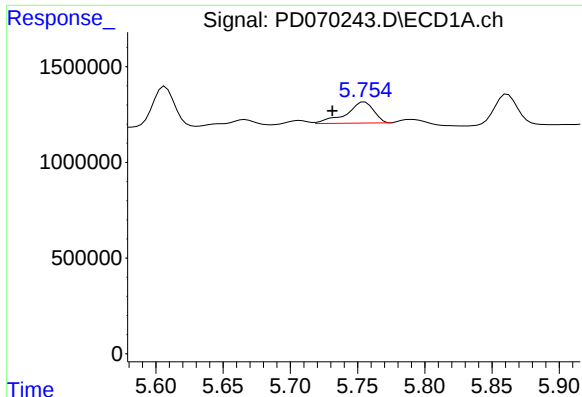

#13 Dieldrin


R.T.: 5.755 min
Delta R.T.: 0.024 min
Response: 1582736
Conc: 1.18 ng/ml

Instrument :
ECD_D
ClientSampleId :

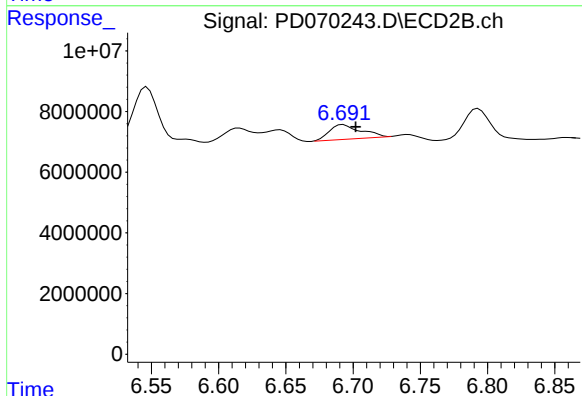


#13 Dieldrin

R.T.: 6.693 min
Delta R.T.: -0.009 min
Response: 7796867
Conc: 0.71 ng/ml

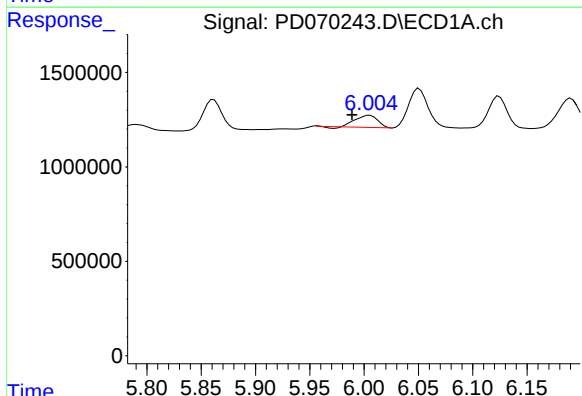


#14 Endrin

R.T.: 6.005 min
Delta R.T.: 0.016 min
Response: 883143
Conc: 0.73 ng/ml

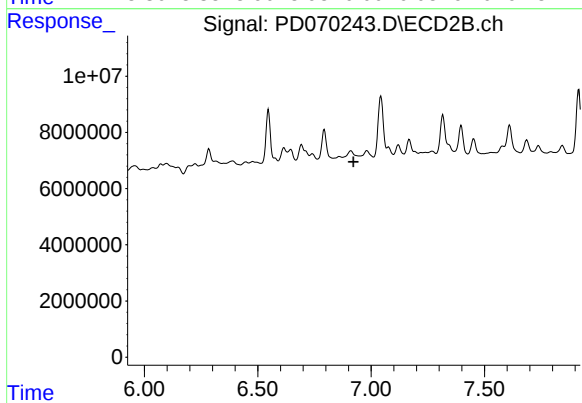

#14 Endrin


R.T.: 0.000 min
Exp R.T. : 6.922 min
Response: 0
Conc: N.D.

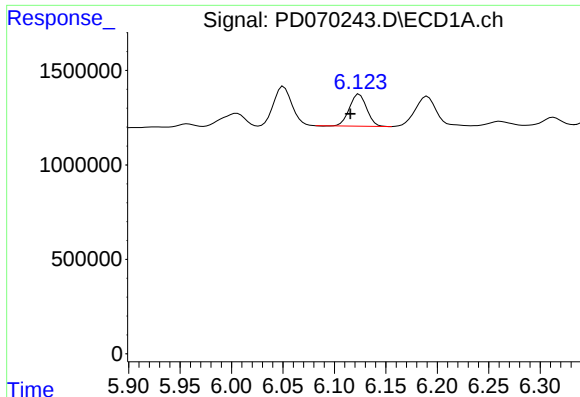

#16 4,4'-DDD


R.T.: 6.124 min
Delta R.T.: 0.009 min
Response: 1988875
Conc: 1.83 ng/ml

Instrument :
ECD_D
ClientSampleId :

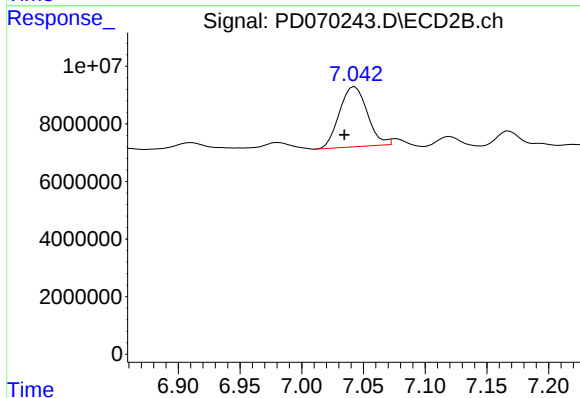


#16 4,4'-DDD

R.T.: 7.043 min
Delta R.T.: 0.008 min
Response: 32815488
Conc: 3.90 ng/ml

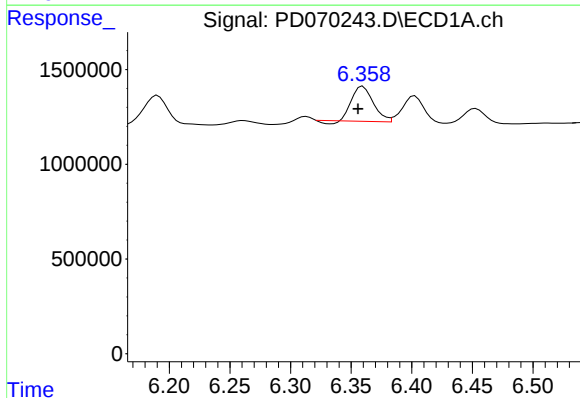


#17 4,4'-DDT

R.T.: 6.360 min
Delta R.T.: 0.004 min
Response: 2225863
Conc: 2.10 ng/ml

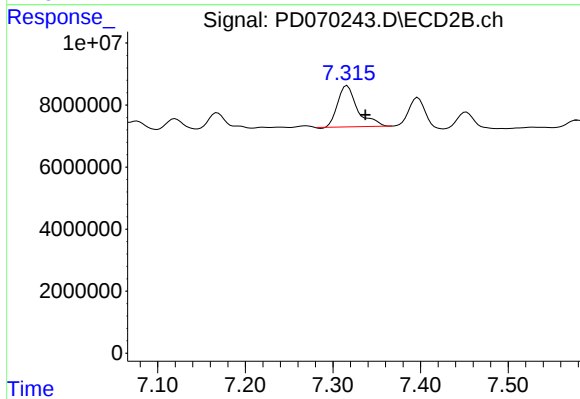

#17 4,4'-DDT


R.T.: 7.316 min
Delta R.T.: -0.021 min
Response: 20992029
Conc: 2.45 ng/ml

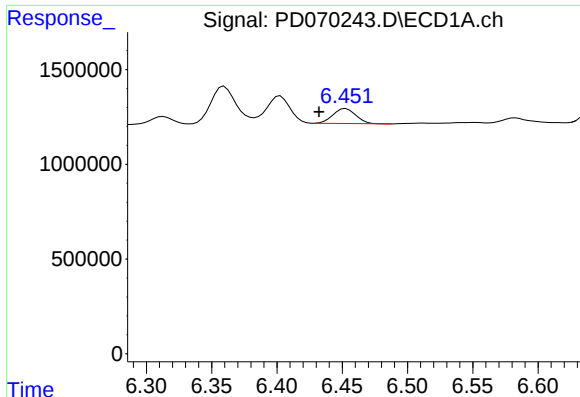

#18 Endrin aldehyde


R.T.: 6.453 min
Delta R.T.: 0.021 min
Response: 960729
Conc: 1.04 ng/ml

Instrument :
ECD_D
ClientSampleId :

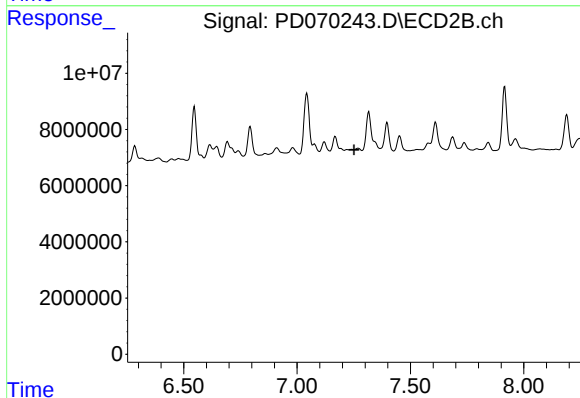


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T. : 7.252 min
Response: 0
Conc: N.D.

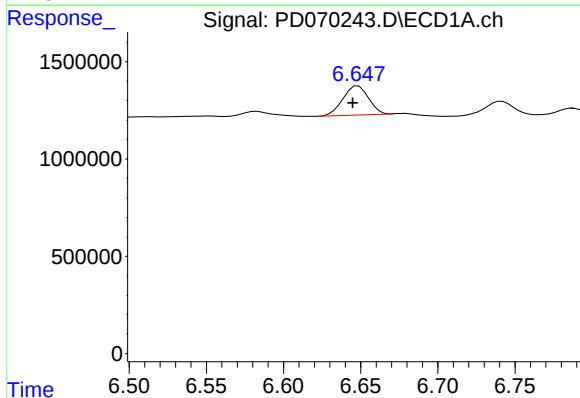


#19 Endosulfan Sulfate

R.T.: 6.648 min
Delta R.T.: 0.003 min
Response: 1722085
Conc: 1.46 ng/ml

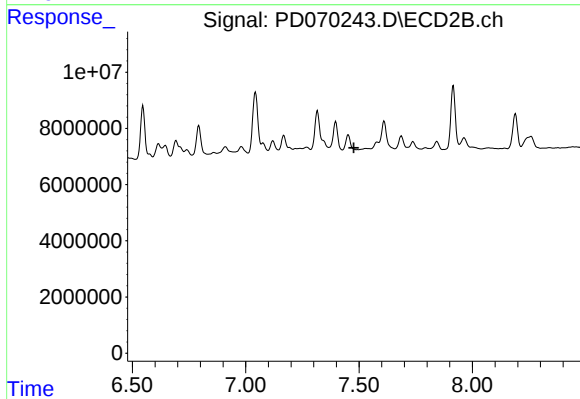

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T. : 7.477 min
Response: 0
Conc: N.D.

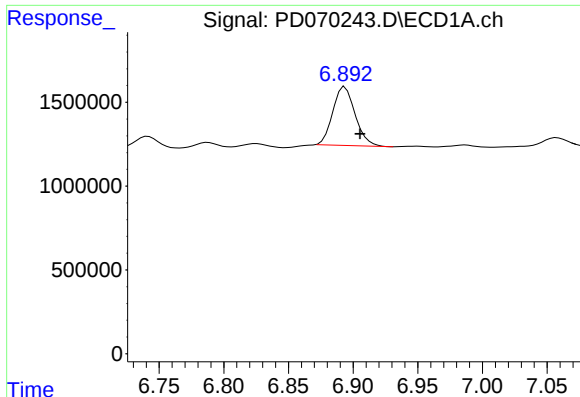

#20 Methoxychlor


R.T.: 6.894 min
Delta R.T.: -0.012 min
Response: 4198310
Conc: 6.81 ng/ml

Instrument :
ECD_D
ClientSampleId :

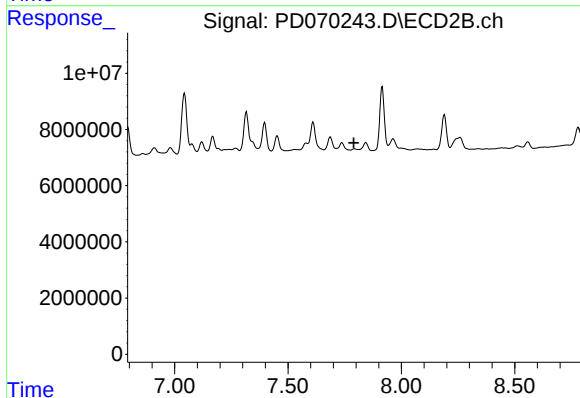


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 7.791 min
Response: 0
Conc: N.D.

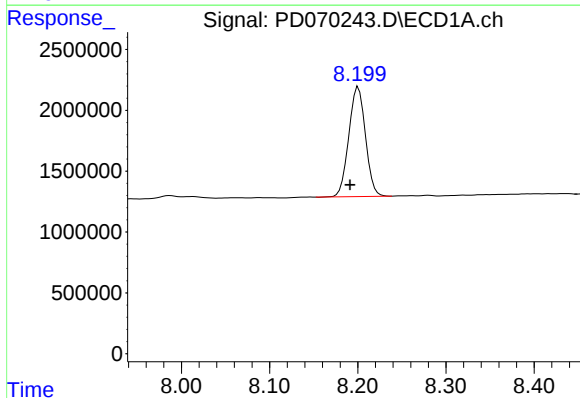

#28 Decachlorobiphenyl

R.T.: 8.201 min
Delta R.T.: 0.009 min
Response: 11851796
Conc: 10.66 ng/ml

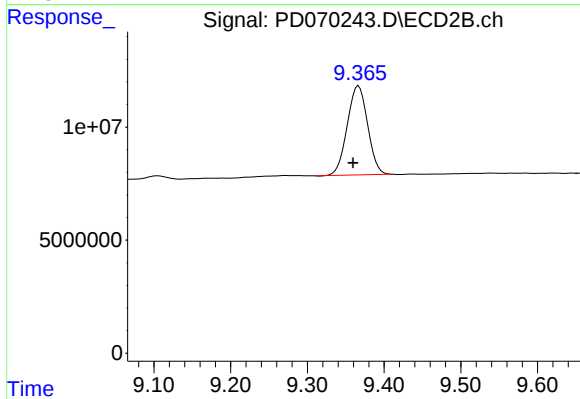

#28 Decachlorobiphenyl

R.T.: 9.367 min
Delta R.T.: 0.007 min
Response: 73127848
Conc: 11.89 ng/ml