

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060923\
 Data File : PD075734.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Jun 2023 12:22
 Operator : AR\AJ
 Sample : PIBLK161
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 09 21:33:49 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060223CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 02 04:01:43 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.547	2.769	48391510	23297799	24.207	22.979
27)	SA Decachlor...	9.089	7.915	117.7E6	48527994	51.306	51.675
Target Compounds							
4)	MA Heptachlor	4.944	0.000	2942853	0	0.907	N.D. #
8)	B Heptachlo...	0.000	4.812f	0	307956	N.D.	0.234
14)	MA Endrin	0.000	5.653	0	112840	N.D.	<MDL
20)	A Methoxychlor	0.000	6.590	0	166697	N.D.	0.345
23)	Toxaphene-2	0.000	5.653	0	112840	N.D.	15.949
25)	Toxaphene-4	0.000	6.590	0	166697	N.D.	8.066
26)	Toxaphene-5	0.000	6.717	0	104230	N.D.	3.219


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060923\
Data File : PD075734.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Jun 2023 12:22
Operator : AR\AJ
Sample : PIBLK161
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 09 21:33:49 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060223CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jun 02 04:01:43 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

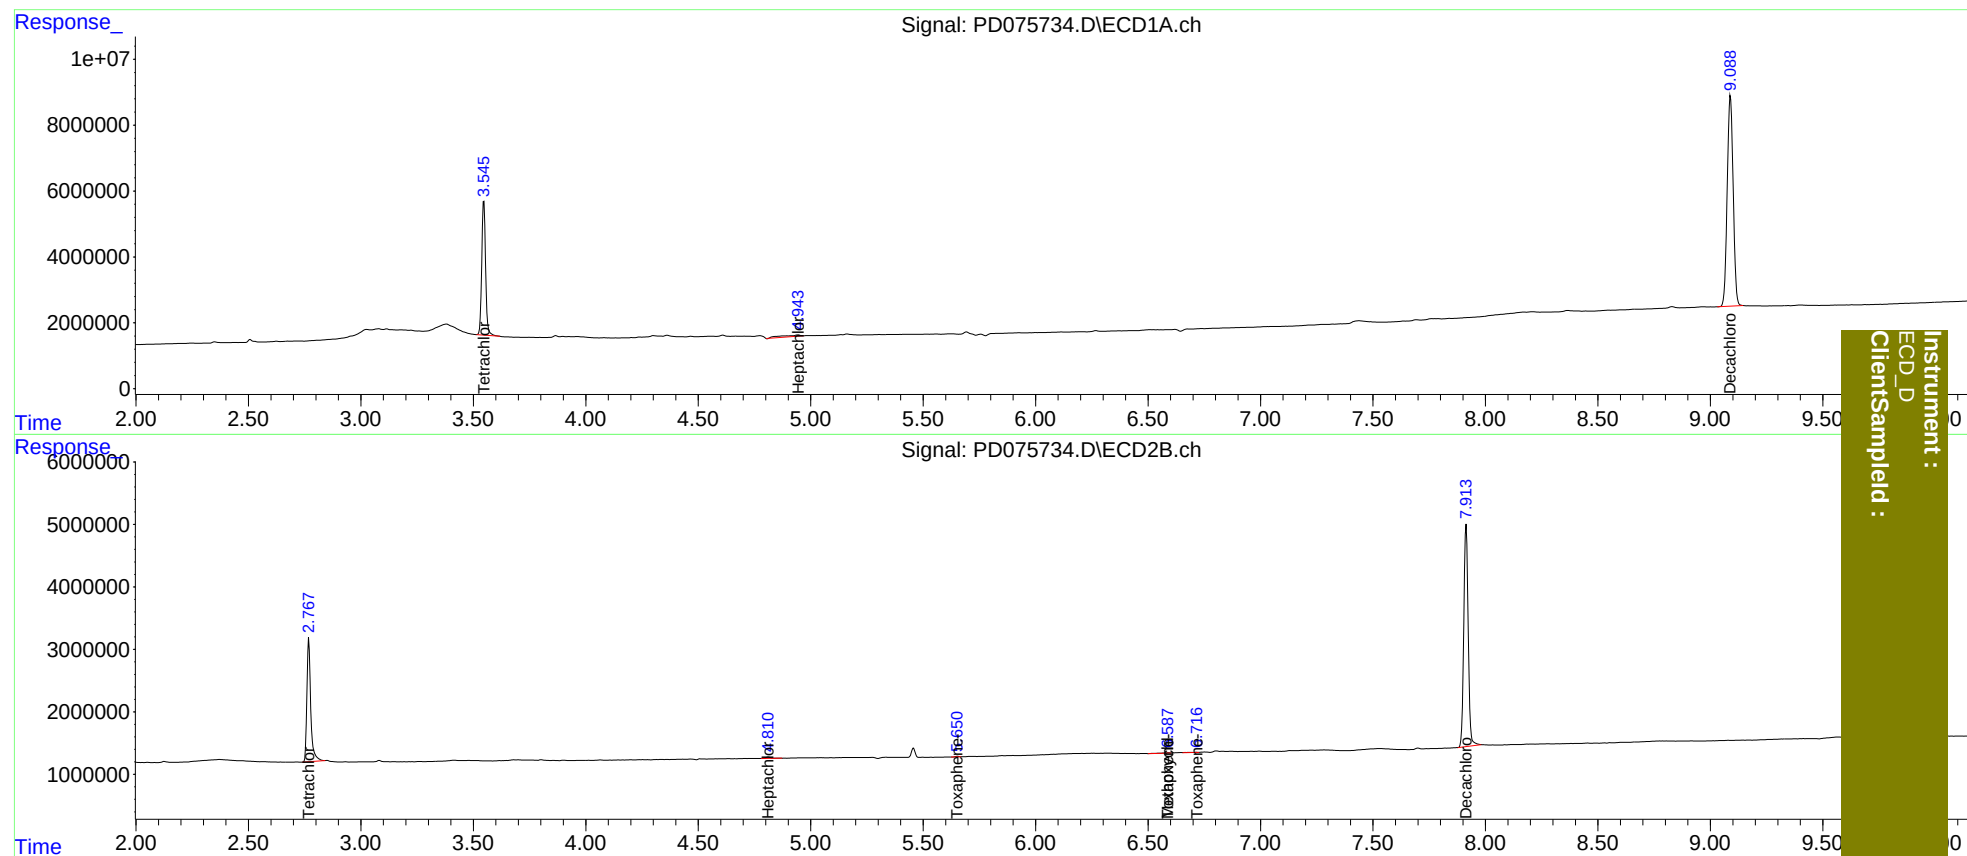


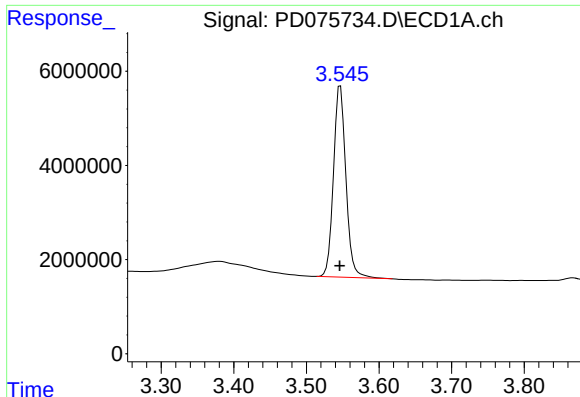

#1 Tetrachloro-m-xylene


R.T.: 3.547 min
Delta R.T.: 0.000 min
Response: 48391510
Conc: 24.21 ng/ml

Instrument :
ECD_D
ClientSampleId :

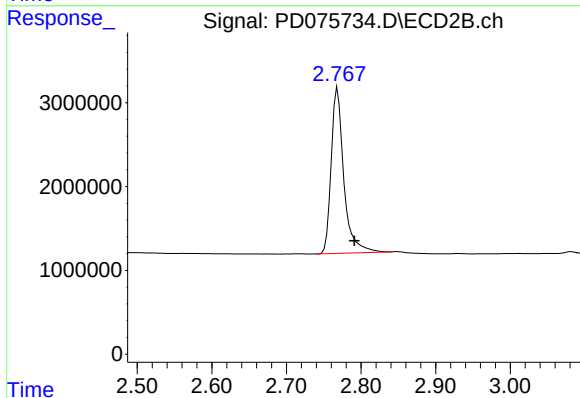


#1 Tetrachloro-m-xylene

R.T.: 2.769 min
Delta R.T.: -0.023 min
Response: 23297799
Conc: 22.98 ng/ml

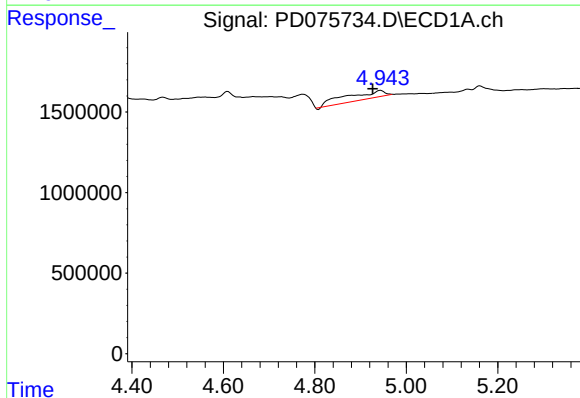


#4 Heptachlor

R.T.: 4.944 min
Delta R.T.: 0.017 min
Response: 2942853
Conc: 0.91 ng/ml

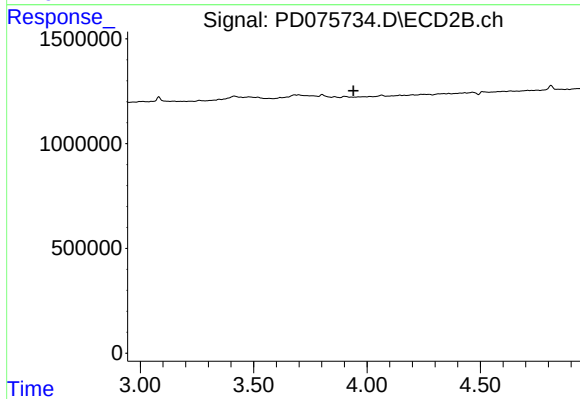

#4 Heptachlor


R.T.: 0.000 min
Exp R.T. : 3.941 min
Response: 0
Conc: N.D.

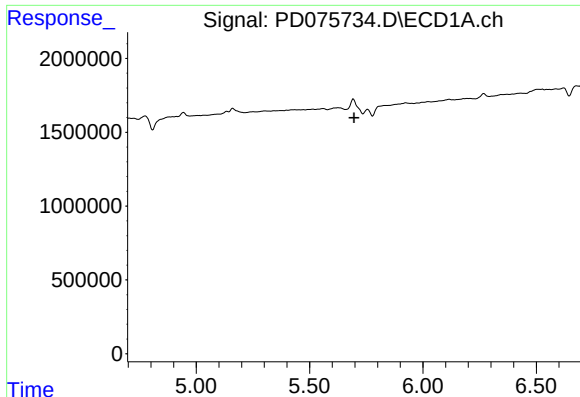

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.697 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

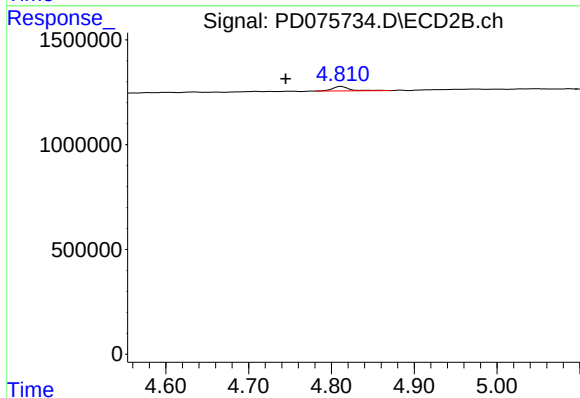


#8 Heptachlor epoxide

R.T.: 4.812 min
Delta R.T.: 0.067 min
Response: 307956
Conc: 0.23 ng/ml

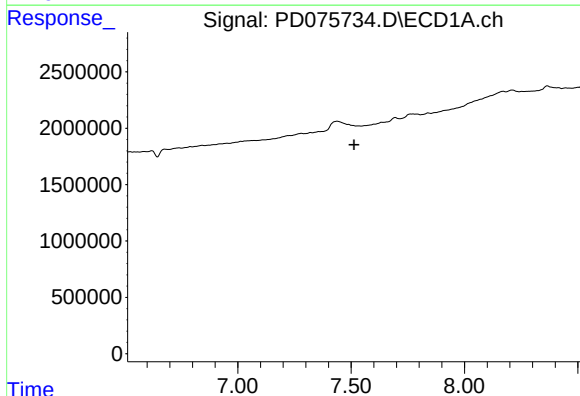


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T.: 7.514 min
Response: 0
Conc: N.D.

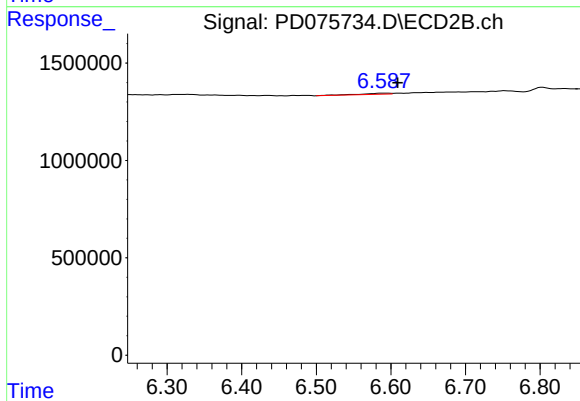

#20 Methoxychlor


R.T.: 6.590 min
Delta R.T.: -0.019 min
Response: 166697
Conc: 0.35 ng/ml

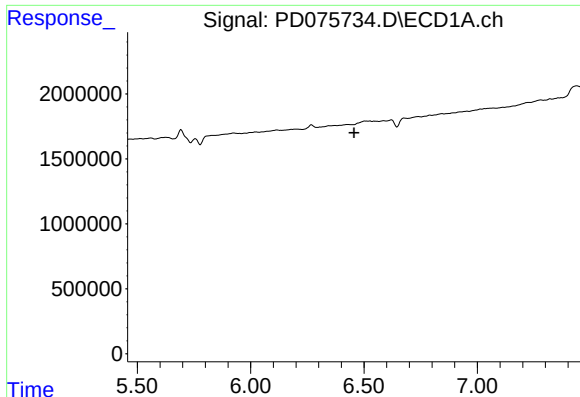

#23 Toxaphene-2


R.T.: 0.000 min
Exp R.T.: 6.457 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

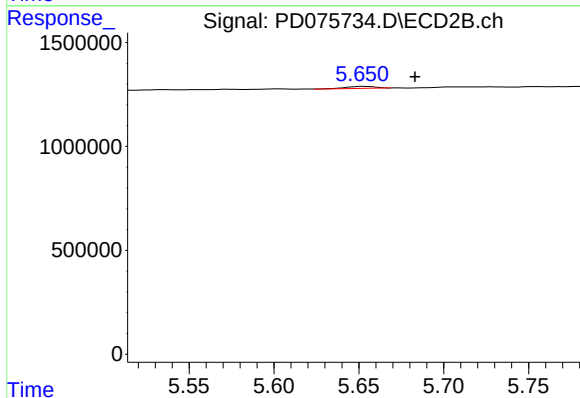


#23 Toxaphene-2

R.T.: 5.653 min
Delta R.T.: -0.030 min
Response: 112840
Conc: 15.95 ng/ml

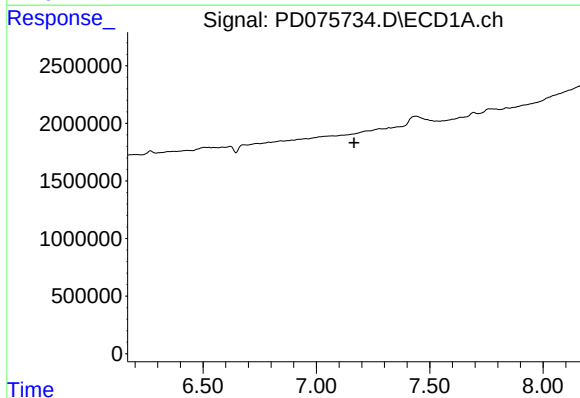


#25 Toxaphene-4

R.T.: 0.000 min
Exp R.T.: 7.166 min
Response: 0
Conc: N.D.

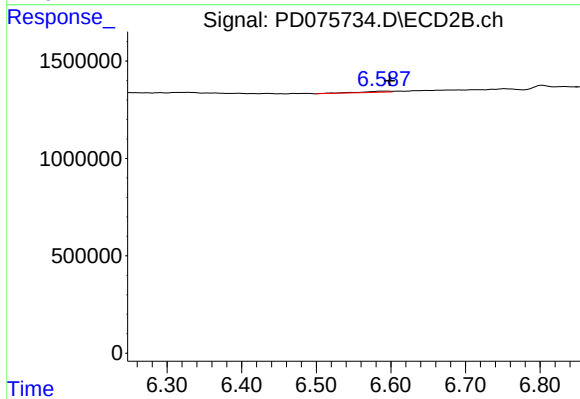

#25 Toxaphene-4


R.T.: 6.590 min
Delta R.T.: -0.008 min
Response: 166697
Conc: 8.07 ng/ml

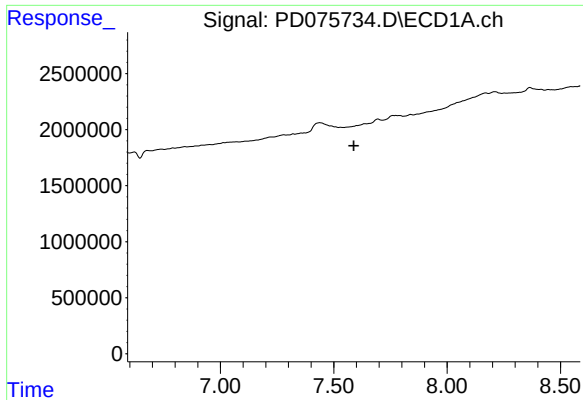

#26 Toxaphene-5


R.T.: 0.000 min
Exp R.T.: 7.589 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

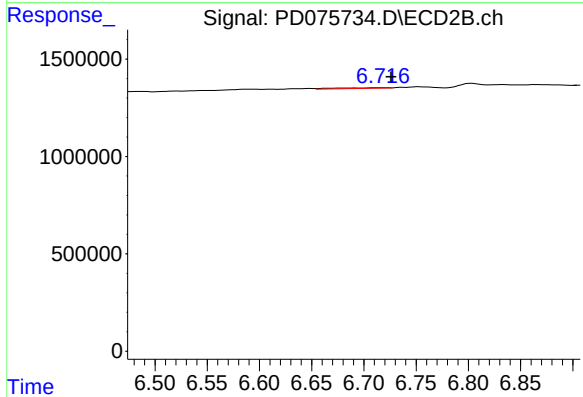


#26 Toxaphene-5

R.T.: 6.717 min
Delta R.T.: -0.009 min
Response: 104230
Conc: 3.22 ng/ml

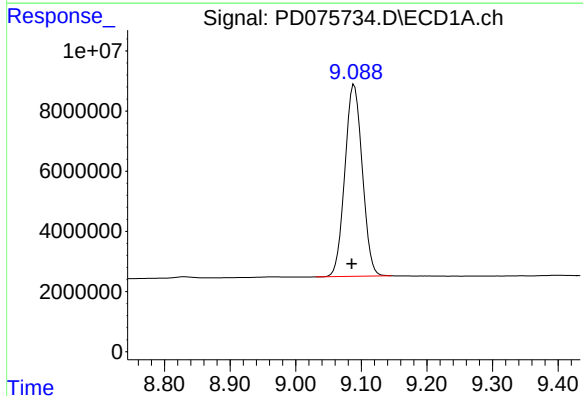

#27 Decachlorobiphenyl

R.T.: 9.089 min
Delta R.T.: 0.004 min
Response: 117672948
Conc: 51.31 ng/ml

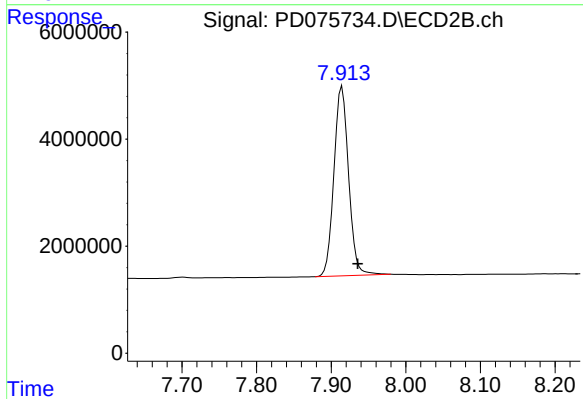

#27 Decachlorobiphenyl

R.T.: 7.915 min
Delta R.T.: -0.021 min
Response: 48527994
Conc: 51.67 ng/ml