

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060923\
 Data File : PD075742.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Jun 2023 15:56
 Operator : AR\AJ
 Sample : 03097-05
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 09 21:42:54 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060223CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 02 04:01:43 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.547	2.769	33099964	15669090	16.557	15.455
27)	SA Decachlor...	9.089	7.914	67474406	27346458	29.419	29.120
Target Compounds							
8)	B Heptachlo...	0.000	4.723	0	465172	N.D.	0.354
9)	A Endosulfan I	6.039f	0.000	1492377	0	0.563	N.D. #
10)	B trans-Chl...	0.000	4.998	0	500586	N.D.	0.394
11)	B cis-Chlor...	6.039	5.018f	1492377	358302	0.496	0.275 #
12)	B 4,4'-DDE	6.206	5.227	2093145	807893	0.747	0.710
13)	MA Dieldrin	6.360	5.358	3549725	1337167	1.193	1.026
15)	B Endosulfa...	0.000	5.888f	0	1242863	N.D.	1.106
17)	MA 4,4'-DDT	0.000	6.025	0	204960	N.D.	0.252
20)	A Methoxychlor	0.000	6.629	0	302119	N.D.	0.626
22)	Toxaphene-1	6.206f	4.998	2093145	500586	102.372	70.248 #
24)	Toxaphene-3	0.000	6.025f	0	204960	N.D.	24.267
25)	Toxaphene-4	0.000	6.629	0	302119	N.D.	14.618


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060923\
Data File : PD075742.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Jun 2023 15:56
Operator : AR\AJ
Sample : 03097-05
Misc :
ALS Vial : 23 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 09 21:42:54 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060223CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jun 02 04:01:43 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

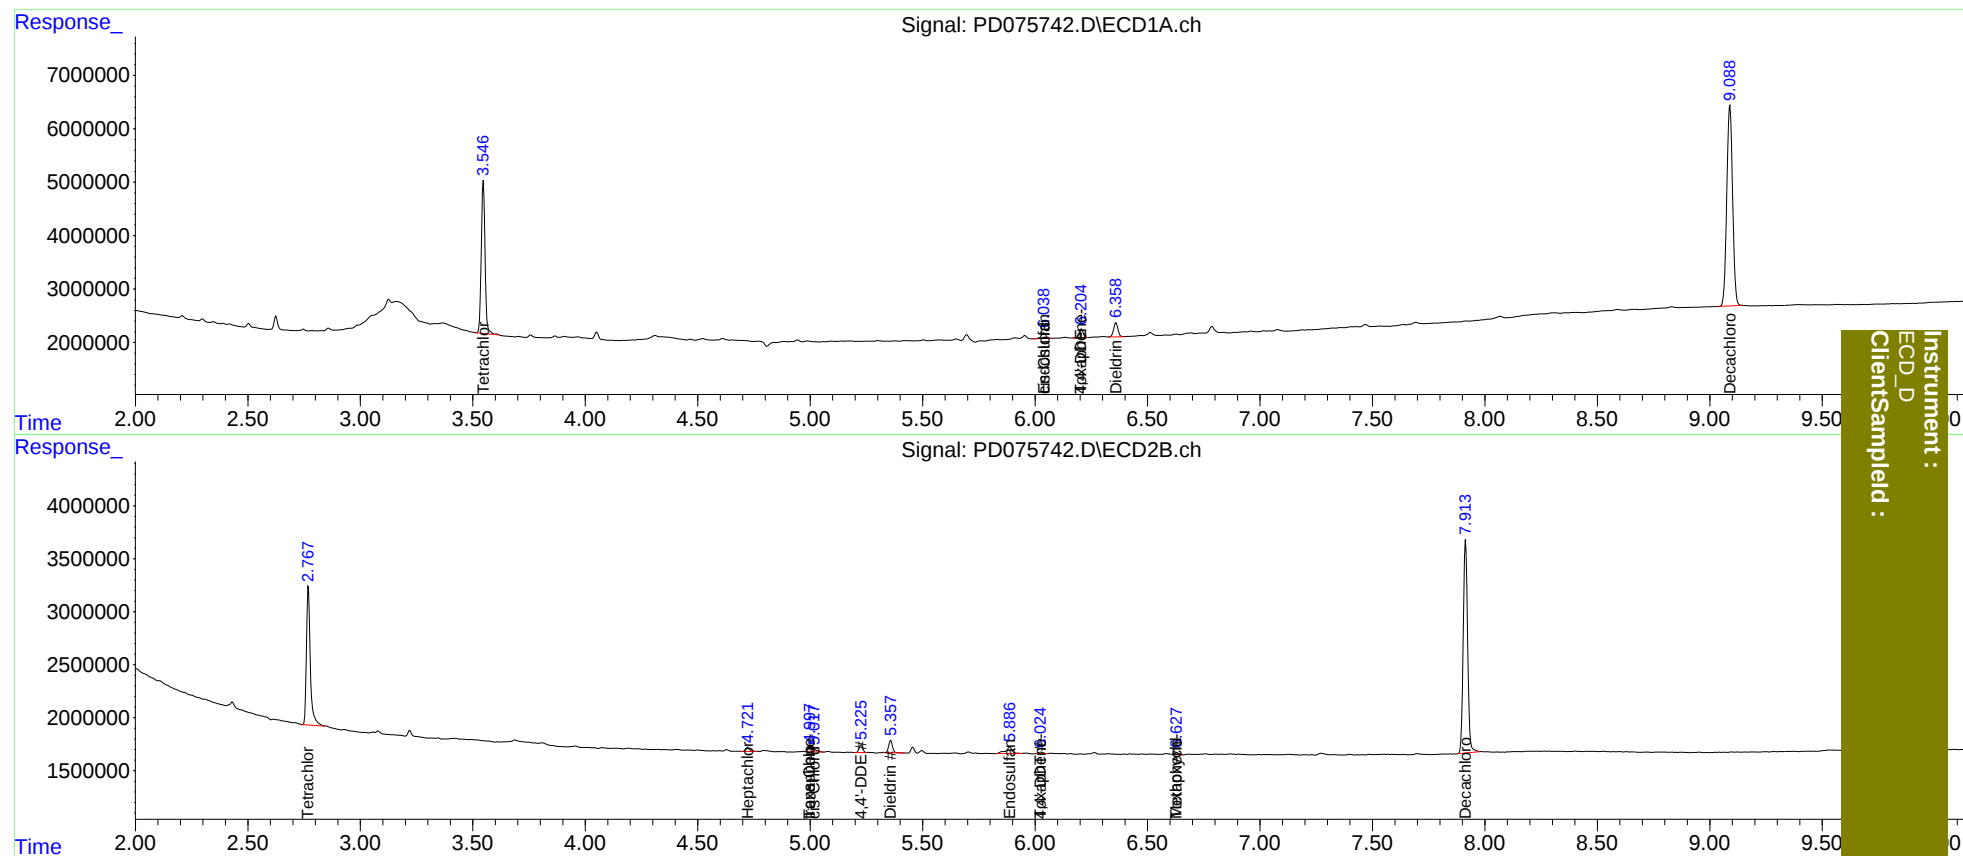


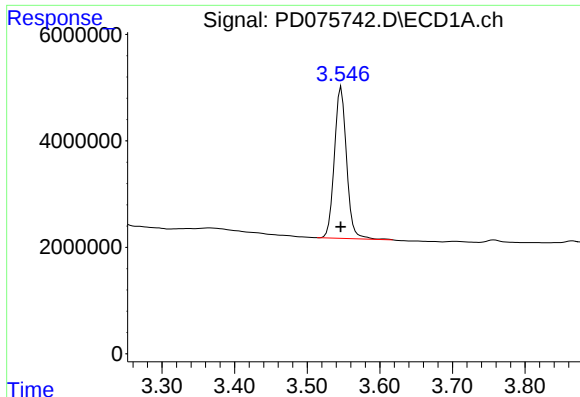

#1 Tetrachloro-m-xylene


R.T.: 3.547 min
Delta R.T.: 0.000 min
Response: 33099964
Conc: 16.56 ng/ml

Instrument :
ECD_D
ClientSampleId :

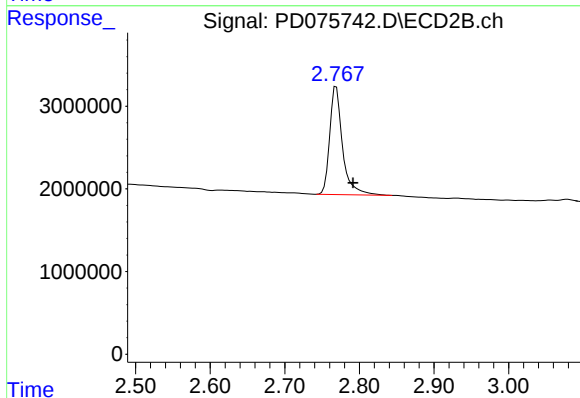


#1 Tetrachloro-m-xylene

R.T.: 2.769 min
Delta R.T.: -0.022 min
Response: 15669090
Conc: 15.45 ng/ml

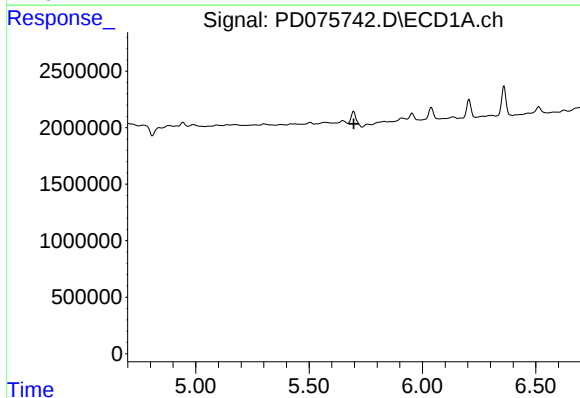


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.697 min
Response: 0
Conc: N.D.

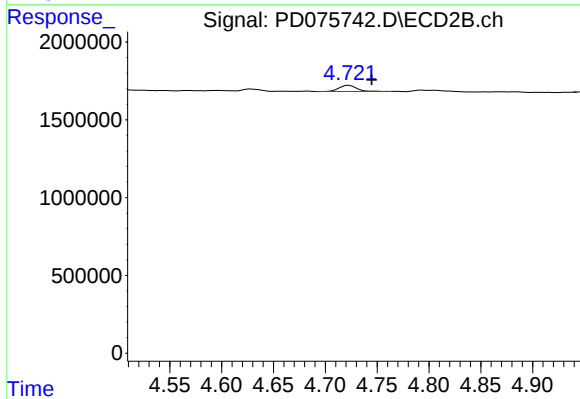

#8 Heptachlor epoxide


R.T.: 4.723 min
Delta R.T.: -0.022 min
Response: 465172
Conc: 0.35 ng/ml

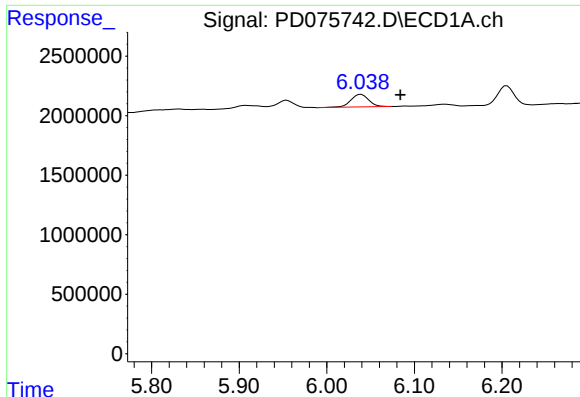

#9 Endosulfan I


R.T.: 6.039 min
Delta R.T.: -0.045 min
Response: 1492377
Conc: 0.56 ng/ml

Instrument :
ECD_D
ClientSampleId :

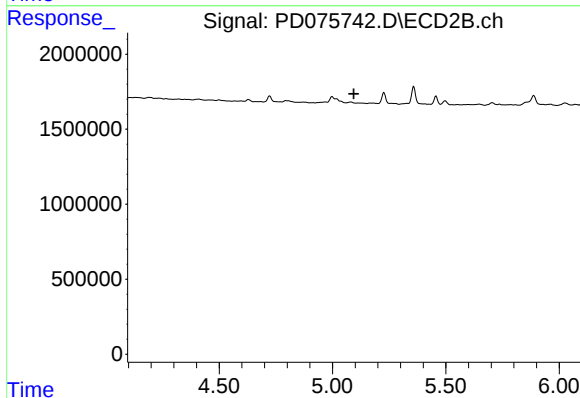


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 5.093 min
Response: 0
Conc: N.D.

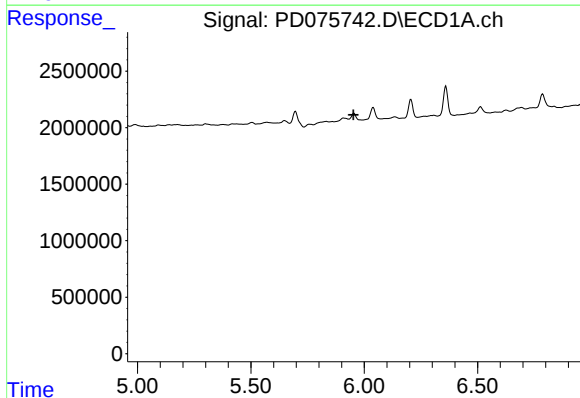


#10 trans-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.953 min
Response: 0
Conc: N.D.

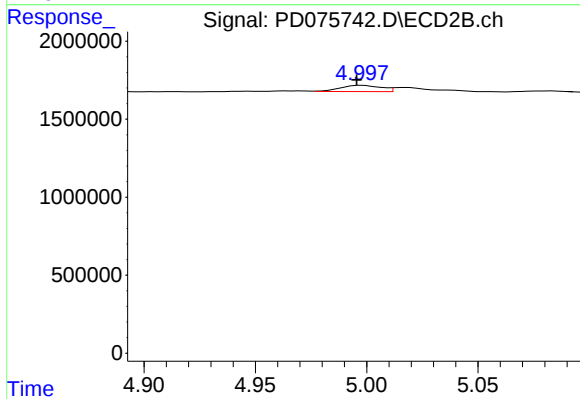

#10 trans-Chlordane


R.T.: 4.998 min
Delta R.T.: 0.003 min
Response: 500586
Conc: 0.39 ng/ml

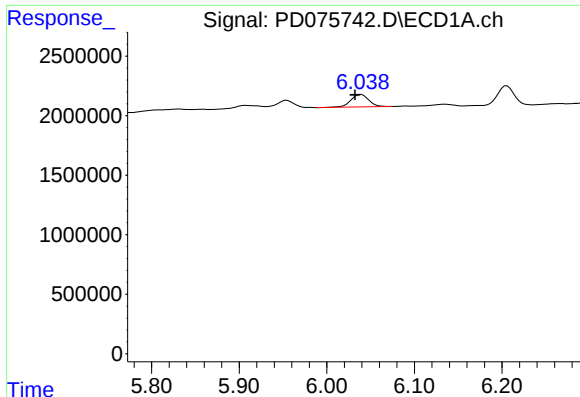

#11 cis-Chlordane


R.T.: 6.039 min
Delta R.T.: 0.007 min
Response: 1492377
Conc: 0.50 ng/ml

Instrument :
ECD_D
ClientSampleId :

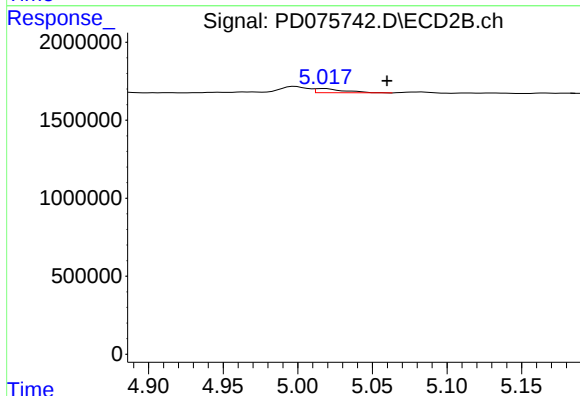


#11 cis-Chlordane

R.T.: 5.018 min
Delta R.T.: -0.042 min
Response: 358302
Conc: 0.27 ng/ml

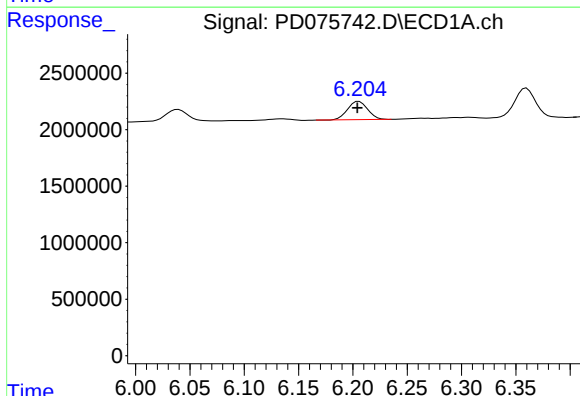


#12 4,4'-DDE

R.T.: 6.206 min
Delta R.T.: 0.001 min
Response: 2093145
Conc: 0.75 ng/ml

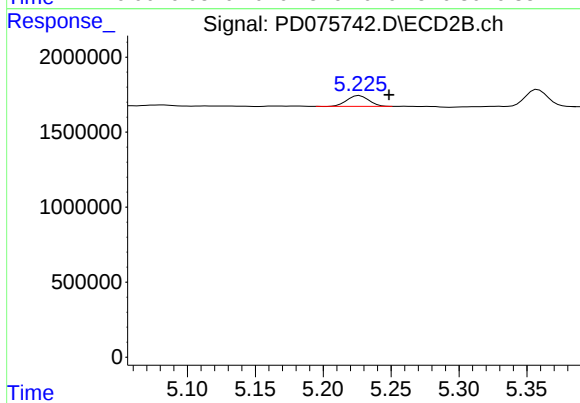

#12 4,4'-DDE


R.T.: 5.227 min
Delta R.T.: -0.022 min
Response: 807893
Conc: 0.71 ng/ml

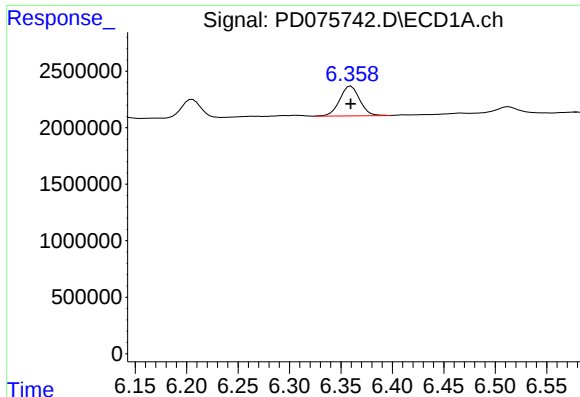

#13 Dieldrin


R.T.: 6.360 min
Delta R.T.: 0.000 min
Response: 3549725
Conc: 1.19 ng/ml

Instrument :
ECD_D
ClientSampleId :

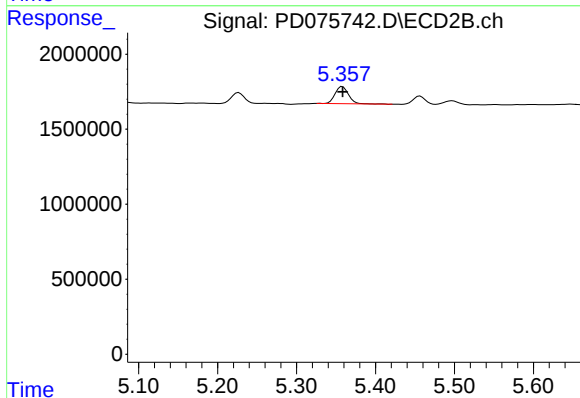


#13 Dieldrin

R.T.: 5.358 min
Delta R.T.: 0.000 min
Response: 1337167
Conc: 1.03 ng/ml

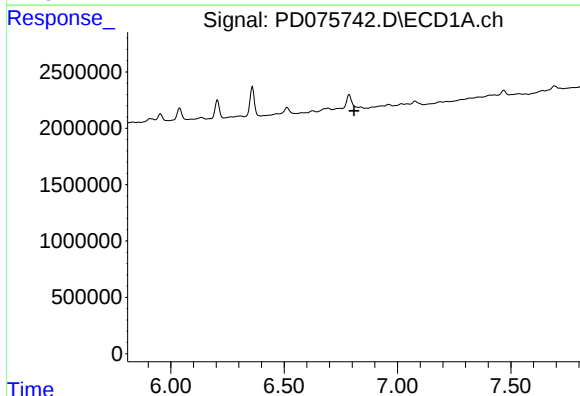


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.809 min
Response: 0
Conc: N.D.

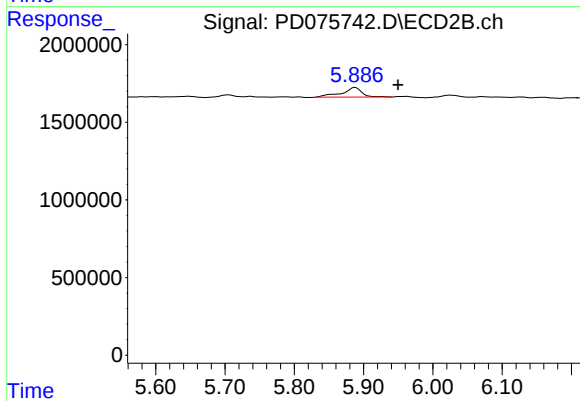

#15 Endosulfan II


R.T.: 5.888 min
Delta R.T.: -0.062 min
Response: 1242863
Conc: 1.11 ng/ml

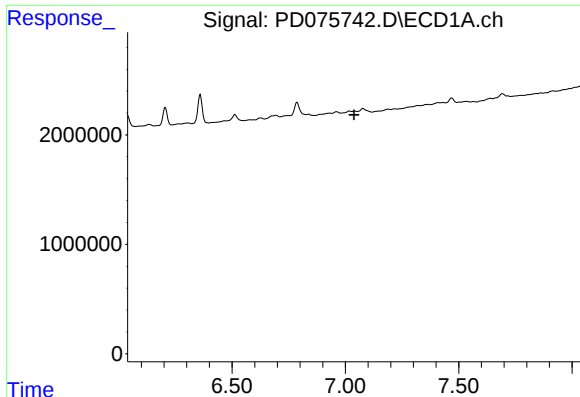

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 7.039 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

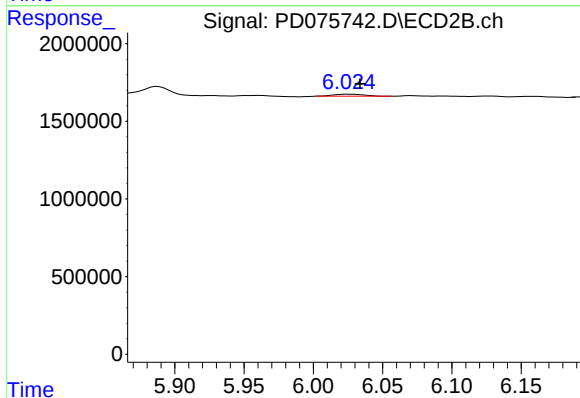


#17 4,4'-DDT

R.T.: 6.025 min
Delta R.T.: -0.008 min
Response: 204960
Conc: 0.25 ng/ml

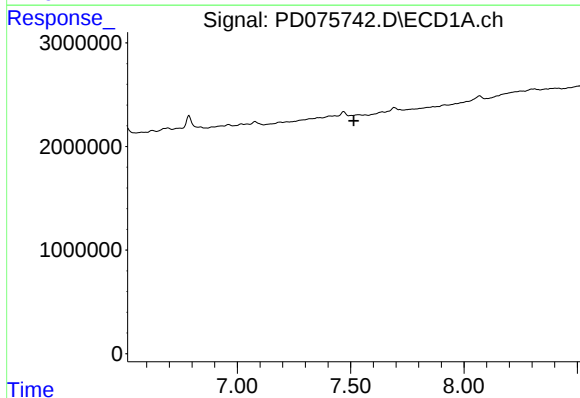


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T.: 7.514 min
Response: 0
Conc: N.D.

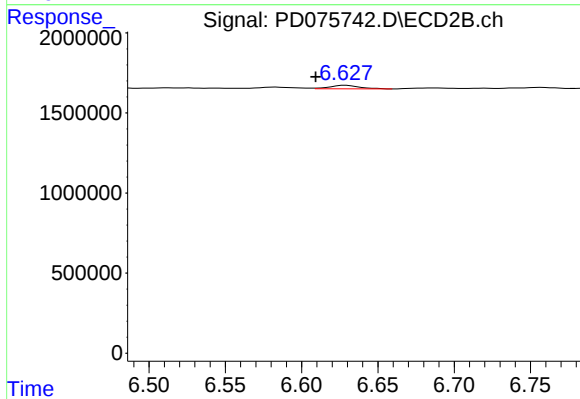

#20 Methoxychlor


R.T.: 6.629 min
Delta R.T.: 0.020 min
Response: 302119
Conc: 0.63 ng/ml

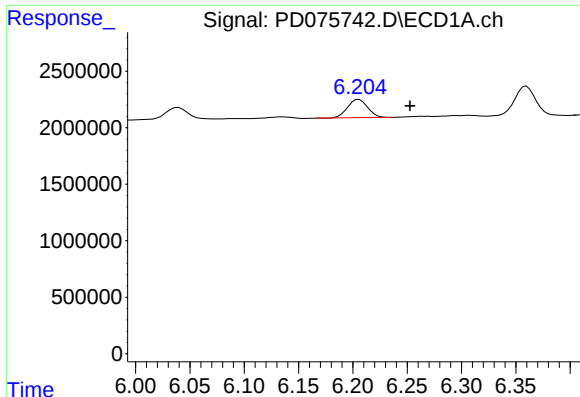

#22 Toxaphene-1


R.T.: 6.206 min
Delta R.T.: -0.047 min
Response: 2093145
Conc: 102.37 ng/ml

Instrument :
ECD_D
ClientSampleId :

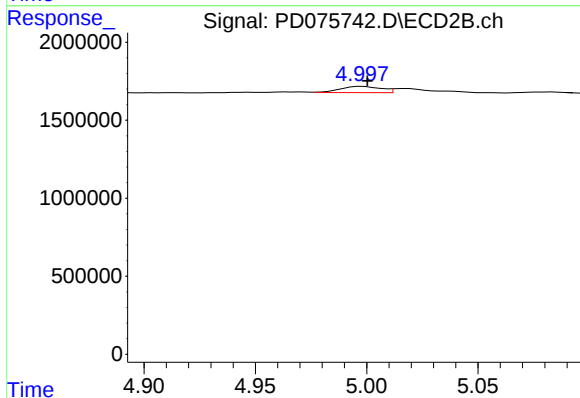


#22 Toxaphene-1

R.T.: 4.998 min
Delta R.T.: -0.002 min
Response: 500586
Conc: 70.25 ng/ml

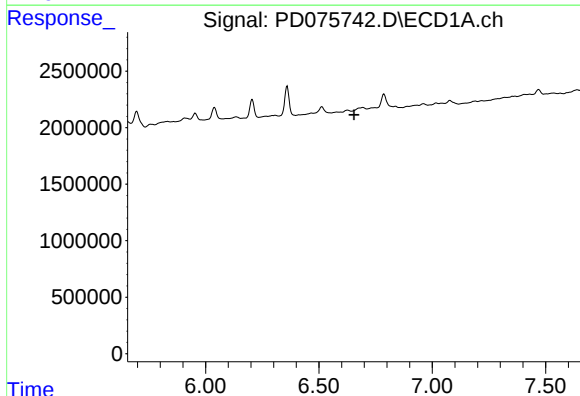


#24 Toxaphene-3

R.T.: 0.000 min
Exp R.T. : 6.656 min
Response: 0
Conc: N.D.

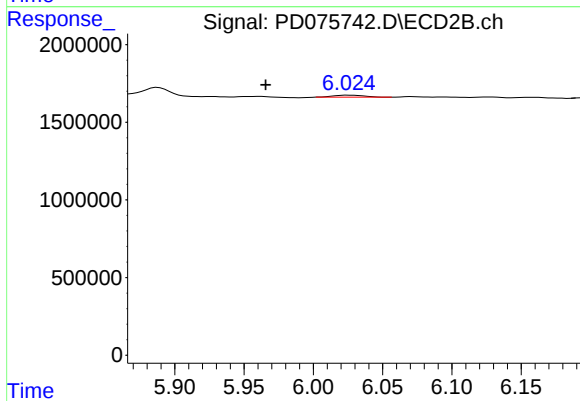

#24 Toxaphene-3


R.T.: 6.025 min
Delta R.T.: 0.060 min
Response: 204960
Conc: 24.27 ng/ml

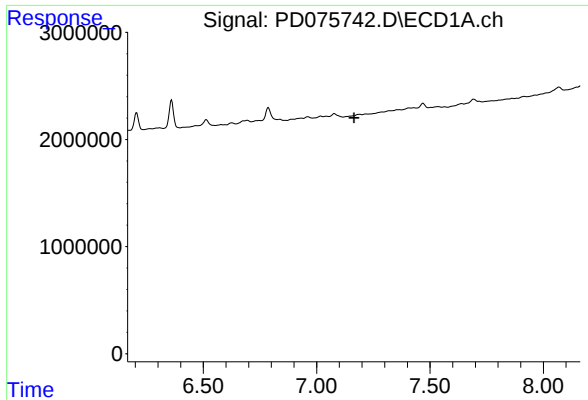

#25 Toxaphene-4


R.T.: 0.000 min
Exp R.T.: 7.166 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

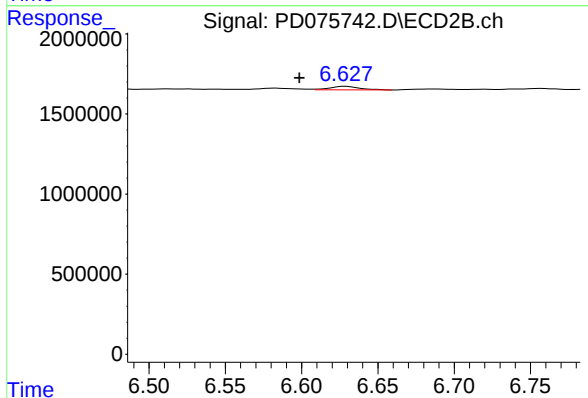


#25 Toxaphene-4

R.T.: 6.629 min
Delta R.T.: 0.030 min
Response: 302119
Conc: 14.62 ng/ml

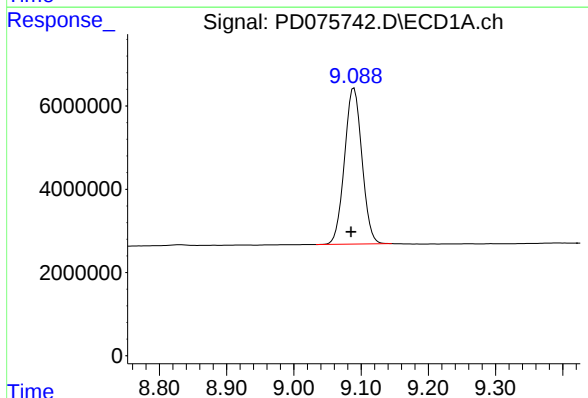

#27 Decachlorobiphenyl

R.T.: 9.089 min
Delta R.T.: 0.004 min
Response: 67474406
Conc: 29.42 ng/ml

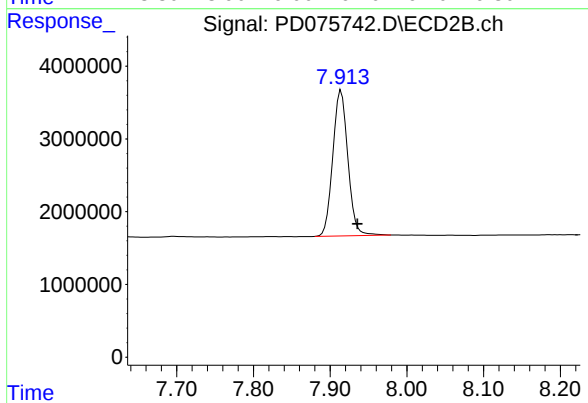

#27 Decachlorobiphenyl

R.T.: 7.914 min
Delta R.T.: -0.021 min
Response: 27346458
Conc: 29.12 ng/ml