

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060923\
 Data File : PD075745.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Jun 2023 16:37
 Operator : AR\AJ
 Sample : 03097-09
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 09 21:44:39 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060223CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 02 04:01:43 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.547	2.770	38546892	16405194	19.282	16.181
27)	SA Decachlor...	9.090	7.914	42128791	16927016	18.368	18.025
Target Compounds							
3)	MA gamma-BHC...	0.000	3.607	0	146777	N.D.	0.106
4)	MA Heptachlor	4.914	0.000	2020663	0	0.623	N.D. #
5)	MB Aldrin	0.000	4.244	0	1612487	N.D.	1.141
7)	B delta-BHC	0.000	4.144	0	211056	N.D.	0.146
9)	A Endosulfan I	0.000	5.056f	0	288667	N.D.	0.250
10)	B trans-Chl...	0.000	5.056f	0	288667	N.D.	0.227
11)	B cis-Chlor...	0.000	5.056	0	288667	N.D.	0.221
15)	B Endosulfa...	6.836	5.958	3228065	1130755	1.262	1.007
22)	Toxaphene-1	0.000	5.056f	0	288667	N.D.	40.509
24)	Toxaphene-3	0.000	5.958	0	1130755	N.D.	133.882


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060923\
Data File : PD075745.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Jun 2023 16:37
Operator : AR\AJ
Sample : 03097-09
Misc :
ALS Vial : 26 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 09 21:44:39 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060223CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jun 02 04:01:43 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

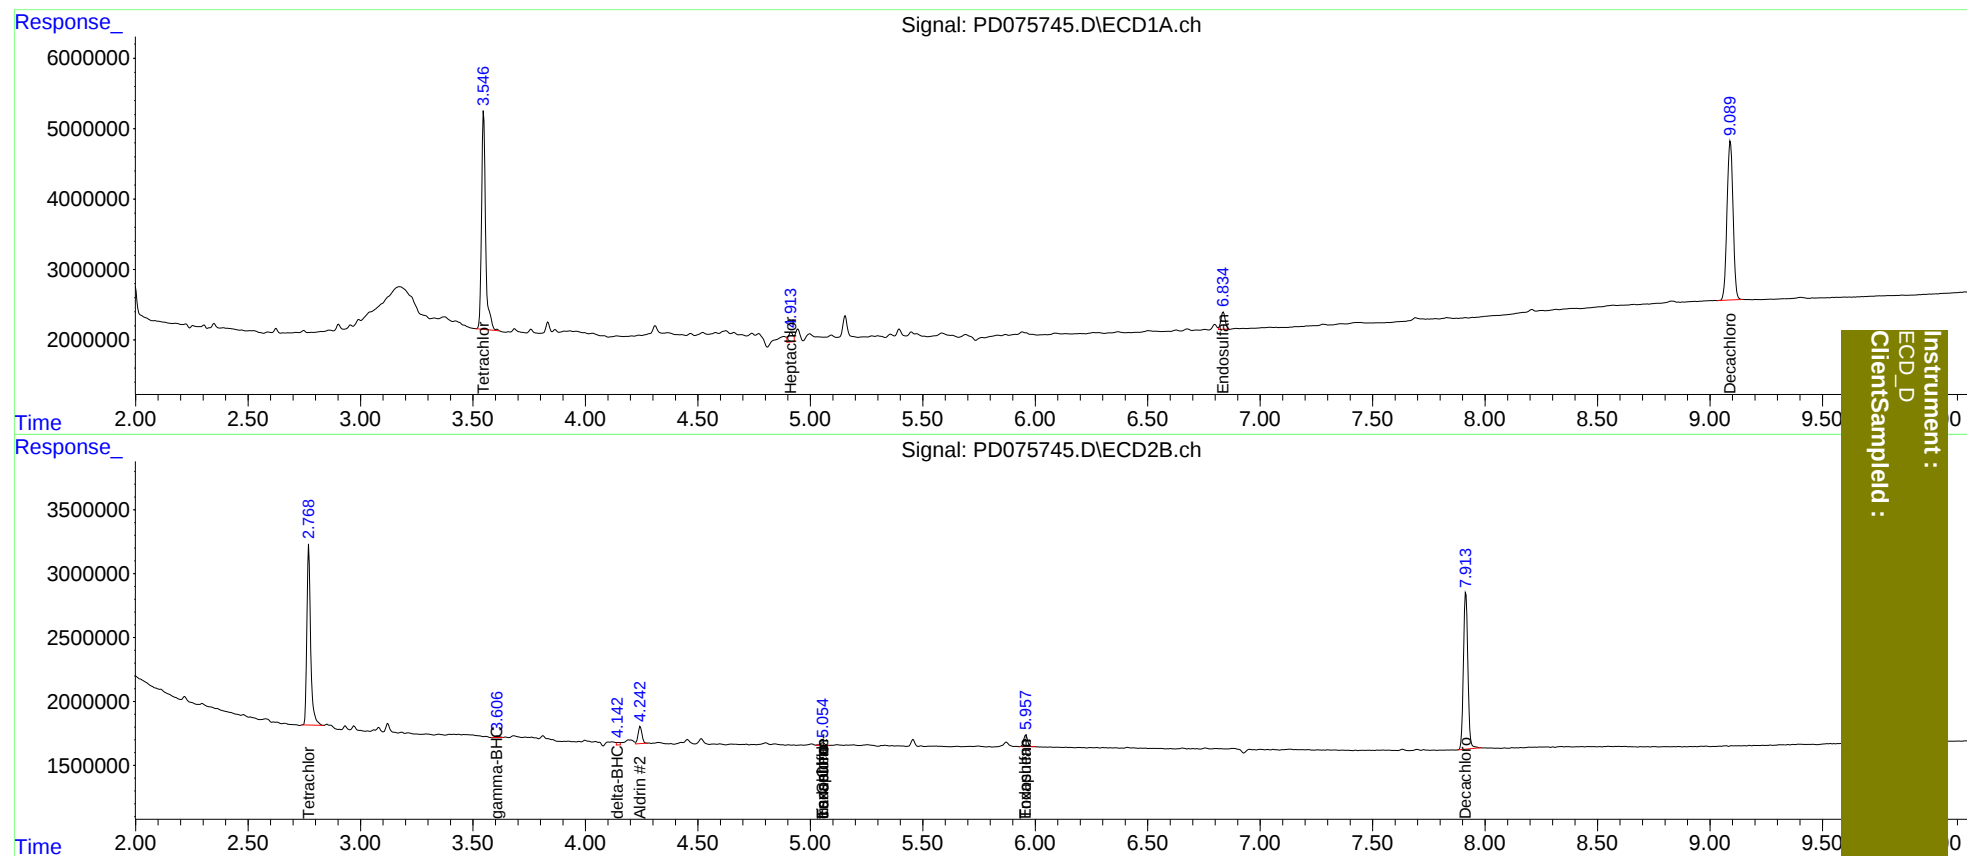


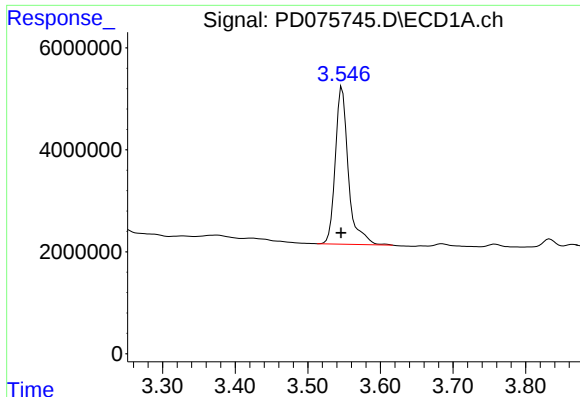

#1 Tetrachloro-m-xylene


R.T.: 3.547 min
Delta R.T.: 0.001 min
Response: 38546892
Conc: 19.28 ng/ml

Instrument :
ECD_D
ClientSampleId :

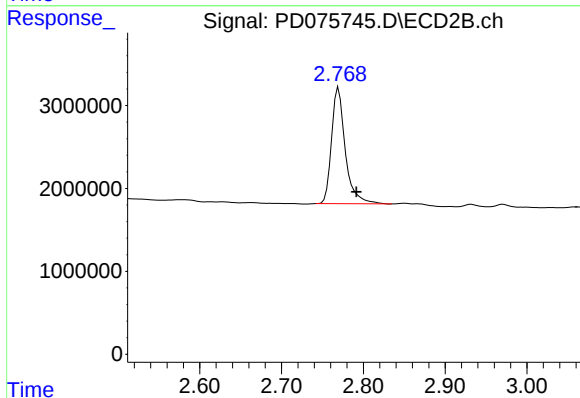


#1 Tetrachloro-m-xylene

R.T.: 2.770 min
Delta R.T.: -0.022 min
Response: 16405194
Conc: 16.18 ng/ml

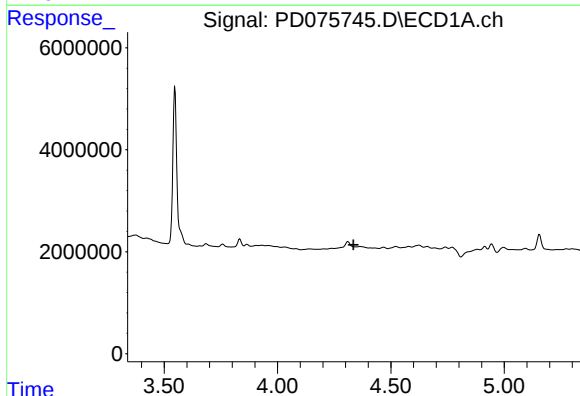


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.336 min
Response: 0
Conc: N.D.

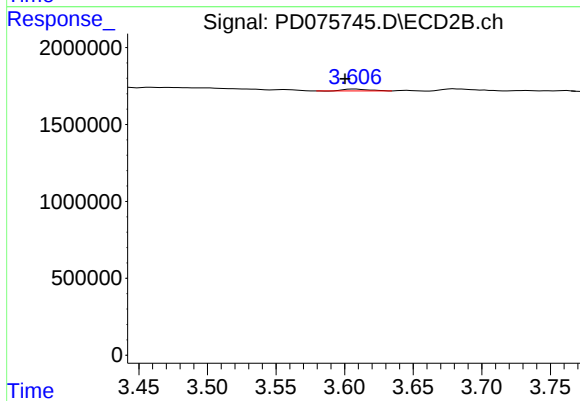

#3 gamma-BHC (Lindane)


R.T.: 3.607 min
Delta R.T.: 0.007 min
Response: 146777
Conc: 0.11 ng/ml

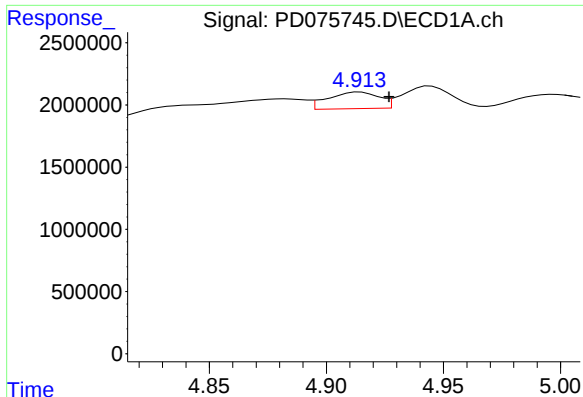

#4 Heptachlor


R.T.: 4.914 min
Delta R.T.: -0.013 min
Response: 2020663
Conc: 0.62 ng/ml

Instrument :
ECD_D
ClientSampleId :

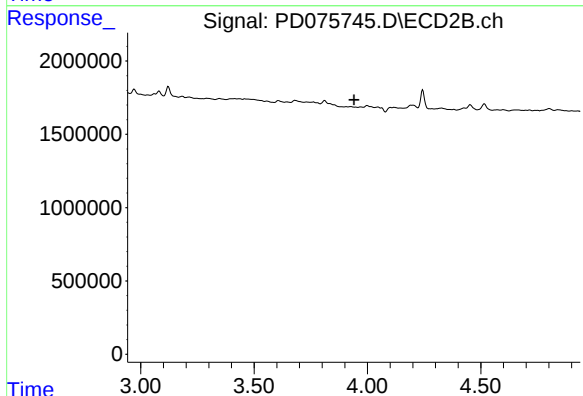


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 3.941 min
Response: 0
Conc: N.D.

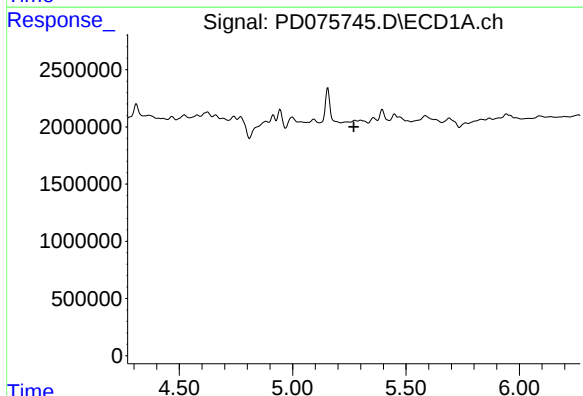


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 5.269 min
Response: 0
Conc: N.D.

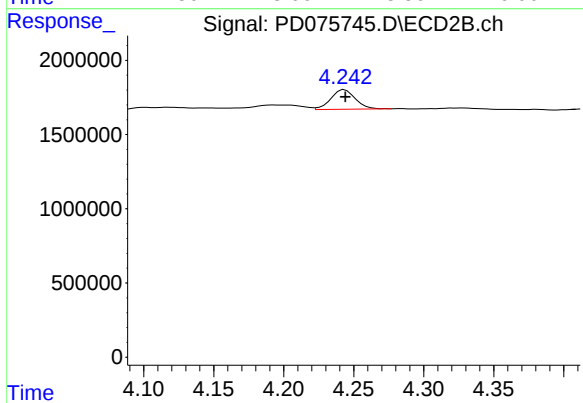

#5 Aldrin


R.T.: 4.244 min
Delta R.T.: 0.000 min
Response: 1612487
Conc: 1.14 ng/ml

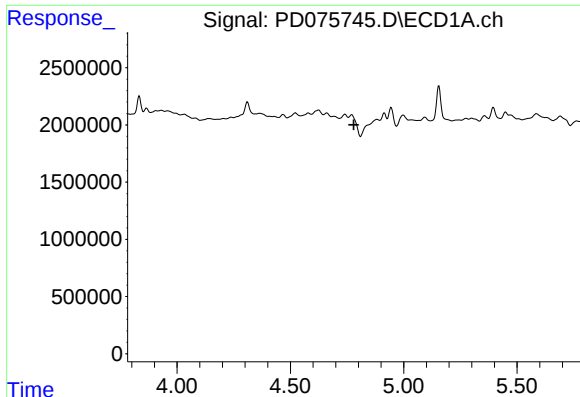

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.779 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

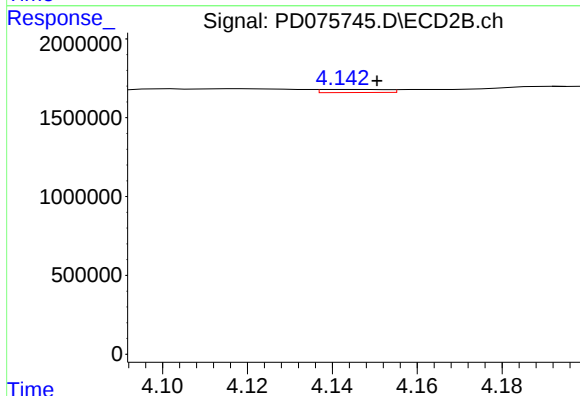


#7 delta-BHC

R.T.: 4.144 min
Delta R.T.: -0.007 min
Response: 211056
Conc: 0.15 ng/ml

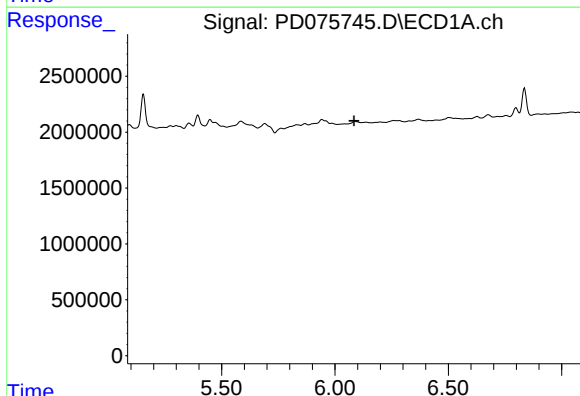


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.084 min
Response: 0
Conc: N.D.

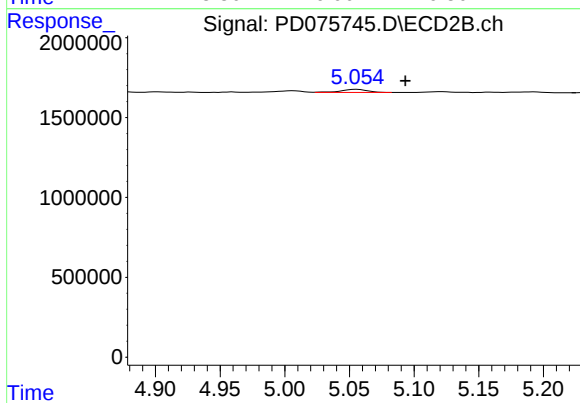

#9 Endosulfan I


R.T.: 5.056 min
Delta R.T.: -0.038 min
Response: 288667
Conc: 0.25 ng/ml

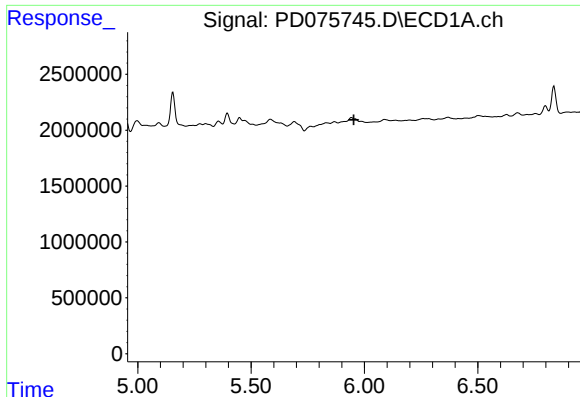

#10 trans-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.953 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

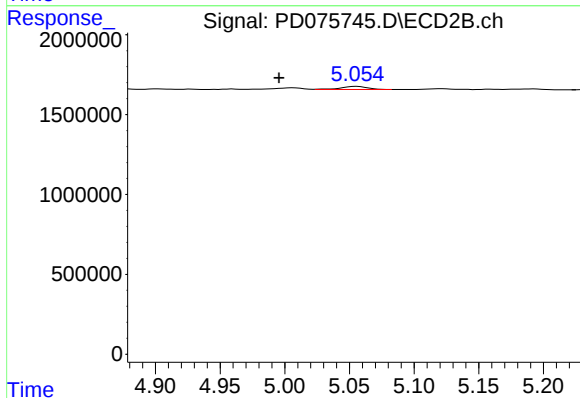


#10 trans-Chlordane

R.T.: 5.056 min
Delta R.T.: 0.060 min
Response: 288667
Conc: 0.23 ng/ml

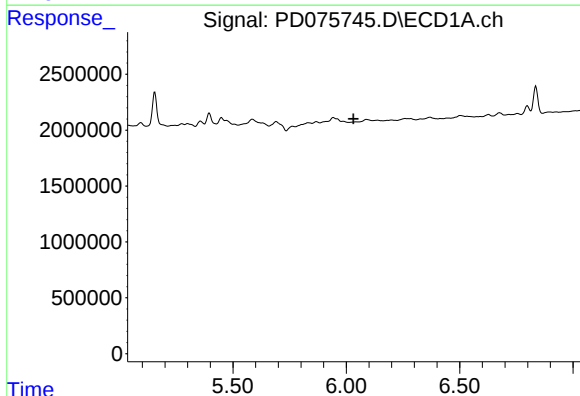


#11 cis-Chlordane

R.T.: 0.000 min
Exp R.T.: 6.032 min
Response: 0
Conc: N.D.

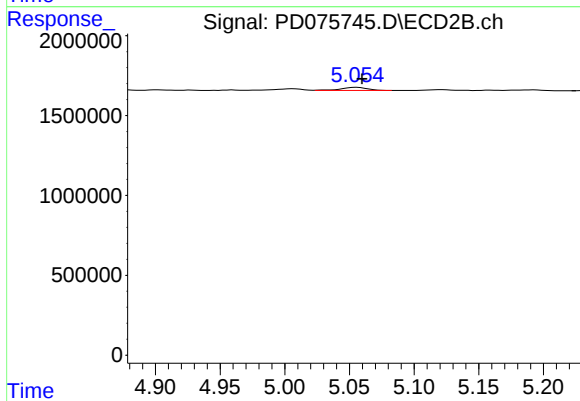

#11 cis-Chlordane


R.T.: 5.056 min
Delta R.T.: -0.004 min
Response: 288667
Conc: 0.22 ng/ml

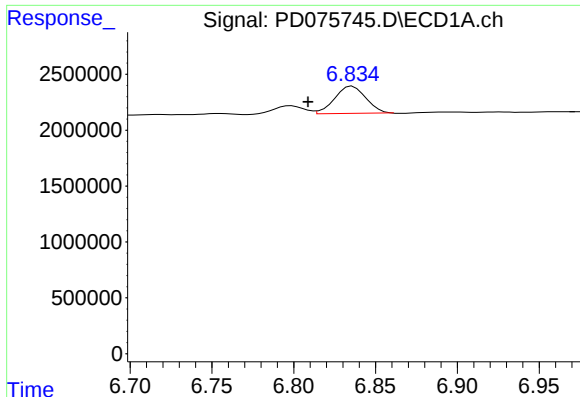

#15 Endosulfan II


R.T.: 6.836 min
Delta R.T.: 0.027 min
Response: 3228065
Conc: 1.26 ng/ml

Instrument :
ECD_D
ClientSampleId :

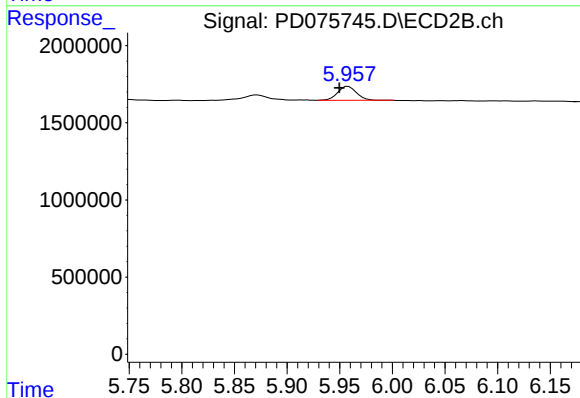


#15 Endosulfan II

R.T.: 5.958 min
Delta R.T.: 0.008 min
Response: 1130755
Conc: 1.01 ng/ml

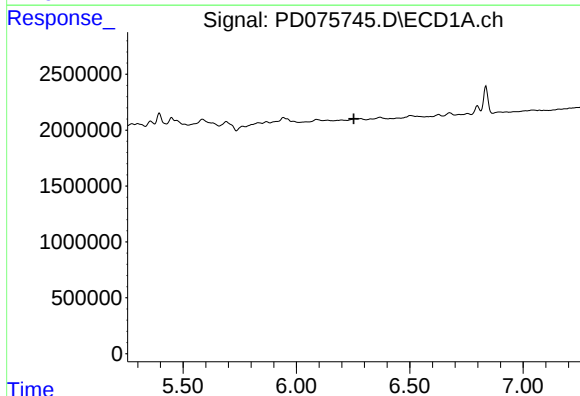


#22 Toxaphene-1

R.T.: 0.000 min
Exp R.T. : 6.253 min
Response: 0
Conc: N.D.

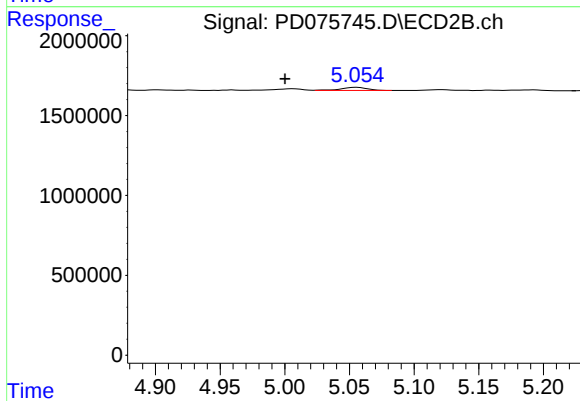

#22 Toxaphene-1


R.T.: 5.056 min
Delta R.T.: 0.055 min
Response: 288667
Conc: 40.51 ng/ml

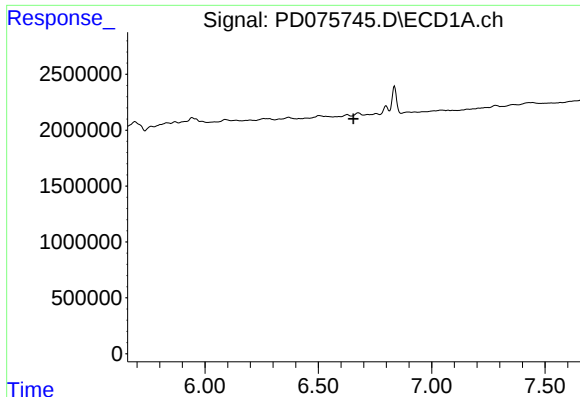

#24 Toxaphene-3


R.T.: 0.000 min
Exp R.T.: 6.656 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

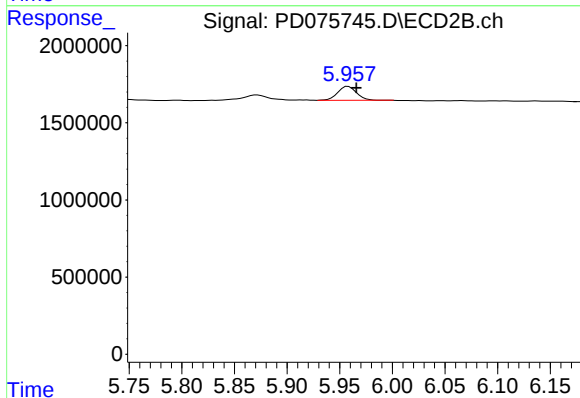


#24 Toxaphene-3

R.T.: 5.958 min
Delta R.T.: -0.008 min
Response: 1130755
Conc: 133.88 ng/ml

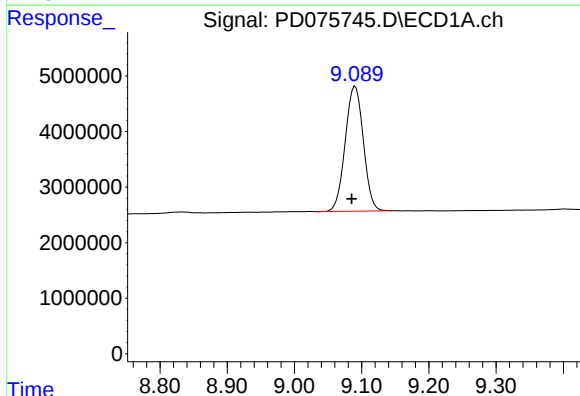

#27 Decachlorobiphenyl

R.T.: 9.090 min
Delta R.T.: 0.005 min
Response: 42128791
Conc: 18.37 ng/ml

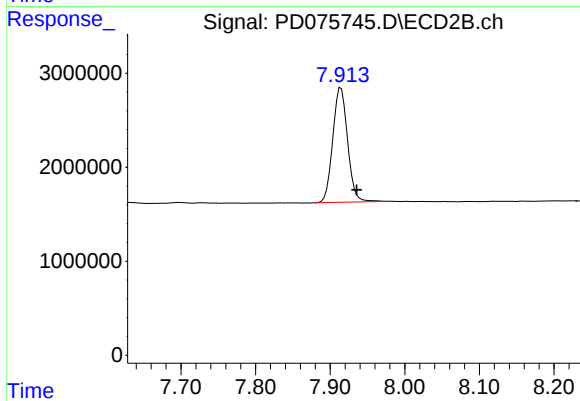

#27 Decachlorobiphenyl

R.T.: 7.914 min
Delta R.T.: -0.021 min
Response: 16927016
Conc: 18.02 ng/ml