

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060923\
 Data File : PD075746.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Jun 2023 16:50
 Operator : AR\AJ
 Sample : 03097-11
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 09 21:45:25 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060223CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 02 04:01:43 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.548	2.770	34359251	15571360	17.187	15.359
2)	SA Decachlor...	9.090	7.915	68304505	26871570	29.781	28.614
Target Compounds							
4)	MA Heptachlor	4.946	0.000	7159844	0	2.208	N.D. #
8)	B Heptachlo...	5.764f	0.000	548275	0	0.179	N.D. #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060923\
Data File : PD075746.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Jun 2023 16:50
Operator : AR\AJ
Sample : 03097-11
Misc :
ALS Vial : 27 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 09 21:45:25 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060223CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jun 02 04:01:43 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

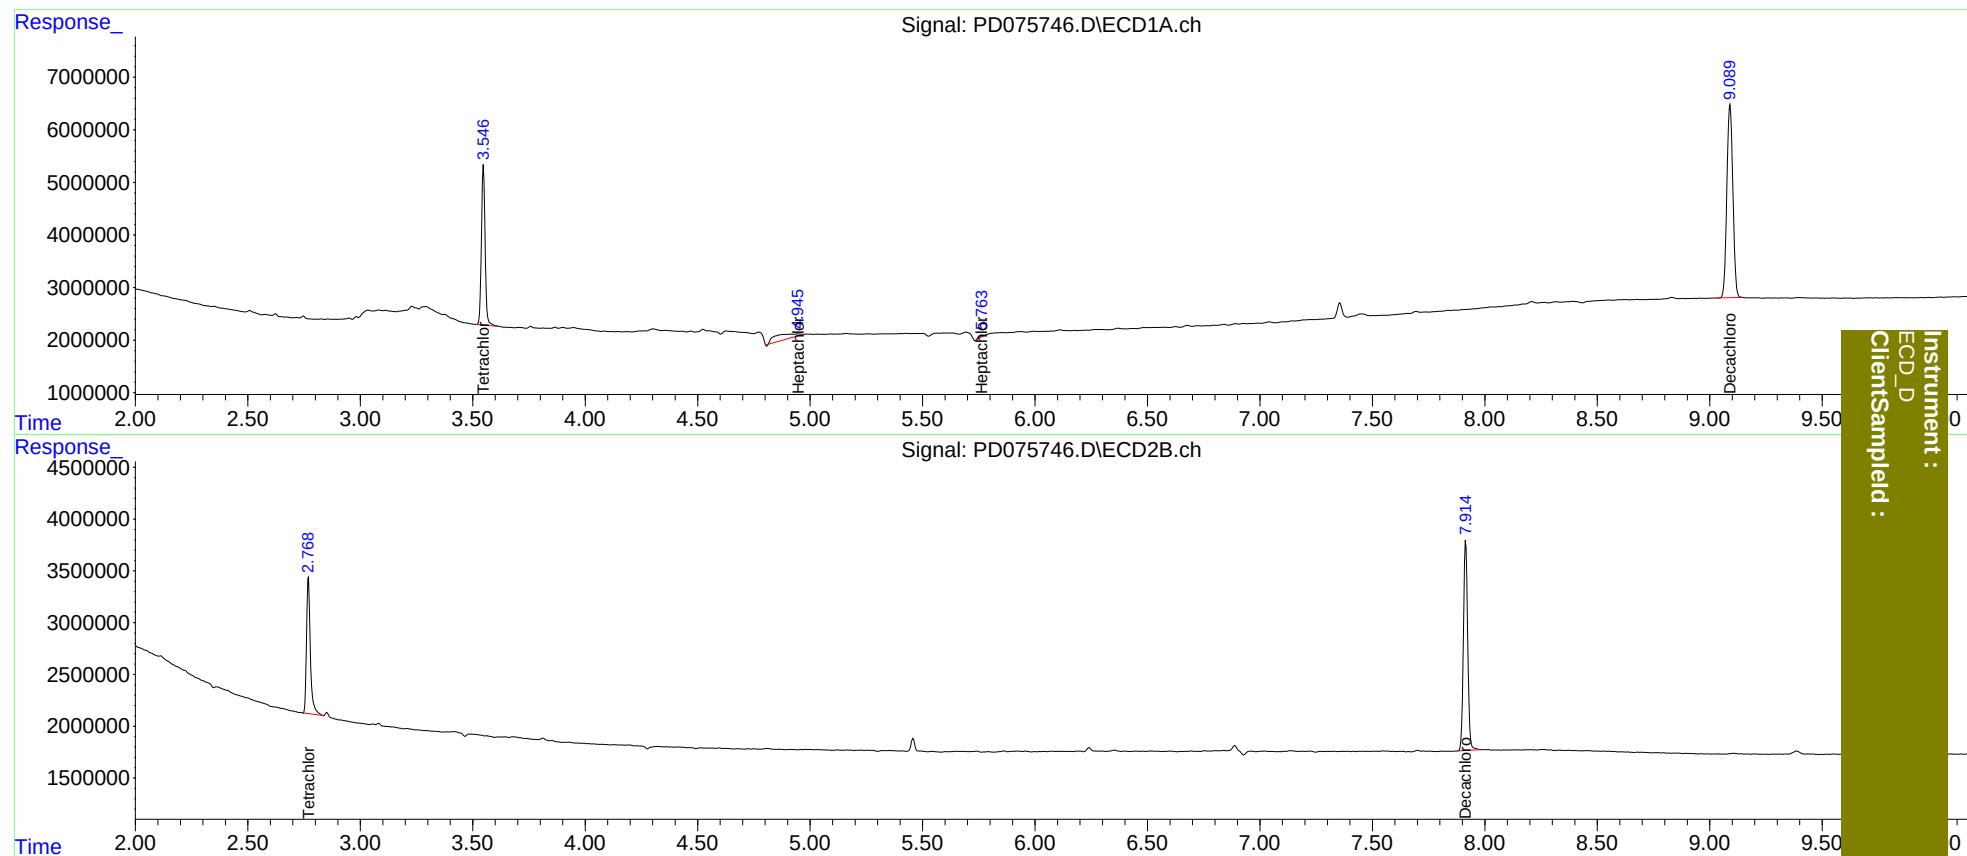


Instrument :
ECD_D
ClientSampled :
0

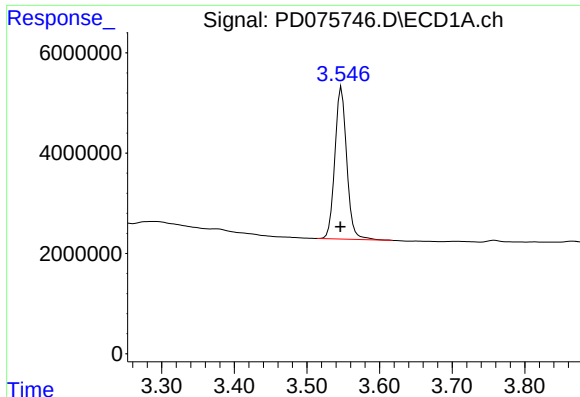

#1 Tetrachloro-m-xylene


R.T.: 3.548 min
Delta R.T.: 0.002 min
Response: 34359251
Conc: 17.19 ng/ml

Instrument :
ECD_D
ClientSampleId :

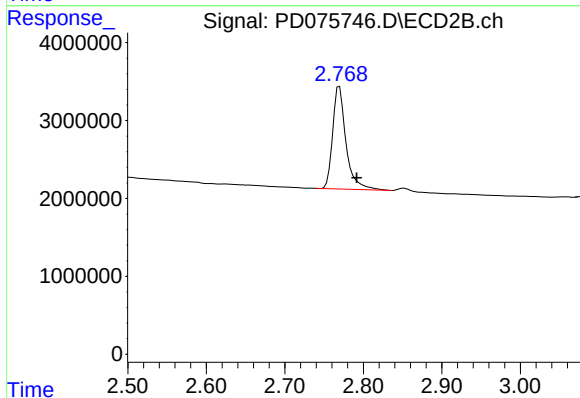


#1 Tetrachloro-m-xylene

R.T.: 2.770 min
Delta R.T.: -0.022 min
Response: 15571360
Conc: 15.36 ng/ml

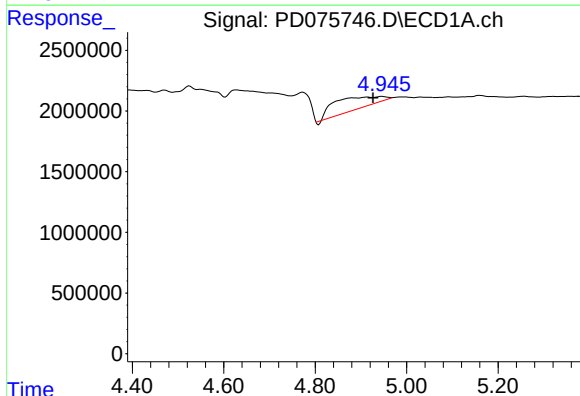


#4 Heptachlor

R.T.: 4.946 min
Delta R.T.: 0.019 min
Response: 7159844
Conc: 2.21 ng/ml

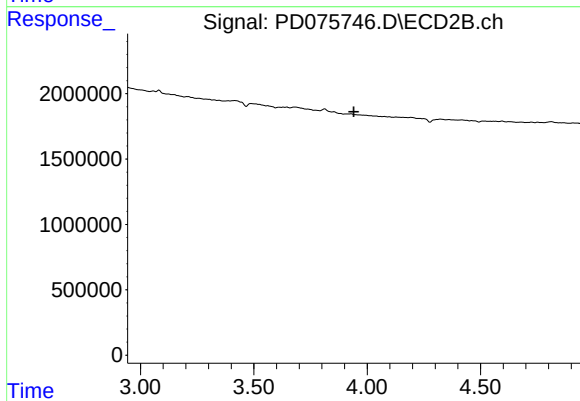

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 3.941 min
Response: 0
Conc: N.D.

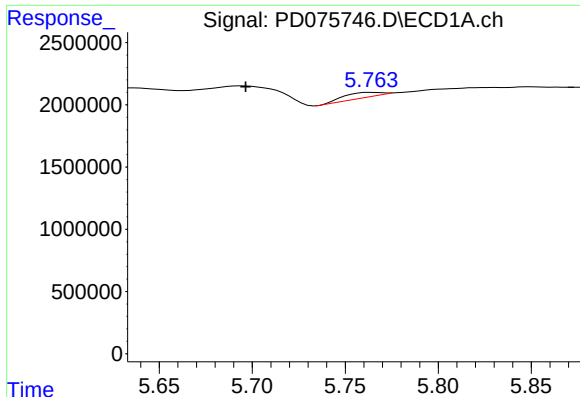

#8 Heptachlor epoxide


R.T.: 5.764 min
Delta R.T.: 0.067 min
Response: 548275
Conc: 0.18 ng/ml

Instrument :
ECD_D
ClientSampleId :

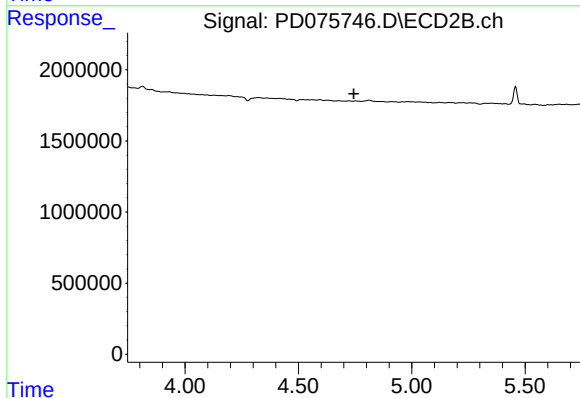


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.745 min
Response: 0
Conc: N.D.

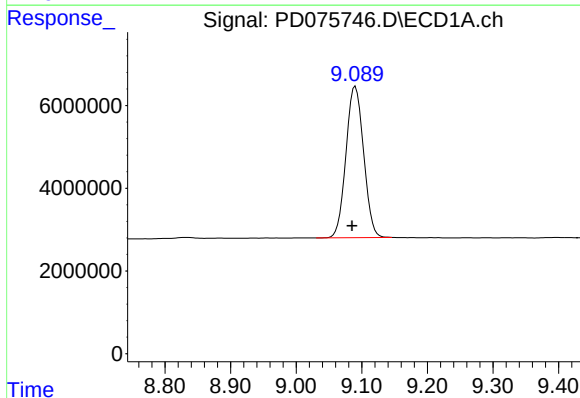

#27 Decachlorobiphenyl

R.T.: 9.090 min
Delta R.T.: 0.005 min
Response: 68304505
Conc: 29.78 ng/ml

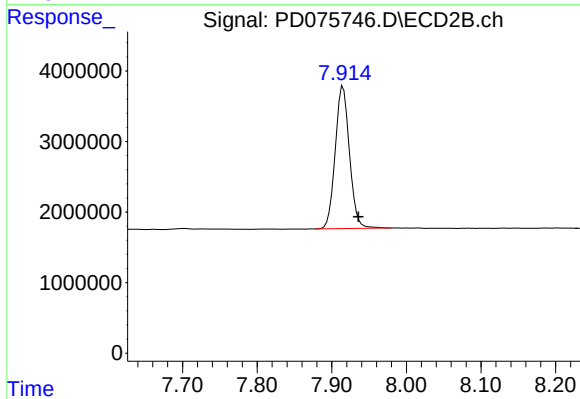

#27 Decachlorobiphenyl

R.T.: 7.915 min
Delta R.T.: -0.020 min
Response: 26871570
Conc: 28.61 ng/ml