

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060923\
 Data File : PD075750.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Jun 2023 17:44
 Operator : AR\AJ
 Sample : 03097-17
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 09 21:48:03 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060223CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 02 04:01:43 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.547	2.770	42387847	18653653	21.204	18.399
27)	SA Decachlor...	9.089	7.915	67357239	26089743	29.368	27.782
Target Compounds							
3)	MA gamma-BHC...	0.000	3.622	0	216081	N.D.	0.156
4)	MA Heptachlor	4.889f	0.000	3105547	0	0.958	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060923\
Data File : PD075750.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Jun 2023 17:44
Operator : AR\AJ
Sample : 03097-17
Misc :
ALS Vial : 31 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 09 21:48:03 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060223CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jun 02 04:01:43 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

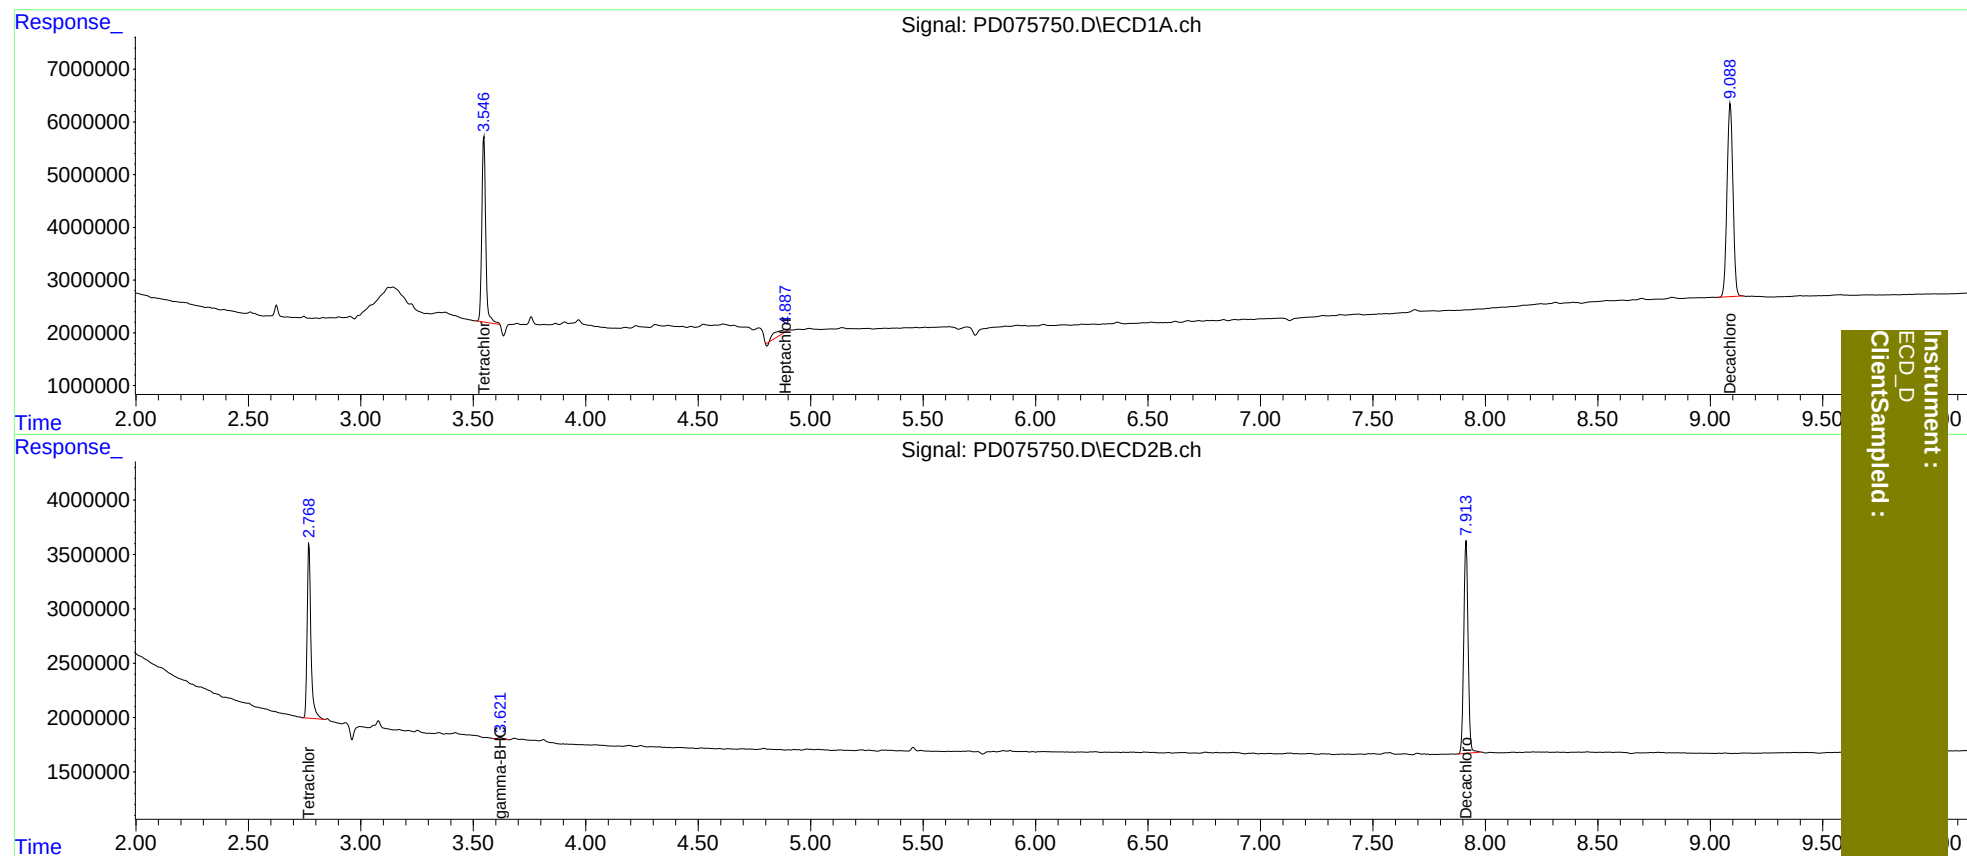


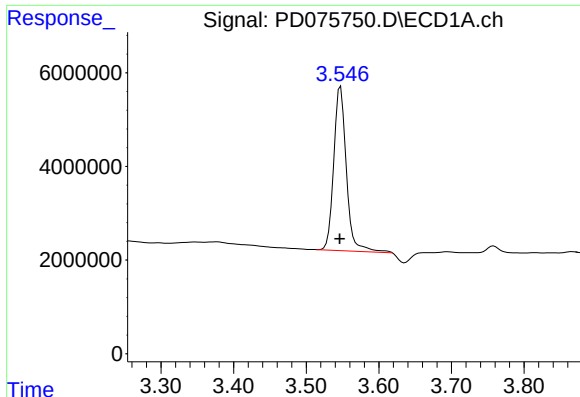

#1 Tetrachloro-m-xylene


R.T.: 3.547 min
Delta R.T.: 0.001 min
Response: 42387847
Conc: 21.20 ng/ml

Instrument :
ECD_D
ClientSampleId :

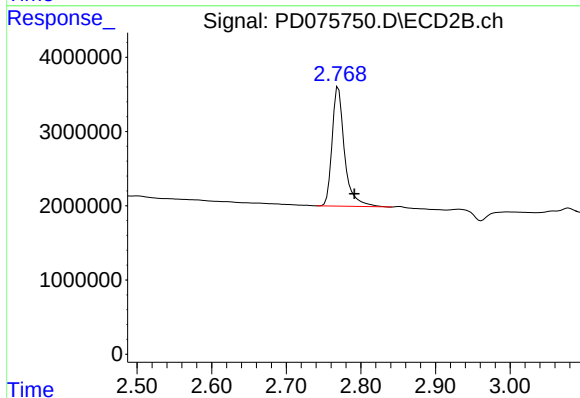


#1 Tetrachloro-m-xylene

R.T.: 2.770 min
Delta R.T.: -0.021 min
Response: 18653653
Conc: 18.40 ng/ml

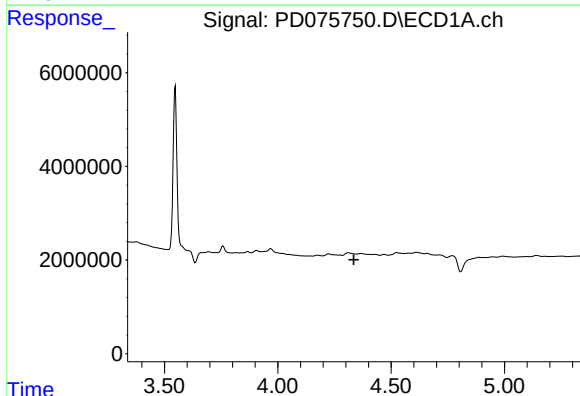


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.336 min
Response: 0
Conc: N.D.

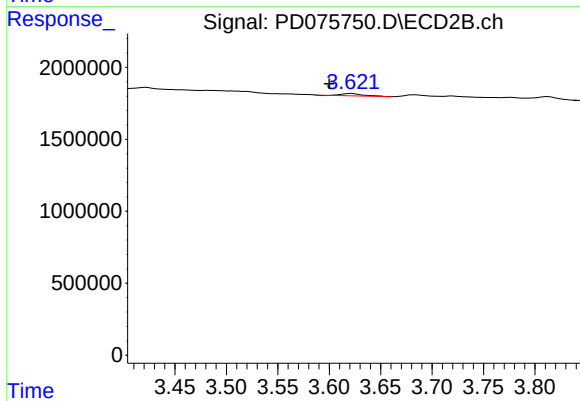

#3 gamma-BHC (Lindane)


R.T.: 3.622 min
Delta R.T.: 0.022 min
Response: 216081
Conc: 0.16 ng/ml

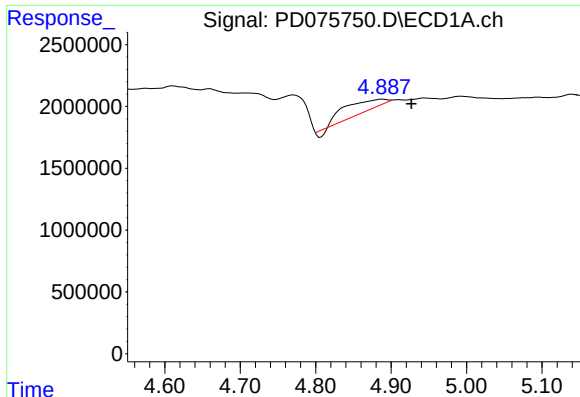

#4 Heptachlor


R.T.: 4.889 min
Delta R.T.: -0.038 min
Response: 3105547
Conc: 0.96 ng/ml

Instrument :
ECD_D
ClientSampleId :

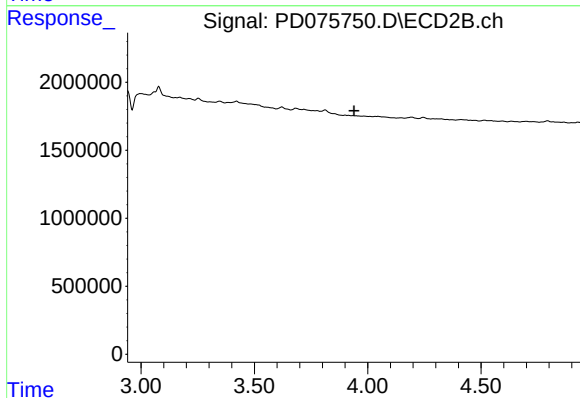


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 3.941 min
Response: 0
Conc: N.D.

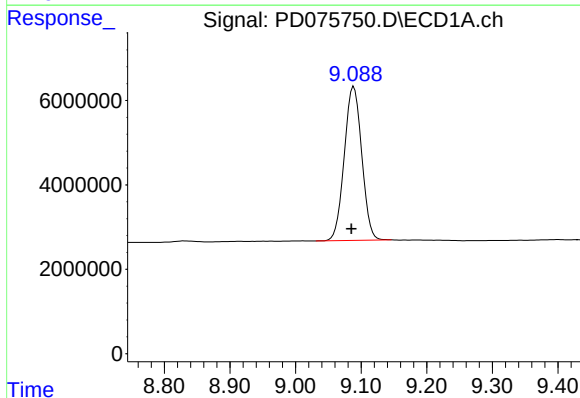

#27 Decachlorobiphenyl

R.T.: 9.089 min
Delta R.T.: 0.004 min
Response: 67357239
Conc: 29.37 ng/ml

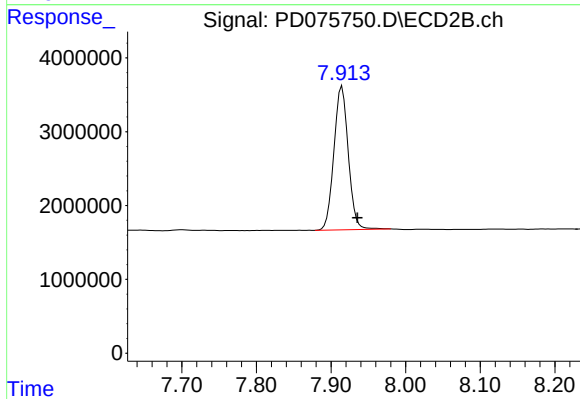

#27 Decachlorobiphenyl

R.T.: 7.915 min
Delta R.T.: -0.021 min
Response: 26089743
Conc: 27.78 ng/ml