

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060923\
 Data File : PD075742.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Jun 2023 15:56
 Operator : AR\AJ
 Sample : 03097-05
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EZEN2

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 06/12/2023
 Supervised By : Ankita Jodhani 06/12/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 09 21:42:54 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060223CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 02 04:01:43 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.547	2.769	33099964	15669090	16.557	15.455
27)	SA Decachlor...	9.089	7.914	67474406	27346458	29.419	29.120
Target Compounds							
8)	B Heptachlo...	5.695	4.721	1859302	484710	0.608m	0.368m#
12)	B 4,4'-DDE	6.206	5.227	2093145	807893	0.747	0.710
13)	MA Dieldrin	6.360	5.357	3549725	1324372	1.193	1.016m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060923\
Data File : PD075742.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Jun 2023 15:56
Operator : AR\AJ
Sample : 03097-05
Misc :
ALS Vial : 23 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 09 21:42:54 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060223CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jun 02 04:01:43 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

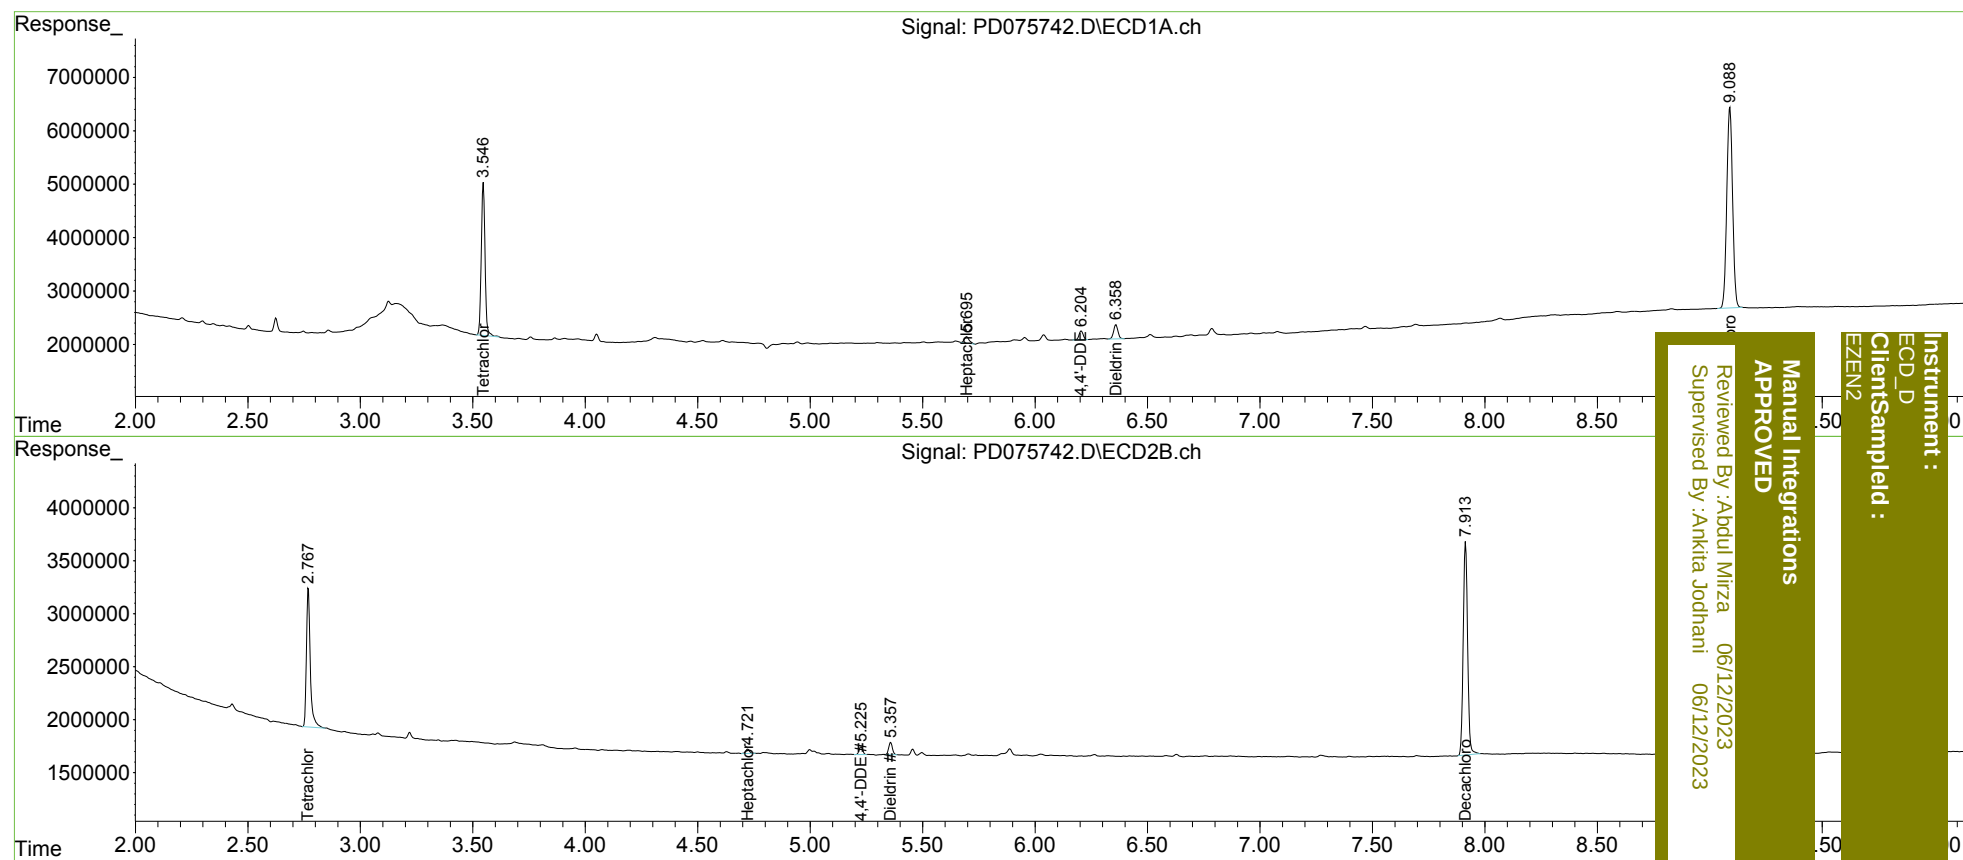

Instrument :
ECD_D
ClientSampled :
EZEN2

Manual Integrations
APPROVED

Reviewed By: Abdul Mirza 06/12/2023
Supervised By: Ankita Jodhani 06/12/2023