

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060923\
 Data File : PD075723.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Jun 2023 09:53
 Operator : AR\AJ
 Sample : PB153306BS
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PLCS306

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 06/19/2023
 Supervised By :Ankita Jodhani 06/19/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 09 21:19:13 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060223CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 02 04:01:43 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.548	2.769	43003827	20676857	21.512	20.394
27)	SA Decachlor...	9.090	7.914	90707069	38698121	39.549	41.207
Target Compounds							
2)	A alpha-BHC	4.004	3.271	16129957	7023931	4.842	4.696
3)	MA gamma-BHC...	4.337	3.601	15375788	6579933	4.917	4.740
4)	MA Heptachlor	4.929	3.941	17014976	6841097	5.246	4.997
5)	MB Aldrin	5.272	4.221	17336566	7187013	5.351	5.086
6)	B beta-BHC	4.534	3.896	7997581	3358725	5.659	4.891m
7)	B delta-BHC	4.781	4.128	13460403	5877250	4.245	4.054
8)	B Heptachlo...	5.699	4.724	16016254	6510444	5.240	4.948
9)	A Endosulfan I	6.086	5.094	14490656	6059232	5.468	5.247
10)	B trans-Chl...	5.955	4.974	15101501	6501133	5.168	5.112
11)	B cis-Chlor...	6.035	5.038	15533322	6704141	5.159	5.144
12)	B 4,4'-DDE	6.207	5.227	27059821	10977836	9.663	9.652
13)	MA Dieldrin	6.361	5.359	30401492	12930187	10.214	9.919
14)	MA Endrin	6.592	5.635	24778706	11242678	9.863	9.793
15)	B Endosulfa...	6.811	5.929	26396240	11305331	10.316	10.063
16)	A 4,4'-DDD	6.725	5.783	22261265	9265138	10.488	10.544
17)	MA 4,4'-DDT	7.040	6.034	18988685	6907872	9.251	8.490
18)	B Endrin al...	6.942	6.108	19002209	8497250	9.189	9.402
19)	B Endosulfa...	7.176	6.331	23974204	10631236	10.036	10.140
20)	A Methoxychlor	7.517	6.609	61095979	23226498	48.995	48.115
21)	B Endrin ke...	7.663	6.838	26771779	12437180	10.114	10.635

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060923\
Data File : PD075723.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Jun 2023 09:53
Operator : AR\AJ
Sample : PB153306BS
Misc :
ALS Vial : 5 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 09 21:19:13 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060223CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jun 02 04:01:43 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

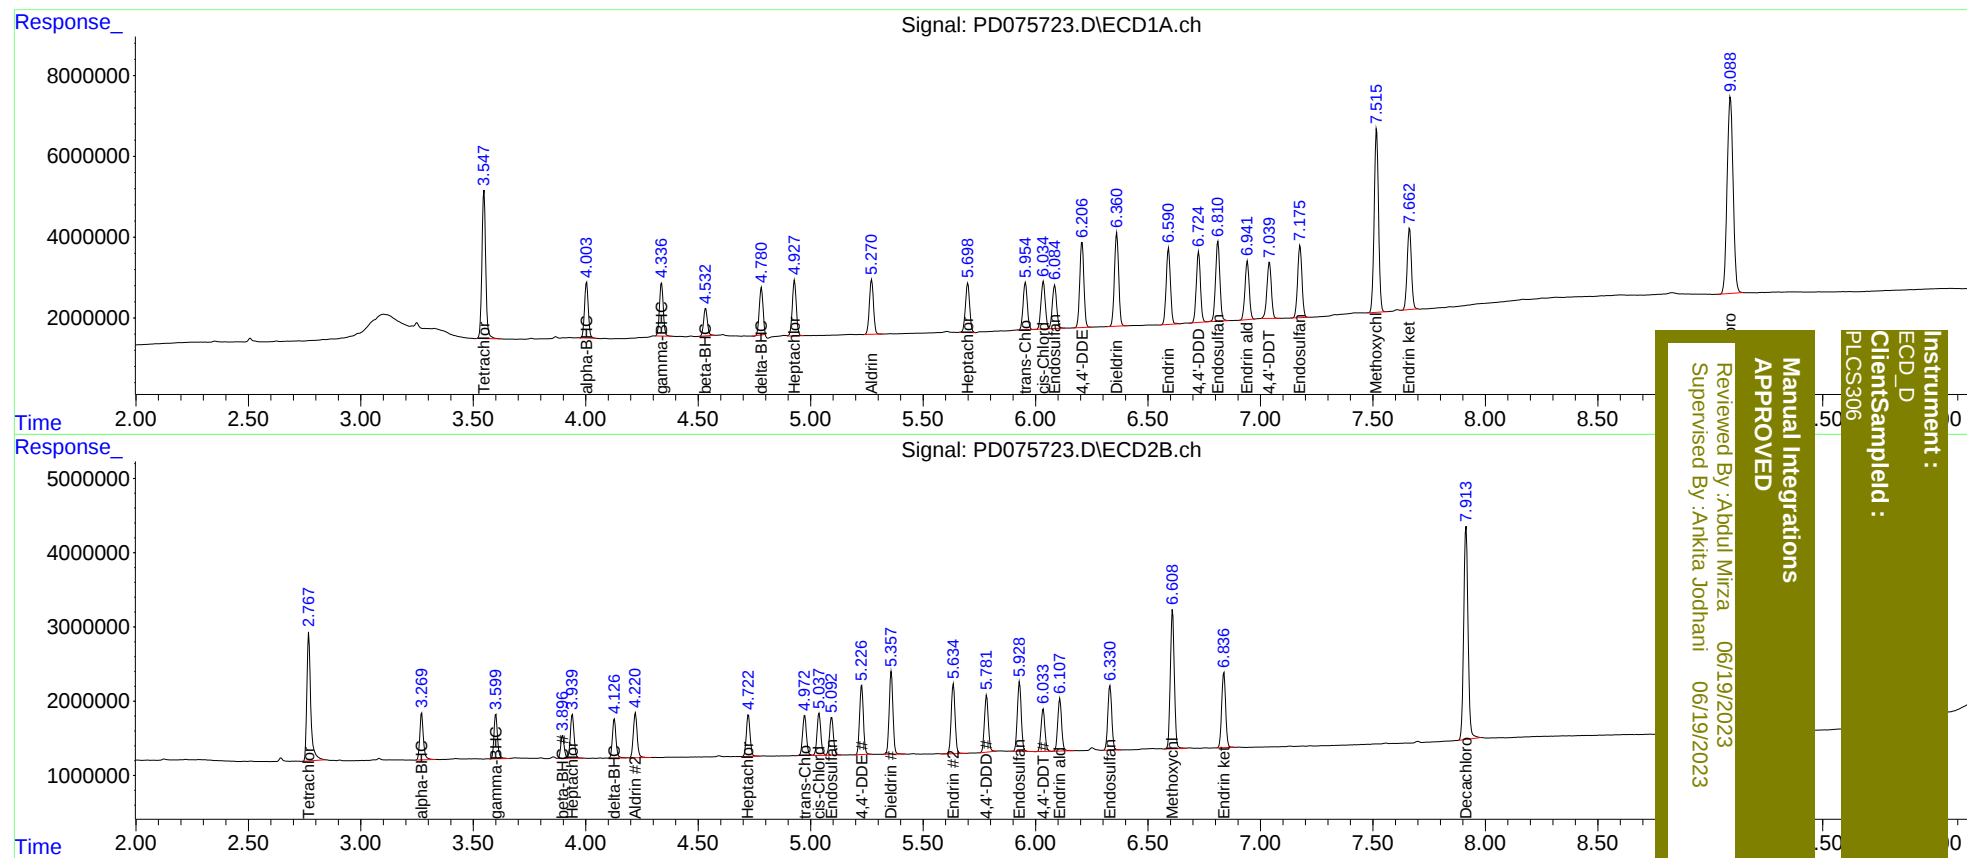

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 06/19/2023
Supervised By: Ankita Jodhani 06/19/2023

Instrument :
ECD_D
Client Sampled :
PLCS306