

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060923\
 Data File : PD075728.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Jun 2023 11:01
 Operator : AR\AJ
 Sample : 03062-05MSD
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EZEL1MSD

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 06/12/2023
 Supervised By : Ankita Jodhani 06/12/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 09 21:26:24 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060223CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 02 04:01:43 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.546	2.768	37899745	18505414	18.958	18.253
27)	SA Decachlor...	9.088	7.914	69559991	29644763	30.329	31.567
Target Compounds							
2)	A alpha-BHC	4.003	3.270	192.0E6	81834773	57.634	54.711
3)	MA gamma-BHC...	4.336	3.600	170.3E6	72656577	54.466	52.342
4)	MA Heptachlor	4.928	3.940	173.7E6	71479156	53.552	52.212
5)	MB Aldrin	5.271	4.221	181.8E6	76208437	56.096	53.926
6)	B beta-BHC	4.532	3.896f	71946941	32285158	50.912	47.013m
7)	B delta-BHC	4.781	4.127	164.2E6	72653824	51.780	50.118
8)	B Heptachlo...	5.698	4.723	155.1E6	64834291	50.747	49.276
9)	A Endosulfan I	6.085	5.094	142.6E6	59945300	53.821	51.907
10)	B trans-Chl...	5.955	4.974	152.9E6	64788351	52.338	50.949
11)	B cis-Chlor...	6.034	5.038	156.5E6	65904626	51.986	50.564
12)	B 4,4'-DDE	6.207	5.227	302.4E6	121.6E6	107.998	106.879
13)	MA Dieldrin	6.361	5.358	331.0E6	138.2E6	111.198	106.019
14)	MA Endrin	6.591	5.634	274.2E6	119.3E6	109.156	103.934
15)	B Endosulfa...	6.810	5.929	267.2E6	114.0E6	104.434	101.480
16)	A 4,4'-DDD	6.724	5.782	241.8E6	96964443	113.926	110.349
17)	MA 4,4'-DDT	7.040	6.034	248.3E6	98206869	120.960	120.701
18)	B Endrin al...	6.941	6.108	192.1E6	82242313	92.910	90.999
19)	B Endosulfa...	7.176	6.331	244.9E6	105.3E6	102.533	100.438
20)	A Methoxychlor	7.516	6.609	647.8E6	248.3E6	519.510	514.443
21)	B Endrin ke...	7.663	6.838	279.2E6	123.7E6	105.464	105.752

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060923\
Data File : PD075728.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Jun 2023 11:01
Operator : AR\AJ
Sample : 03062-05MSD
Misc :
ALS Vial : 10 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 09 21:26:24 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060223CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jun 02 04:01:43 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

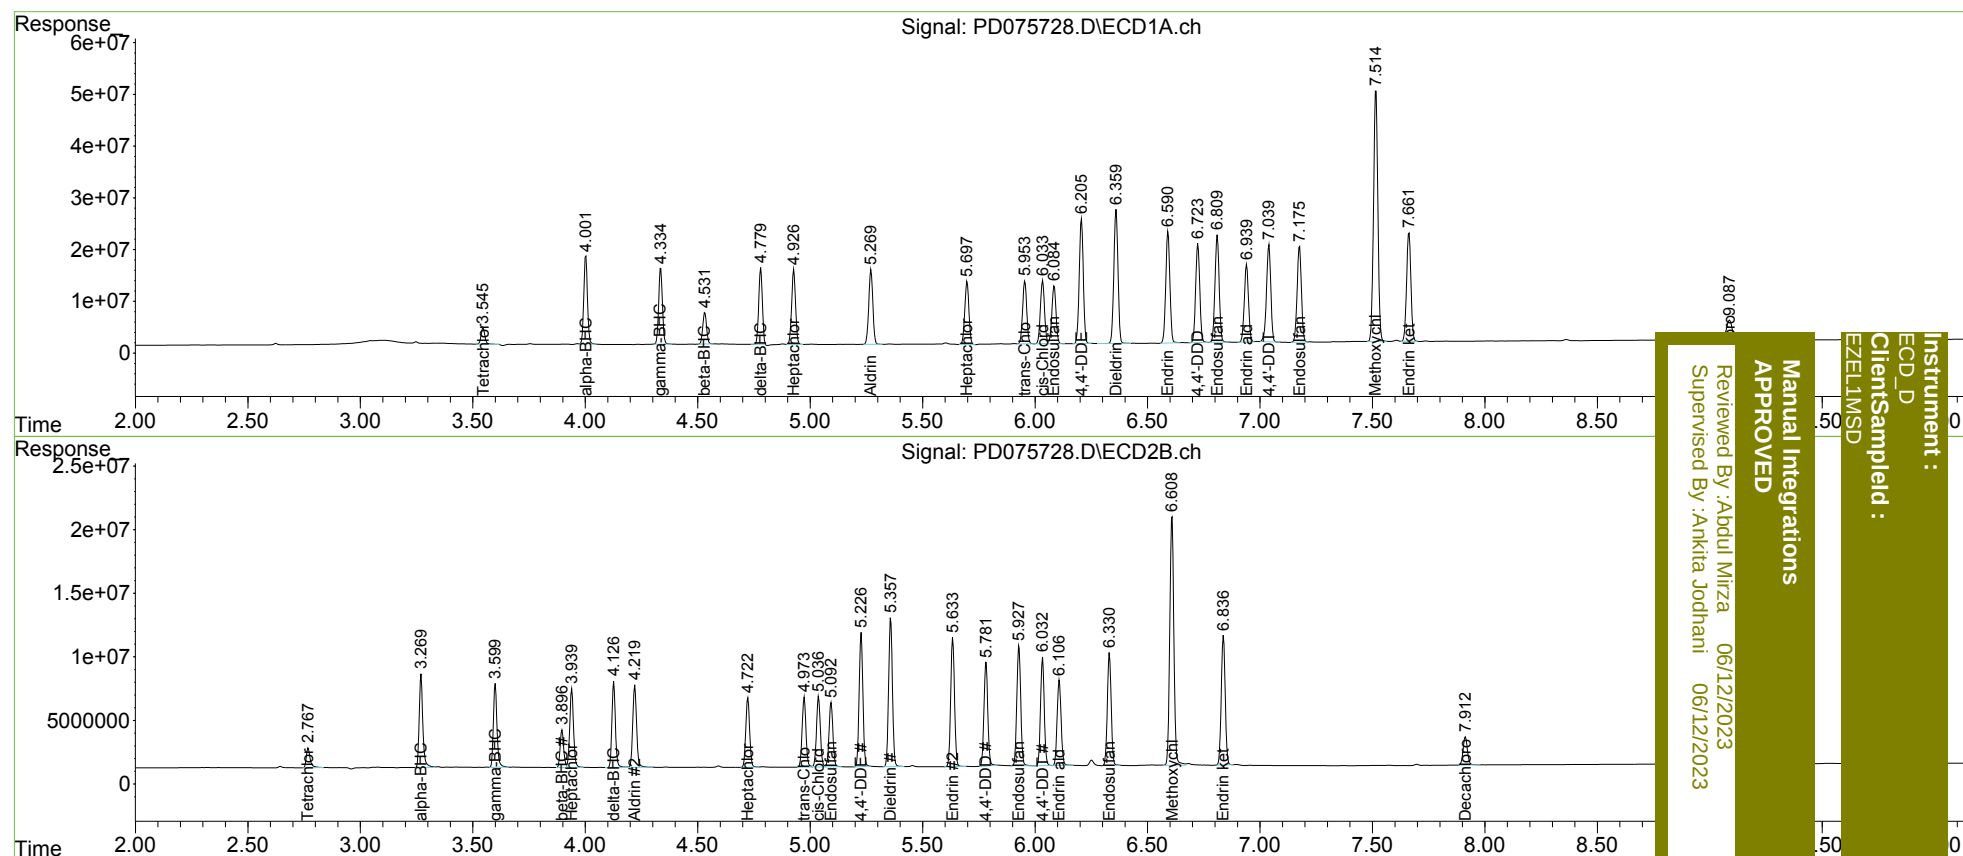

Instrument :
ECD_D
Client Sampled :
EZELMSD
Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 06/12/2023
Supervised By: Ankita Jodhani 06/12/2023