

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060923\
 Data File : PD075740.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Jun 2023 15:29
 Operator : AR\AJ
 Sample : 03097-02MS
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EZEN4MS

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 06/12/2023
 Supervised By :Ankita Jodhani 06/12/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 09 21:40:42 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060223CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 02 04:01:43 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.547	2.769	30091346	14286985	15.052	14.092
27)	SA Decachlor...	9.090	7.914	60407511	24995982	26.338	26.617
Target Compounds							
2)	A alpha-BHC	4.004	3.271	142.8E6	60321308	42.859	40.328
3)	MA gamma-BHC...	4.337	3.601	127.7E6	53417119	40.834	38.482
4)	MA Heptachlor	4.929	3.941	127.3E6	51314658	39.261	37.483
5)	MB Aldrin	5.272	4.222	132.2E6	54268584	40.788	38.401
6)	B beta-BHC	4.534	3.896	53960030	24290097	38.184	35.371m
7)	B delta-BHC	4.782	4.128	119.1E6	52956404	37.552	36.530
8)	B Heptachlo...	5.699	4.724	117.8E6	47694936	38.537	36.250
9)	A Endosulfan I	6.086	5.094	107.2E6	44057208	40.458	38.150
10)	B trans-Chl...	5.956	4.974	113.4E6	47346756	38.810	37.233
11)	B cis-Chlor...	6.035	5.038	116.9E6	48088419	38.819	36.895
12)	B 4,4'-DDE	6.207	5.228	222.9E6	87746571	79.597	77.146
13)	MA Dieldrin	6.362	5.359	247.6E6	101.6E6	83.179	77.942
14)	MA Endrin	6.592	5.635	206.6E6	89095777	82.231	77.607
15)	B Endosulfa...	6.811	5.929	204.0E6	84000653	79.742	74.773
16)	A 4,4'-DDD	6.725	5.783	180.8E6	70789175	85.201	80.561
17)	MA 4,4'-DDT	7.041	6.034	183.8E6	69500092	89.530	85.419
18)	B Endrin al...	6.942	6.109	144.2E6	60399786	69.725	66.831
19)	B Endosulfa...	7.176	6.331	186.1E6	78271973	77.920	74.652
20)	A Methoxychlor	7.516	6.610	493.7E6	185.9E6	395.887	385.024
21)	B Endrin ke...	7.663	6.838	210.9E6	92416285	79.664	79.028

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060923\
Data File : PD075740.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Jun 2023 15:29
Operator : AR\AJ
Sample : 03097-02MS
Misc :
ALS Vial : 21 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 09 21:40:42 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060223CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jun 02 04:01:43 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

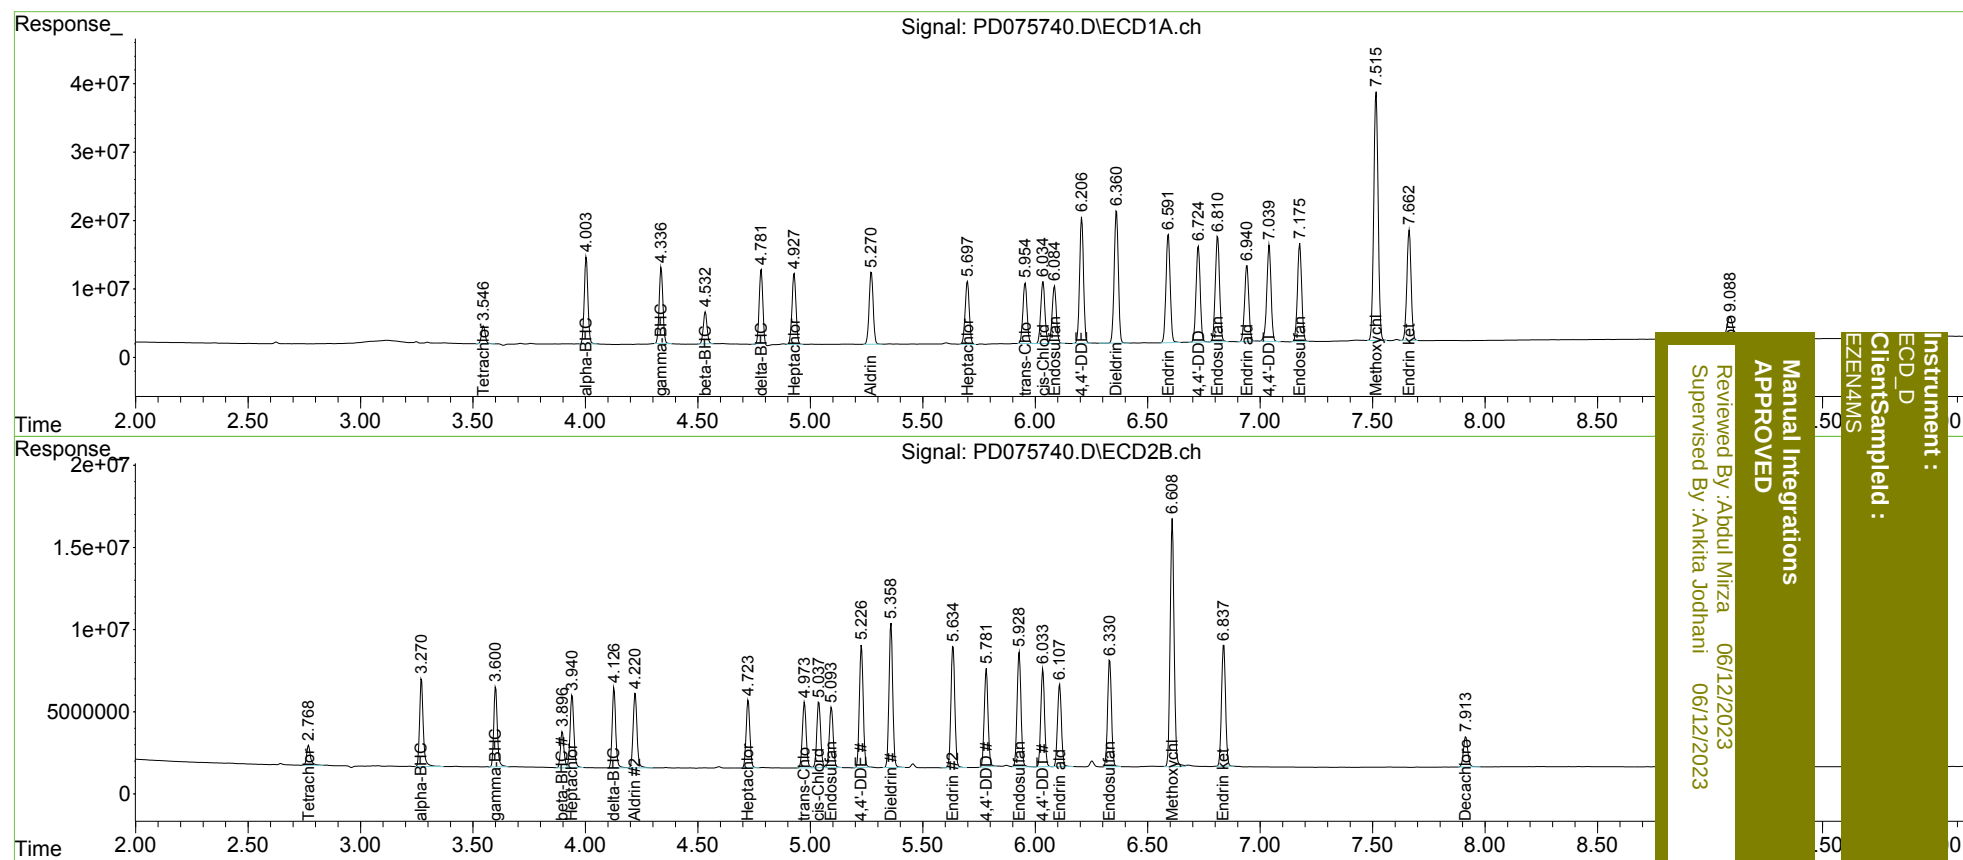

Instrument :
ECD_D
ClientSampled :
EZEN4MS
Manual Integrations
APPROVED
Reviewed By :Abdul Mirza 06/12/2023
Supervised By :Ankita Jodhani 06/12/2023