

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060923\
 Data File : PD075741.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Jun 2023 15:43
 Operator : AR\AJ
 Sample : 03097-03MSD
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EZEN4MSD

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 06/12/2023
 Supervised By : Ankita Jodhani 06/12/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 09 21:41:46 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060223CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 02 04:01:43 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.547	2.769	29869476	14303575	14.941	14.108
27)	SA Decachlor...	9.091	7.915	60730015	24419109	26.479	26.003
Target Compounds							
2)	A alpha-BHC	4.004	3.271	142.0E6	60075501	42.624	40.164
3)	MA gamma-BHC...	4.337	3.601	127.0E6	52993554	40.616	38.176
4)	MA Heptachlor	4.929	3.941	125.8E6	50772119	38.796	37.086
5)	MB Aldrin	5.272	4.222	131.3E6	53553878	40.512	37.896
6)	B beta-BHC	4.533	3.896	53372724	23231585	37.768	33.829m
7)	B delta-BHC	4.782	4.128	120.0E6	52454414	37.835	36.184
8)	B Heptachlo...	5.699	4.724	116.6E6	47098097	38.163	35.796
9)	A Endosulfan I	6.086	5.095	106.1E6	43597126	40.047	37.751
10)	B trans-Chl...	5.956	4.975	112.7E6	46749069	38.560	36.763
11)	B cis-Chlor...	6.035	5.039	115.8E6	47457088	38.471	36.411
12)	B 4,4'-DDE	6.208	5.228	219.7E6	86661617	78.443	76.192
13)	MA Dieldrin	6.362	5.360	244.5E6	99978069	82.140	76.694
14)	MA Endrin	6.593	5.635	203.2E6	87845996	80.898	76.518
15)	B Endosulfa...	6.811	5.930	200.8E6	82928167	78.475	73.818
16)	A 4,4'-DDD	6.726	5.783	177.9E6	69764512	83.806	79.395
17)	MA 4,4'-DDT	7.041	6.035	182.3E6	68744212	88.793	84.490
18)	B Endrin al...	6.942	6.109	142.2E6	59629982	68.752	65.979
19)	B Endosulfa...	7.177	6.332	183.0E6	77030008	76.593	73.467
20)	A Methoxychlor	7.517	6.610	488.9E6	184.0E6	392.068	381.202
21)	B Endrin ke...	7.664	6.839	210.2E6	91219310	79.416	78.004

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060923\
Data File : PD075741.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Jun 2023 15:43
Operator : AR\AJ
Sample : 03097-03MSD
Misc :
ALS Vial : 22 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 09 21:41:46 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060223CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jun 02 04:01:43 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

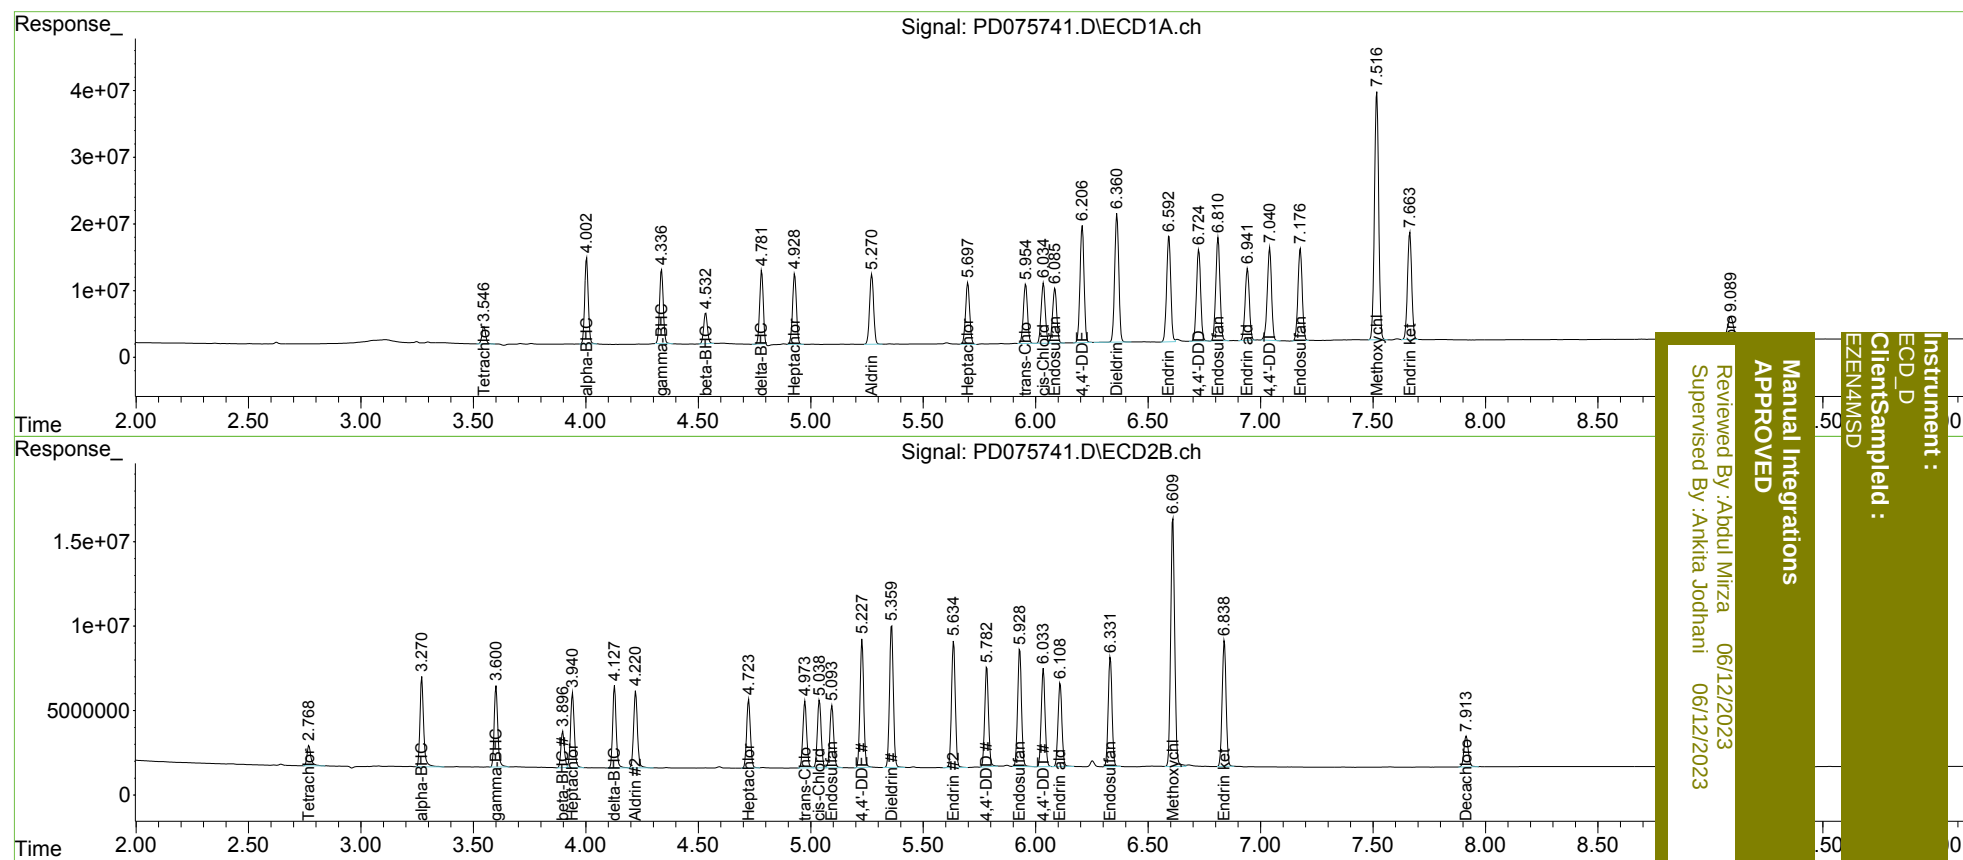

Instrument :
ECD_D
ClientSampled :
EZEN4MSD

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 06/12/2023
Supervised By :Ankita Jodhani 06/12/2023