

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061119\
 Data File : PD053550.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 11 Jun 2019 9:28
 Operator : SM\AJ
 Sample : PB120440BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PBLK40

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 12 04:40:19 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052119CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed May 22 06:53:42 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.322	3.984	15699284	24656309	21.427	25.043
27) SA Decachlor...	8.024	9.035	23894101	37316143	36.121	36.126
Target Compounds						
6) B beta-BHC	0.000	4.821	0	468743	N.D.	0.799


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061119\
Data File : PD053550.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 11 Jun 2019 9:28
Operator : SM\AJ
Sample : PB120440BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PBLK40

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 12 04:40:19 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052119CLP.M
Quant Title : GC Extractables
QLast Update : Wed May 22 06:53:42 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

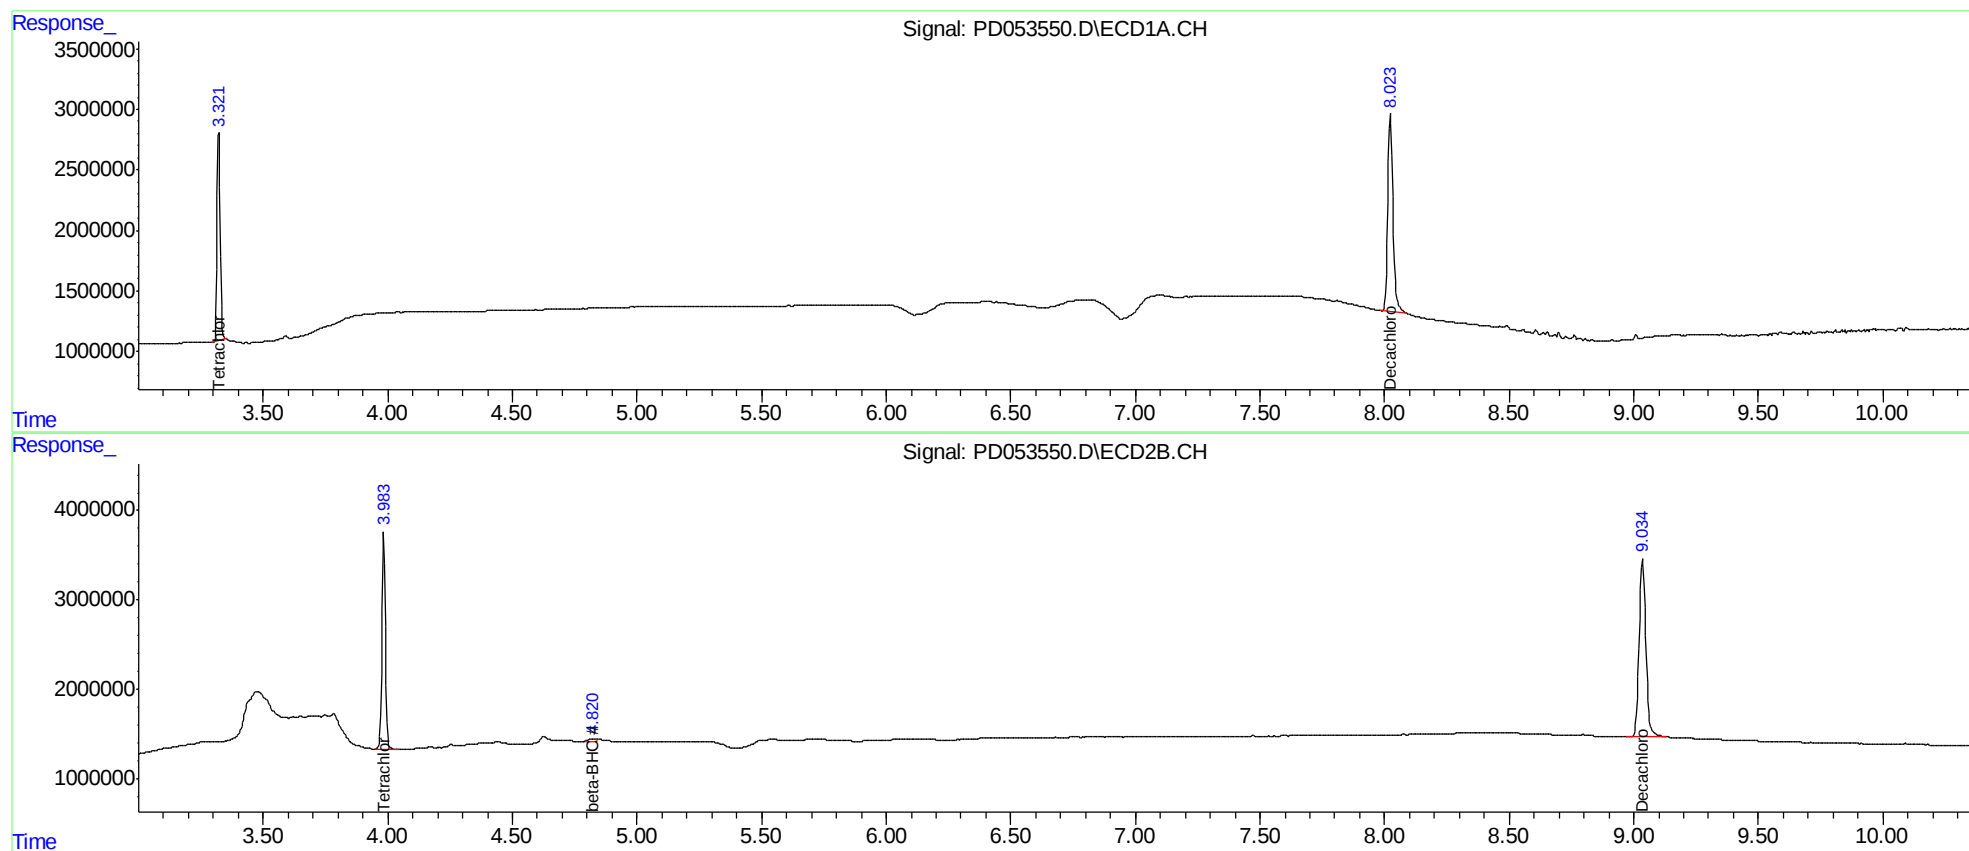


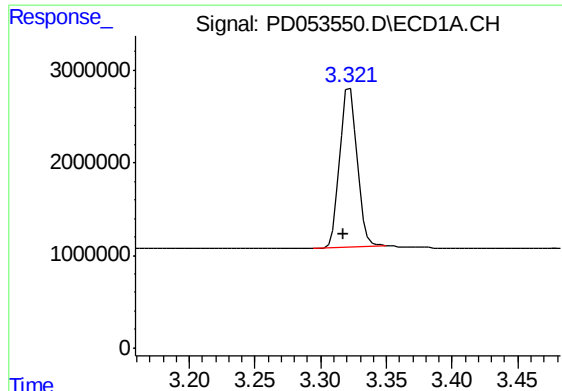

#1 Tetrachloro-m-xylene


R.T.: 3.322 min
Delta R.T.: 0.005 min
Response: 15699284
Conc: 21.43 ng/ml

Instrument :
ECD_D
ClientSampleId :
PBLK40

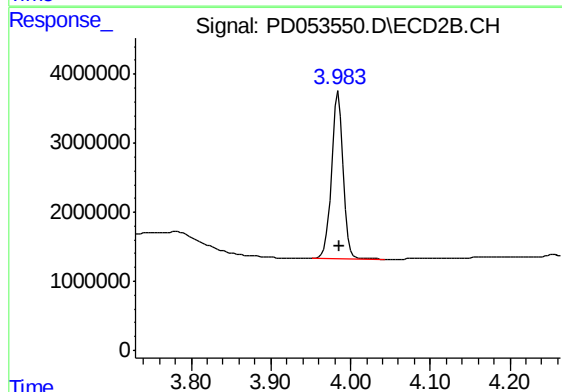


#1 Tetrachloro-m-xylene

R.T.: 3.984 min
Delta R.T.: -0.001 min
Response: 24656309
Conc: 25.04 ng/ml

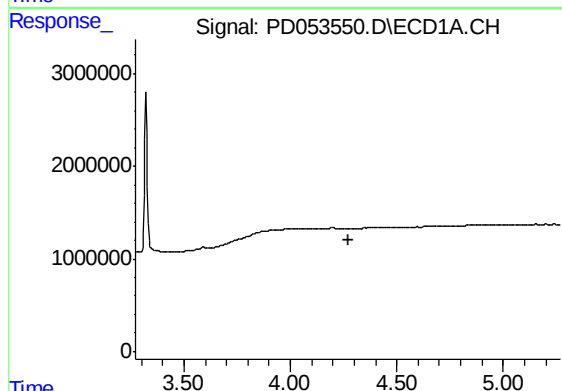


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.272 min
Response: 0
Conc: N.D.

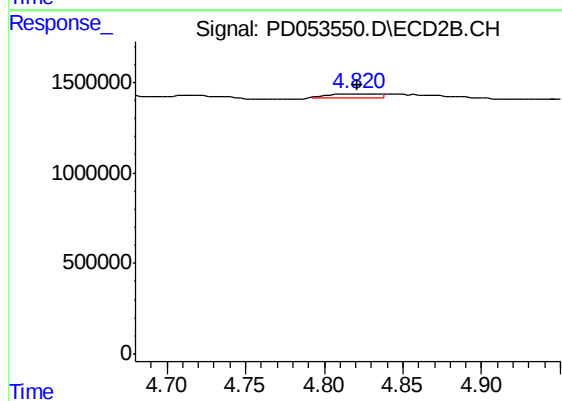

#6 beta-BHC


R.T.: 4.821 min
Delta R.T.: 0.000 min
Response: 468743
Conc: 0.80 ng/ml

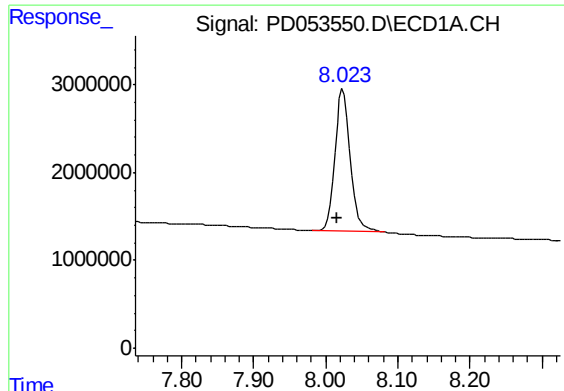

#27 Decachlorobiphenyl

R.T.: 8.024 min
Delta R.T.: 0.009 min
Response: 23894101
Conc: 36.12 ng/ml

Instrument :
ECD_D
ClientSampleId :
PBLK40

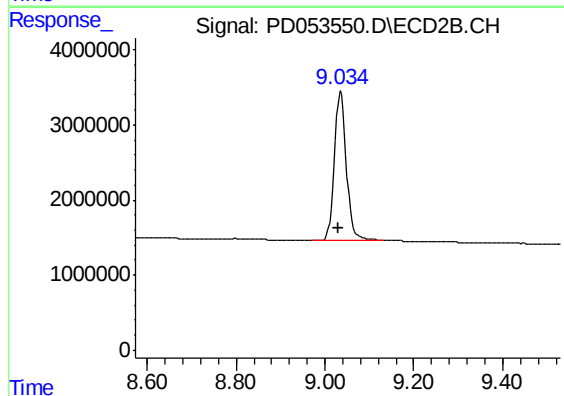

#27 Decachlorobiphenyl

R.T.: 9.035 min
Delta R.T.: 0.006 min
Response: 37316143
Conc: 36.13 ng/ml