

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061119\
 Data File : PD053573.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 11 Jun 2019 15:58
 Operator : SM\AJ
 Sample : PIBLK42
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PIBLK42

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 12 04:46:10 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052119CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed May 22 06:53:42 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.316	3.985	15511581	23479368	21.170	23.848
27) SA Decachlor...	8.013	9.028	23791992	35897852	35.966	34.753
Target Compounds						
6) B beta-BHC	0.000	4.869f	0	862488	N.D.	1.470


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061119\
Data File : PD053573.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 11 Jun 2019 15:58
Operator : SM\AJ
Sample : PIBLK42
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PIBLK42

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 12 04:46:10 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052119CLP.M
Quant Title : GC Extractables
QLast Update : Wed May 22 06:53:42 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

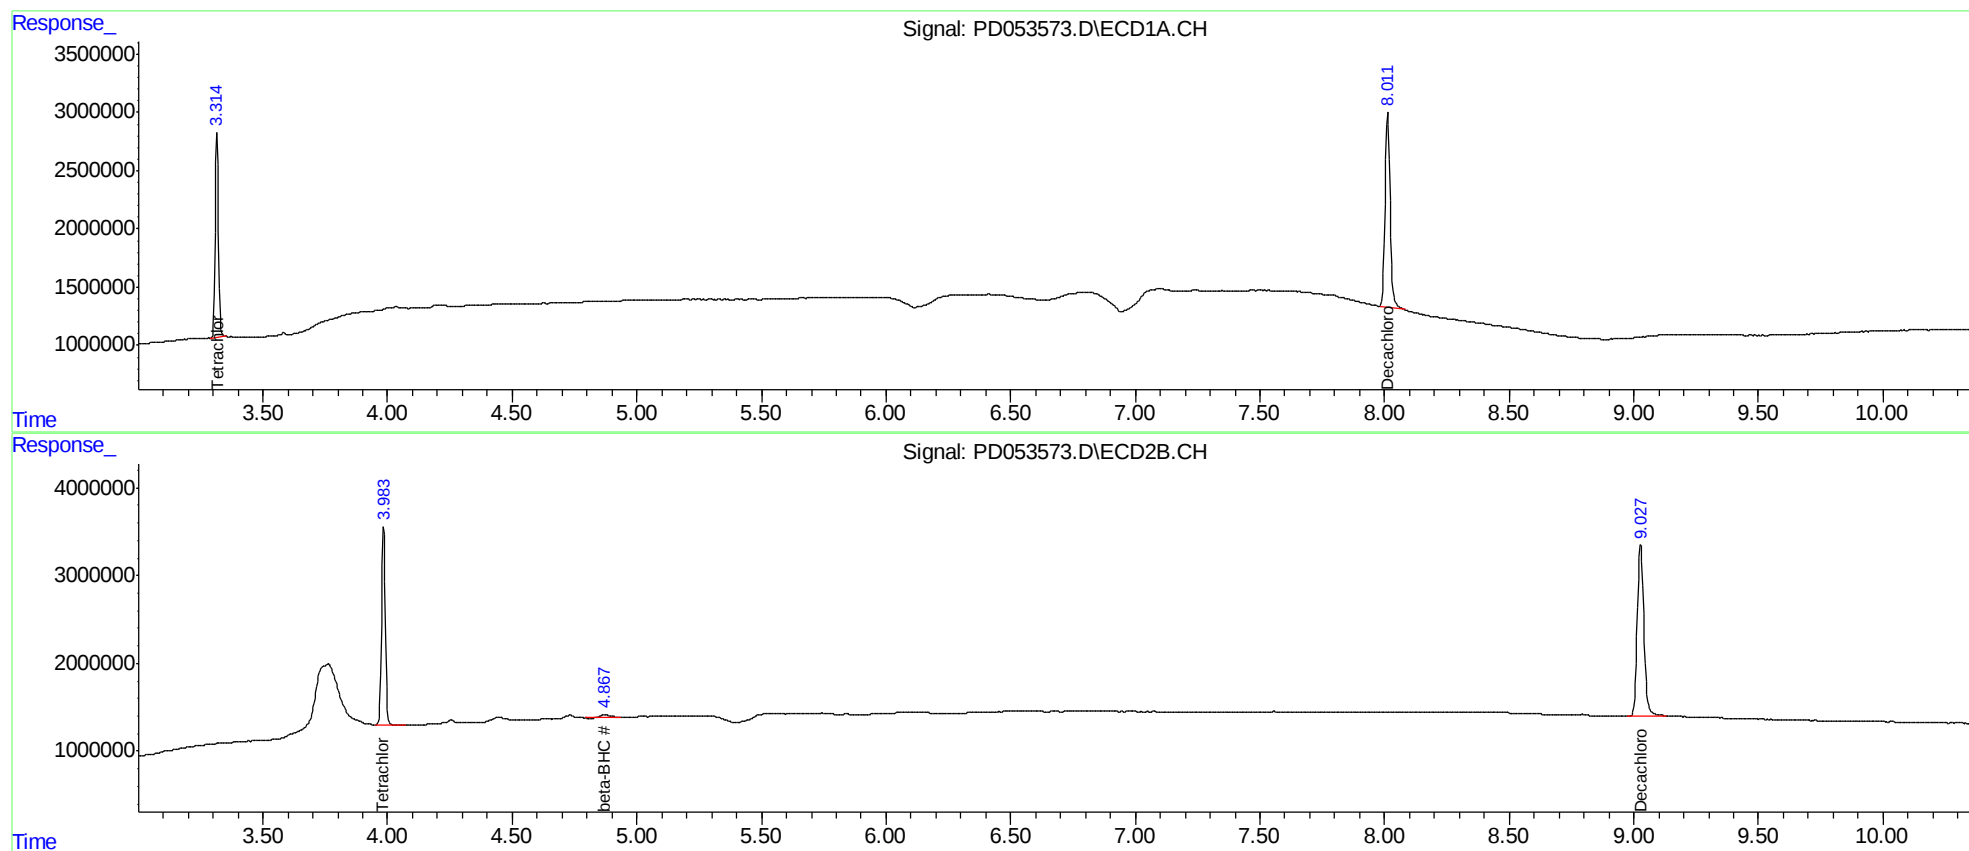


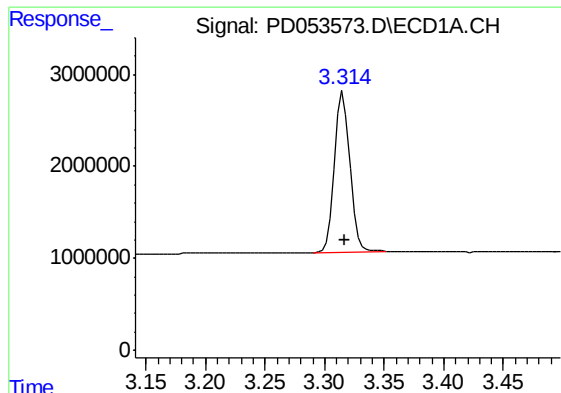

#1 Tetrachloro-m-xylene


R.T.: 3.316 min
Delta R.T.: -0.001 min
Response: 15511581
Conc: 21.17 ng/ml

Instrument :
ECD_D
ClientSampleId :
PIBLK42

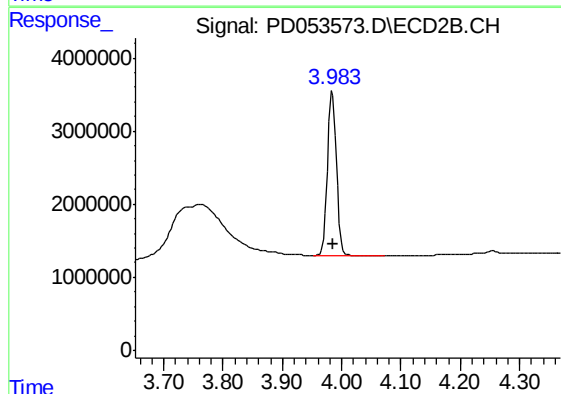


#1 Tetrachloro-m-xylene

R.T.: 3.985 min
Delta R.T.: 0.000 min
Response: 23479368
Conc: 23.85 ng/ml

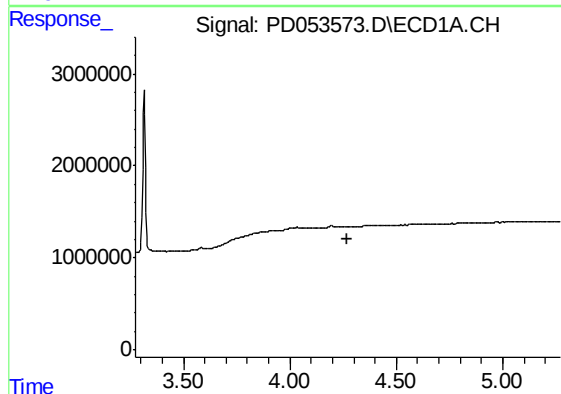


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.272 min
Response: 0
Conc: N.D.

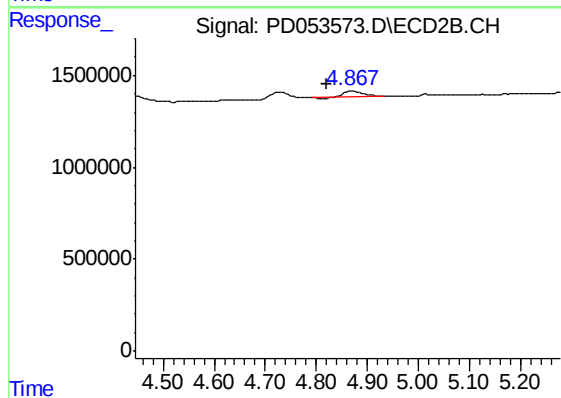

#6 beta-BHC


R.T.: 4.869 min
Delta R.T.: 0.048 min
Response: 862488
Conc: 1.47 ng/ml

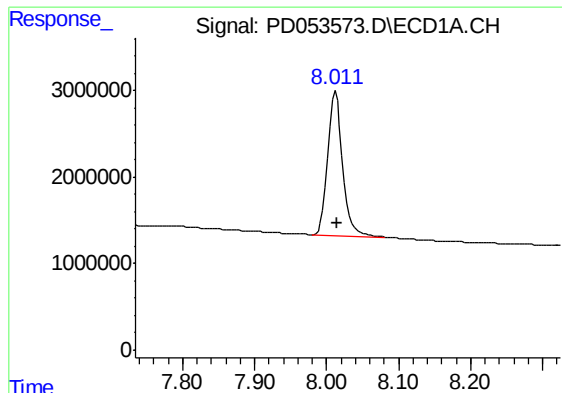

#27 Decachlorobiphenyl

R.T.: 8.013 min
Delta R.T.: -0.002 min
Response: 23791992
Conc: 35.97 ng/ml

Instrument :
ECD_D
ClientSampleId :
PIBLK42

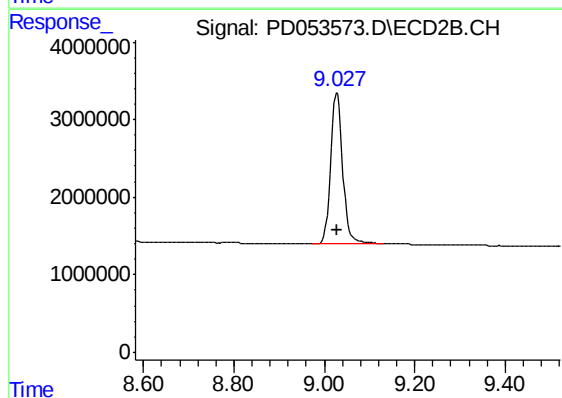

#27 Decachlorobiphenyl

R.T.: 9.028 min
Delta R.T.: -0.001 min
Response: 35897852
Conc: 34.75 ng/ml